

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120319\
 Data File : PD056242.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2019 00:31
 Operator : SG\AJ
 Sample : PIBLK44
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK44

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 01:35:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.291	3.961	18580779	28591120	22.435	23.781
27) SA	Decachlor...	7.970	9.001	38697786	52116056	42.856	43.316
Target Compounds							
6) B	beta-BHC	0.000	4.840f	0	2347212	N.D.	2.848
16) A	4,4'-DDD	0.000	6.736f	0	1112844	N.D.	0.946


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120319\
Data File : PD056242.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2019 00:31
Operator : SG\AJ
Sample : PIBLK44
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK44

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 01:35:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

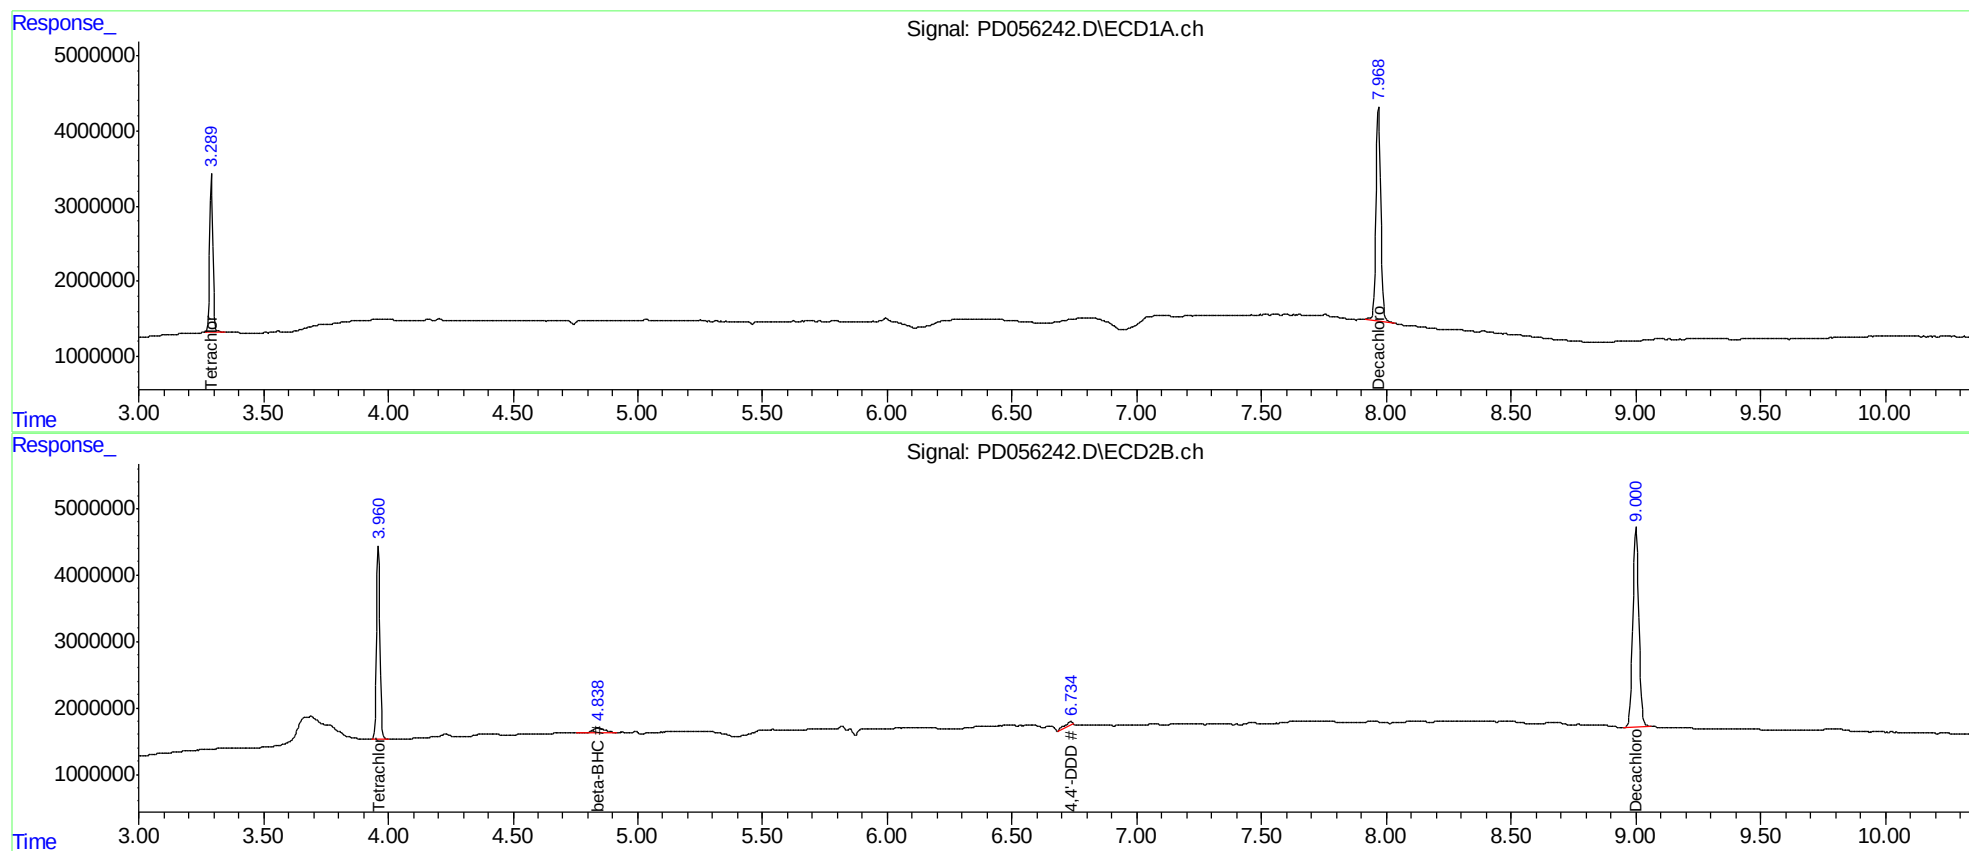


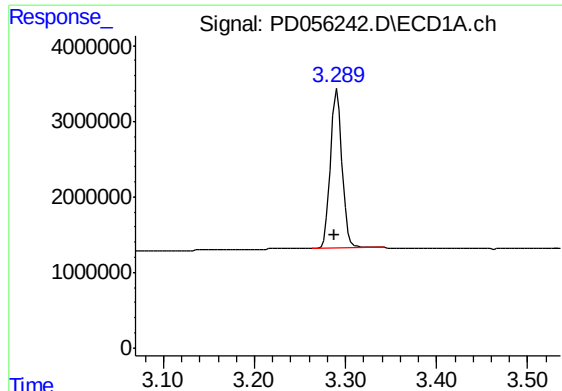

#1 Tetrachloro-m-xylene


R.T.: 3.291 min
Delta R.T.: 0.003 min
Response: 18580779
Conc: 22.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK44

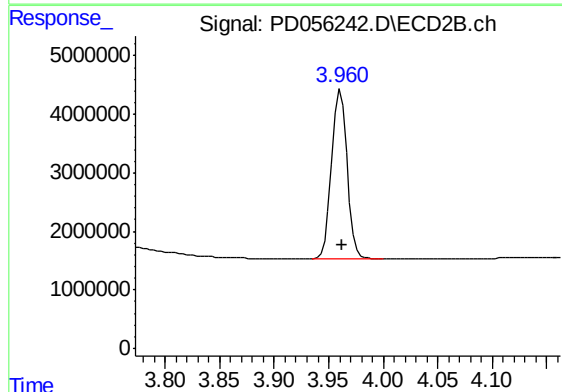


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.002 min
Response: 28591120
Conc: 23.78 ng/ml

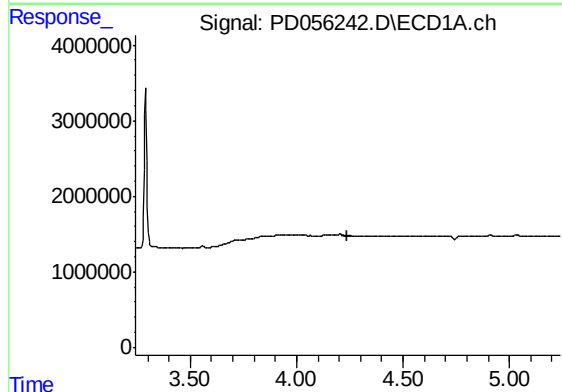


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.240 min
Response: 0
Conc: N.D.

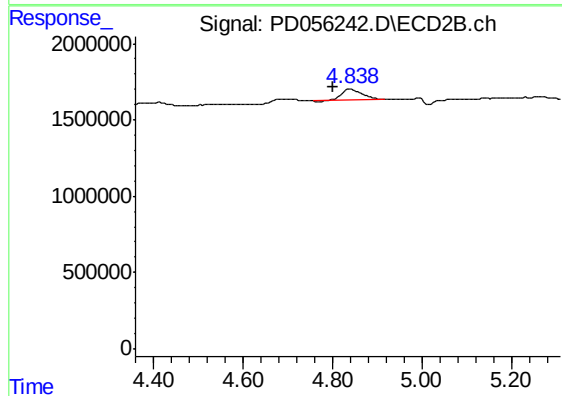

#6 beta-BHC


R.T.: 4.840 min
Delta R.T.: 0.039 min
Response: 2347212
Conc: 2.85 ng/ml

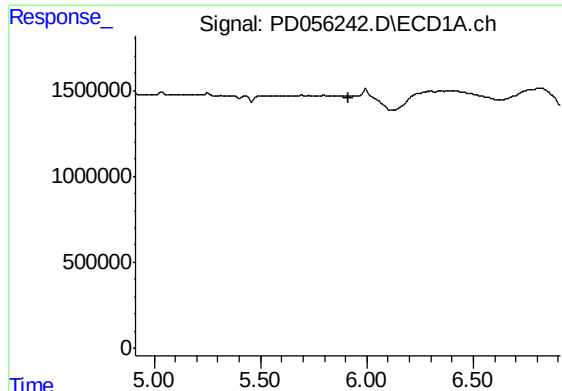

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.912 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK44

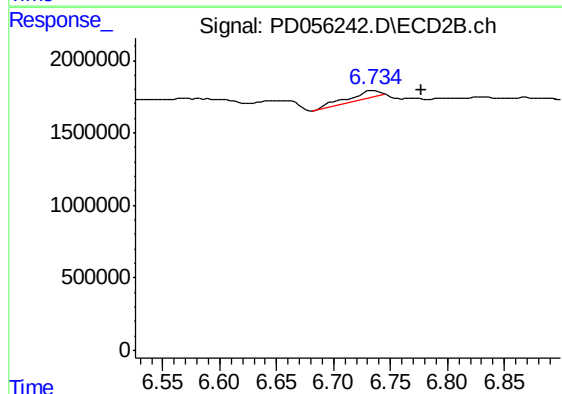


#16 4,4'-DDD

R.T.: 6.736 min
Delta R.T.: -0.042 min
Response: 1112844
Conc: 0.95 ng/ml

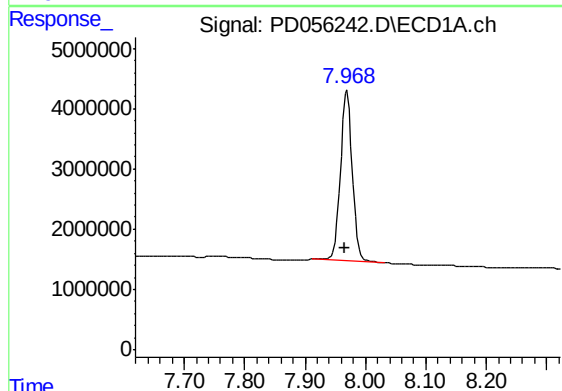

#27 Decachlorobiphenyl

R.T.: 7.970 min
Delta R.T.: 0.004 min
Response: 38697786
Conc: 42.86 ng/ml

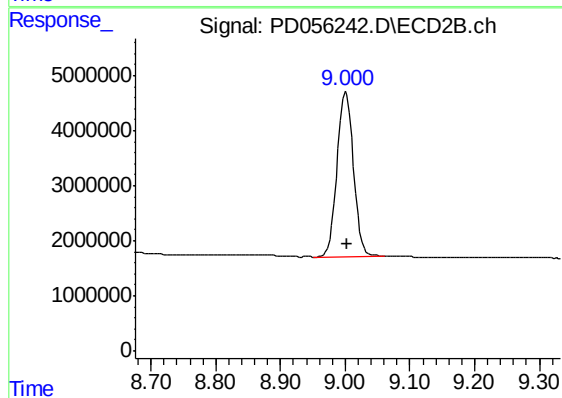

#27 Decachlorobiphenyl

R.T.: 9.001 min
Delta R.T.: -0.001 min
Response: 52116056
Conc: 43.32 ng/ml