

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120319\
 Data File : PD056249.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2019 02:24
 Operator : SG\AJ
 Sample : K6007-20
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BM6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 02:56:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.963	12154110	17959542	14.675	14.938
27)	SA Decachlor...	7.965	9.001	22794694	29696255	25.244	24.682
Target Compounds							
10)	B trans-Chl...	0.000	6.033	0	7093884	N.D.	4.290
15)	B Endosulfa...	0.000	6.875	0	2623870	N.D.	1.791
20)	A Methoxychlor	0.000	7.472f	0	267262	N.D.	0.441


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120319\
Data File : PD056249.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2019 02:24
Operator : SG\AJ
Sample : K6007-20
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0BM6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 02:56:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

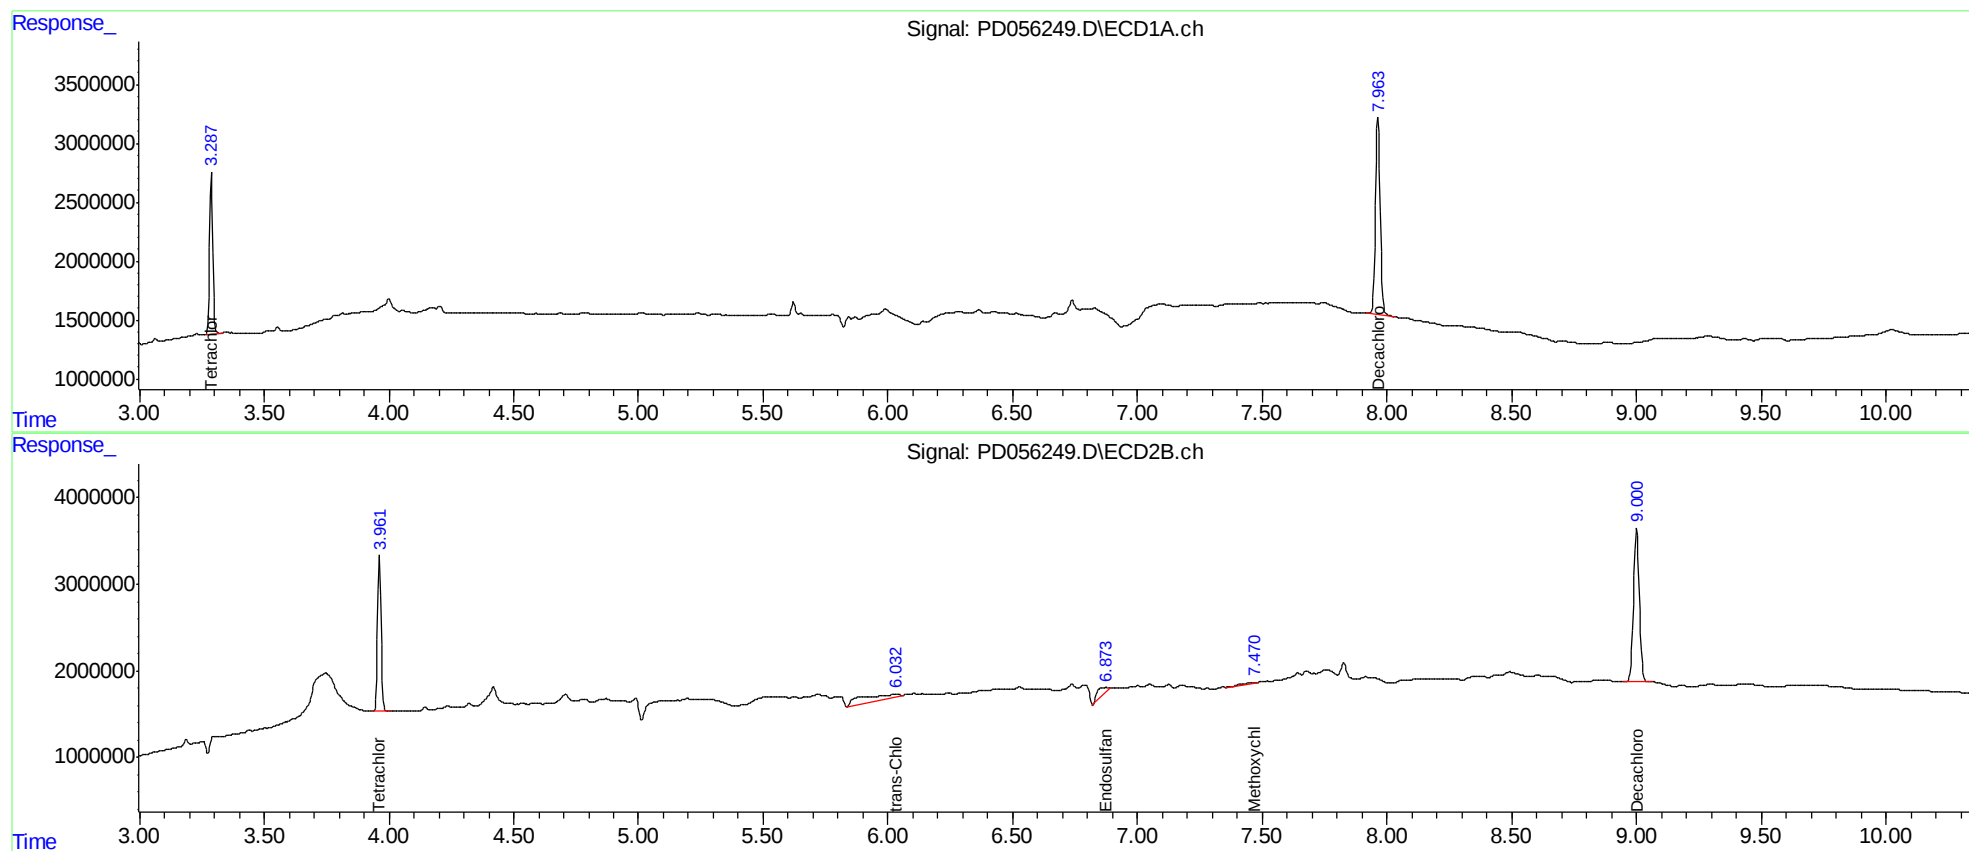


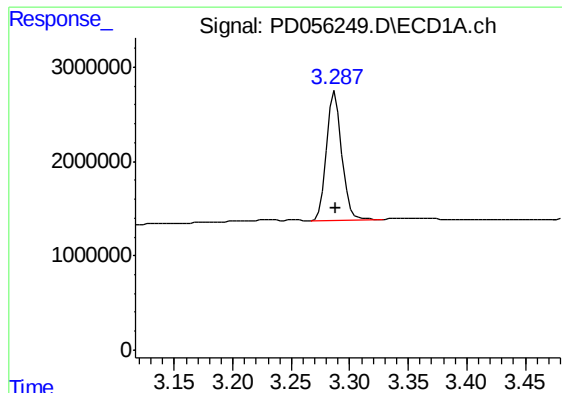

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: 0.000 min
Response: 12154110
Conc: 14.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BM6

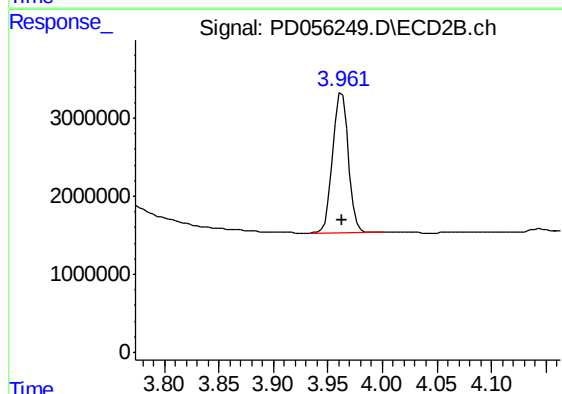


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 17959542
Conc: 14.94 ng/ml

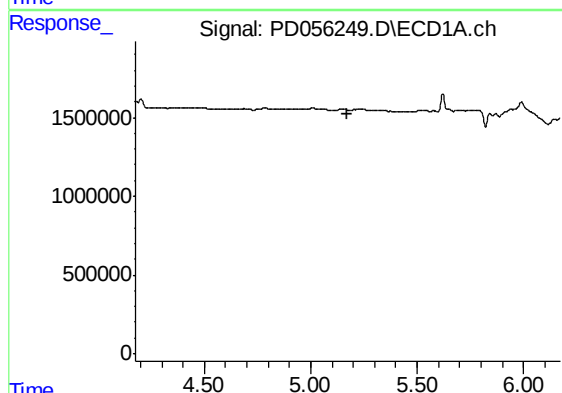


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.175 min
Response: 0
Conc: N.D.

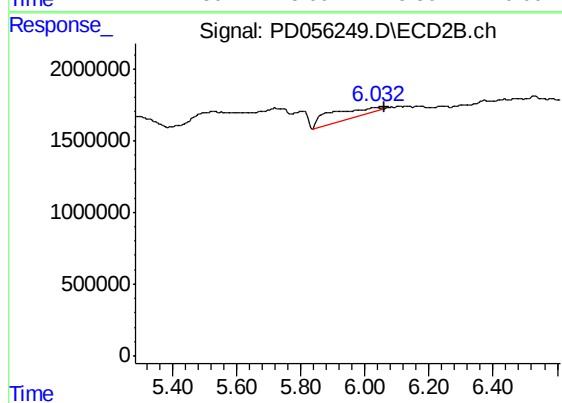

#10 trans-Chlordane


R.T.: 6.033 min
Delta R.T.: -0.027 min
Response: 7093884
Conc: 4.29 ng/ml

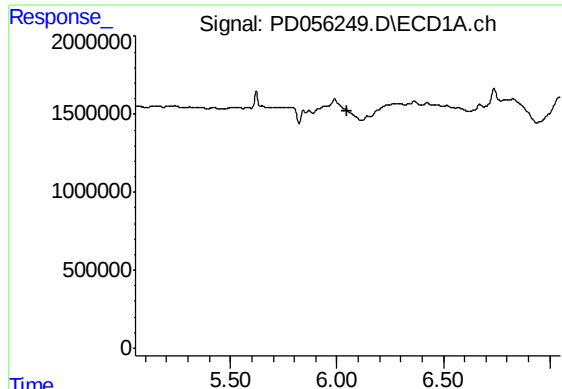

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BM6

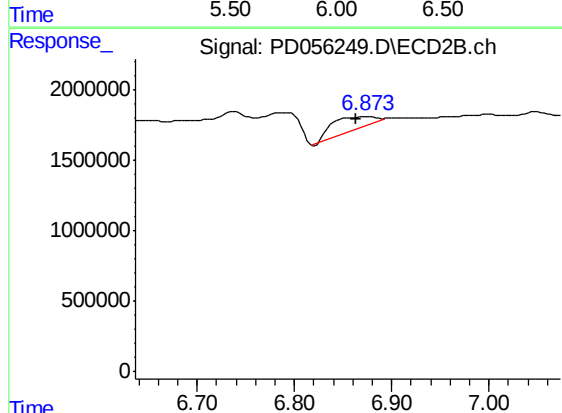


#15 Endosulfan II

R.T.: 6.875 min
Delta R.T.: 0.011 min
Response: 2623870
Conc: 1.79 ng/ml

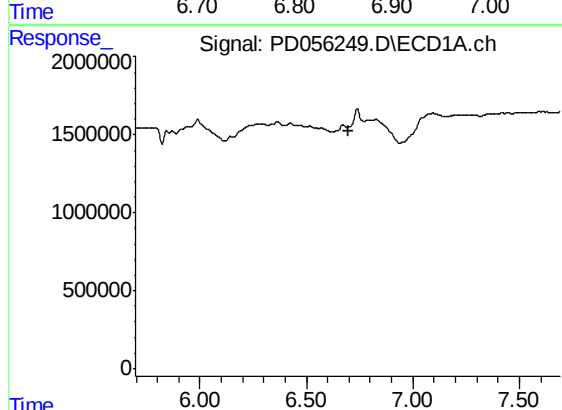


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.696 min
Response: 0
Conc: N.D.

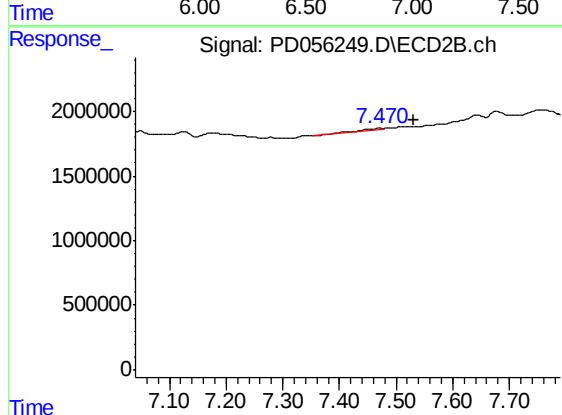

#20 Methoxychlor


R.T.: 7.472 min
Delta R.T.: -0.061 min
Response: 267262
Conc: 0.44 ng/ml

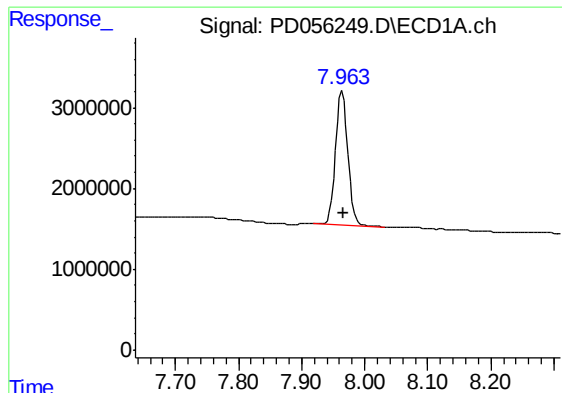

#27 Decachlorobiphenyl

R.T.: 7.965 min
Delta R.T.: 0.000 min
Response: 22794694
Conc: 25.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BM6

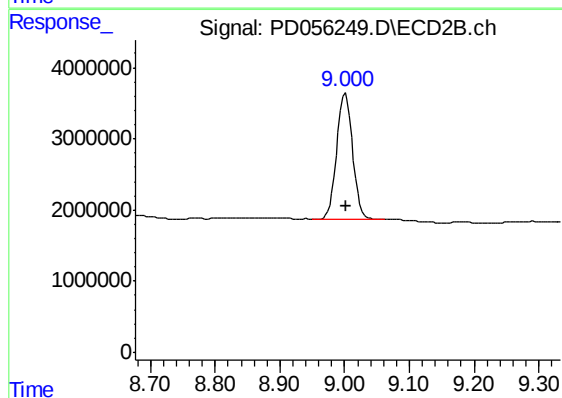

#27 Decachlorobiphenyl

R.T.: 9.001 min
Delta R.T.: -0.002 min
Response: 29696255
Conc: 24.68 ng/ml