

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120319\
 Data File : PD056256.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2019 04:02
 Operator : SG\AJ
 Sample : K6007-06
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BL4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 04:42:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.962	15608221	23526935	18.846	19.569
27)	SA Decachlor...	7.965	9.002	30114999	35879797	33.351	29.822
Target Compounds							
3)	MA gamma-BHC...	0.000	4.613	0	545442	N.D.	0.338
7)	B delta-BHC	0.000	5.047f	0	774856	N.D.	0.465
9)	A Endosulfan I	0.000	6.218f	0	173540	N.D.	0.120
10)	B trans-Chl...	0.000	6.046	0	4531213	N.D.	2.740
13)	MA Dieldrin	5.508	6.429	1851218	824911	1.822	0.525 #
14)	MA Endrin	5.836f	0.000	2702867	0	3.234	N.D. #
15)	B Endosulfa...	0.000	6.850	0	574430	N.D.	0.392
16)	A 4,4'-DDD	0.000	6.782	0	4812468	N.D.	4.090
17)	MA 4,4'-DDT	6.141	7.126f	2366463	1432397	3.363	1.212 #
19)	B Endosulfa...	0.000	7.182	0	410921	N.D.	0.307
20)	A Methoxychlor	6.670	7.577f	3022834	1154842	8.919	1.906 #
22)	Toxaphene-1	5.508	6.369	1851218	808823	205.466	72.043 #
25)	Toxaphene-4	6.141	7.126	2366463	1432397	95.517	25.942 #
26)	Toxaphene-5	0.000	7.577	0	1154842	N.D.	45.183


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120319\
Data File : PD056256.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2019 04:02
Operator : SG\AJ
Sample : K6007-06
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0BL4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 04:42:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

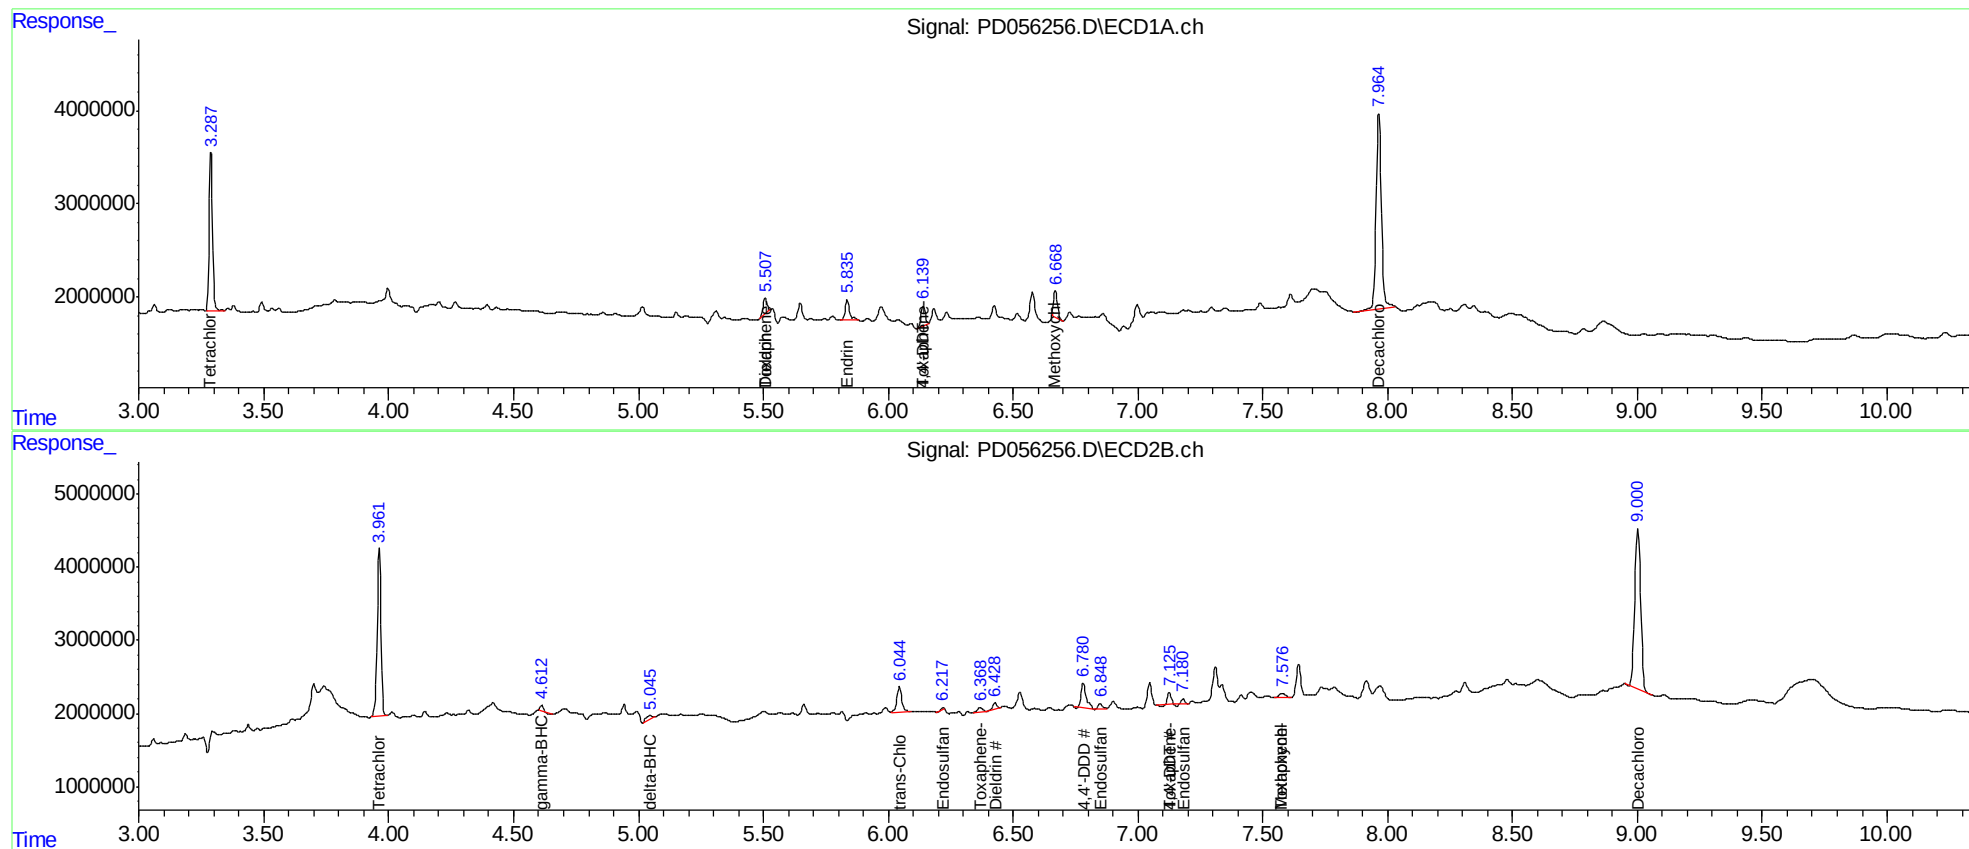




#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: 0.000 min
Response: 15608221
Conc: 18.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BL4

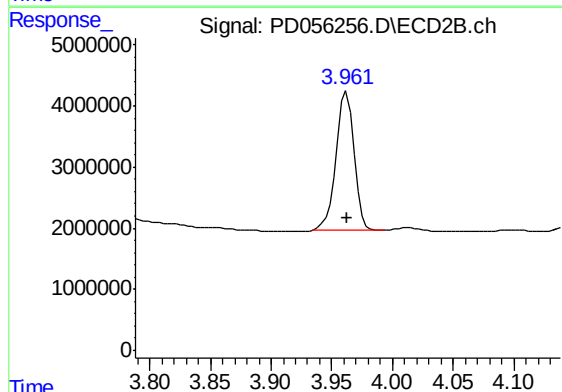


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 23526935
Conc: 19.57 ng/ml




#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.991 min
Response: 0
Conc: N.D.

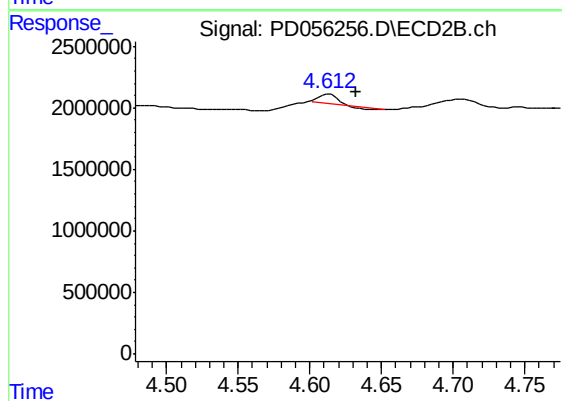

#3 gamma-BHC (Lindane)


R.T.: 4.613 min
Delta R.T.: -0.019 min
Response: 545442
Conc: 0.34 ng/ml



#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.436 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BL4

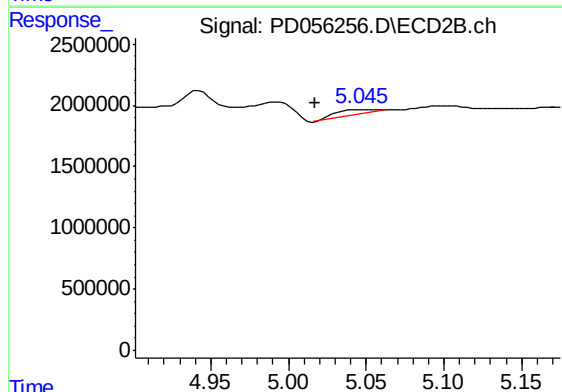


#7 delta-BHC

R.T.: 5.047 min
Delta R.T.: 0.030 min
Response: 774856
Conc: 0.47 ng/ml




#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.284 min
Response: 0
Conc: N.D.

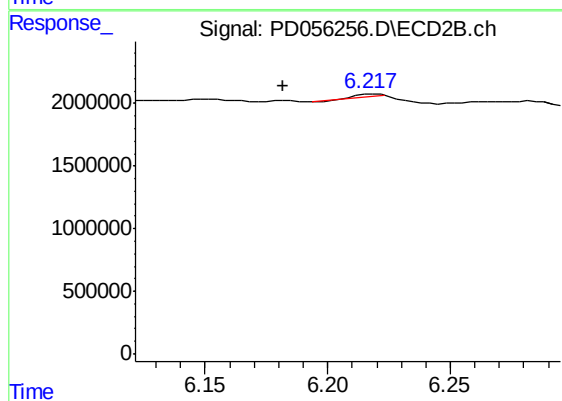

#9 Endosulfan I


R.T.: 6.218 min
Delta R.T.: 0.036 min
Response: 173540
Conc: 0.12 ng/ml



#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BL4

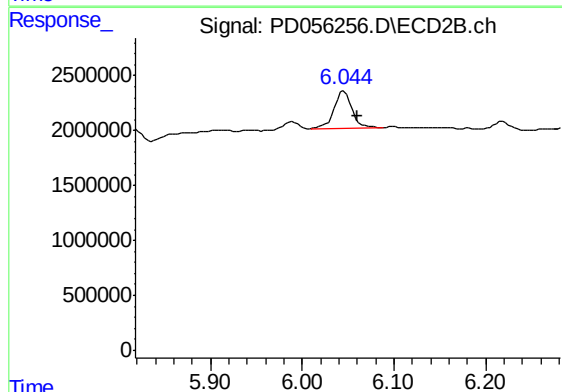


#10 trans-Chlordane

R.T.: 6.046 min
Delta R.T.: -0.014 min
Response: 4531213
Conc: 2.74 ng/ml




#13 Dieldrin

R.T.: 5.508 min
Delta R.T.: -0.016 min
Response: 1851218
Conc: 1.82 ng/ml

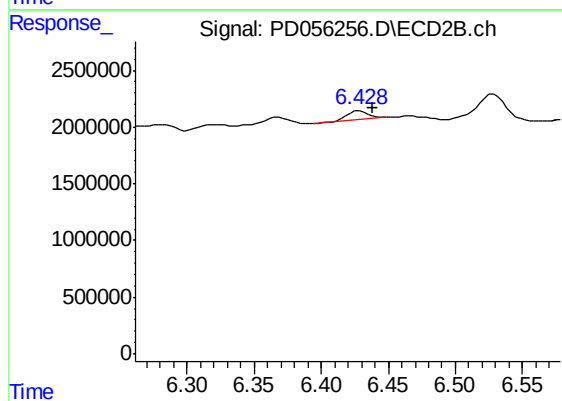

#13 Dieldrin


R.T.: 6.429 min
Delta R.T.: -0.009 min
Response: 824911
Conc: 0.52 ng/ml

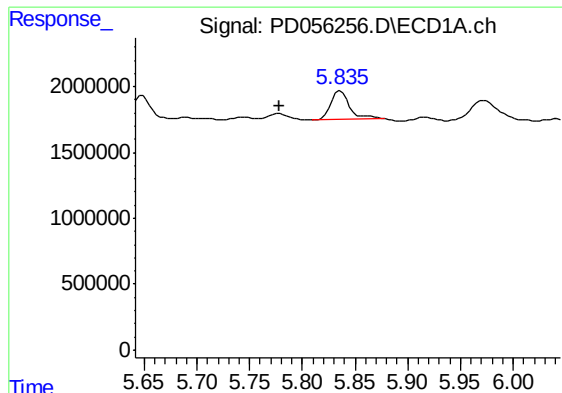

#14 Endrin


R.T.: 5.836 min
Delta R.T.: 0.059 min
Response: 2702867
Conc: 3.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BL4

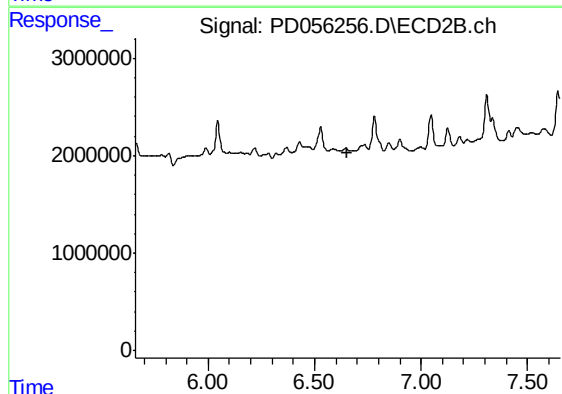


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.655 min
Response: 0
Conc: N.D.




#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.051 min
Response: 0
Conc: N.D.

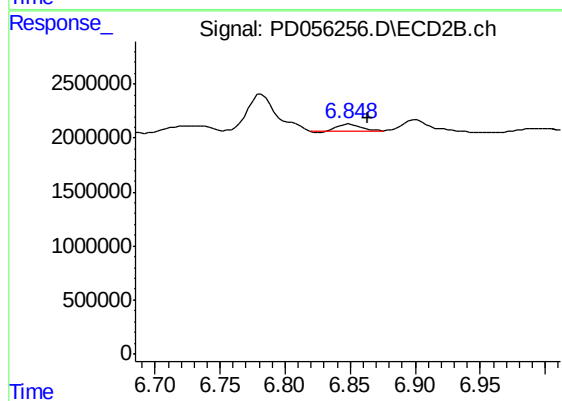

#15 Endosulfan II


R.T.: 6.850 min
Delta R.T.: -0.014 min
Response: 574430
Conc: 0.39 ng/ml

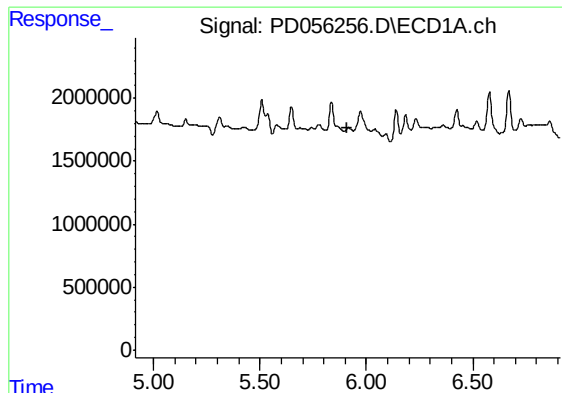

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.912 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BL4

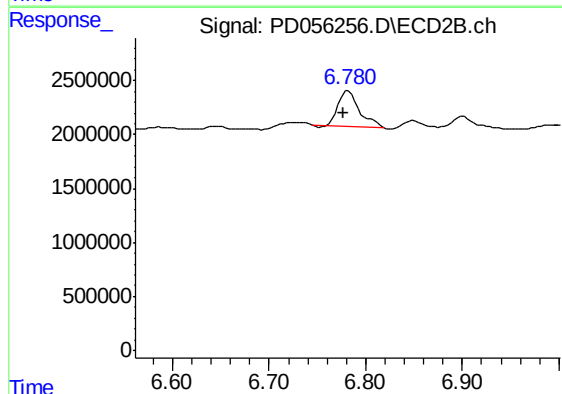


#16 4,4'-DDD

R.T.: 6.782 min
Delta R.T.: 0.004 min
Response: 4812468
Conc: 4.09 ng/ml

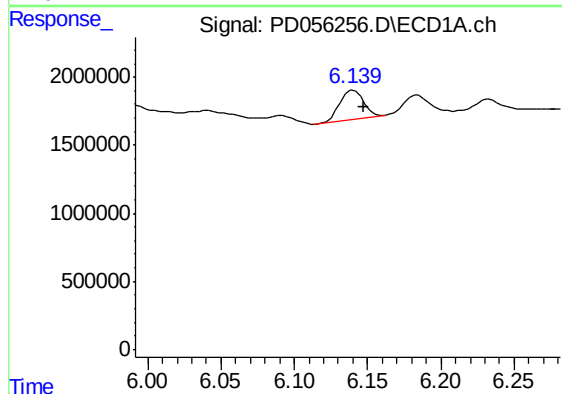


#17 4,4'-DDT

R.T.: 6.141 min
Delta R.T.: -0.007 min
Response: 2366463
Conc: 3.36 ng/ml

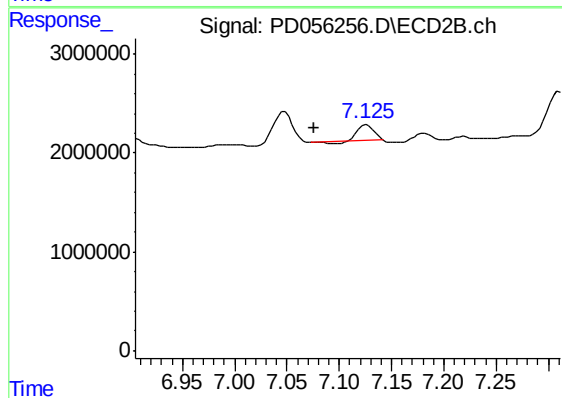

#17 4,4'-DDT


R.T.: 7.126 min
Delta R.T.: 0.051 min
Response: 1432397
Conc: 1.21 ng/ml



#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BL4

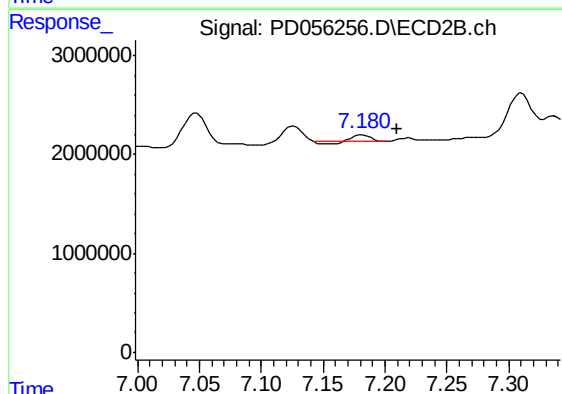


#19 Endosulfan Sulfate

R.T.: 7.182 min
Delta R.T.: -0.028 min
Response: 410921
Conc: 0.31 ng/ml

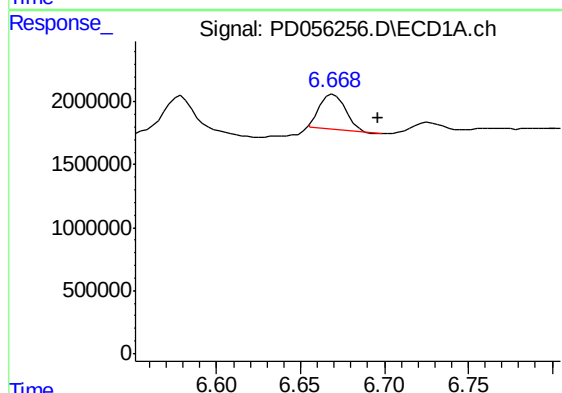


#20 Methoxychlor

R.T.: 6.670 min
Delta R.T.: -0.026 min
Response: 3022834
Conc: 8.92 ng/ml

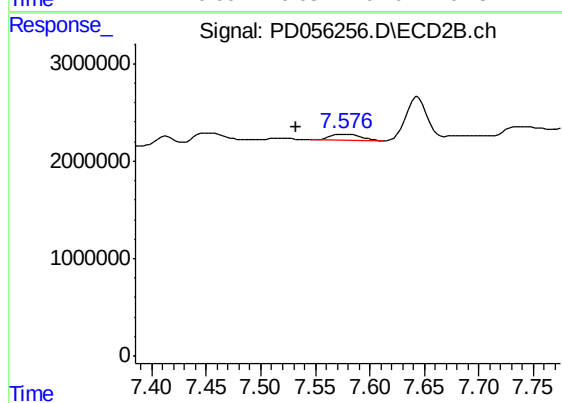

#20 Methoxychlor


R.T.: 7.577 min
Delta R.T.: 0.045 min
Response: 1154842
Conc: 1.91 ng/ml

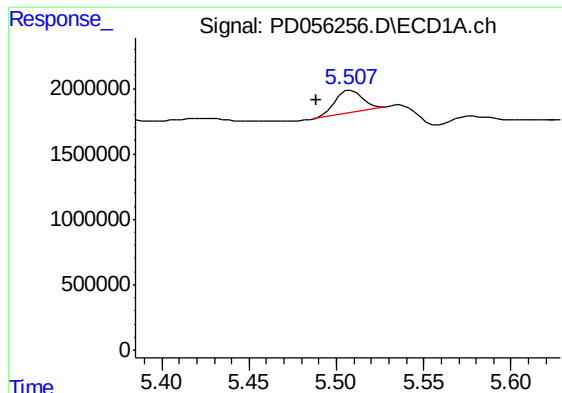

#22 Toxaphene-1


R.T.: 5.508 min
Delta R.T.: 0.020 min
Response: 1851218
Conc: 205.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BL4

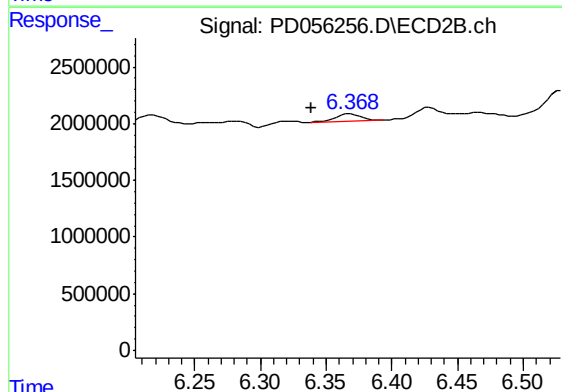


#22 Toxaphene-1

R.T.: 6.369 min
Delta R.T.: 0.030 min
Response: 808823
Conc: 72.04 ng/ml




#25 Toxaphene-4

R.T.: 6.141 min
Delta R.T.: 0.058 min
Response: 2366463
Conc: 95.52 ng/ml

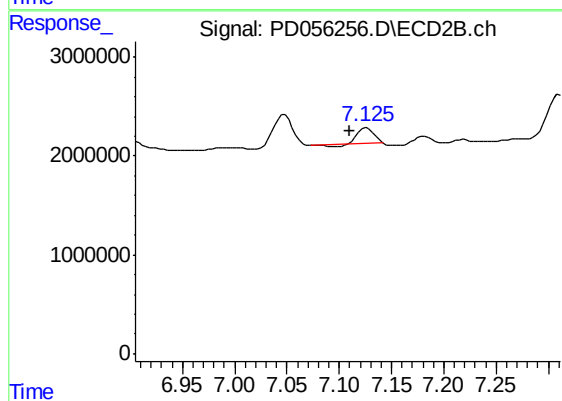

#25 Toxaphene-4


R.T.: 7.126 min
Delta R.T.: 0.017 min
Response: 1432397
Conc: 25.94 ng/ml



#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T.: 6.808 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BL4

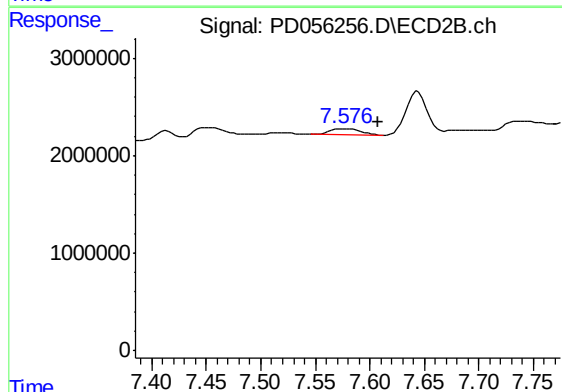


#26 Toxaphene-5

R.T.: 7.577 min
Delta R.T.: -0.030 min
Response: 1154842
Conc: 45.18 ng/ml



#27 Decachlorobiphenyl

R.T.: 7.965 min
Delta R.T.: 0.000 min
Response: 30114999
Conc: 33.35 ng/ml

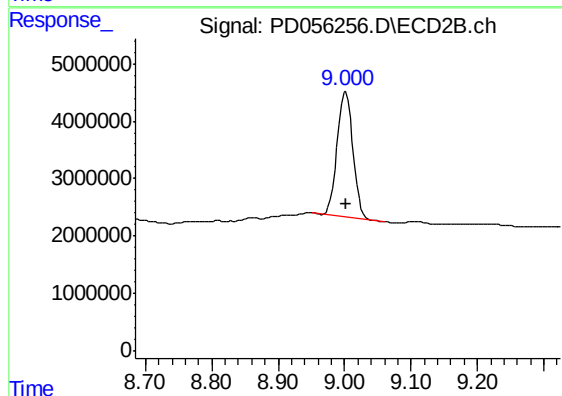

#27 Decachlorobiphenyl

R.T.: 9.002 min
Delta R.T.: 0.000 min
Response: 35879797
Conc: 29.82 ng/ml