

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120319\
 Data File : PD056258.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2019 04:30
 Operator : SG\AJ
 Sample : PIBLK45
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK45

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 04:43:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.288	3.962	18630165	27589710	22.495	22.948
27) SA	Decachlor...	7.965	9.001	37689821	49094969	41.740	40.805
Target Compounds							
8) B	Heptachlo...	0.000	5.821	0	1222986	N.D.	0.789
16) A	4,4'-DDD	0.000	6.738f	0	1751481	N.D.	1.488
20) A	Methoxychlor	0.000	7.464f	0	584718	N.D.	0.965


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120319\
Data File : PD056258.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2019 04:30
Operator : SG\AJ
Sample : PIBLK45
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK45

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 04:43:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

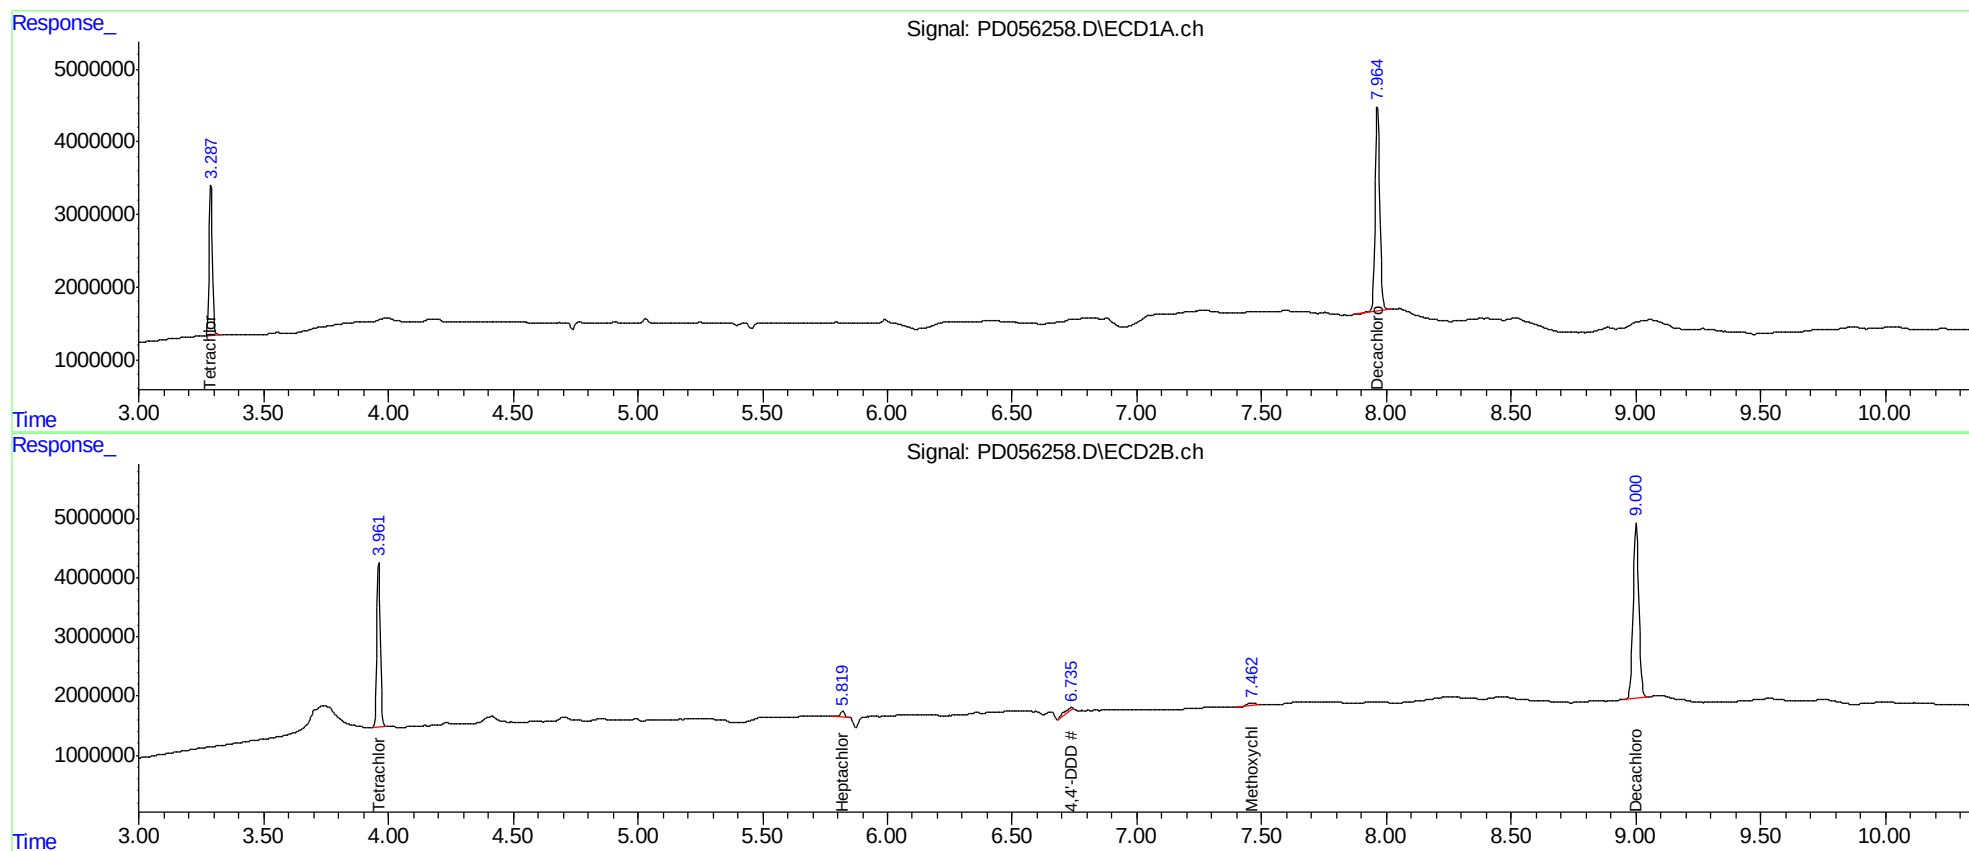


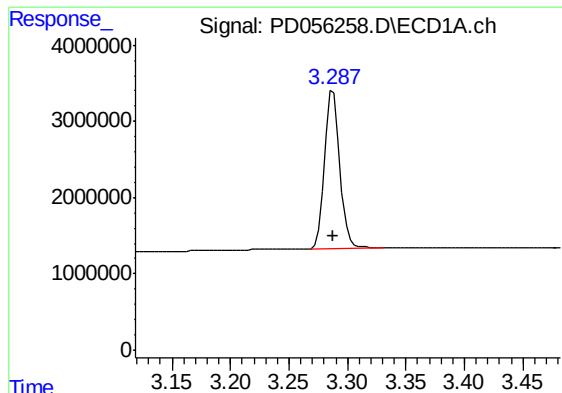

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: 0.000 min
Response: 18630165
Conc: 22.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK45

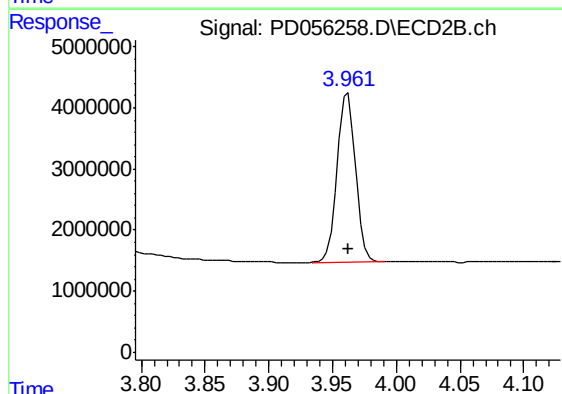


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 27589710
Conc: 22.95 ng/ml

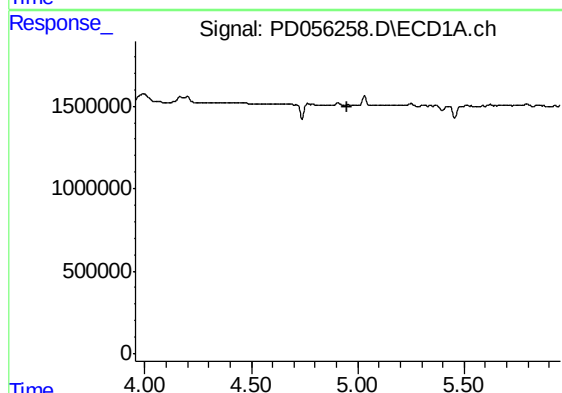


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

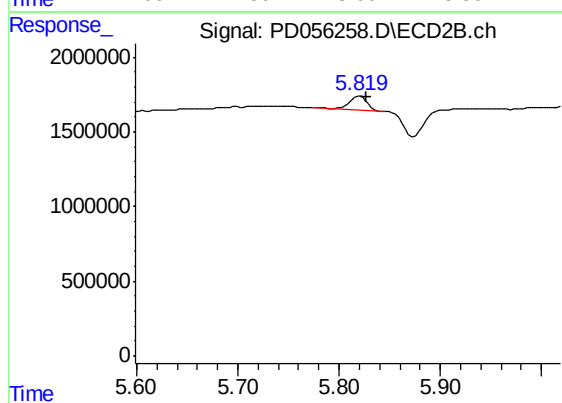

#8 Heptachlor epoxide


R.T.: 5.821 min
Delta R.T.: -0.006 min
Response: 1222986
Conc: 0.79 ng/ml

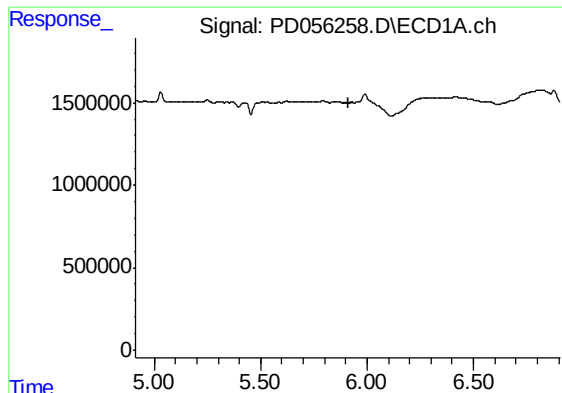

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 5.912 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK45

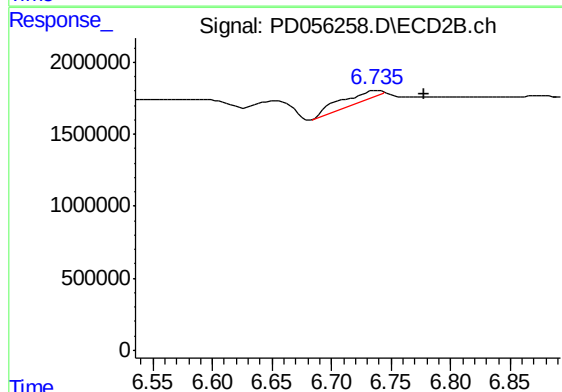


#16 4,4'-DDD

R.T.: 6.738 min
Delta R.T.: -0.039 min
Response: 1751481
Conc: 1.49 ng/ml

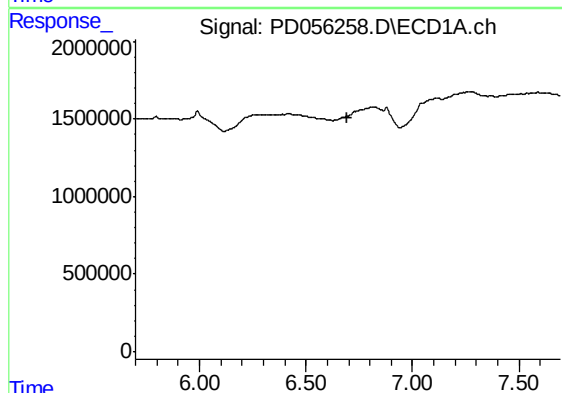


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.696 min
Response: 0
Conc: N.D.

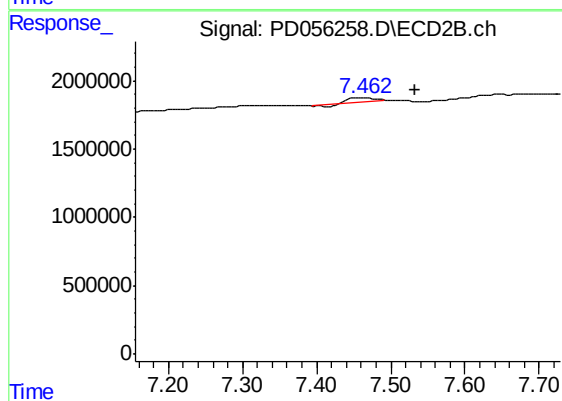

#20 Methoxychlor


R.T.: 7.464 min
Delta R.T.: -0.068 min
Response: 584718
Conc: 0.97 ng/ml

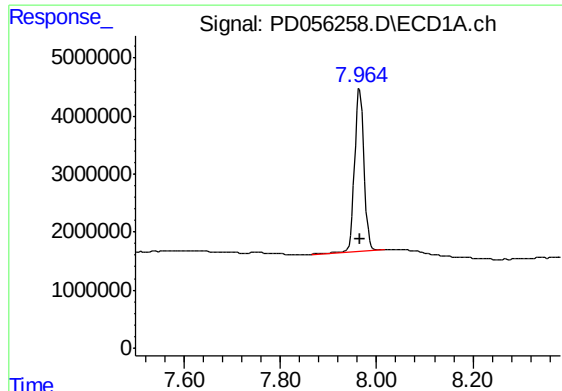

#27 Decachlorobiphenyl

R.T.: 7.965 min
Delta R.T.: 0.000 min
Response: 37689821
Conc: 41.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK45

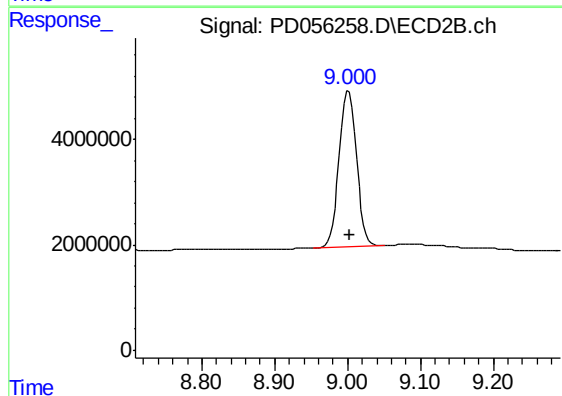

#27 Decachlorobiphenyl

R.T.: 9.001 min
Delta R.T.: 0.000 min
Response: 49094969
Conc: 40.81 ng/ml