

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120320\
 Data File : PD060560.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2020 10:28
 Operator : DD\AJ
 Sample : L4865-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleID :
 C0B88

Manual Integrations
 APPROVED

mohammad
 12/4/2020 12:33:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 00:31:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 28 01:50:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.504	4.022	10552088	35815179	9.266	9.742
2) SA Decachlor...	8.291	9.107	17391539	35979832	12.843	12.414
Target Compounds						
12) B 4,4'-DDE	5.683	6.362	1049773	3938418	0.735m	0.991m#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120320\
Data File : PD060560.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2020 10:28
Operator : DD\AJ
Sample : L4865-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 00:31:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112720CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 28 01:50:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

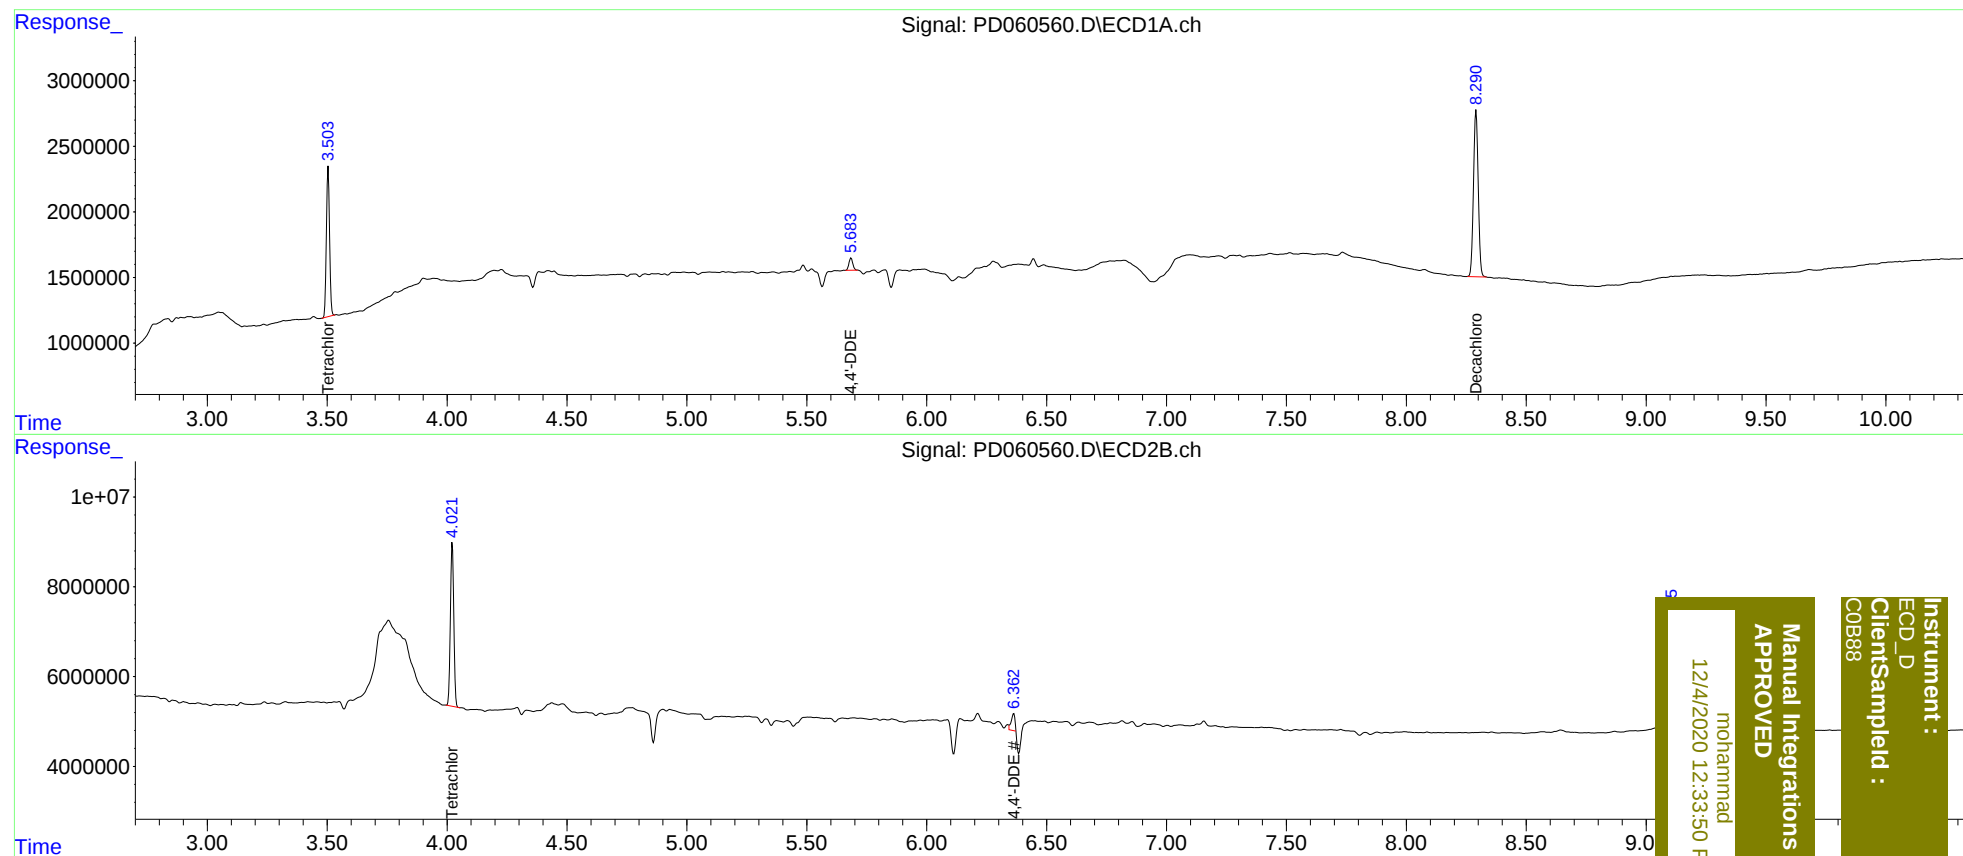

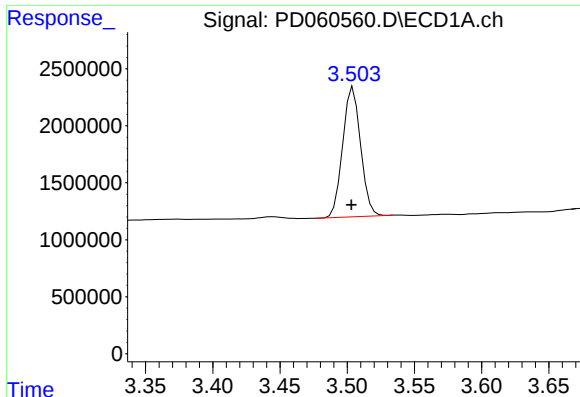


#1 Tetrachloro-m-xylene

R.T.: 3.504 min
Delta R.T.: 0.001 min
Response: 10552088
Conc: 9.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0B88


Manual Integrations
APPROVED

mohammad
12/4/2020 12:33:50 PM

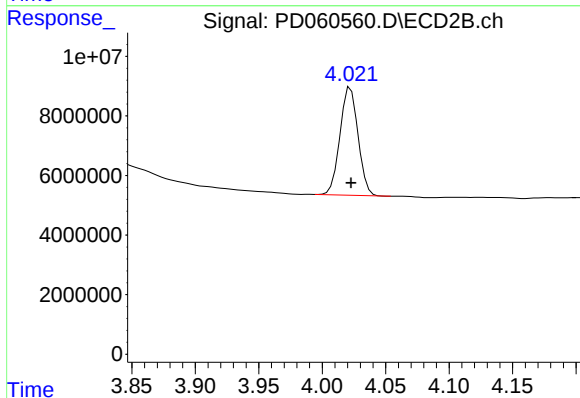


#1 Tetrachloro-m-xylene

R.T.: 4.022 min
Delta R.T.: 0.000 min
Response: 35815179
Conc: 9.74 ng/ml

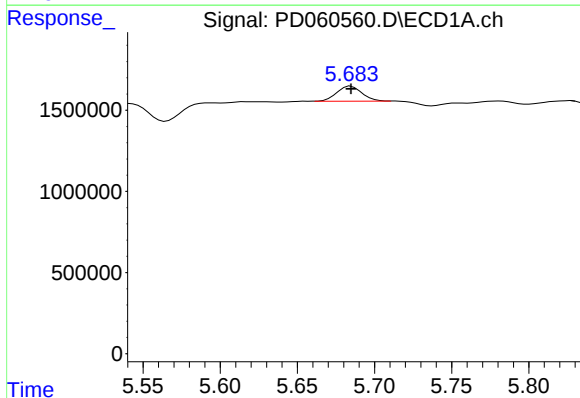


#12 4,4'-DDE

R.T.: 5.683 min
Delta R.T.: -0.001 min
Response: 1049773
Conc: 0.73 ng/ml m

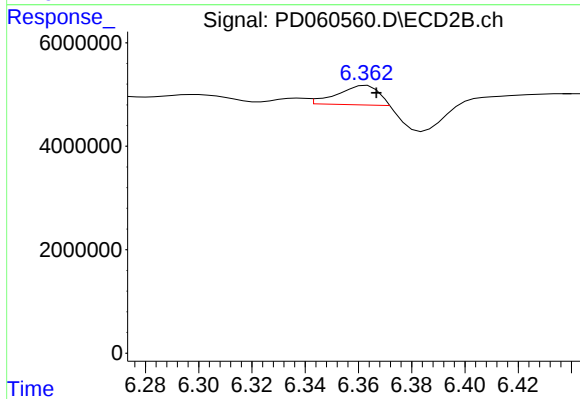

#12 4,4'-DDE

R.T.: 6.362 min
Delta R.T.: -0.005 min
Response: 3938418
Conc: 0.99 ng/ml m

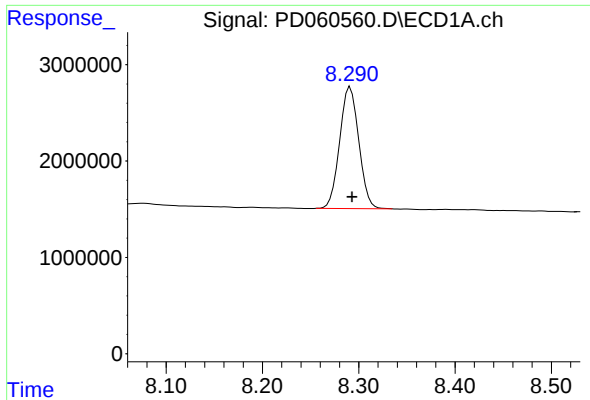


#27 Decachlorobiphenyl

R.T.: 8.291 min
Delta R.T.: -0.002 min
Response: 17391539
Conc: 12.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0B88

Manual Integrations
APPROVED

mohammad
12/4/2020 12:33:50 PM

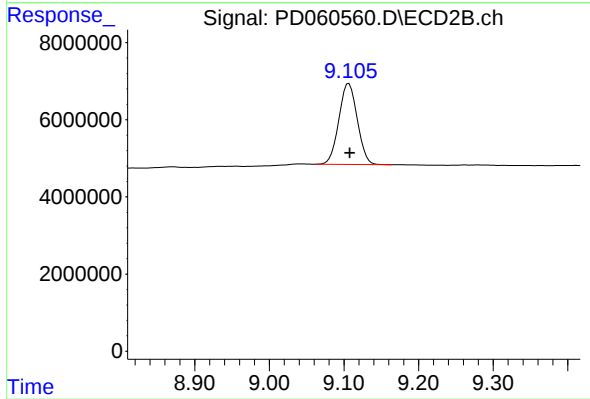

#27 Decachlorobiphenyl

R.T.: 9.107 min
Delta R.T.: -0.001 min
Response: 35979832
Conc: 12.41 ng/ml