

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120321\
 Data File : PD067217.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2021 17:07
 Operator : AR\AJ
 Sample : M4833-11 2X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ESQM9

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/03/2021
 Supervised By :mohammad ahmed 12/06/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 04:57:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 05:28:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.437	3.967	12585184	49703536	5.764	6.204
2) SA Decachlor...	8.163	9.026	9811407	53125446	8.642	10.477
Target Compounds						
11) B cis-Chlor...	5.421	6.144	97563689	27612186	35.160m	3.732 #
12) B 4,4'-DDE	5.579	6.305	24806062	360.0E6	9.912m	53.720 #
16) A 4,4'-DDD	6.094	6.800	44341369	221.1E6	20.973m	37.812 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120321\
Data File : PD067217.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2021 17:07
Operator : AR\AJ
Sample : M4833-11 2X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 04:57:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:28:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

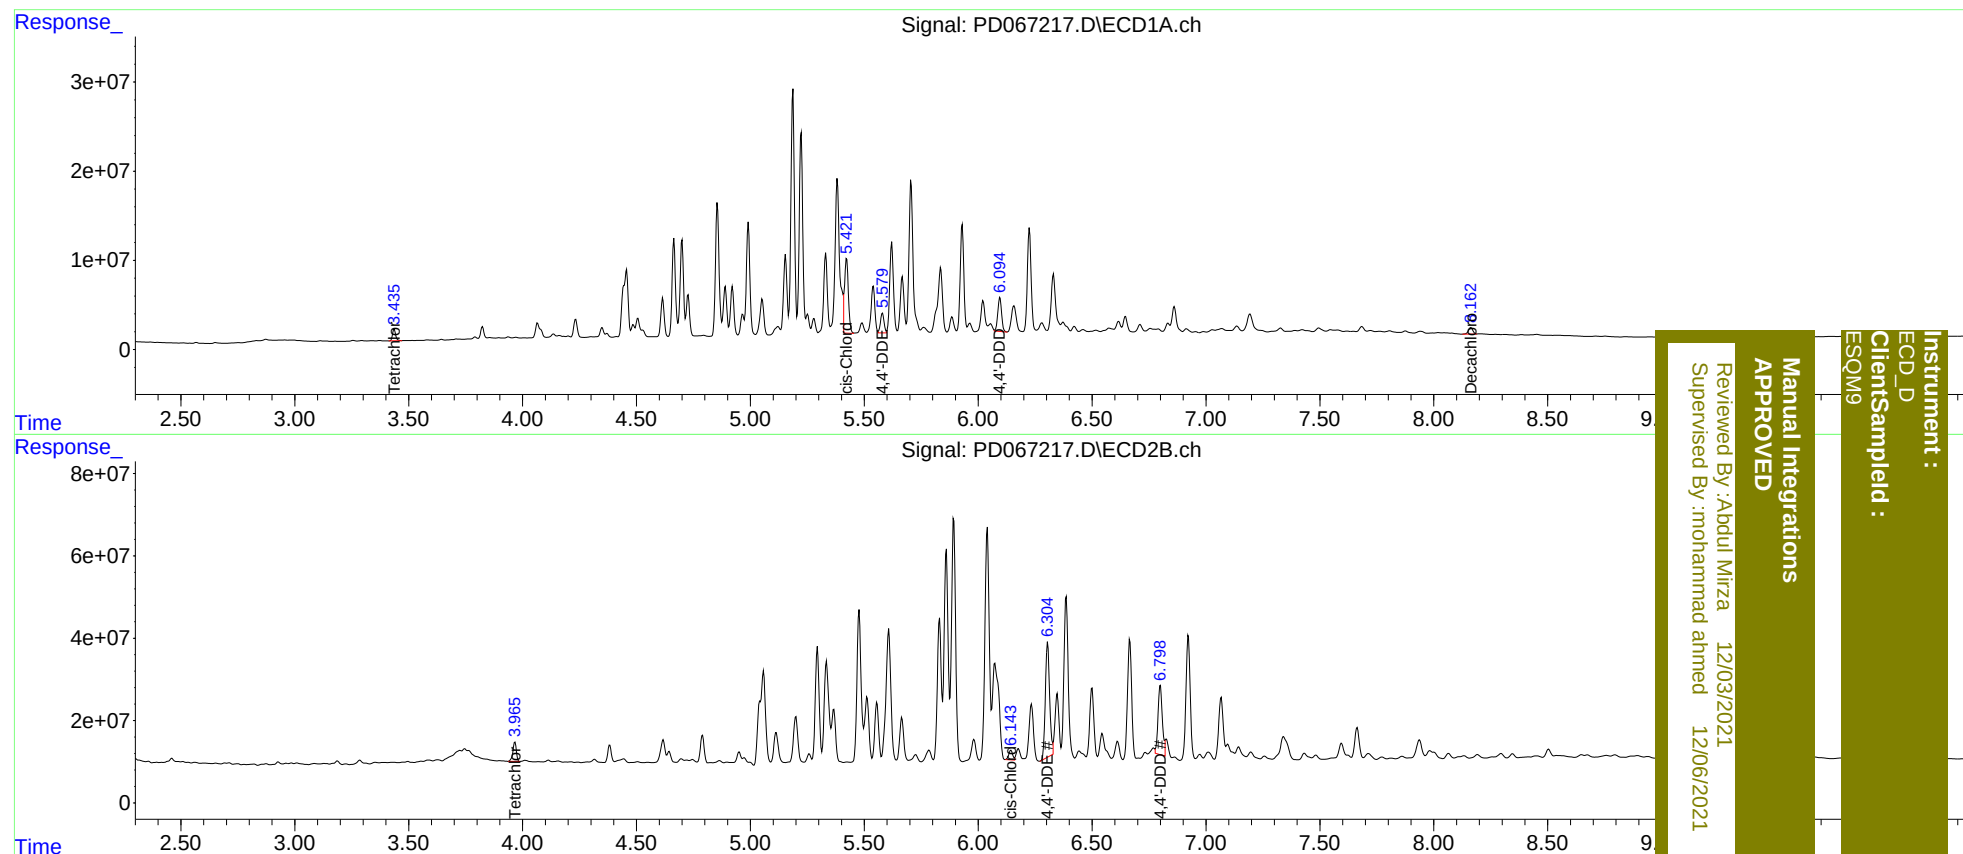

Reviewed By: Abdul Mirza 12/03/2021
Supervised By: mohammad ahmed 12/06/2021

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
ESQM9