

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120418\
 Data File : PD050659.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Dec 2018 18:12
 Operator : AJ\SJ
 Sample : J6203-06
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 03:01:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120318CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 04 00:43:01 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
27) SA Decachlor...	0.000	9.142	0	5200062	N.D.	0.240
Target Compounds						
6) B beta-BHC	0.000	4.940f	0	25351800	N.D.	1.575
7) B delta-BHC	0.000	5.086	0	10926152	N.D.	0.274
15) B Endosulfa...	0.000	6.970	0	6904116	N.D.	0.275

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120418\
Data File : PD050659.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Dec 2018 18:12
Operator : AJ\SJ
Sample : J6203-06
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 03:01:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120318CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 04 00:43:01 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

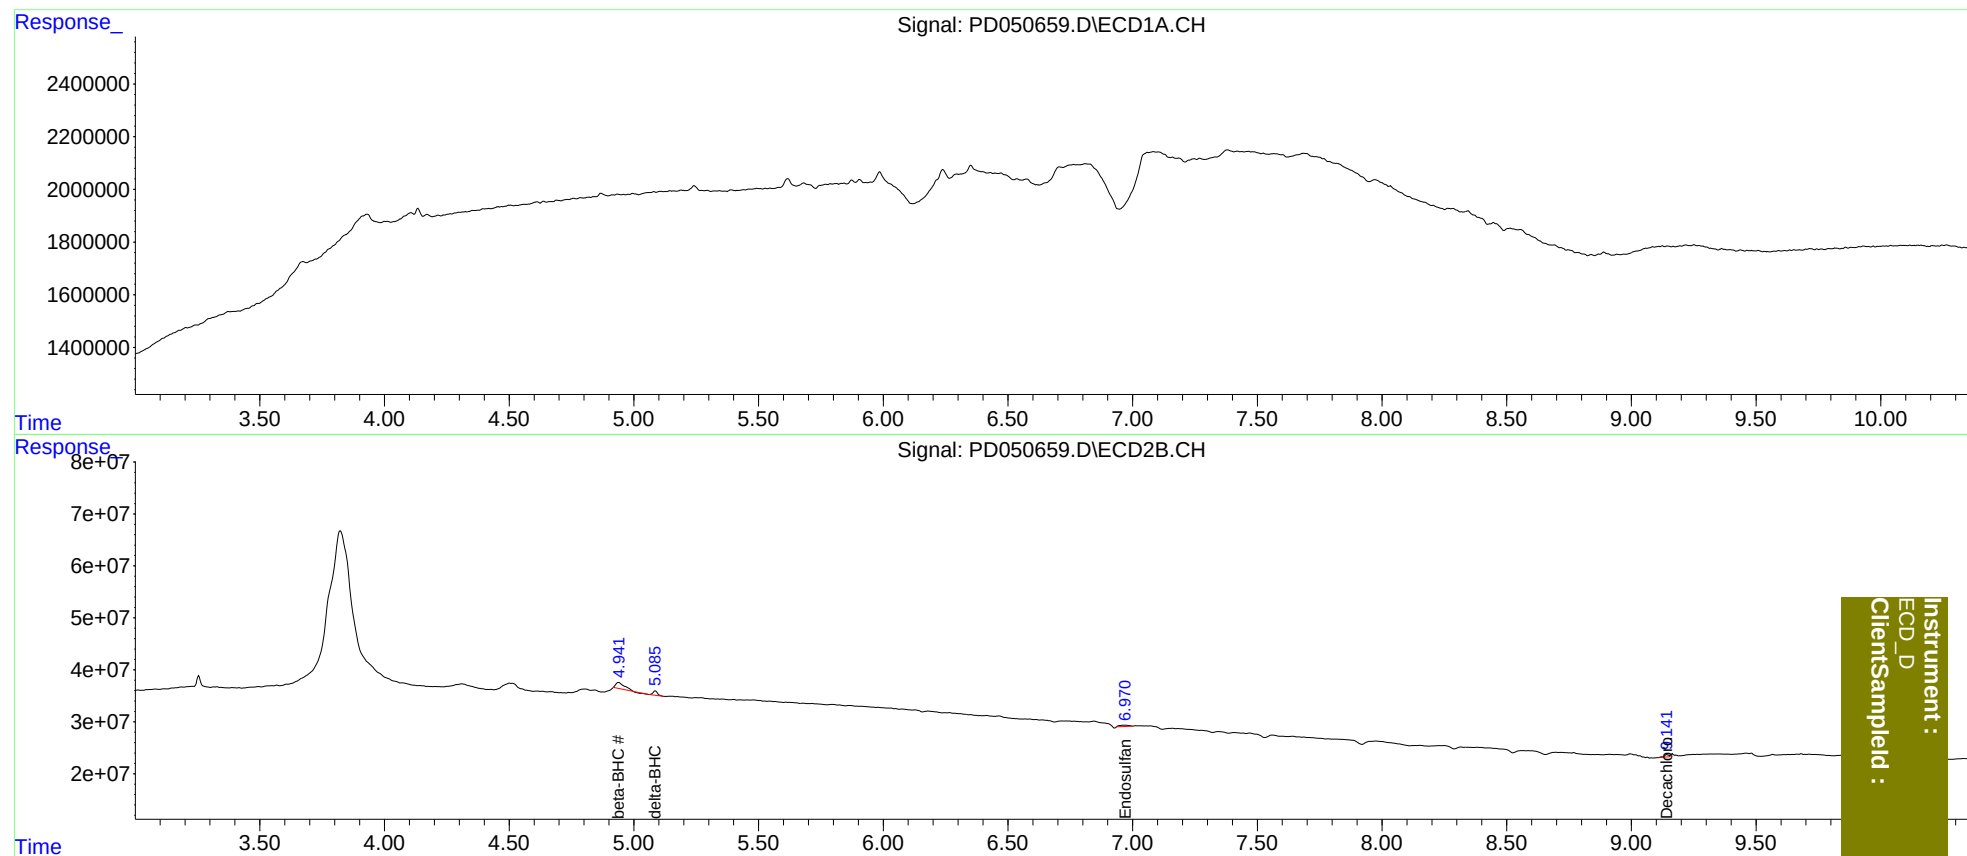


Instrument :
ECD_D
ClientSampled :

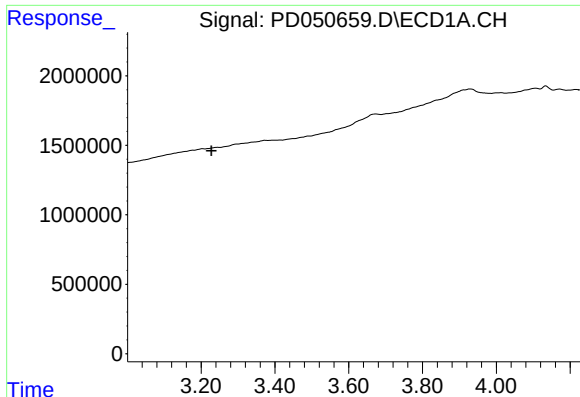

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.228 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

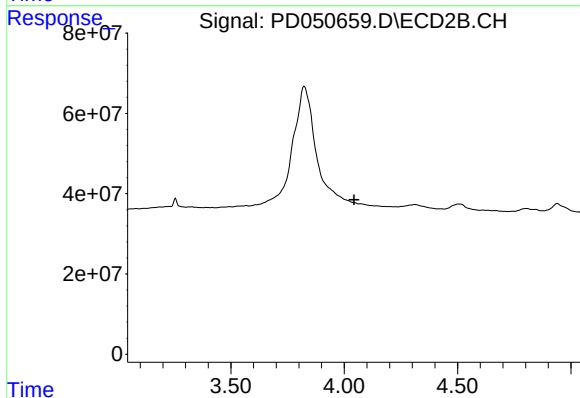


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.044 min
Response: 0
Conc: N.D.

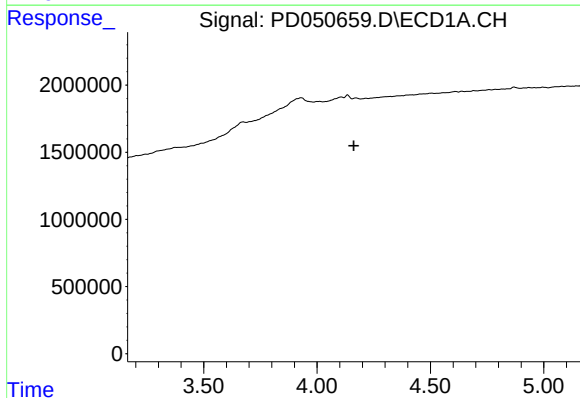


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.162 min
Response: 0
Conc: N.D.

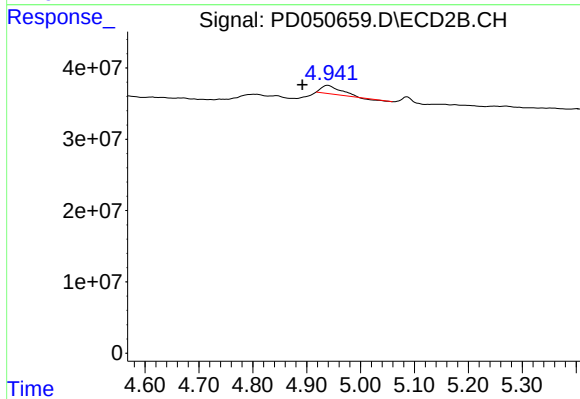

#6 beta-BHC


R.T.: 4.940 min
Delta R.T.: 0.047 min
Response: 25351800
Conc: 1.57 ng/ml

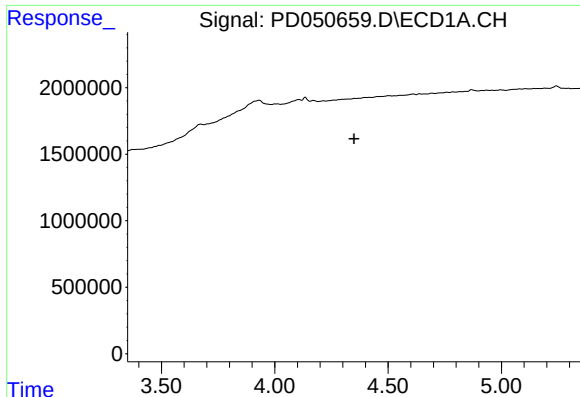

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.351 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

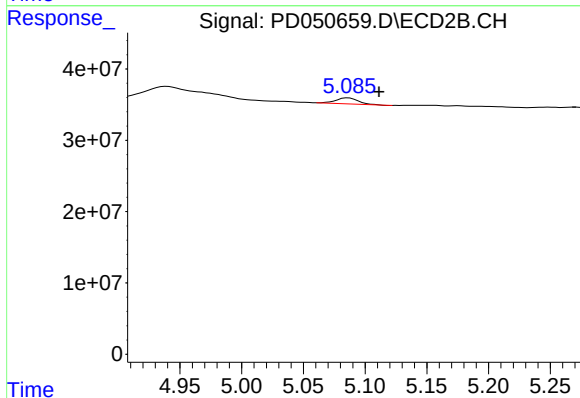


#7 delta-BHC

R.T.: 5.086 min
Delta R.T.: -0.025 min
Response: 10926152
Conc: 0.27 ng/ml

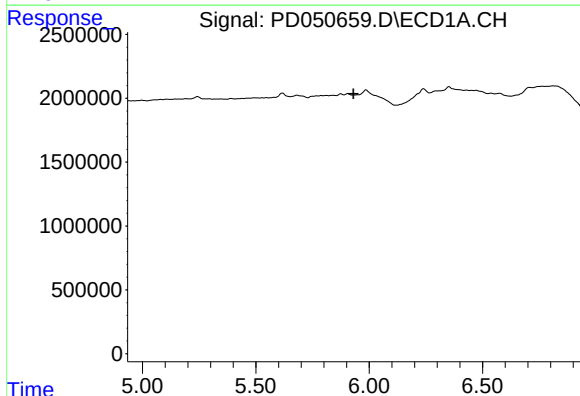


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.931 min
Response: 0
Conc: N.D.

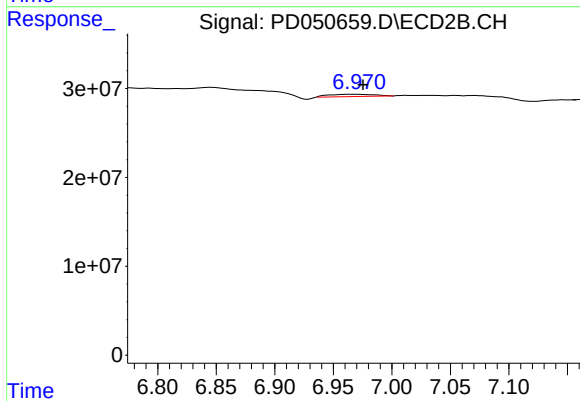

#15 Endosulfan II


R.T.: 6.970 min
Delta R.T.: -0.005 min
Response: 6904116
Conc: 0.27 ng/ml

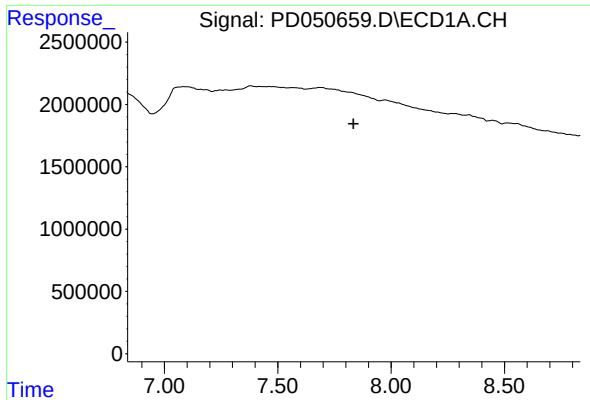

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.834 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

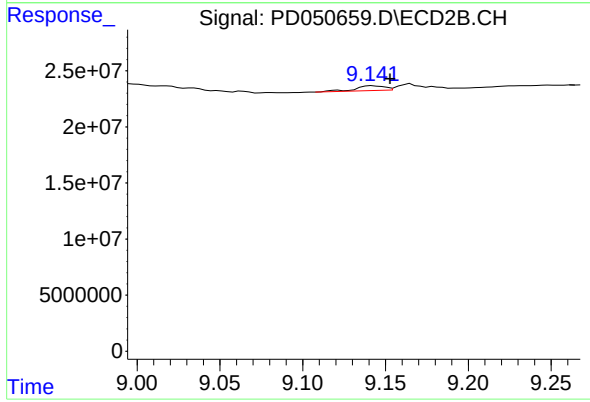

#27 Decachlorobiphenyl

R.T.: 9.142 min
Delta R.T.: -0.010 min
Response: 5200062
Conc: 0.24 ng/ml