

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120420\
 Data File : PD060576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2020 17:32
 Operator : DD\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 03:20:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 04 03:19:35 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.501	4.022	12243998	39995761	10.551	10.064
27)	SA Decachlor...	8.290	9.105	31729282	67916988	21.308	20.780
Target Compounds							
2)	A alpha-BHC	3.942	4.412	16852423	59088001	10.094	9.979
3)	MA gamma-BHC...	4.228	4.698	16501147	53912234	10.352	9.954
4)	MA Heptachlor	4.534	5.209	17062146	53636057	10.254	10.145
9)	A Endosulfan I	5.573	6.260	14896767	43678930	10.295	10.115
13)	MA Dieldrin	5.817	6.518	31858122	95139751	20.124	20.186
14)	MA Endrin	6.077	6.736	26454125	53967779	20.501	14.515 #
16)	A 4,4'-DDD	6.201	6.855	25475781	74175016	19.838	19.847
17)	MA 4,4'-DDT	6.443	7.155	25836767	72075523	19.876	19.986
20)	A Methoxychlor	6.991	7.611	70914823	190.0E6	103.292	103.600

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120420\
Data File : PD060576.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2020 17:32
Operator : DD\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 03:20:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 04 03:19:35 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

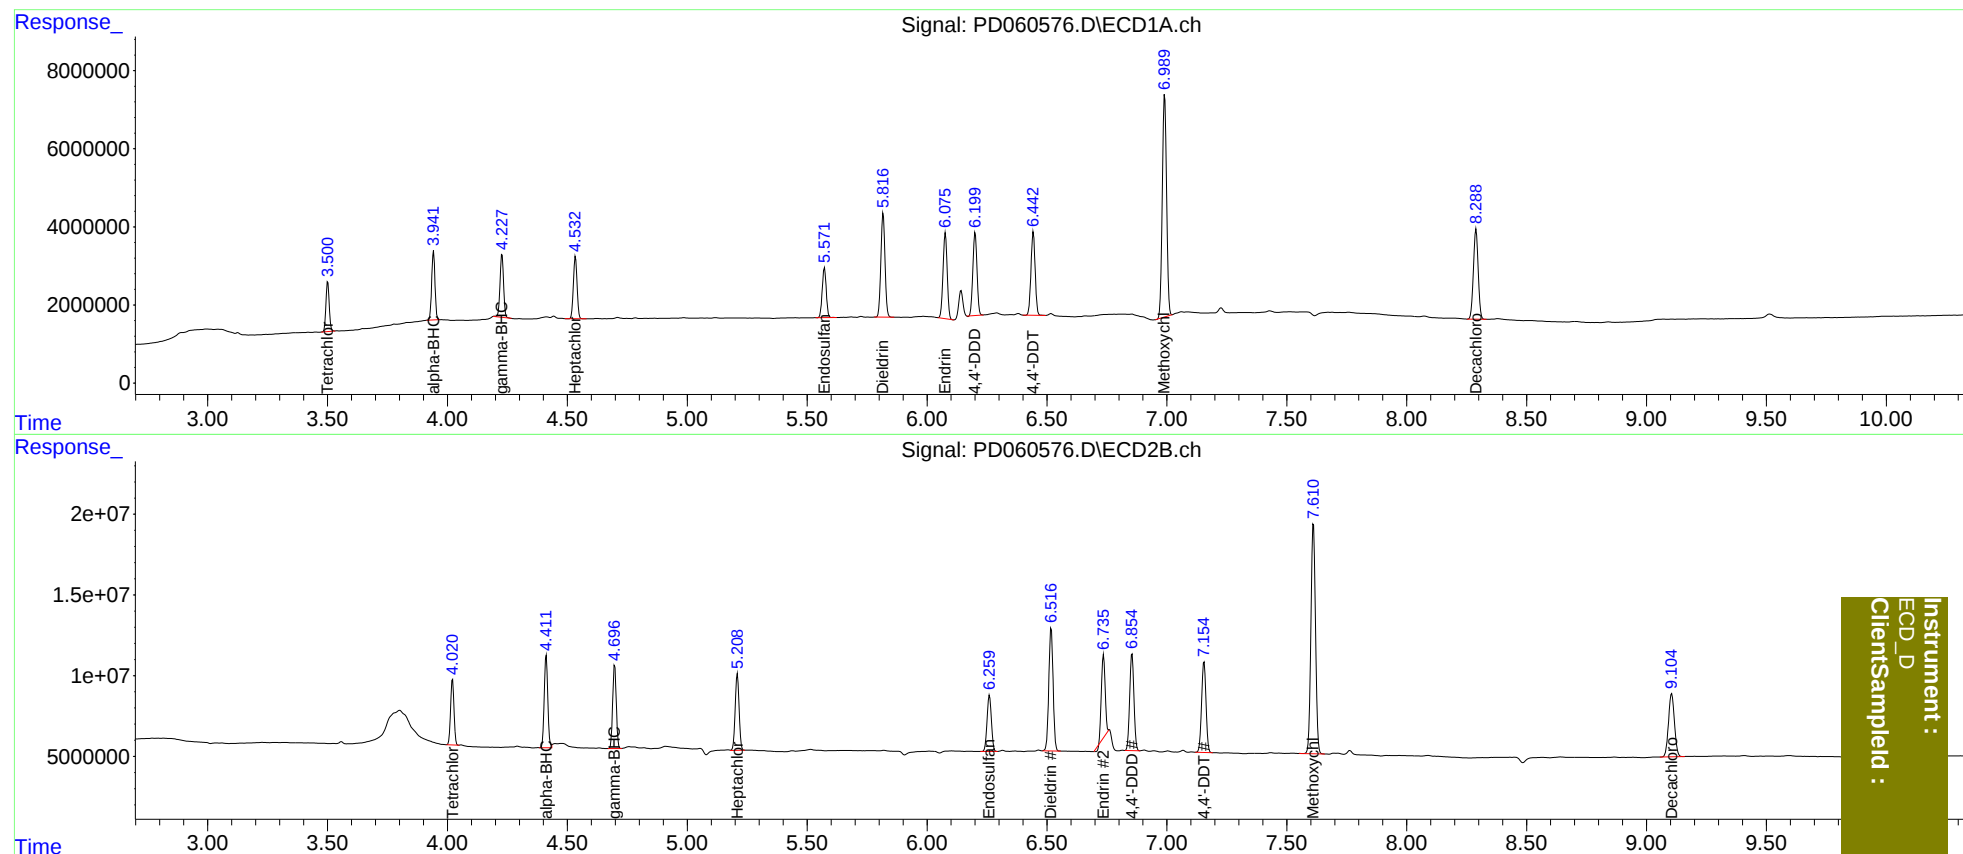


Instrument :
ECD_D
ClientSampled :

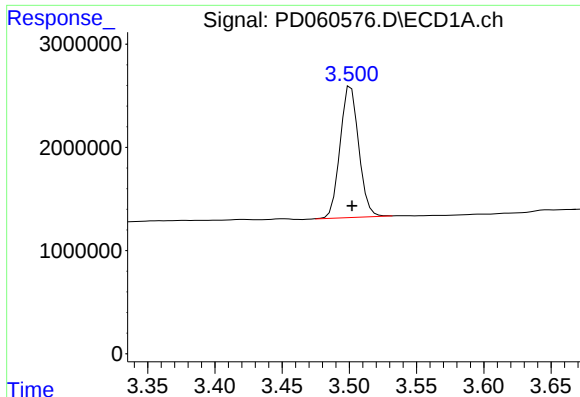

#1 Tetrachloro-m-xylene


R.T.: 3.501 min
Delta R.T.: 0.000 min
Response: 12243998
Conc: 10.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

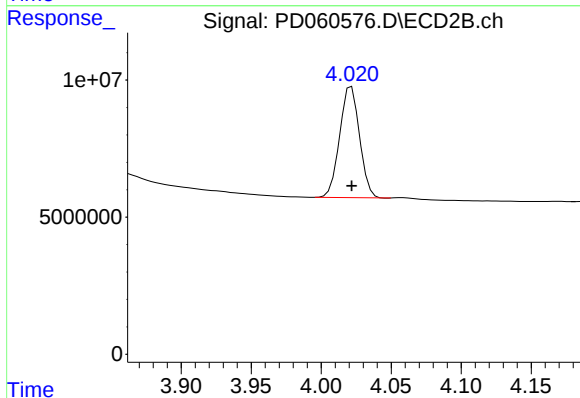


#1 Tetrachloro-m-xylene

R.T.: 4.022 min
Delta R.T.: 0.000 min
Response: 39995761
Conc: 10.06 ng/ml

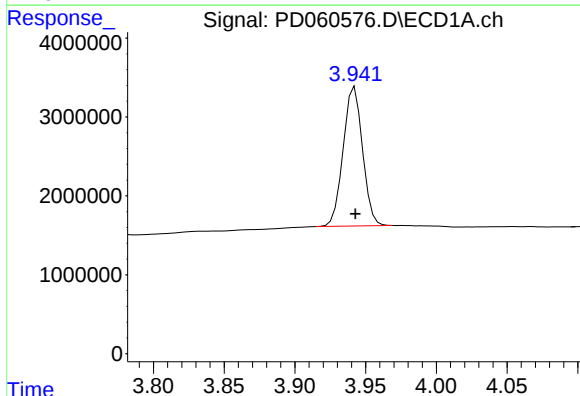


#2 alpha-BHC

R.T.: 3.942 min
Delta R.T.: 0.000 min
Response: 16852423
Conc: 10.09 ng/ml

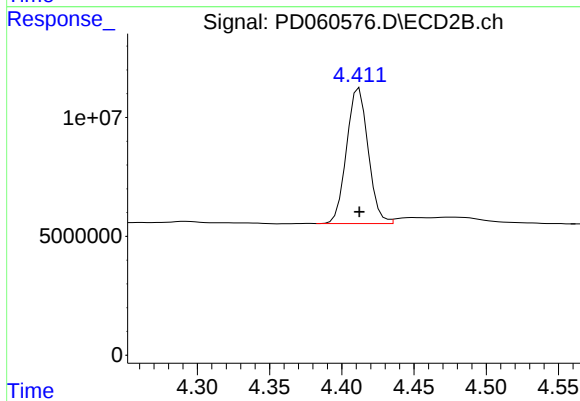

#2 alpha-BHC


R.T.: 4.412 min
Delta R.T.: 0.000 min
Response: 59088001
Conc: 9.98 ng/ml

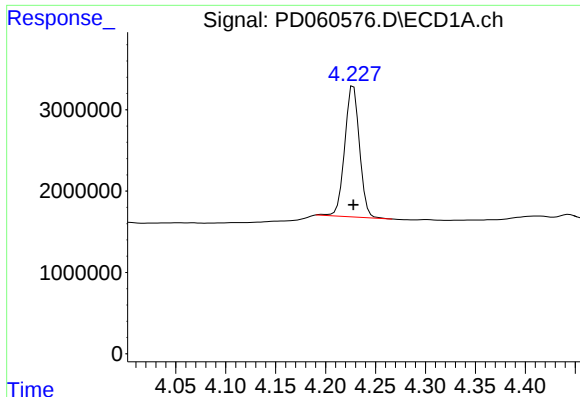

#3 gamma-BHC (Lindane)


R.T.: 4.228 min
Delta R.T.: 0.000 min
Response: 16501147
Conc: 10.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

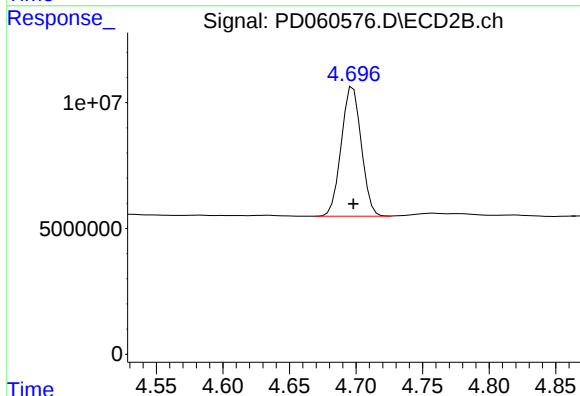


#3 gamma-BHC (Lindane)

R.T.: 4.698 min
Delta R.T.: 0.000 min
Response: 53912234
Conc: 9.95 ng/ml

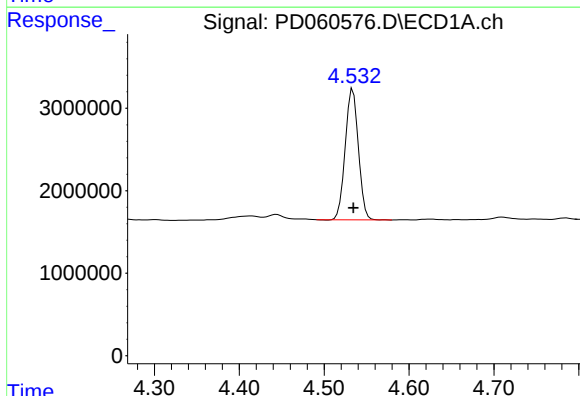


#4 Heptachlor

R.T.: 4.534 min
Delta R.T.: 0.000 min
Response: 17062146
Conc: 10.25 ng/ml

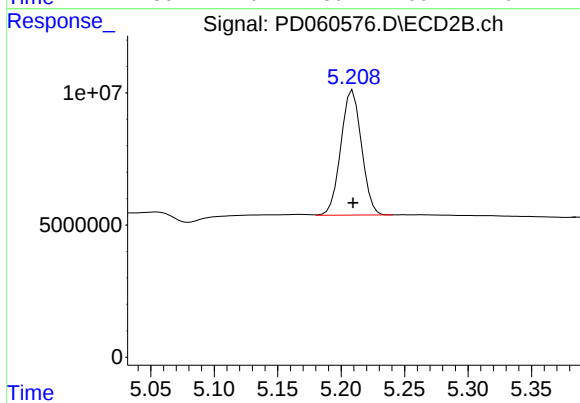

#4 Heptachlor


R.T.: 5.209 min
Delta R.T.: 0.000 min
Response: 53636057
Conc: 10.14 ng/ml

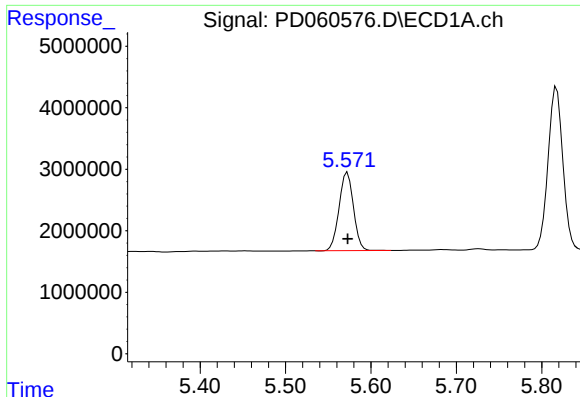

#9 Endosulfan I


R.T.: 5.573 min
Delta R.T.: 0.000 min
Response: 14896767
Conc: 10.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

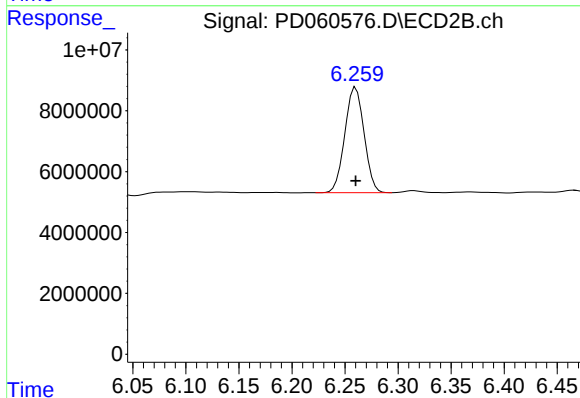


#9 Endosulfan I

R.T.: 6.260 min
Delta R.T.: 0.000 min
Response: 43678930
Conc: 10.11 ng/ml

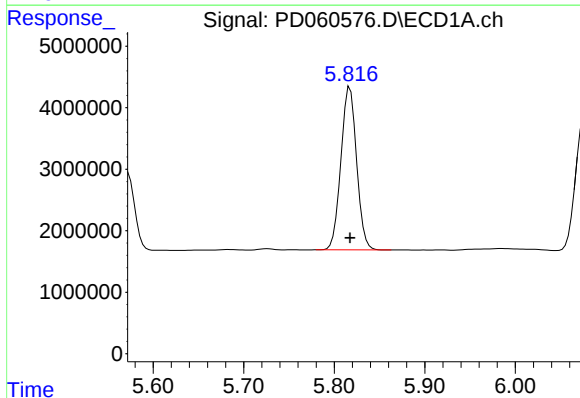


#13 Dieldrin

R.T.: 5.817 min
Delta R.T.: 0.000 min
Response: 31858122
Conc: 20.12 ng/ml

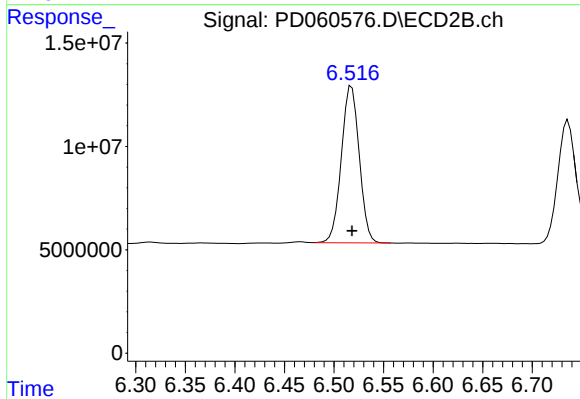

#13 Dieldrin


R.T.: 6.518 min
Delta R.T.: 0.000 min
Response: 95139751
Conc: 20.19 ng/ml

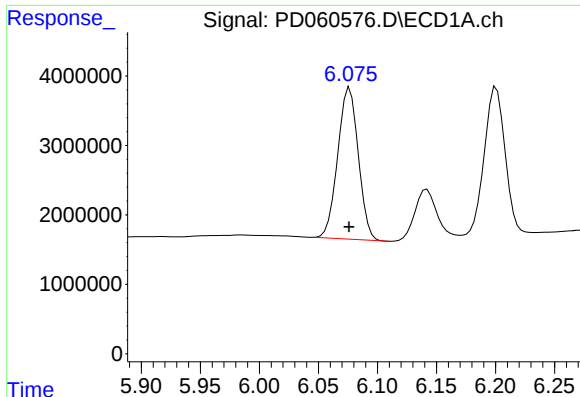

#14 Endrin


R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 26454125
Conc: 20.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

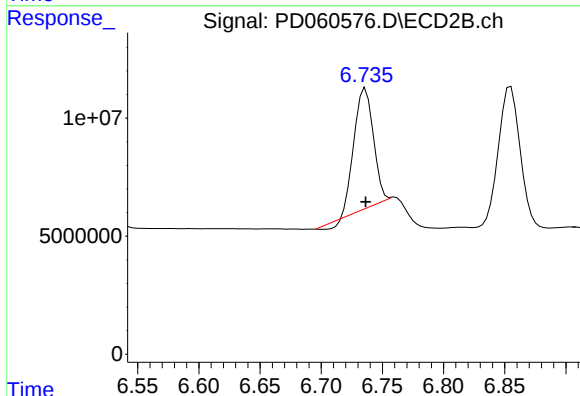


#14 Endrin

R.T.: 6.736 min
Delta R.T.: 0.000 min
Response: 53967779
Conc: 14.52 ng/ml

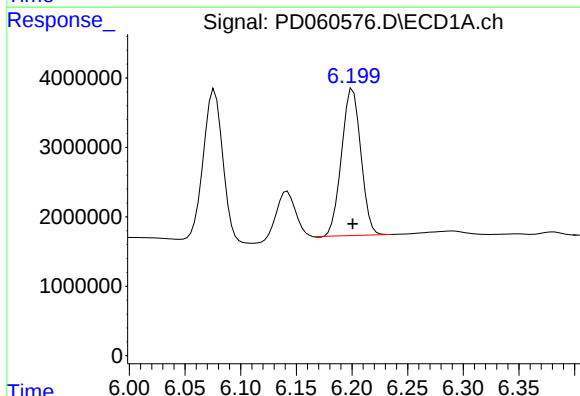


#16 4,4'-DDD

R.T.: 6.201 min
Delta R.T.: 0.000 min
Response: 25475781
Conc: 19.84 ng/ml

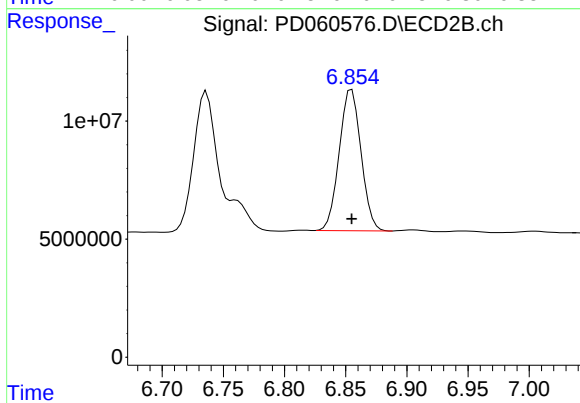

#16 4,4'-DDD


R.T.: 6.855 min
Delta R.T.: 0.000 min
Response: 74175016
Conc: 19.85 ng/ml

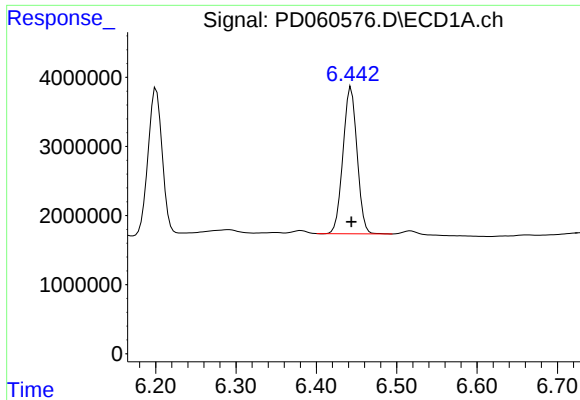

#17 4,4'-DDT


R.T.: 6.443 min
Delta R.T.: 0.000 min
Response: 25836767
Conc: 19.88 ng/ml

Instrument :
ECD_D
ClientSampleId :

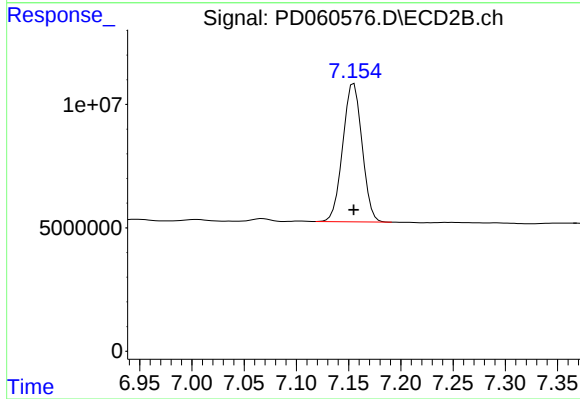


#17 4,4'-DDT

R.T.: 7.155 min
Delta R.T.: 0.000 min
Response: 72075523
Conc: 19.99 ng/ml

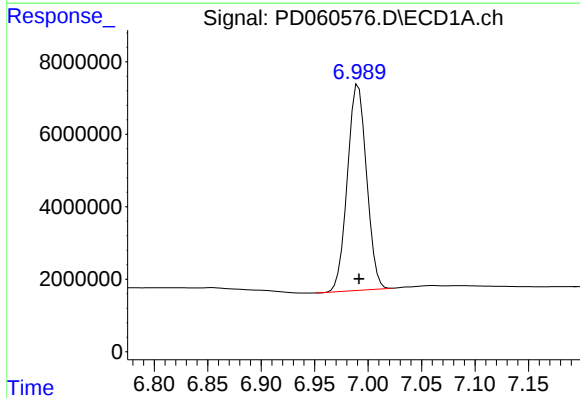


#20 Methoxychlor

R.T.: 6.991 min
Delta R.T.: 0.000 min
Response: 70914823
Conc: 103.29 ng/ml

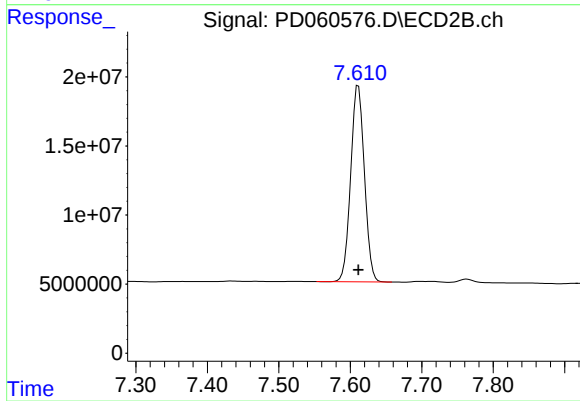

#20 Methoxychlor


R.T.: 7.611 min
Delta R.T.: 0.000 min
Response: 190033131
Conc: 103.60 ng/ml

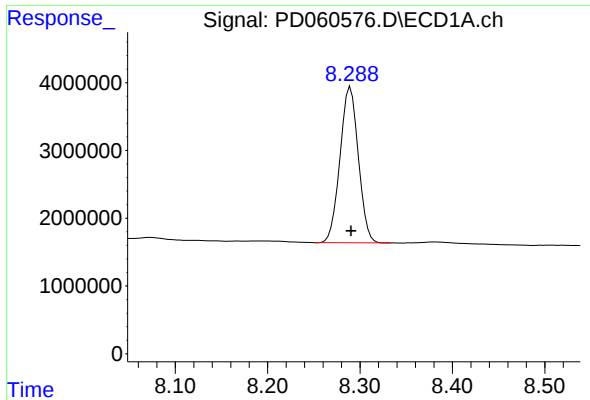

#27 Decachlorobiphenyl

R.T.: 8.290 min
Delta R.T.: 0.000 min
Response: 31729282
Conc: 21.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

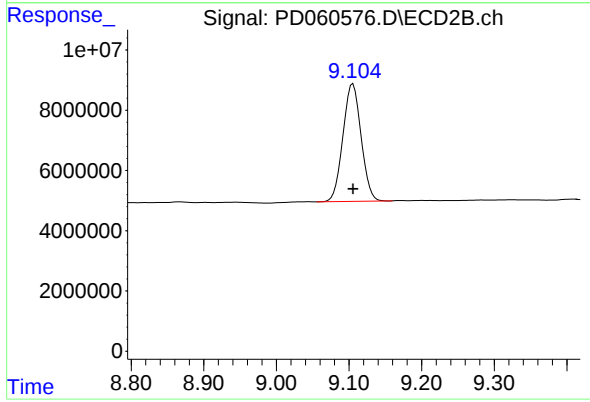

#27 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 67916988
Conc: 20.78 ng/ml