

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120420\
 Data File : PD060578.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2020 18:00
 Operator : DD\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 03:20:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 04 03:19:35 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.502	4.022	23210243	79482866	20.000	20.000
27)	SA Decachlor...	8.290	9.106	59562699	130.7E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.943	4.412	33390829	118.4E6	20.000	20.000
3)	MA gamma-BHC...	4.228	4.698	31879827	108.3E6	20.000	20.000
4)	MA Heptachlor	4.535	5.209	33278069	105.7E6	20.000	20.000
9)	A Endosulfan I	5.573	6.260	28940181	86368082	20.000	20.000
13)	MA Dieldrin	5.818	6.518	63322881	188.5E6	40.000	40.000
14)	MA Endrin	6.076	6.736	51614308	148.7E6	40.000	40.000
16)	A 4,4'-DDD	6.201	6.855	51368832	149.5E6	40.000	40.000
17)	MA 4,4'-DDT	6.443	7.155	51997158	144.3E6	40.000	40.000
20)	A Methoxychlor	6.992	7.611	137.3E6	366.9E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120420\
Data File : PD060578.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2020 18:00
Operator : DD\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 03:20:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 04 03:19:35 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

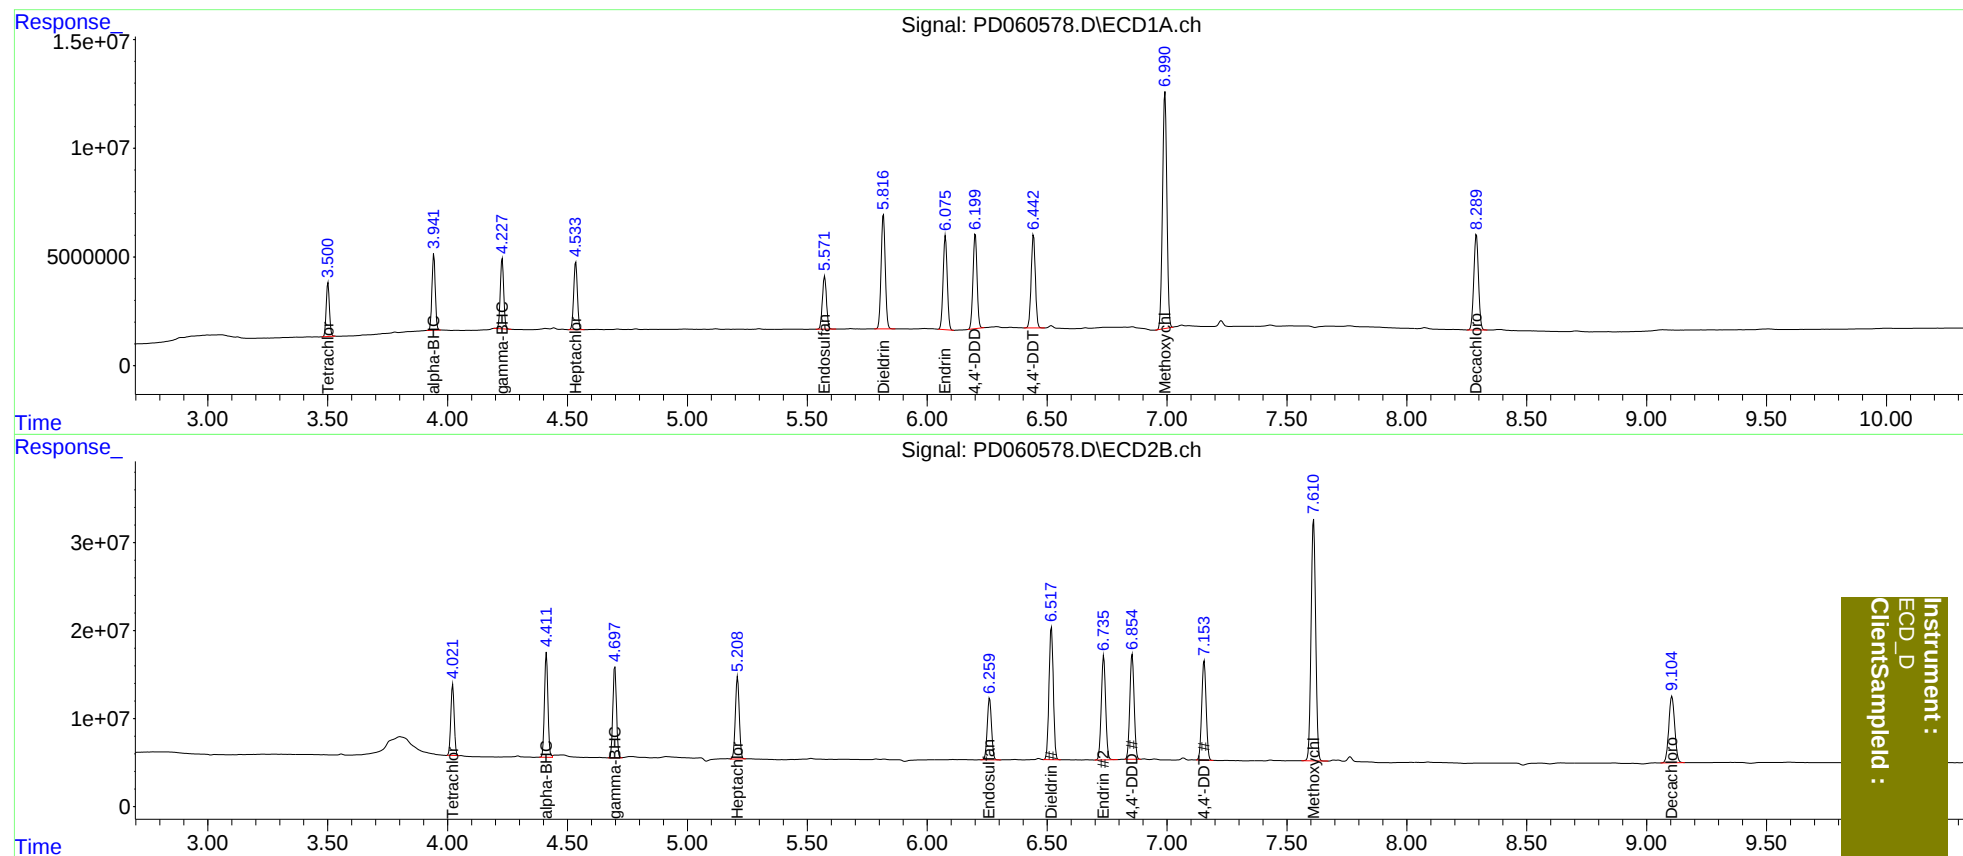


Instrument :
ECD_D
ClientSampled :

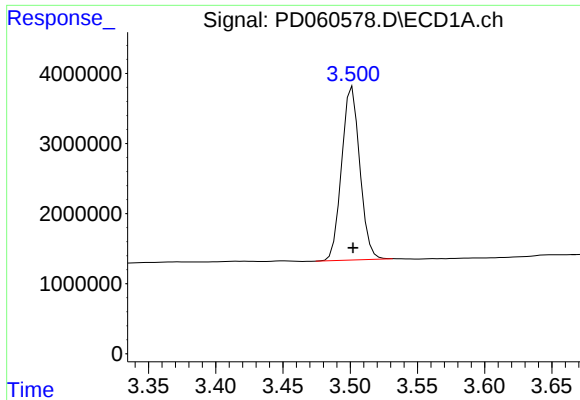

#1 Tetrachloro-m-xylene


R.T.: 3.502 min
Delta R.T.: 0.000 min
Response: 23210243
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

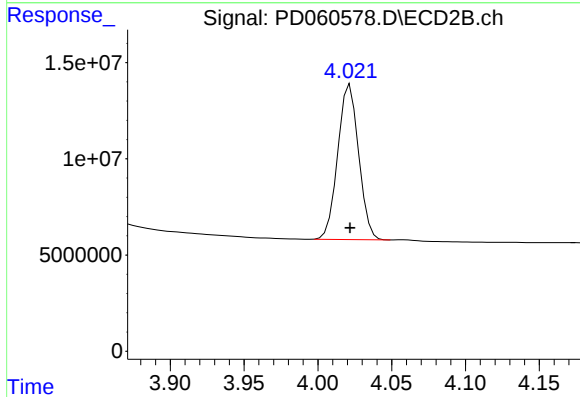


#1 Tetrachloro-m-xylene

R.T.: 4.022 min
Delta R.T.: 0.000 min
Response: 79482866
Conc: 20.00 ng/ml

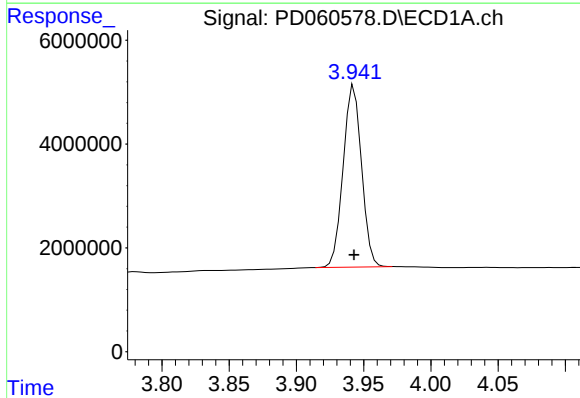


#2 alpha-BHC

R.T.: 3.943 min
Delta R.T.: 0.000 min
Response: 33390829
Conc: 20.00 ng/ml

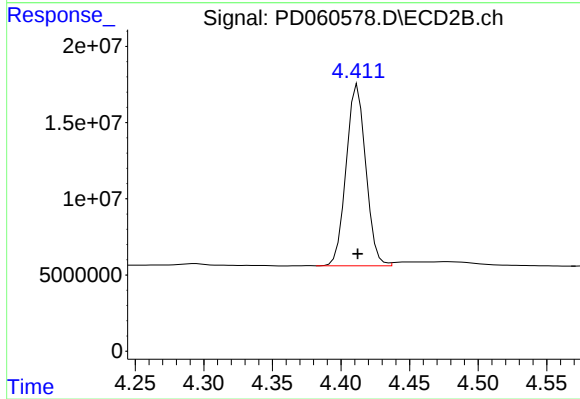

#2 alpha-BHC


R.T.: 4.412 min
Delta R.T.: 0.000 min
Response: 118425161
Conc: 20.00 ng/ml

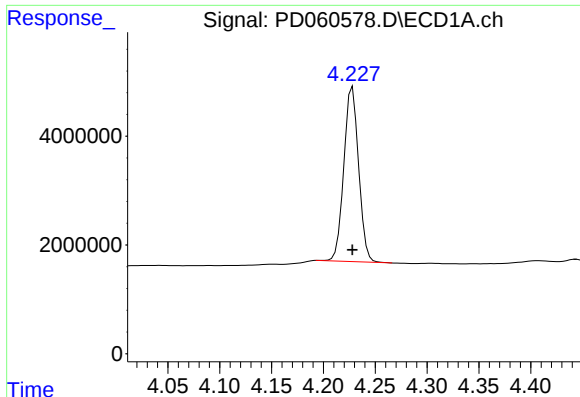

#3 gamma-BHC (Lindane)


R.T.: 4.228 min
Delta R.T.: 0.000 min
Response: 31879827
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

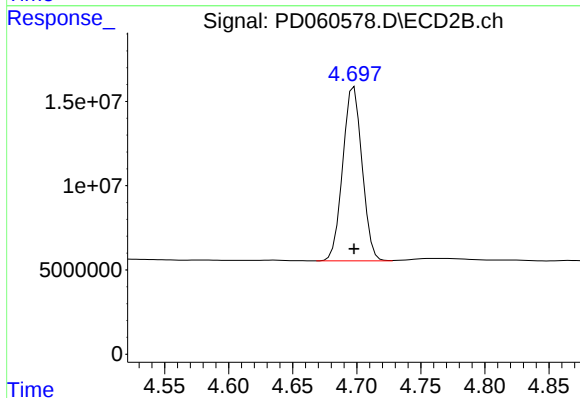


#3 gamma-BHC (Lindane)

R.T.: 4.698 min
Delta R.T.: 0.000 min
Response: 108321841
Conc: 20.00 ng/ml

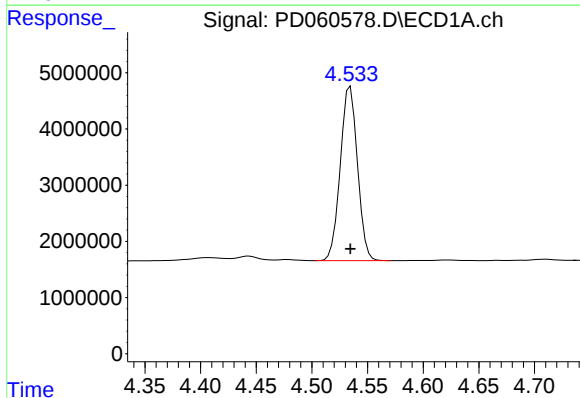


#4 Heptachlor

R.T.: 4.535 min
Delta R.T.: 0.000 min
Response: 33278069
Conc: 20.00 ng/ml

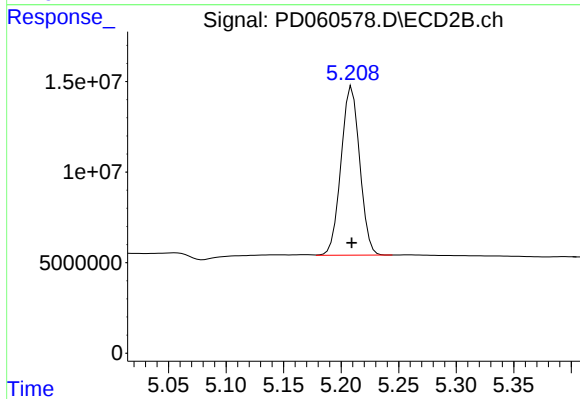

#4 Heptachlor


R.T.: 5.209 min
Delta R.T.: 0.000 min
Response: 105739167
Conc: 20.00 ng/ml

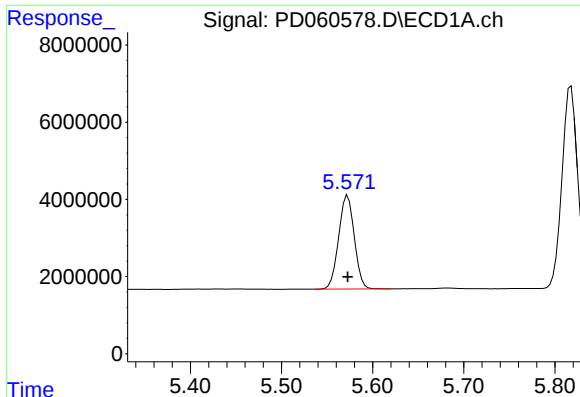

#9 Endosulfan I


R.T.: 5.573 min
Delta R.T.: 0.000 min
Response: 28940181
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

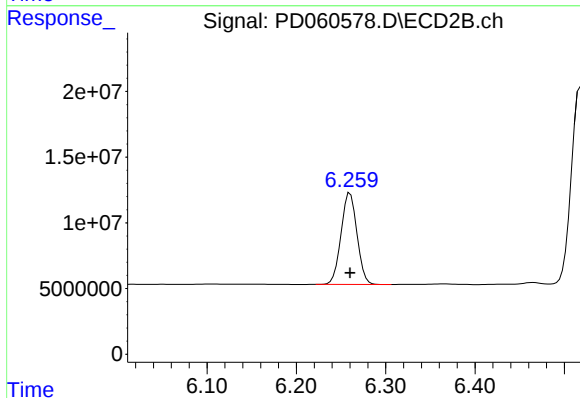


#9 Endosulfan I

R.T.: 6.260 min
Delta R.T.: 0.000 min
Response: 86368082
Conc: 20.00 ng/ml

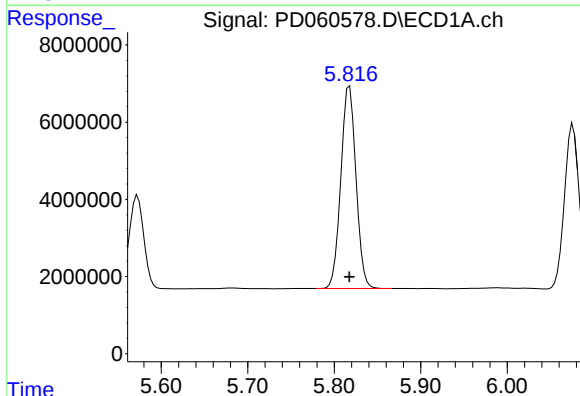


#13 Dieldrin

R.T.: 5.818 min
Delta R.T.: 0.000 min
Response: 63322881
Conc: 40.00 ng/ml

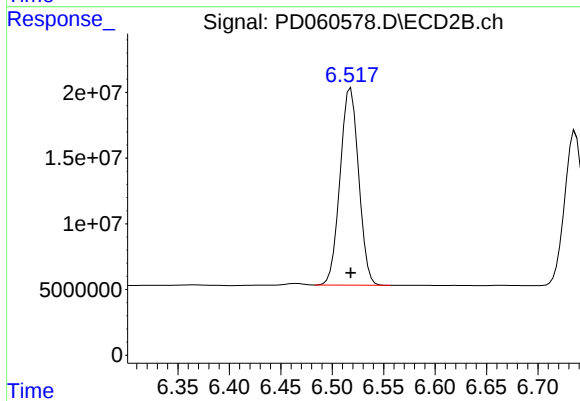

#13 Dieldrin


R.T.: 6.518 min
Delta R.T.: 0.000 min
Response: 188528958
Conc: 40.00 ng/ml

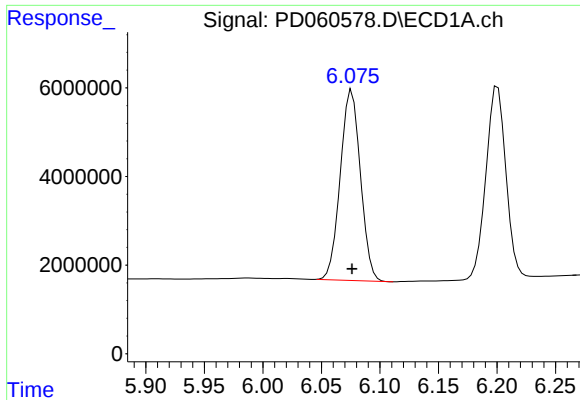

#14 Endrin


R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 51614308
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

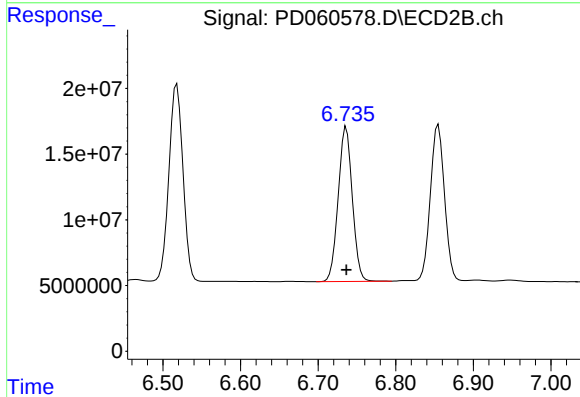


#14 Endrin

R.T.: 6.736 min
Delta R.T.: 0.000 min
Response: 148718070
Conc: 40.00 ng/ml

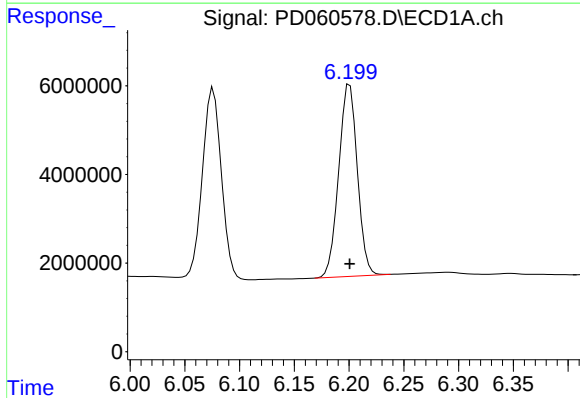


#16 4,4'-DDD

R.T.: 6.201 min
Delta R.T.: 0.000 min
Response: 51368832
Conc: 40.00 ng/ml

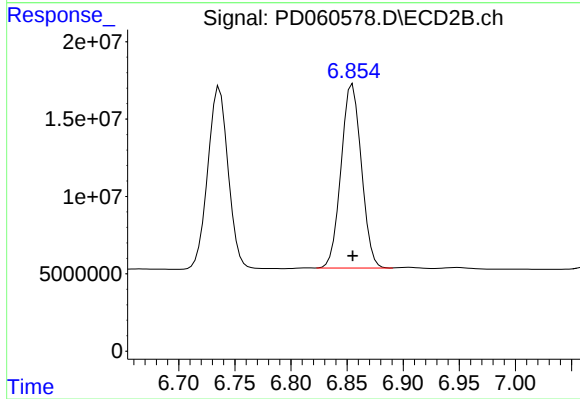

#16 4,4'-DDD


R.T.: 6.855 min
Delta R.T.: 0.000 min
Response: 149493170
Conc: 40.00 ng/ml

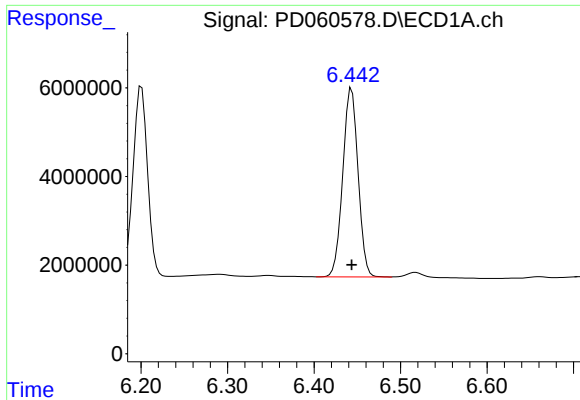

#17 4,4'-DDT


R.T.: 6.443 min
Delta R.T.: 0.000 min
Response: 51997158
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

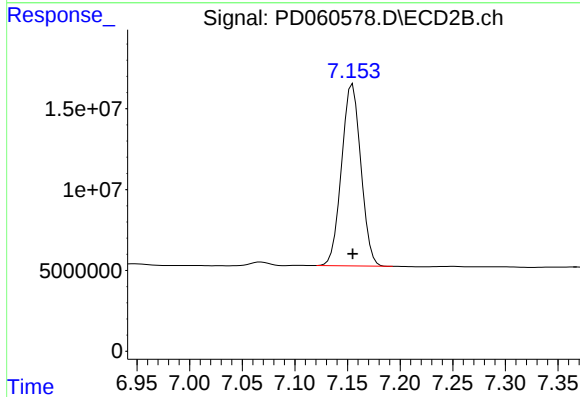


#17 4,4'-DDT

R.T.: 7.155 min
Delta R.T.: 0.000 min
Response: 144255357
Conc: 40.00 ng/ml

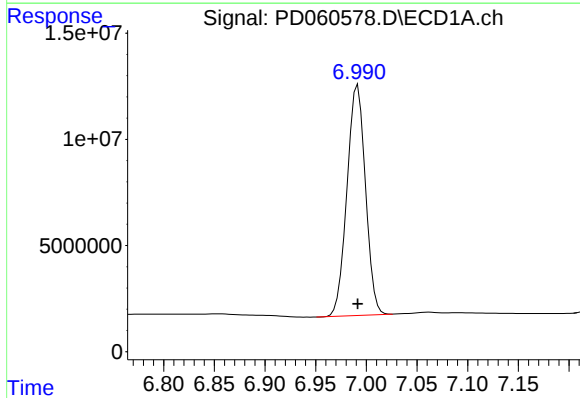


#20 Methoxychlor

R.T.: 6.992 min
Delta R.T.: 0.000 min
Response: 137310040
Conc: 200.00 ng/ml

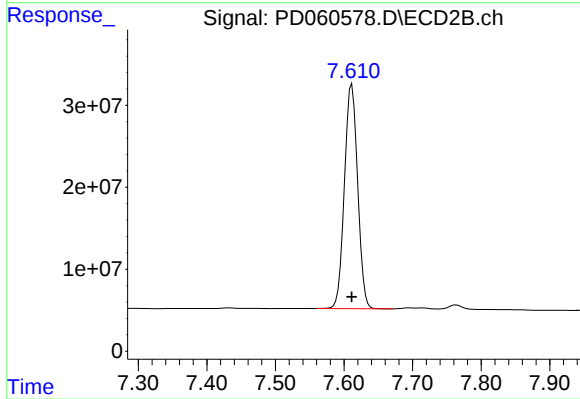

#20 Methoxychlor


R.T.: 7.611 min
Delta R.T.: 0.000 min
Response: 366861093
Conc: 200.00 ng/ml

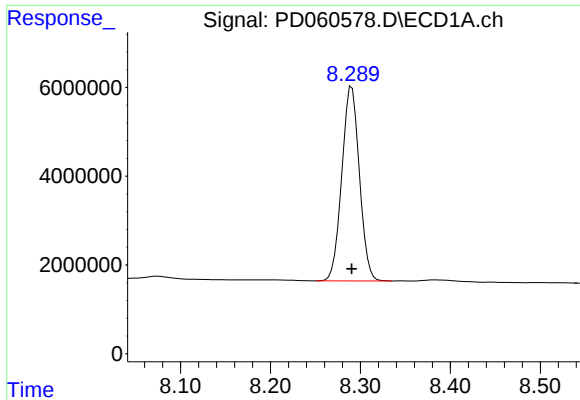

#27 Decachlorobiphenyl

R.T.: 8.290 min
Delta R.T.: 0.000 min
Response: 59562699
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

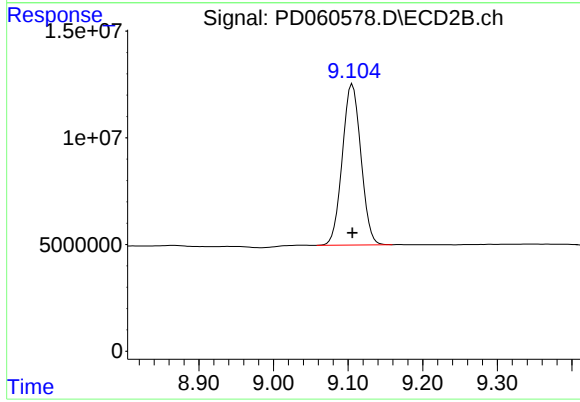

#27 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 130733333
Conc: 40.00 ng/ml