

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120420\
 Data File : PD060580.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2020 18:28
 Operator : DD\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 03:20:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 04 03:19:35 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.502	4.021	44942149	157.5E6	38.726	39.638
27)	SA Decachlor...	8.289	9.105	113.3E6	250.9E6	76.088	76.770
Target Compounds							
2)	A alpha-BHC	3.943	4.412	67424384	238.9E6	40.385	40.341
3)	MA gamma-BHC...	4.228	4.698	63515965	217.5E6	39.847	40.158
4)	MA Heptachlor	4.534	5.209	65860260	216.8E6	39.582	41.001
9)	A Endosulfan I	5.573	6.261	56763571	171.1E6	39.228	39.624
13)	MA Dieldrin	5.818	6.518	128.2E6	377.0E6	80.983	79.995
14)	MA Endrin	6.076	6.736	101.6E6	293.7E6	78.772	78.996
16)	A 4,4'-DDD	6.200	6.855	103.4E6	299.8E6	80.540	80.223
17)	MA 4,4'-DDT	6.444	7.155	105.9E6	290.4E6	81.500	80.516
20)	A Methoxychlor	6.991	7.611	266.7E6	698.3E6	388.430	380.703

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120420\
Data File : PD060580.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2020 18:28
Operator : DD\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 03:20:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 04 03:19:35 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

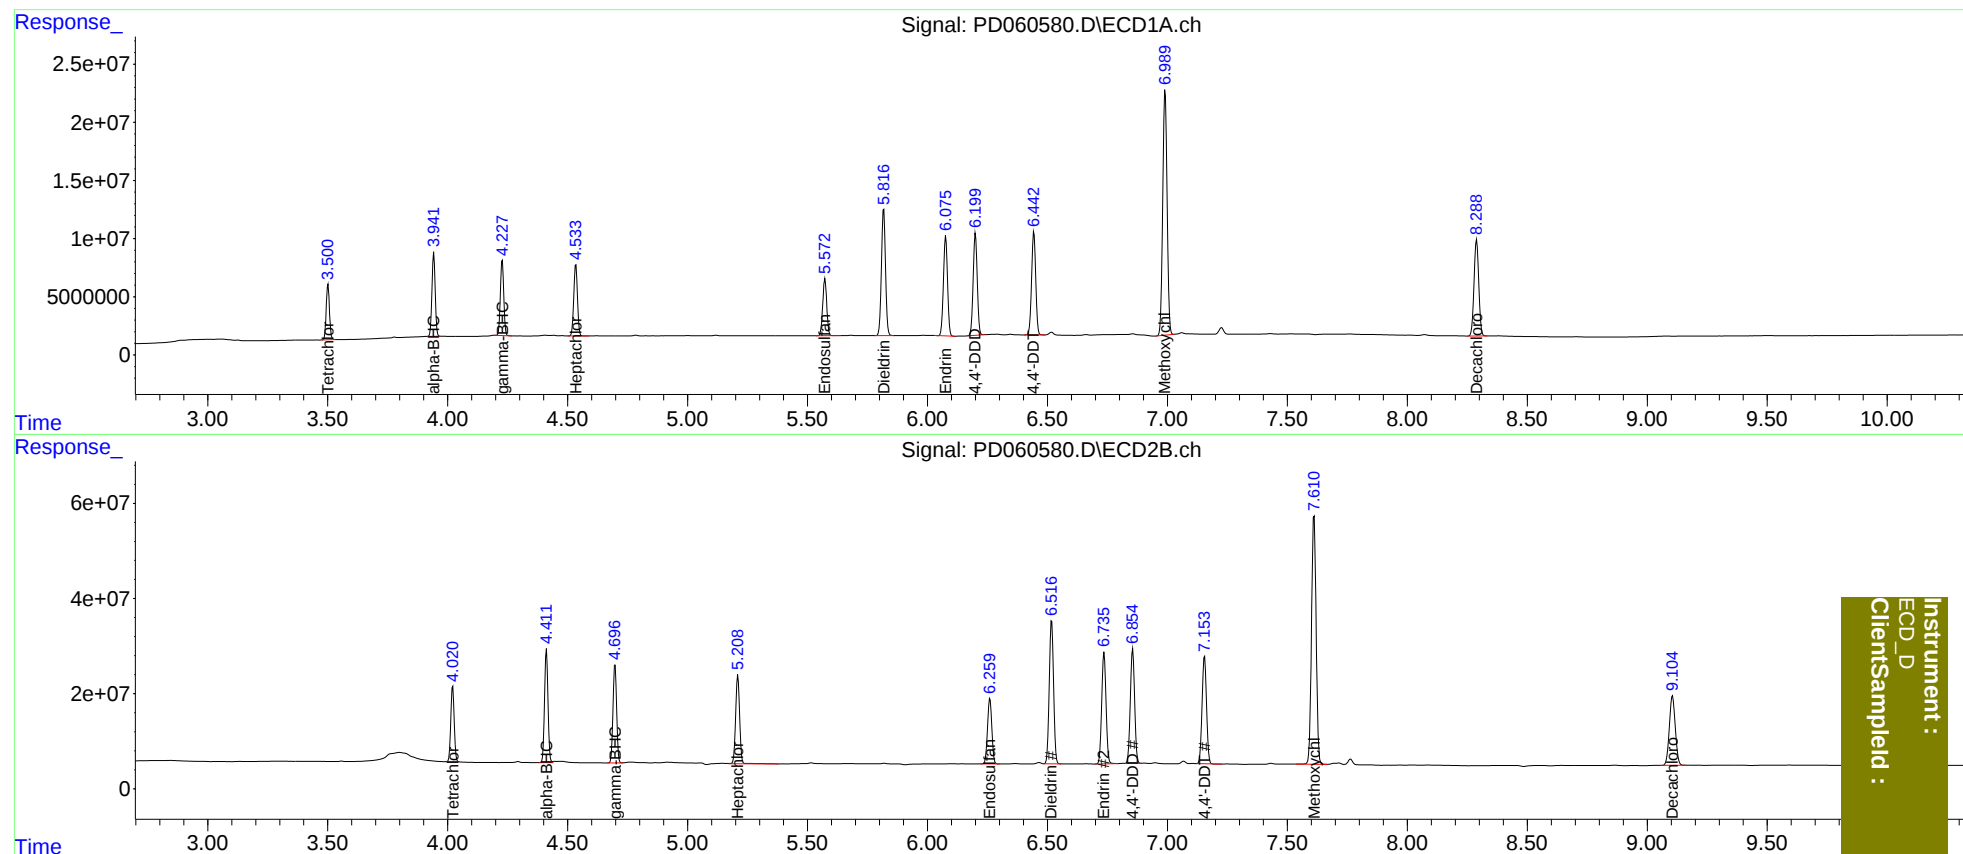


Instrument :
ECD_D
ClientSample :
INDA401

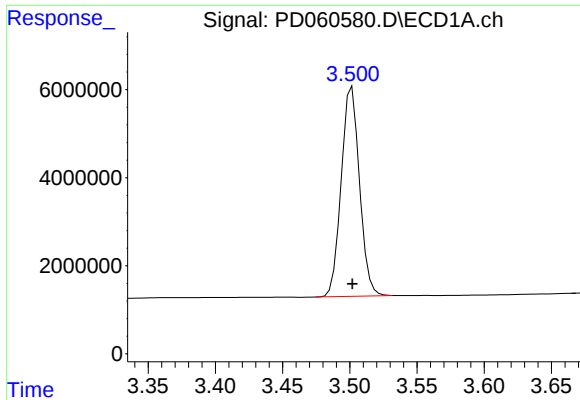

#1 Tetrachloro-m-xylene


R.T.: 3.502 min
Delta R.T.: 0.000 min
Response: 44942149
Conc: 38.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

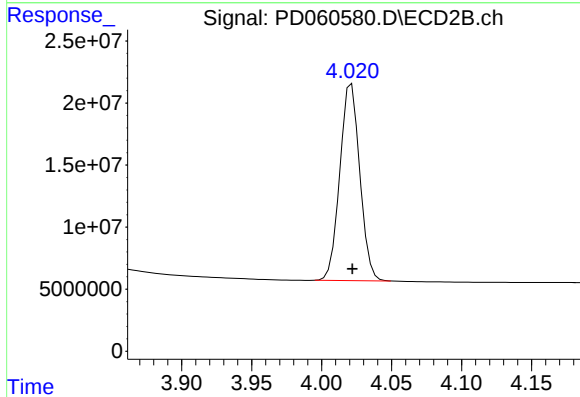


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 157526087
Conc: 39.64 ng/ml

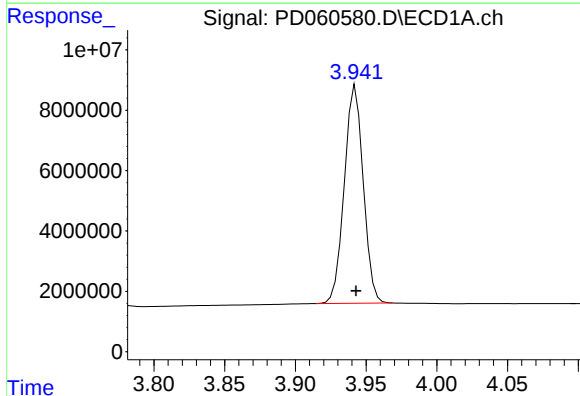


#2 alpha-BHC

R.T.: 3.943 min
Delta R.T.: 0.000 min
Response: 67424384
Conc: 40.38 ng/ml

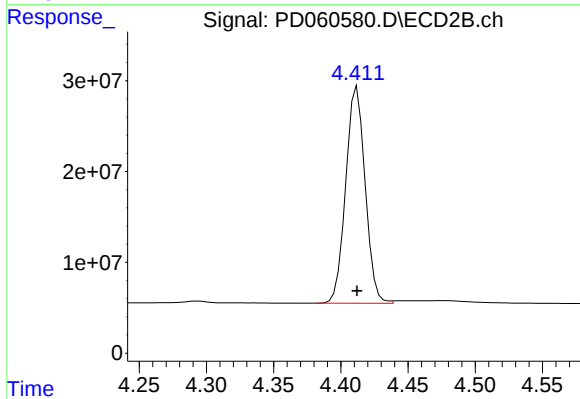

#2 alpha-BHC


R.T.: 4.412 min
Delta R.T.: 0.000 min
Response: 238869196
Conc: 40.34 ng/ml

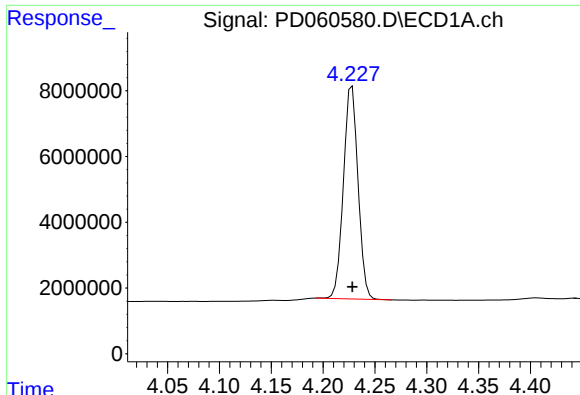

#3 gamma-BHC (Lindane)


R.T.: 4.228 min
Delta R.T.: 0.000 min
Response: 63515965
Conc: 39.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

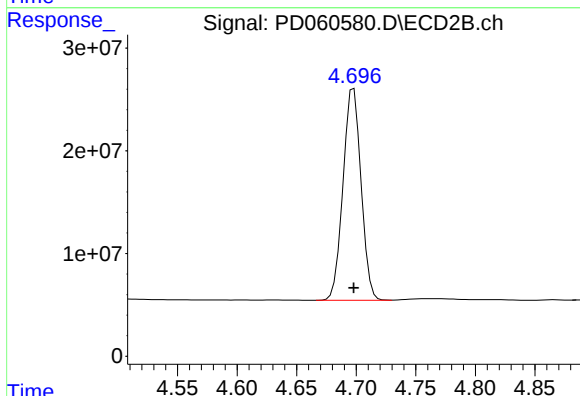


#3 gamma-BHC (Lindane)

R.T.: 4.698 min
Delta R.T.: 0.000 min
Response: 217497215
Conc: 40.16 ng/ml

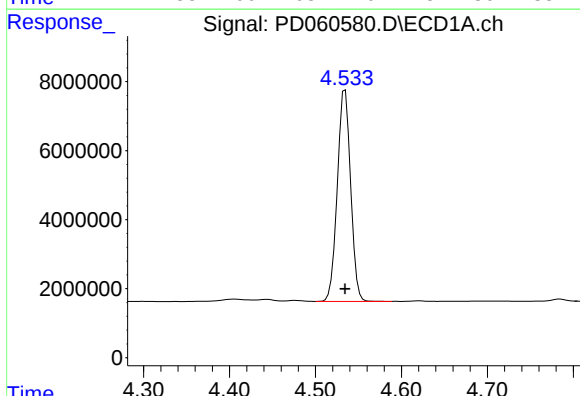


#4 Heptachlor

R.T.: 4.534 min
Delta R.T.: 0.000 min
Response: 65860260
Conc: 39.58 ng/ml

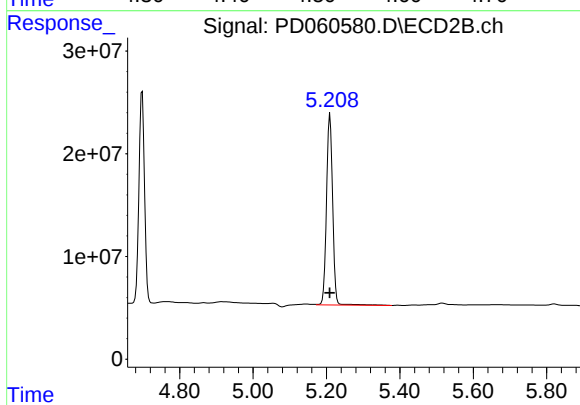

#4 Heptachlor


R.T.: 5.209 min
Delta R.T.: 0.000 min
Response: 216772555
Conc: 41.00 ng/ml

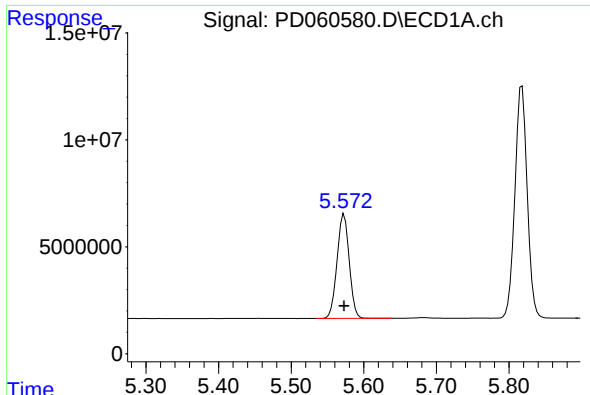

#9 Endosulfan I


R.T.: 5.573 min
Delta R.T.: 0.000 min
Response: 56763571
Conc: 39.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

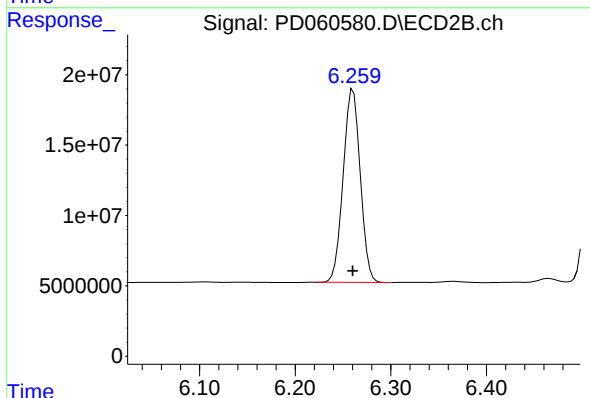


#9 Endosulfan I

R.T.: 6.261 min
Delta R.T.: 0.000 min
Response: 171111172
Conc: 39.62 ng/ml

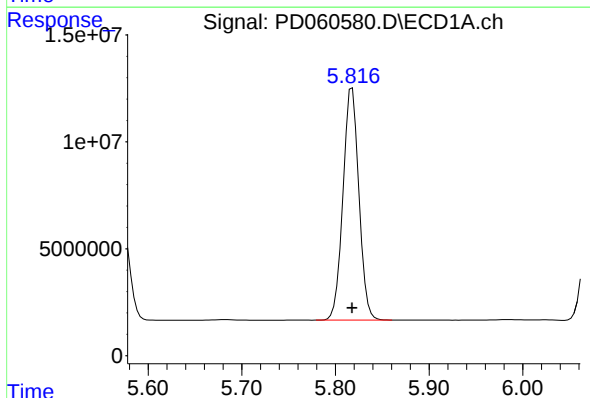


#13 Dieldrin

R.T.: 5.818 min
Delta R.T.: 0.000 min
Response: 128202113
Conc: 80.98 ng/ml

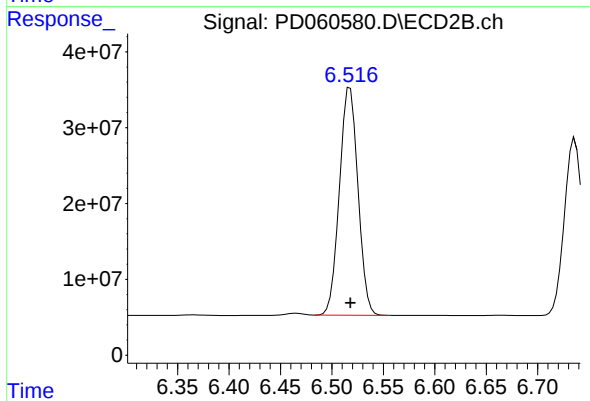

#13 Dieldrin


R.T.: 6.518 min
Delta R.T.: 0.000 min
Response: 377036155
Conc: 80.00 ng/ml

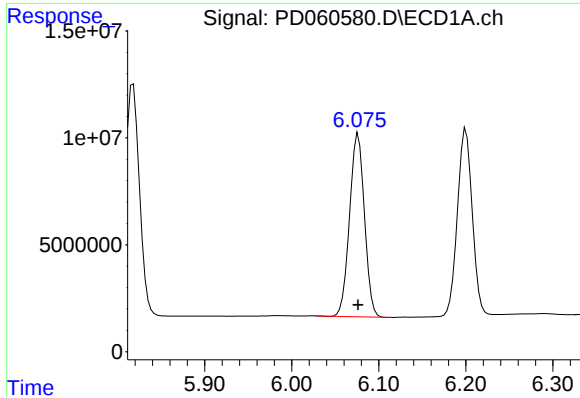

#14 Endrin


R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 101644127
Conc: 78.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

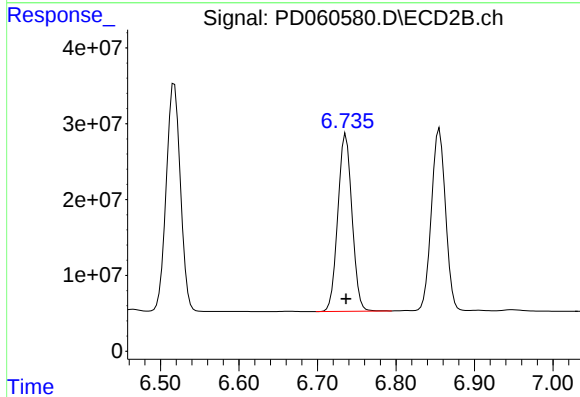


#14 Endrin

R.T.: 6.736 min
Delta R.T.: 0.000 min
Response: 293703859
Conc: 79.00 ng/ml

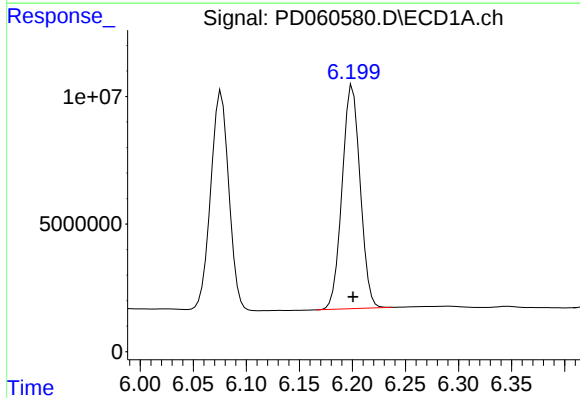


#16 4,4'-DDD

R.T.: 6.200 min
Delta R.T.: 0.000 min
Response: 103430850
Conc: 80.54 ng/ml

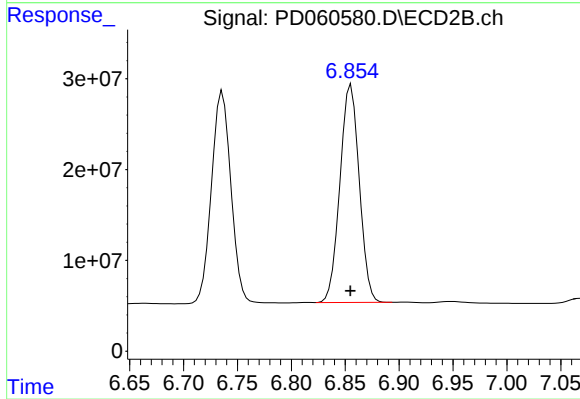

#16 4,4'-DDD


R.T.: 6.855 min
Delta R.T.: 0.000 min
Response: 299819695
Conc: 80.22 ng/ml

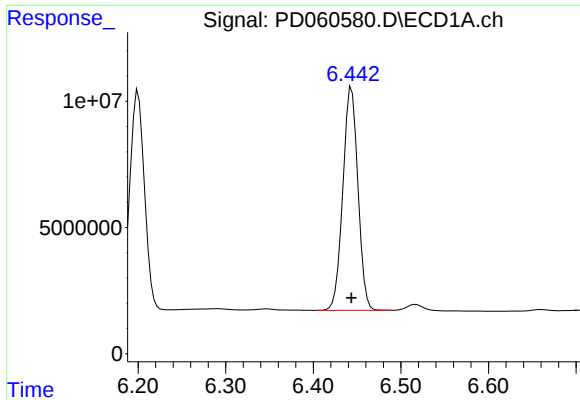

#17 4,4'-DDT


R.T.: 6.444 min
Delta R.T.: 0.000 min
Response: 105944459
Conc: 81.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

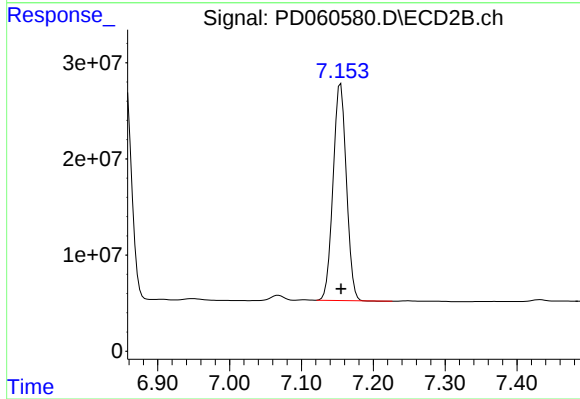


#17 4,4'-DDT

R.T.: 7.155 min
Delta R.T.: 0.000 min
Response: 290372604
Conc: 80.52 ng/ml

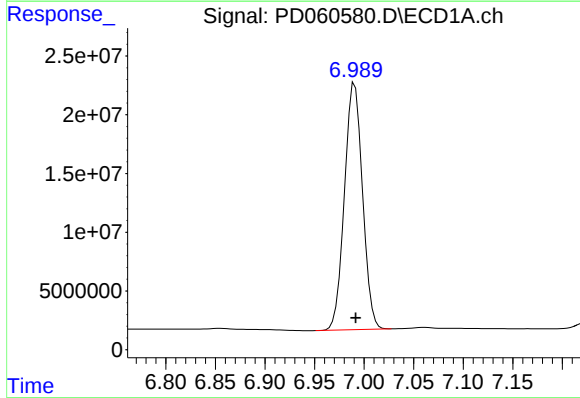


#20 Methoxychlor

R.T.: 6.991 min
Delta R.T.: -0.001 min
Response: 266676393
Conc: 388.43 ng/ml

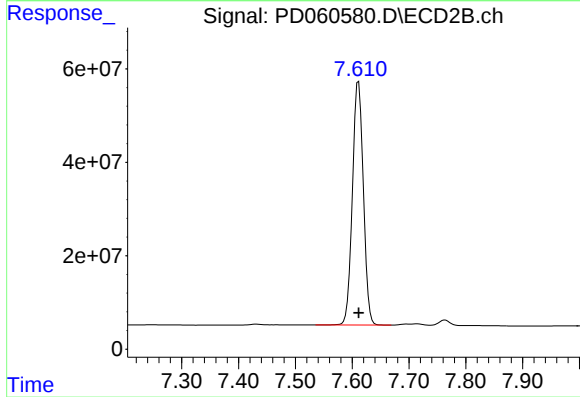

#20 Methoxychlor


R.T.: 7.611 min
Delta R.T.: 0.000 min
Response: 698325192
Conc: 380.70 ng/ml

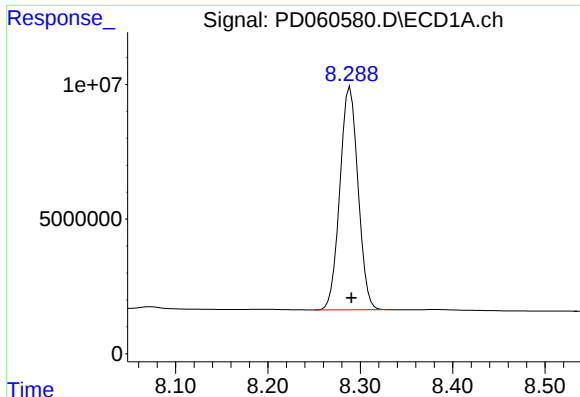

#27 Decachlorobiphenyl

R.T.: 8.289 min
Delta R.T.: -0.001 min
Response: 113300831
Conc: 76.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

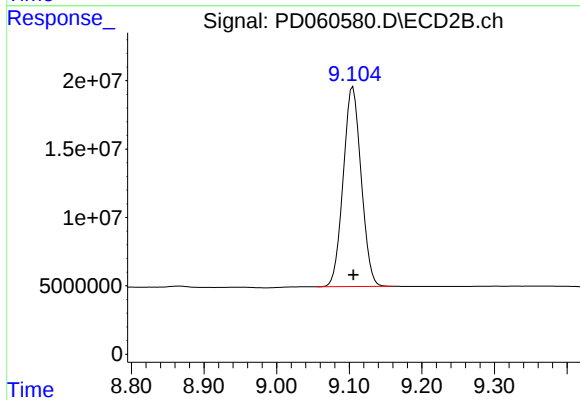

#27 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 250910426
Conc: 76.77 ng/ml