

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120420\
 Data File : PD060582.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2020 18:56
 Operator : DD\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 03:20:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 04 03:19:35 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.502	4.022	84959780	296.8E6	73.209	74.678
27)	SA Decachlor...	8.289	9.105	210.9E6	467.4E6	141.605	143.014
Target Compounds							
2)	A alpha-BHC	3.943	4.412	132.8E6	461.3E6	79.553	77.907
3)	MA gamma-BHC...	4.229	4.698	123.5E6	416.6E6	77.460	76.923
4)	MA Heptachlor	4.535	5.210	127.8E6	405.0E6	76.790	76.597
9)	A Endosulfan I	5.573	6.261	108.9E6	324.2E6	75.290	75.085
13)	MA Dieldrin	5.818	6.518	250.8E6	718.8E6	158.431	152.502
14)	MA Endrin	6.077	6.736	195.2E6	555.3E6	151.259	149.353
16)	A 4,4'-DDD	6.201	6.855	201.0E6	572.0E6	156.523	153.057
17)	MA 4,4'-DDT	6.444	7.155	208.4E6	561.2E6	160.344	155.615
20)	A Methoxychlor	6.991	7.612	495.9E6	1283.3E6	722.291	699.589

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120420\
Data File : PD060582.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2020 18:56
Operator : DD\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 03:20:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 04 03:19:35 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

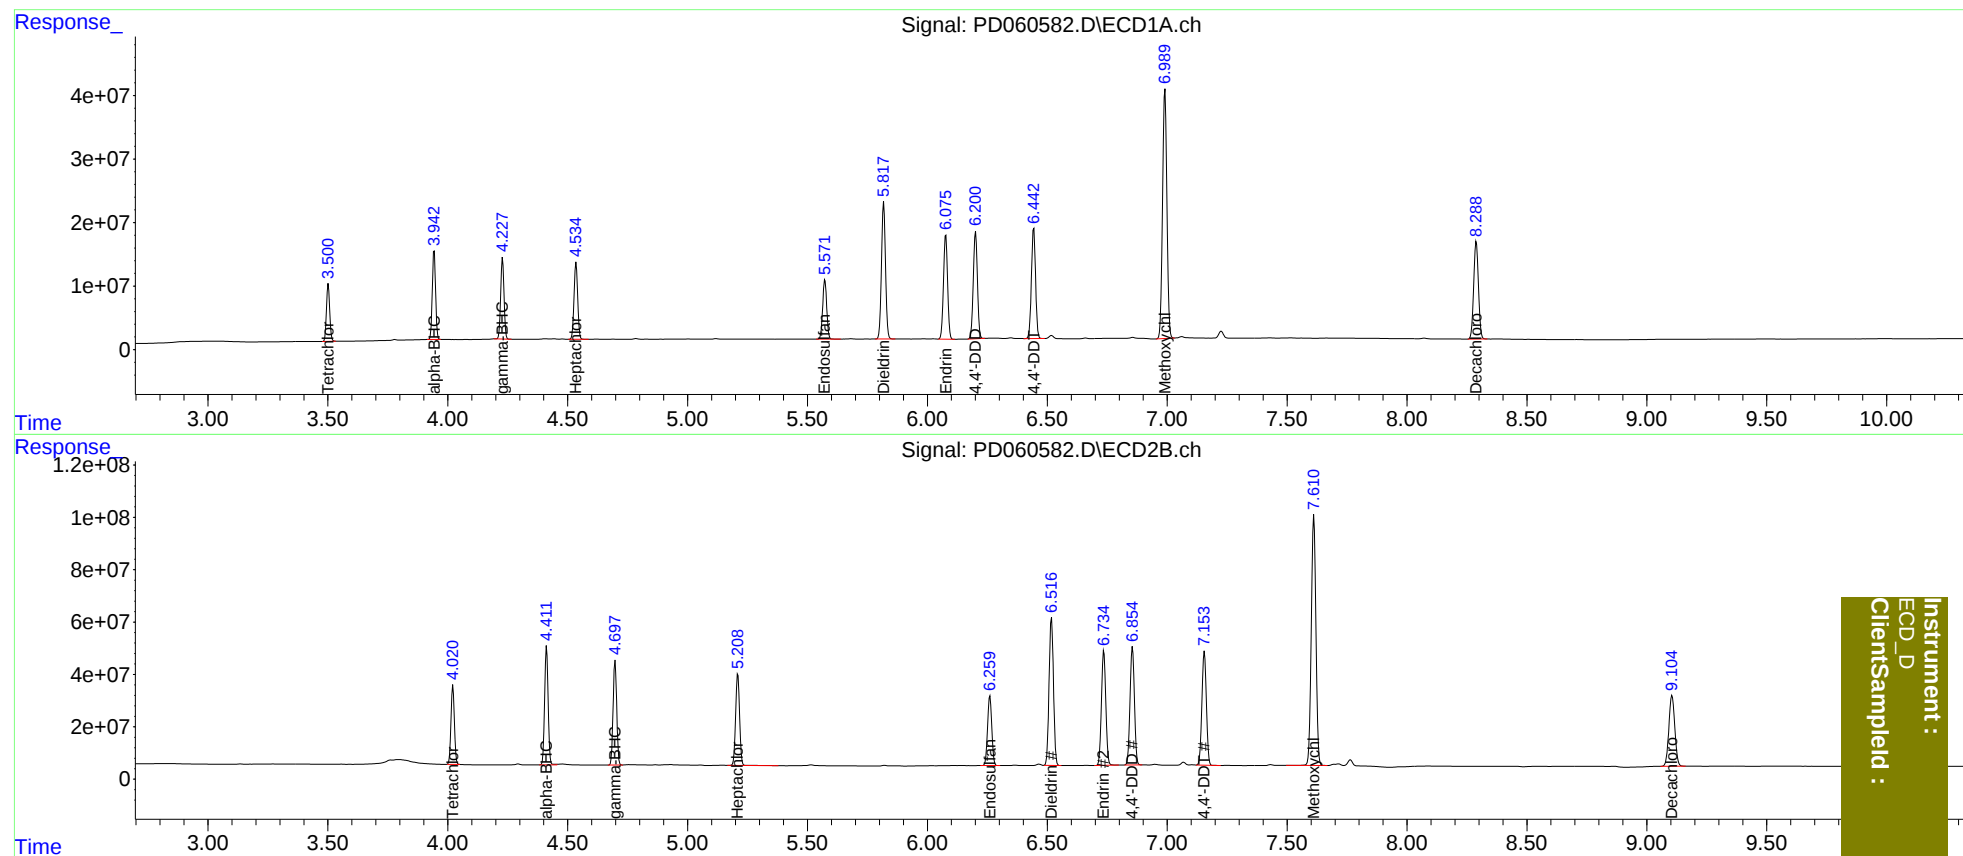


Instrument :
ECD_D
ClientSampled :

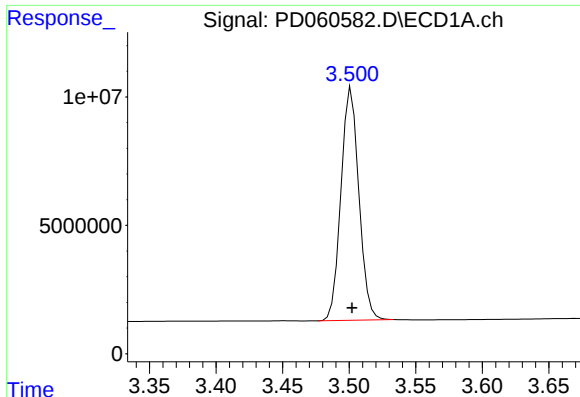

#1 Tetrachloro-m-xylene


R.T.: 3.502 min
Delta R.T.: 0.000 min
Response: 84959780
Conc: 73.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

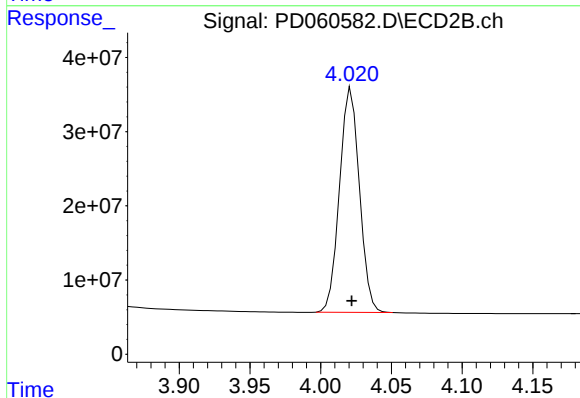


#1 Tetrachloro-m-xylene

R.T.: 4.022 min
Delta R.T.: 0.000 min
Response: 296779396
Conc: 74.68 ng/ml

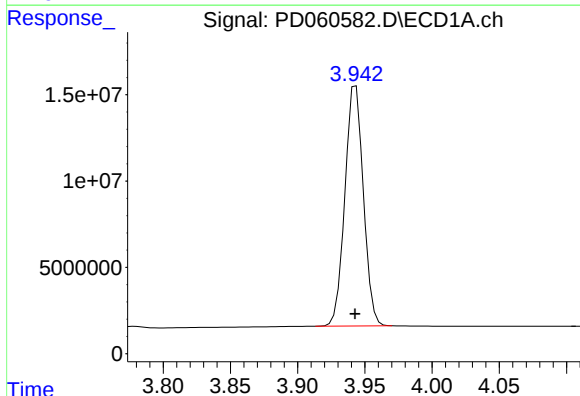


#2 alpha-BHC

R.T.: 3.943 min
Delta R.T.: 0.000 min
Response: 132817516
Conc: 79.55 ng/ml

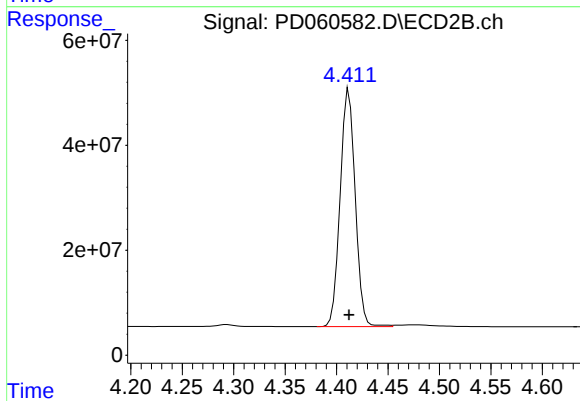

#2 alpha-BHC


R.T.: 4.412 min
Delta R.T.: 0.000 min
Response: 461310409
Conc: 77.91 ng/ml

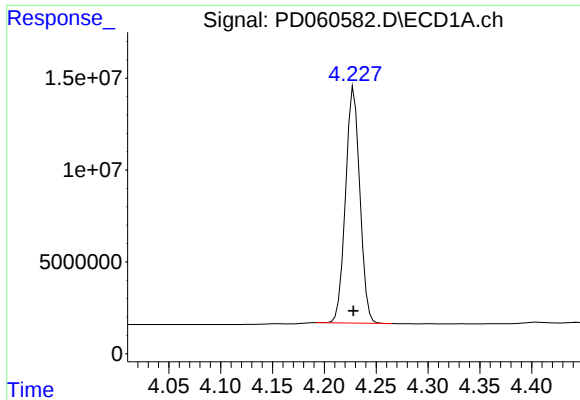

#3 gamma-BHC (Lindane)


R.T.: 4.229 min
Delta R.T.: 0.000 min
Response: 123469854
Conc: 77.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

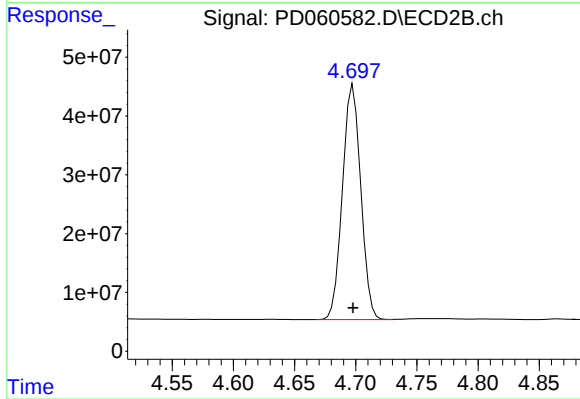


#3 gamma-BHC (Lindane)

R.T.: 4.698 min
Delta R.T.: 0.000 min
Response: 416621911
Conc: 76.92 ng/ml

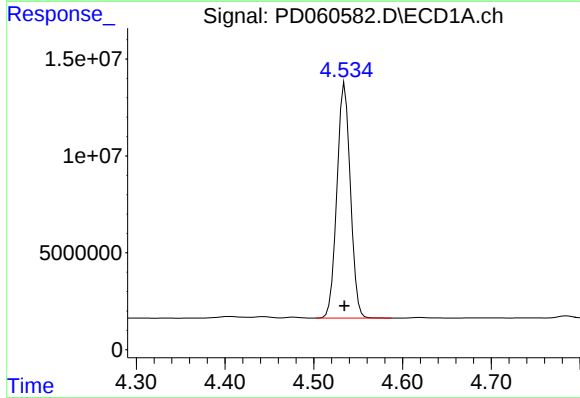


#4 Heptachlor

R.T.: 4.535 min
Delta R.T.: 0.000 min
Response: 127771370
Conc: 76.79 ng/ml

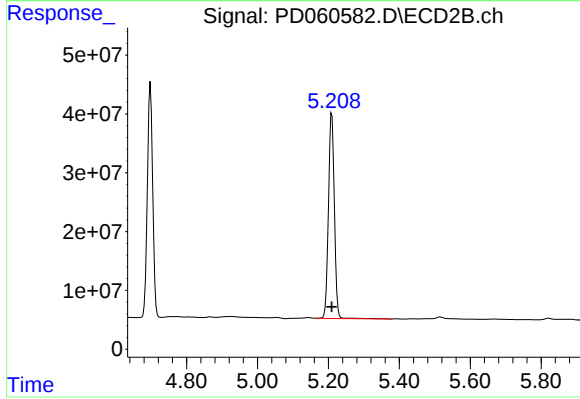

#4 Heptachlor


R.T.: 5.210 min
Delta R.T.: 0.000 min
Response: 404962530
Conc: 76.60 ng/ml

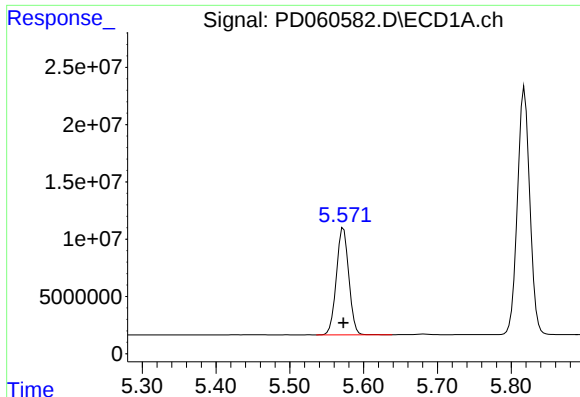

#9 Endosulfan I


R.T.: 5.573 min
Delta R.T.: 0.000 min
Response: 108945907
Conc: 75.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

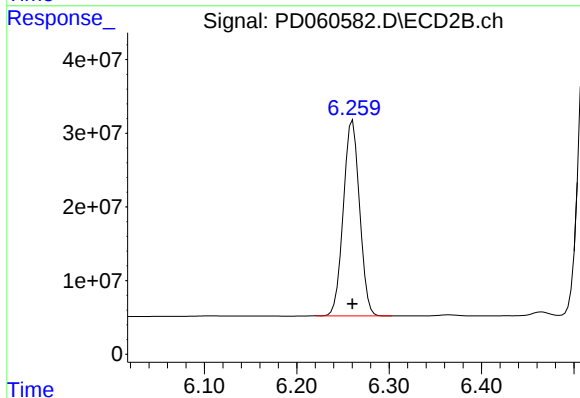


#9 Endosulfan I

R.T.: 6.261 min
Delta R.T.: 0.000 min
Response: 324248925
Conc: 75.09 ng/ml

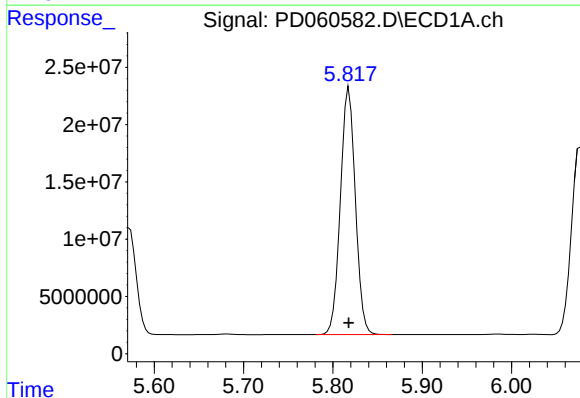


#13 Dieldrin

R.T.: 5.818 min
Delta R.T.: 0.000 min
Response: 250808263
Conc: 158.43 ng/ml

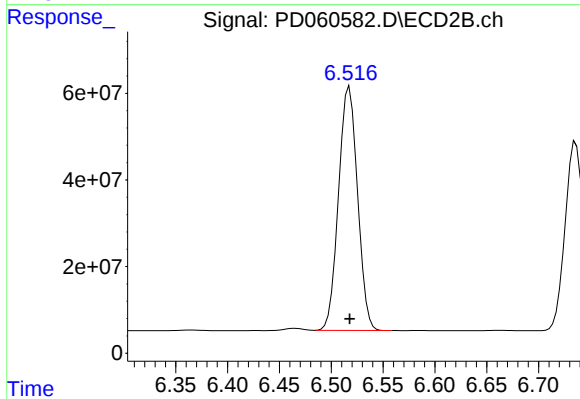

#13 Dieldrin


R.T.: 6.518 min
Delta R.T.: 0.000 min
Response: 718774918
Conc: 152.50 ng/ml

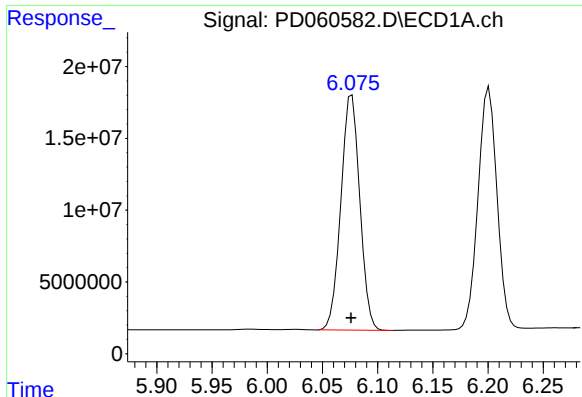

#14 Endrin


R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 195178574
Conc: 151.26 ng/ml

Instrument :
ECD_D
ClientSampleId :

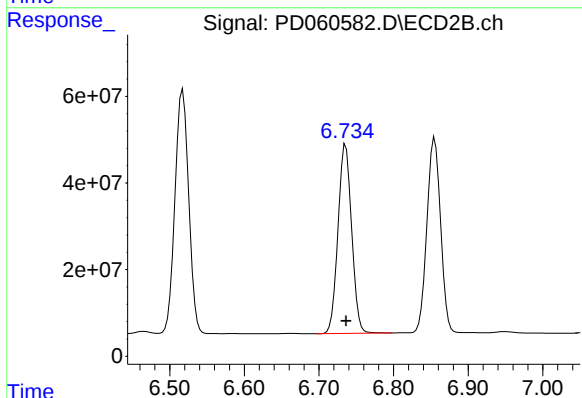


#14 Endrin

R.T.: 6.736 min
Delta R.T.: 0.000 min
Response: 555286020
Conc: 149.35 ng/ml

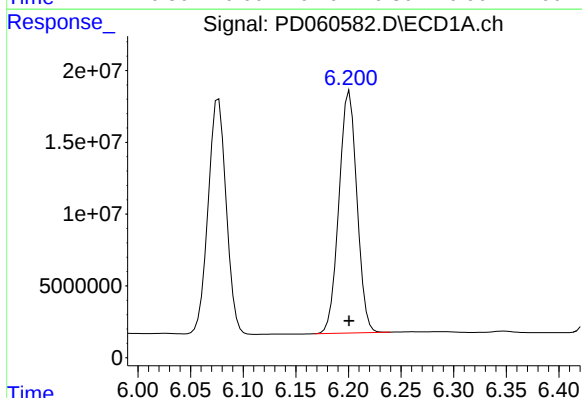


#16 4,4'-DDD

R.T.: 6.201 min
Delta R.T.: 0.000 min
Response: 201009826
Conc: 156.52 ng/ml

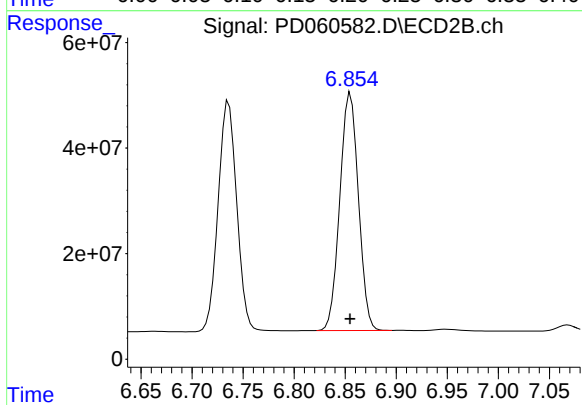

#16 4,4'-DDD


R.T.: 6.855 min
Delta R.T.: 0.000 min
Response: 572022989
Conc: 153.06 ng/ml

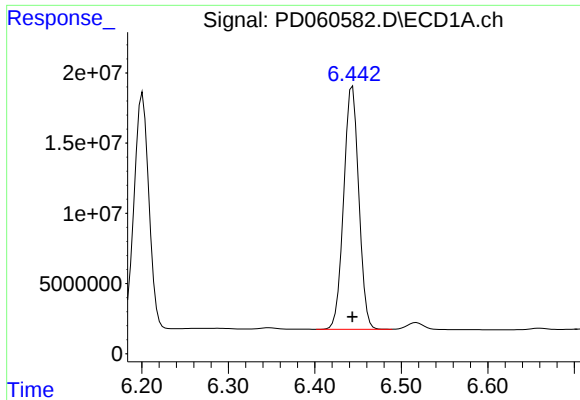

#17 4,4'-DDT


R.T.: 6.444 min
Delta R.T.: 0.000 min
Response: 208435586
Conc: 160.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

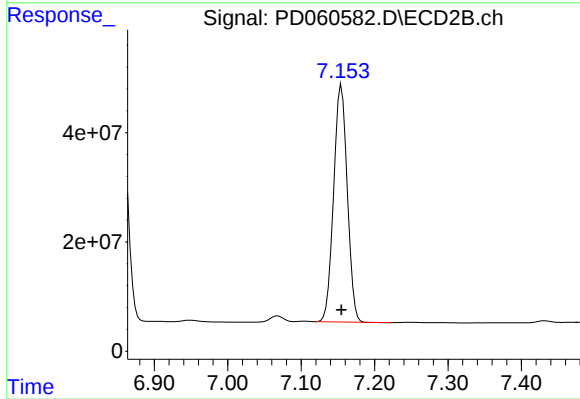


#17 4,4'-DDT

R.T.: 7.155 min
Delta R.T.: 0.000 min
Response: 561205980
Conc: 155.61 ng/ml

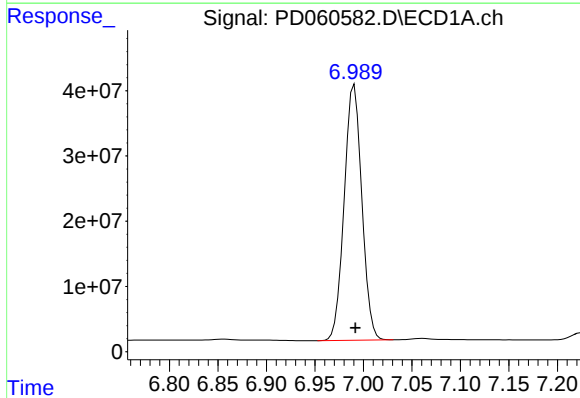


#20 Methoxychlor

R.T.: 6.991 min
Delta R.T.: 0.000 min
Response: 495889280
Conc: 722.29 ng/ml

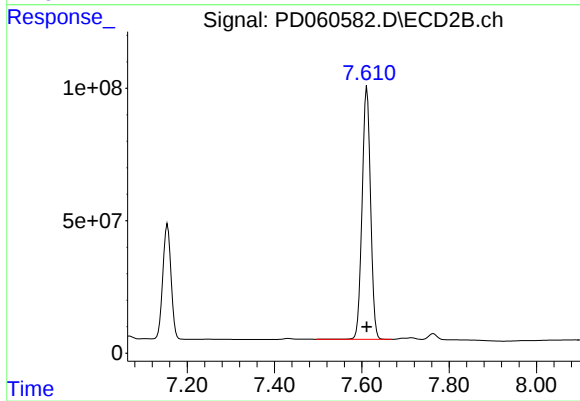

#20 Methoxychlor


R.T.: 7.612 min
Delta R.T.: 0.000 min
Response: 1283259838
Conc: 699.59 ng/ml

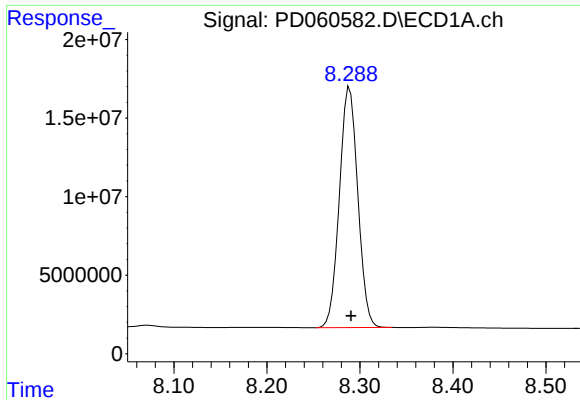

#27 Decachlorobiphenyl

R.T.: 8.289 min
Delta R.T.: -0.001 min
Response: 210858905
Conc: 141.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

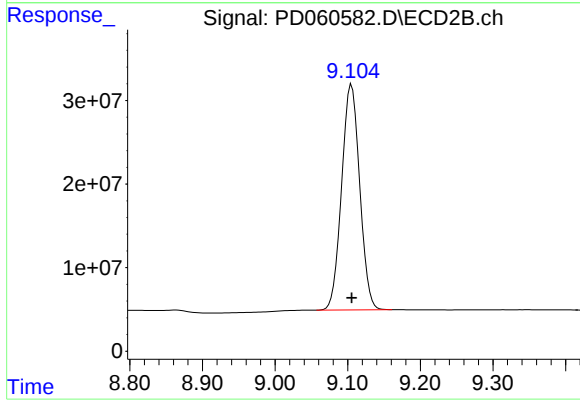

#27 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 467418640
Conc: 143.01 ng/ml