

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120420\
 Data File : PD060580.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2020 18:28
 Operator : DD\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA401

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 03:25:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 04 03:19:35 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.502	4.021	44942149	157.5E6	38.726	39.638
27)	SA Decachlor...	8.289	9.105	113.3E6	250.9E6	76.088	76.770
Target Compounds							
2)	A alpha-BHC	3.943	4.412	67424384	238.9E6	40.385	40.341
3)	MA gamma-BHC...	4.228	4.698	63515965	217.5E6	39.847	40.158
4)	MA Heptachlor	4.534	5.209	65860260	210.7E6	39.582	39.861
9)	A Endosulfan I	5.573	6.261	56763571	171.1E6	39.228	39.624
13)	MA Dieldrin	5.818	6.518	128.2E6	377.0E6	80.983	79.995
14)	MA Endrin	6.076	6.736	101.6E6	293.7E6	78.772	78.996
16)	A 4,4'-DDD	6.200	6.855	103.4E6	299.8E6	80.540	80.223
17)	MA 4,4'-DDT	6.444	7.155	105.9E6	290.4E6	81.500	80.516
20)	A Methoxychlor	6.991	7.611	266.7E6	698.1E6	388.430	380.594

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120420\
Data File : PD060580.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2020 18:28
Operator : DD\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 03:25:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 04 03:19:35 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

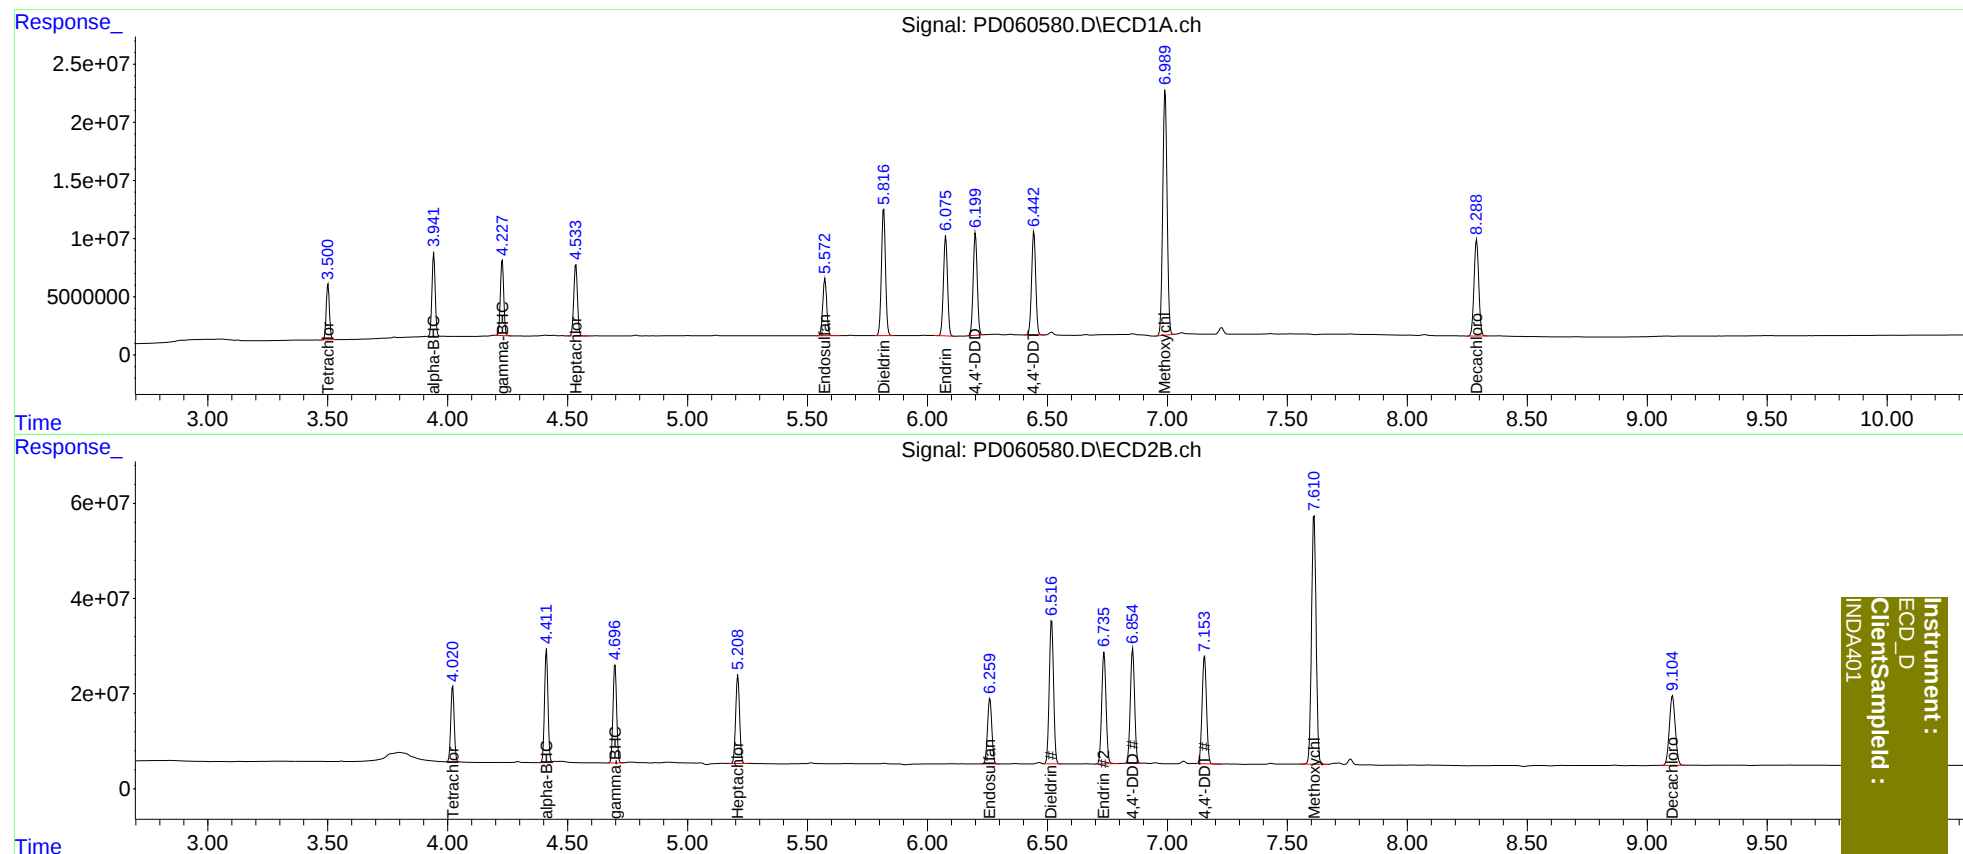

Instrument :
ECD_D
ClientSample :
INDA401