

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120420\
 Data File : PD060582.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2020 18:56
 Operator : DD\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA501

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 03:24:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 04 03:19:35 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.502	4.022	84959780	296.8E6	73.209	74.678
27)	SA Decachlor...	8.289	9.105	210.9E6	467.4E6	141.605	143.014
Target Compounds							
2)	A alpha-BHC	3.943	4.412	132.8E6	461.3E6	79.553	77.907
3)	MA gamma-BHC...	4.229	4.698	123.5E6	416.6E6	77.460	76.923
4)	MA Heptachlor	4.535	5.210	127.8E6	398.9E6	76.790	75.449
9)	A Endosulfan I	5.573	6.261	108.9E6	324.2E6	75.290	75.085
13)	MA Dieldrin	5.818	6.518	250.8E6	718.8E6	158.431	152.502
14)	MA Endrin	6.077	6.736	195.2E6	555.3E6	151.259	149.353
16)	A 4,4'-DDD	6.201	6.855	201.0E6	572.0E6	156.523	153.057
17)	MA 4,4'-DDT	6.444	7.155	208.4E6	561.2E6	160.344	155.615
20)	A Methoxychlor	6.991	7.612	495.9E6	1281.1E6	722.291	698.404

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120420\
Data File : PD060582.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2020 18:56
Operator : DD\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 03:24:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 04 03:19:35 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

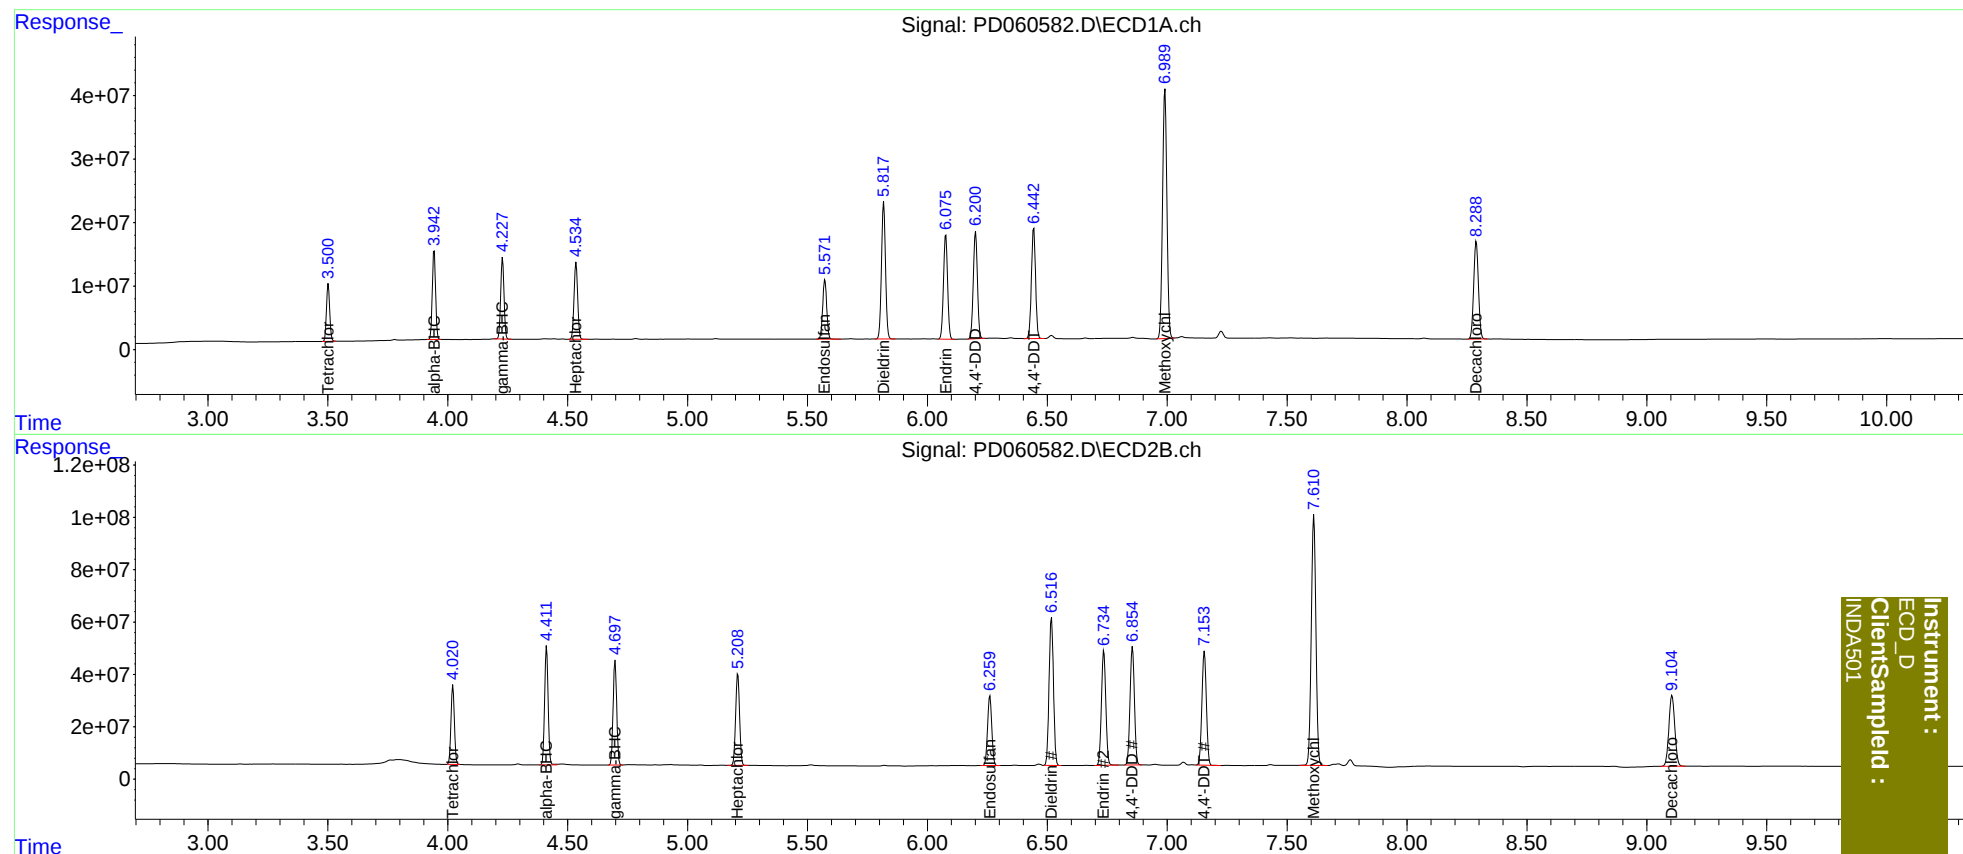

Instrument :
ECD_D
ClientSample :
INDA501