

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120420\
 Data File : PD060567.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2020 15:26
 Operator : DD\AJ
 Sample : RESC10
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 04:03:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 04 03:58:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.502	4.022	22639586	78227124	19.378	19.888
2)	SA Decachlor...	8.290	9.107	57806070	126.5E6	38.776	39.085
Target Compounds							
2)	A alpha-BHC	3.943	4.412	16455155	58398138	9.771	9.895
3)	MA gamma-BHC...	4.228	4.698	15719641	53428184	9.746	9.964
4)	MA Heptachlor	4.534	5.210	16901979	53192814	10.065	10.111
5)	MB Aldrin	4.785	5.516	15978395	49795976	9.934	10.001
6)	B beta-BHC	4.478	4.866	8028254	23484578	10.470	9.869
7)	B delta-BHC	4.686	5.085	15904854	44838640	9.932	9.407
8)	B Heptachlo...	5.231	5.903	15263892	41491711	9.990	9.632
9)	A Endosulfan I	5.572	6.261	14542304	41534315	10.009	9.703
10)	B trans-Chl...	5.460	6.137	15690413	46989601	9.920	9.970
11)	B cis-Chlor...	5.519	6.210	15486631	44013007	9.943	9.760
12)	B 4,4'-DDE	5.683	6.365	29514771	87075889	19.609	19.717
13)	MA Dieldrin	5.818	6.518	31040354	92172370	19.546	19.734
14)	MA Endrin	6.076	6.736	26727681	76167602	20.657	20.662
15)	B Endosulfa...	6.349	6.944	25217595	70989209	19.938	19.749
16)	A 4,4'-DDD	6.200	6.855	25161091	72788147	19.582	19.754
17)	MA 4,4'-DDT	6.443	7.155	25753290	71328638	19.773	19.879
18)	B Endrin al...	6.518	7.068	21985967	61675448	20.484	20.308
19)	B Endosulfa...	6.732	7.292	24097684	71977132	20.215	20.143
20)	A Methoxychlor	6.991	7.612	69723756	189.4E6	102.518	105.003
21)	B Endrin ke...	7.228	7.764	30122956	75830036	20.808	19.975

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120420\
Data File : PD060567.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2020 15:26
Operator : DD\AJ
Sample : RESC10
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 04:03:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 04 03:58:39 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

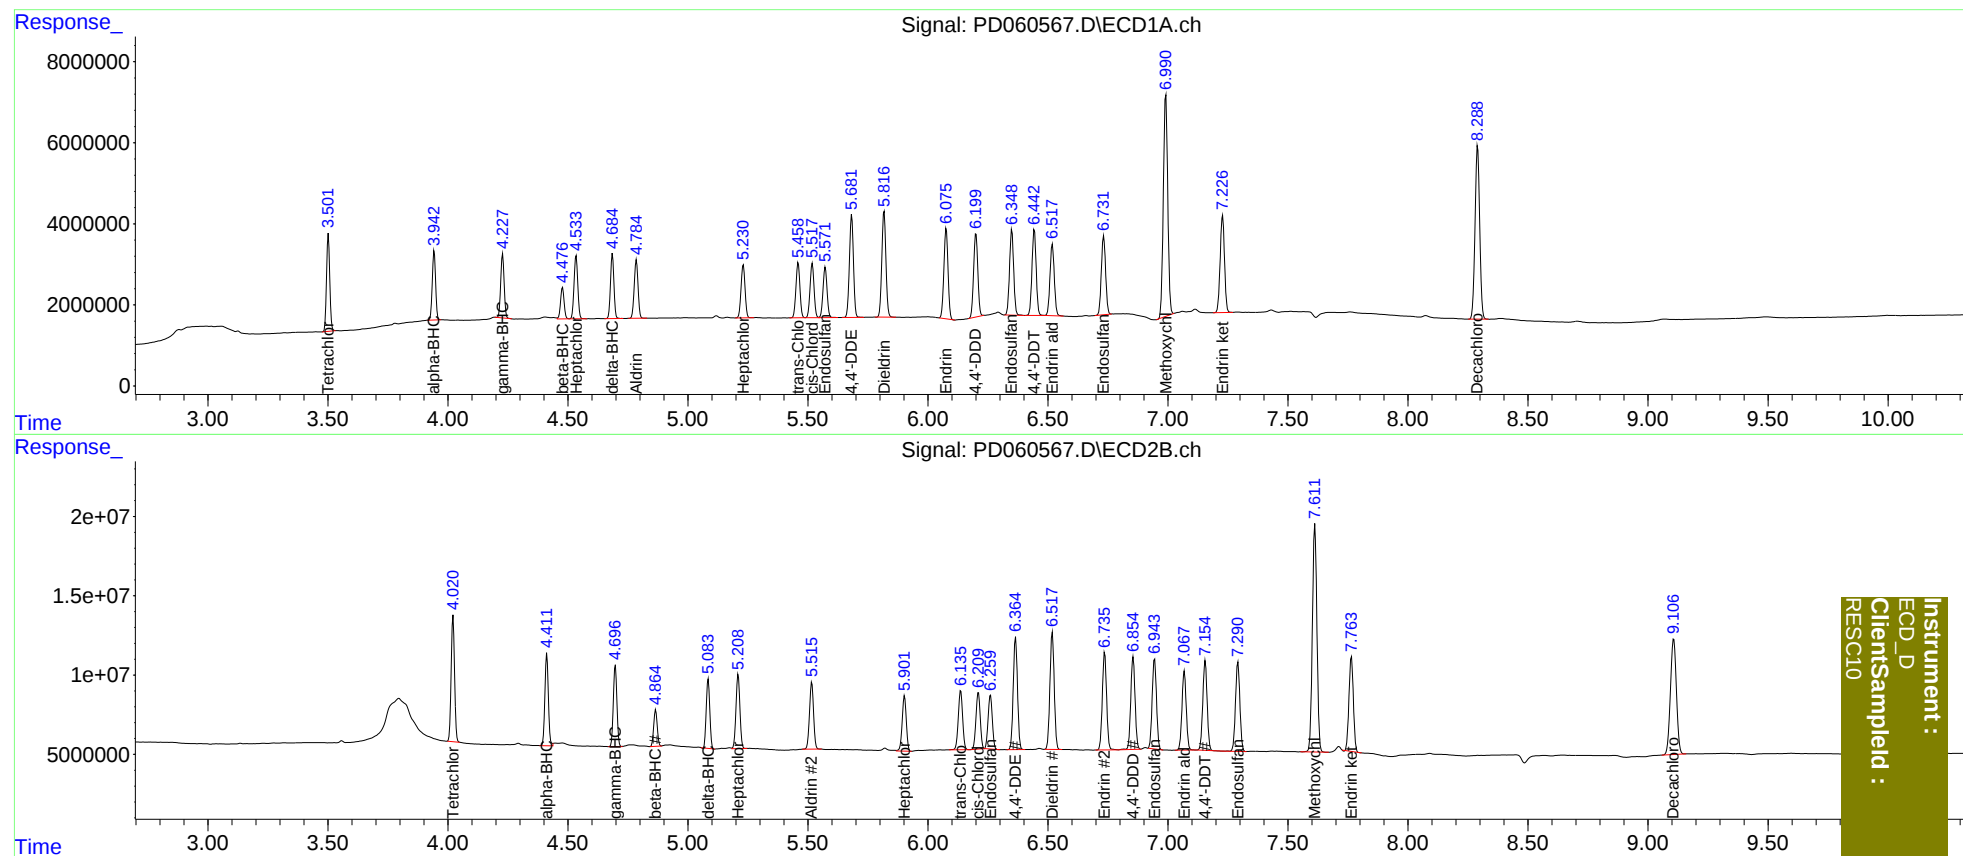

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120420\
Data File : PD060567.D
Acq On : 03 Dec 2020 15:26
Operator : DD\AJ
Sample : RESC10
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
Title : GC Extractables
Last Update : Fri Dec 04 03:58:39 2020
Integrator: ChemStation

RT#1	RT#2	Resolution
3.502	3.943	100.00%
3.943	4.228	100.00%
4.228	4.478	100.00%
4.478	4.534	100.00%
4.534	4.686	100.00%
4.686	4.785	100.00%
4.785	5.231	100.00%
5.231	5.460	100.00%
5.460	5.519	100.00%
5.519	5.572	100.00%
5.572	5.683	100.00%
5.683	5.818	100.00%
5.818	6.076	100.00%
6.076	6.200	100.00%
6.200	6.349	100.00%
6.349	6.443	100.00%
6.443	6.518	100.00%
6.518	6.732	100.00%
6.732	6.991	100.00%
6.991	7.228	100.00%
7.228	8.290	100.00%

Signal #2

4.022	4.412	100.00%
4.412	4.698	100.00%
4.698	4.866	100.00%
4.866	5.085	100.00%
5.085	5.210	100.00%
5.210	5.516	100.00%
5.516	5.903	100.00%
5.903	6.137	100.00%
6.137	6.210	100.00%
6.210	6.261	100.00%
6.261	6.365	100.00%
6.365	6.518	100.00%
6.518	6.736	100.00%
6.736	6.855	100.00%
6.855	6.944	100.00%
6.944	7.068	100.00%
7.068	7.155	100.00%
7.155	7.292	100.00%
7.292	7.612	100.00%
7.612	7.764	100.00%
7.764	9.107	100.00%