

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120425\
 Data File : PD091451.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2025 12:50
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 04:20:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX111525.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 15 05:17:12 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.871	169.0E6	2059.9E6	51.742	58.602
7)	SA Decachlor...	9.069	8.057	232.1E6	2179.8E6	48.725	56.010
Target Compounds							
2)	Toxaphene-1	6.238	5.463	16998467	188.1E6	403.223	539.775 #
3)	Toxaphene-2	6.440	5.634	34057853	125.9E6	482.998	557.705
4)	Toxaphene-3	7.145	6.744	53647491	581.1E6	482.200	555.353
5)	Toxaphene-4	7.561	7.185	62562666	381.3E6	481.818	563.543
6)	Toxaphene-5	7.927	7.316	37578630	223.0E6	483.518	532.920

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120425\
Data File : PD091451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2025 12:50
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 04:20:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX111525.M
Quant Title : GC Extractables
QLast Update : Sat Nov 15 05:17:12 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x0.25µm

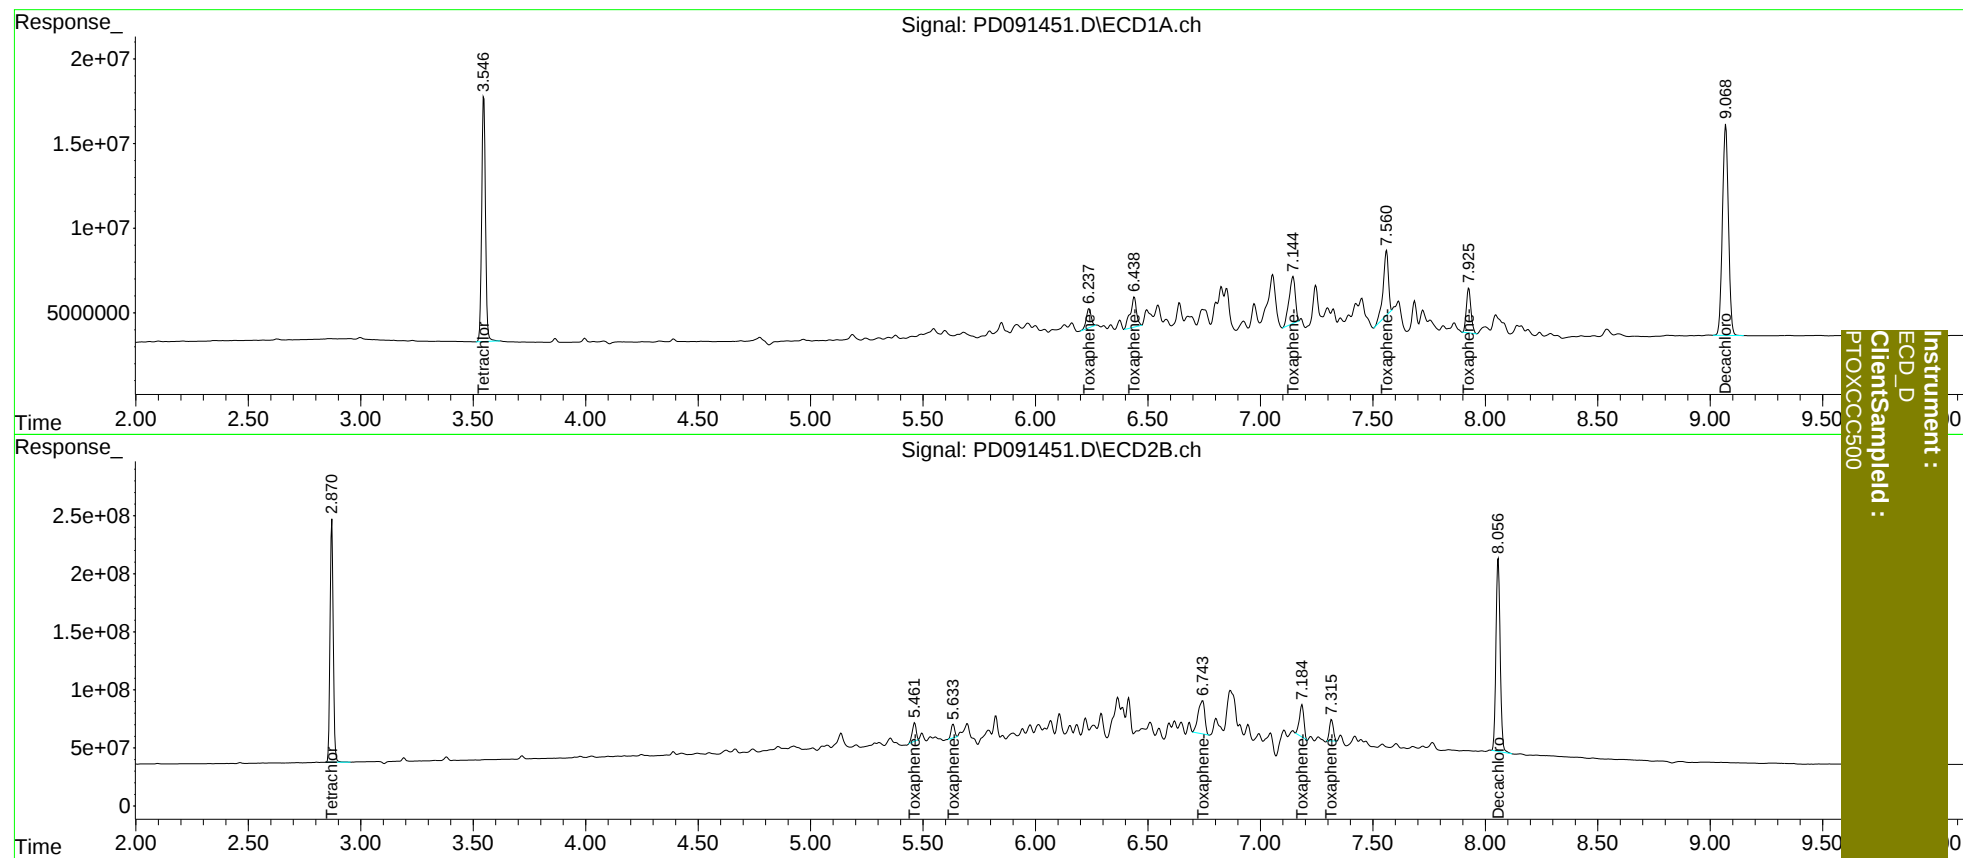

Instrument :
ECD_D
ClientSampled :
PTOXCCC500