

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120425\
 Data File : PD091455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2025 14:25
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 04:20:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX111525.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 15 05:17:12 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.871	156.2E6	1905.8E6	47.819	54.218
7)	SA Decachlor...	9.069	8.057	218.0E6	2012.0E6	45.766	51.699
Target Compounds							
2)	Toxaphene-1	6.240	5.463	22591908	188.2E6	535.905	539.955
3)	Toxaphene-2	6.440	5.635	31855419	116.6E6	451.763	516.853
4)	Toxaphene-3	7.146	6.743	49518184	532.9E6	445.085	509.371
5)	Toxaphene-4	7.562	7.186	57801106	356.8E6	445.147	527.339
6)	Toxaphene-5	7.927	7.317	34759517	205.5E6	447.245	490.995

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120425\
Data File : PD091455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2025 14:25
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 04:20:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX111525.M
Quant Title : GC Extractables
QLast Update : Sat Nov 15 05:17:12 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x0.25µm

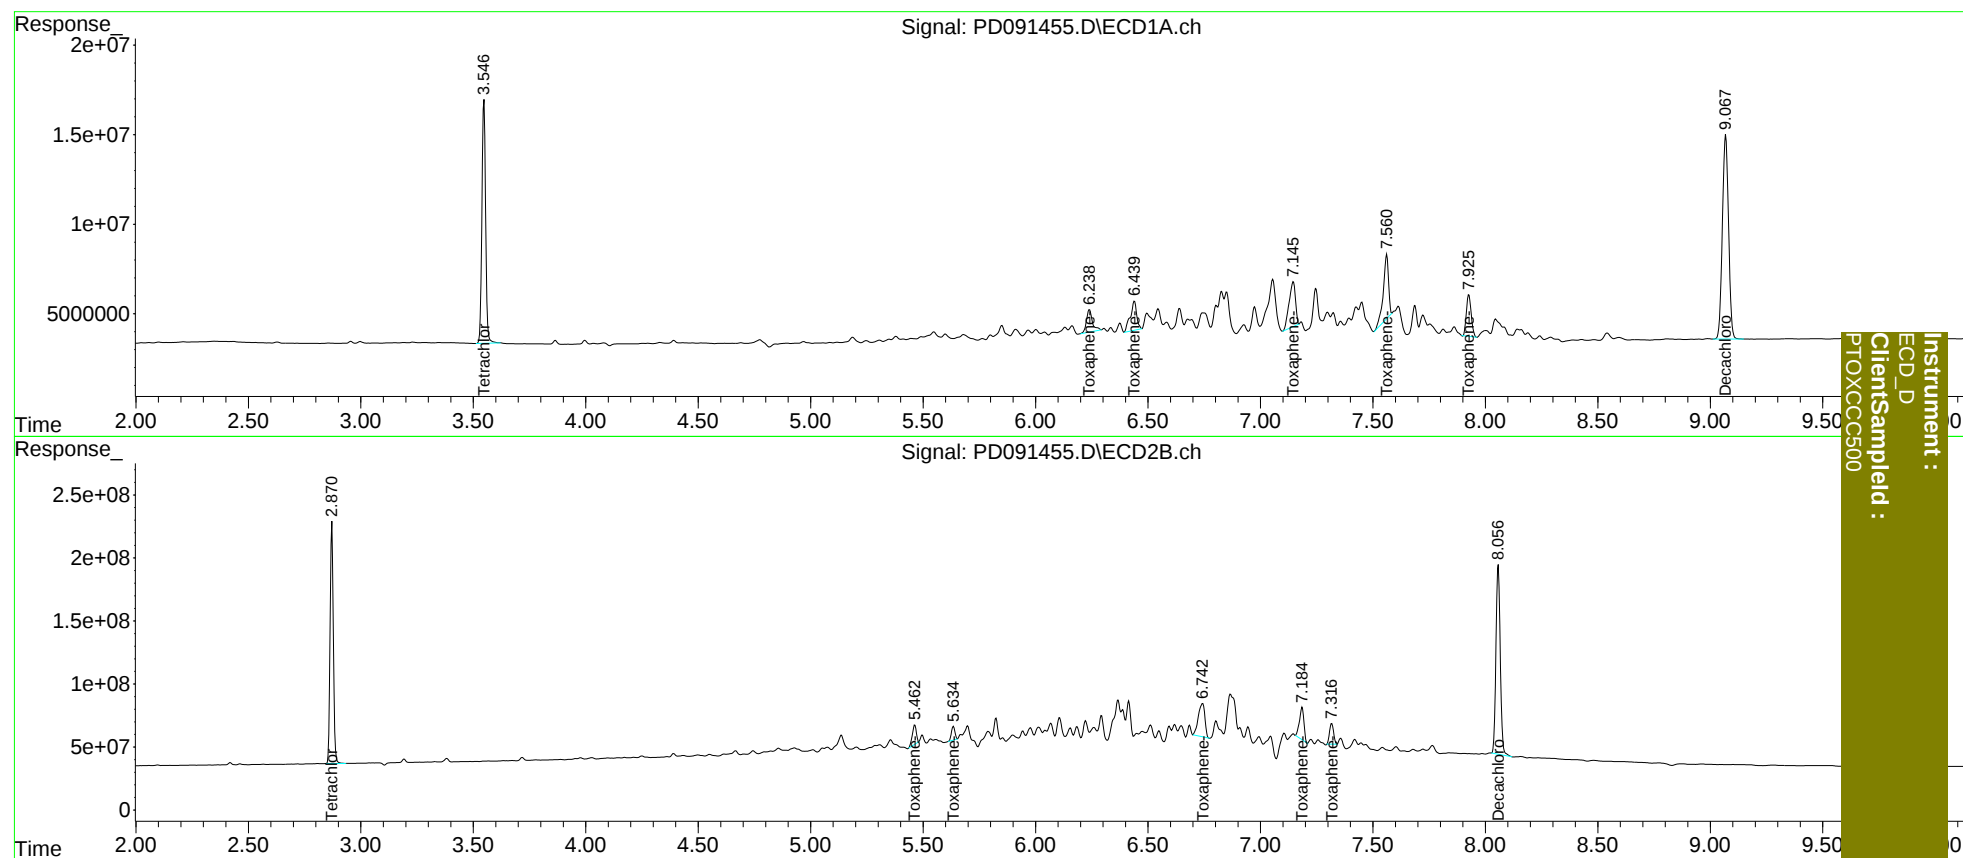

Instrument :
ECD_D
ClientSampled :
PTOXCCC500