

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120519\
 Data File : PD056269.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2019 10:51
 Operator : SG\AJ
 Sample : K6088-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BN6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 02:59:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.962	6767899	10442086	8.172	8.685
27)	SA Decachlor...	7.962	8.999	12254275	16666043	13.571	13.852
Target Compounds							
7)	B delta-BHC	0.000	4.991f	0	1830209	N.D.	1.099
16)	A 4,4'-DDD	0.000	6.736f	0	151822	N.D.	0.129


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120519\
Data File : PD056269.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2019 10:51
Operator : SG\AJ
Sample : K6088-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 02:59:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

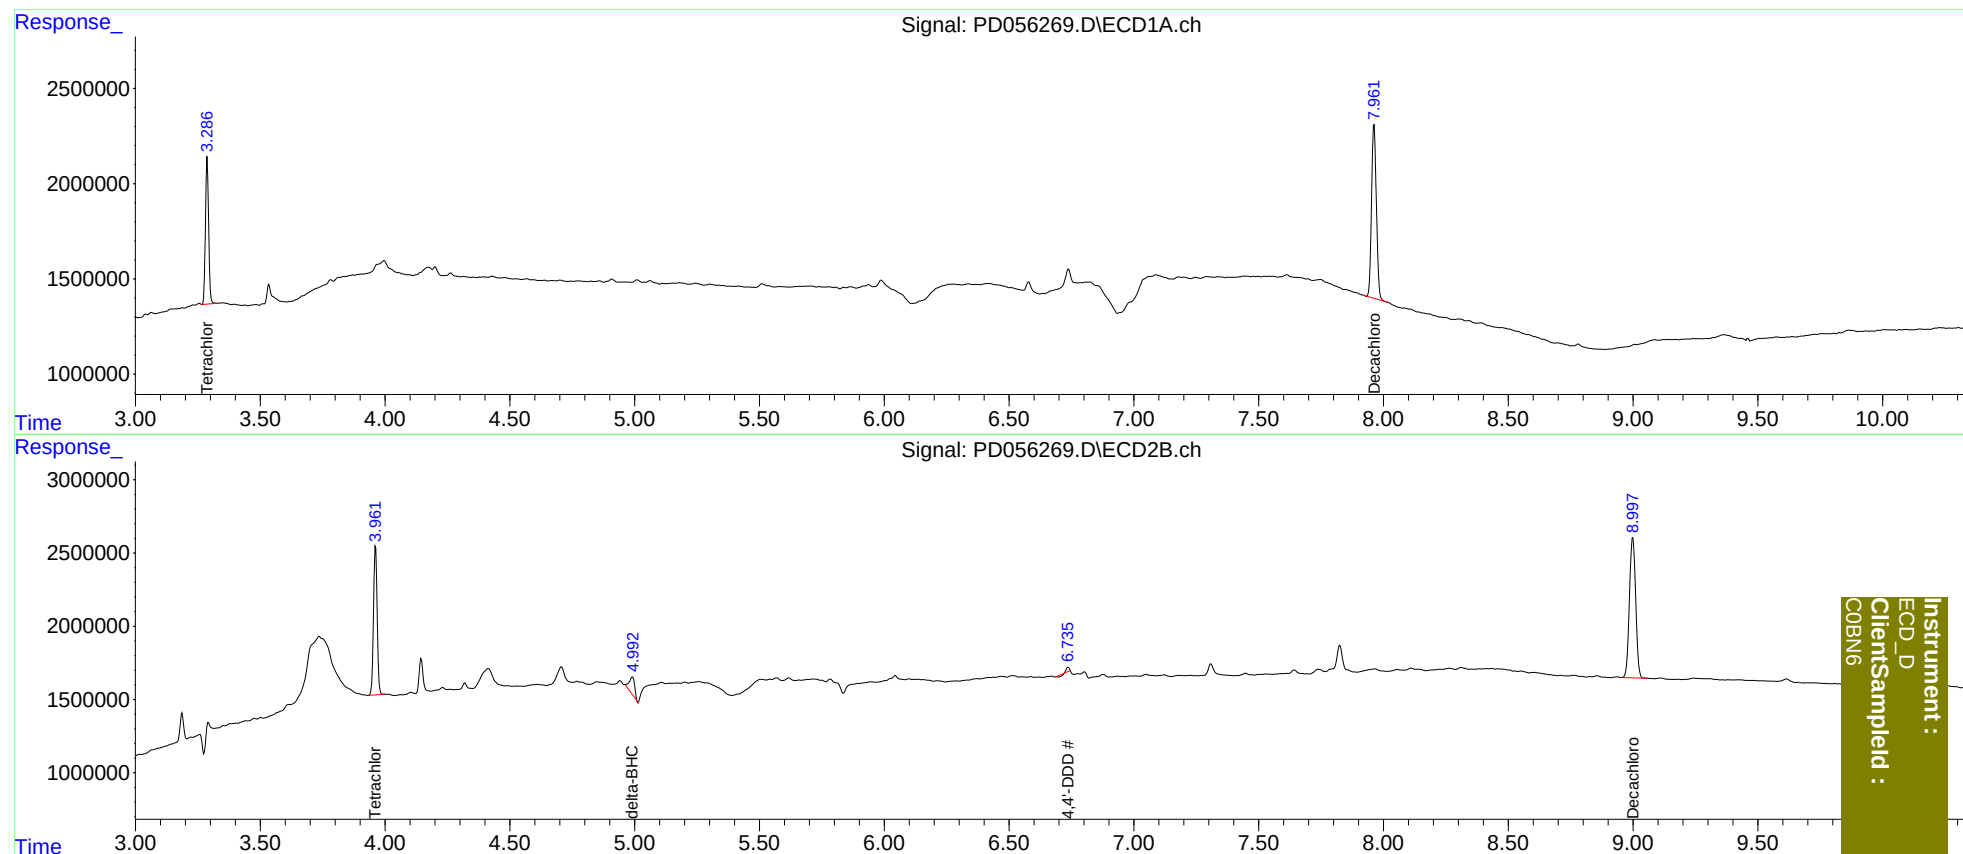


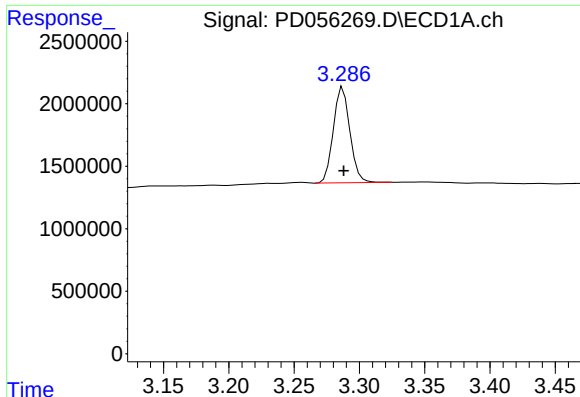

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: 0.000 min
Response: 6767899
Conc: 8.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BN6

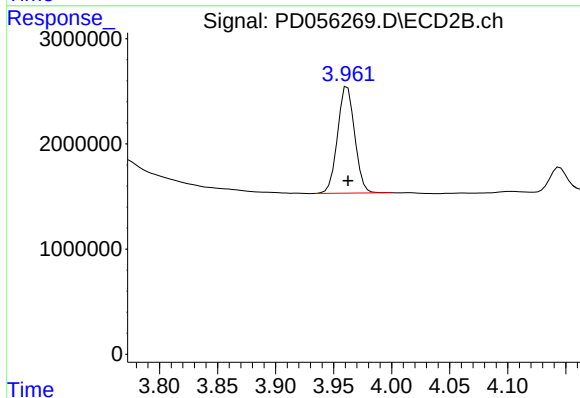


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 10442086
Conc: 8.69 ng/ml

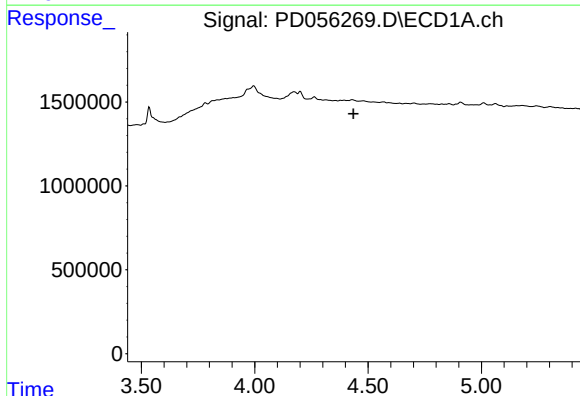


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.436 min
Response: 0
Conc: N.D.

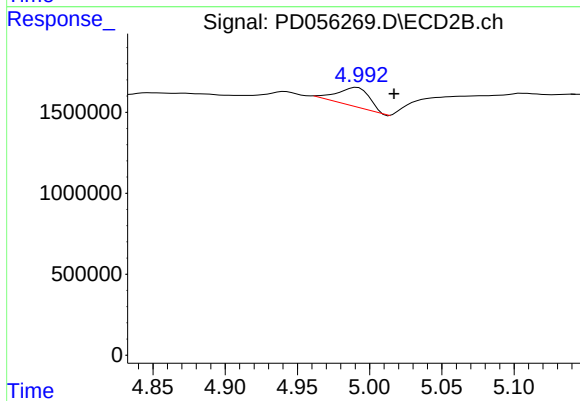

#7 delta-BHC


R.T.: 4.991 min
Delta R.T.: -0.026 min
Response: 1830209
Conc: 1.10 ng/ml

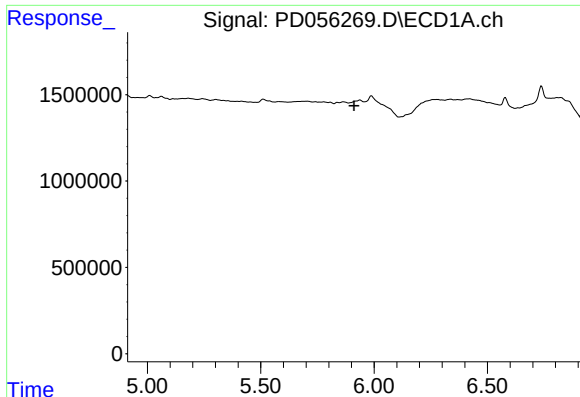

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.912 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BN6

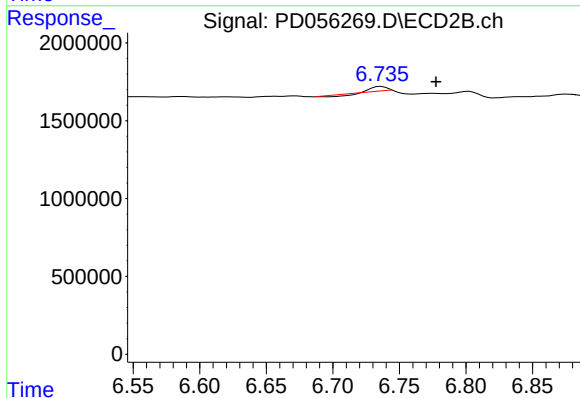


#16 4,4'-DDD

R.T.: 6.736 min
Delta R.T.: -0.041 min
Response: 151822
Conc: 0.13 ng/ml

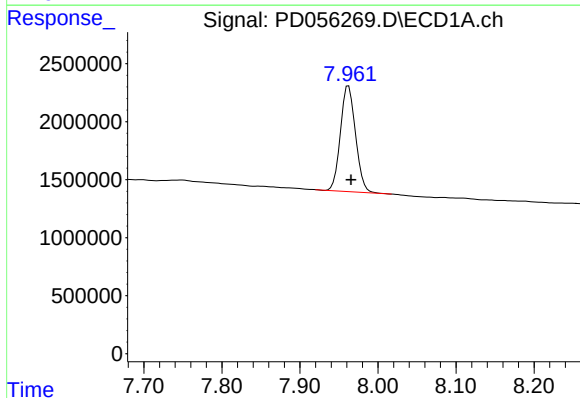

#27 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: -0.003 min
Response: 12254275
Conc: 13.57 ng/ml

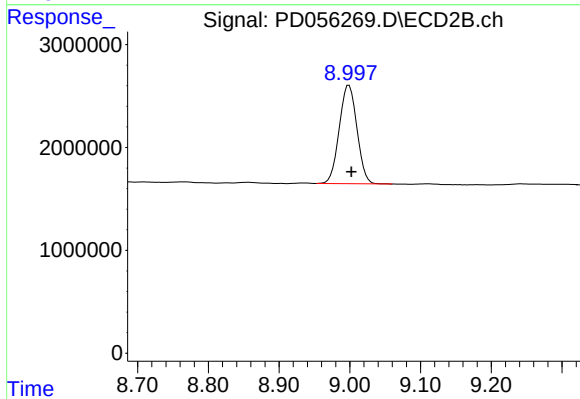

#27 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: -0.004 min
Response: 16666043
Conc: 13.85 ng/ml