

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120519\
 Data File : PD056272.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2019 11:33
 Operator : SG\AJ
 Sample : K6088-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BP2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 02:59:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.962	5873032	9277178	7.091	7.716
2)	SA Decachlor...	7.962	8.998	9044422	11624458	10.016	9.662
Target Compounds							
10)	B trans-Chl...	0.000	6.083	0	2002567	N.D.	1.211
11)	B cis-Chlor...	0.000	6.083f	0	2002567	N.D.	1.243
16)	A 4,4'-DDD	0.000	6.736f	0	309650	N.D.	0.263


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120519\
Data File : PD056272.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2019 11:33
Operator : SG\AJ
Sample : K6088-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 02:59:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

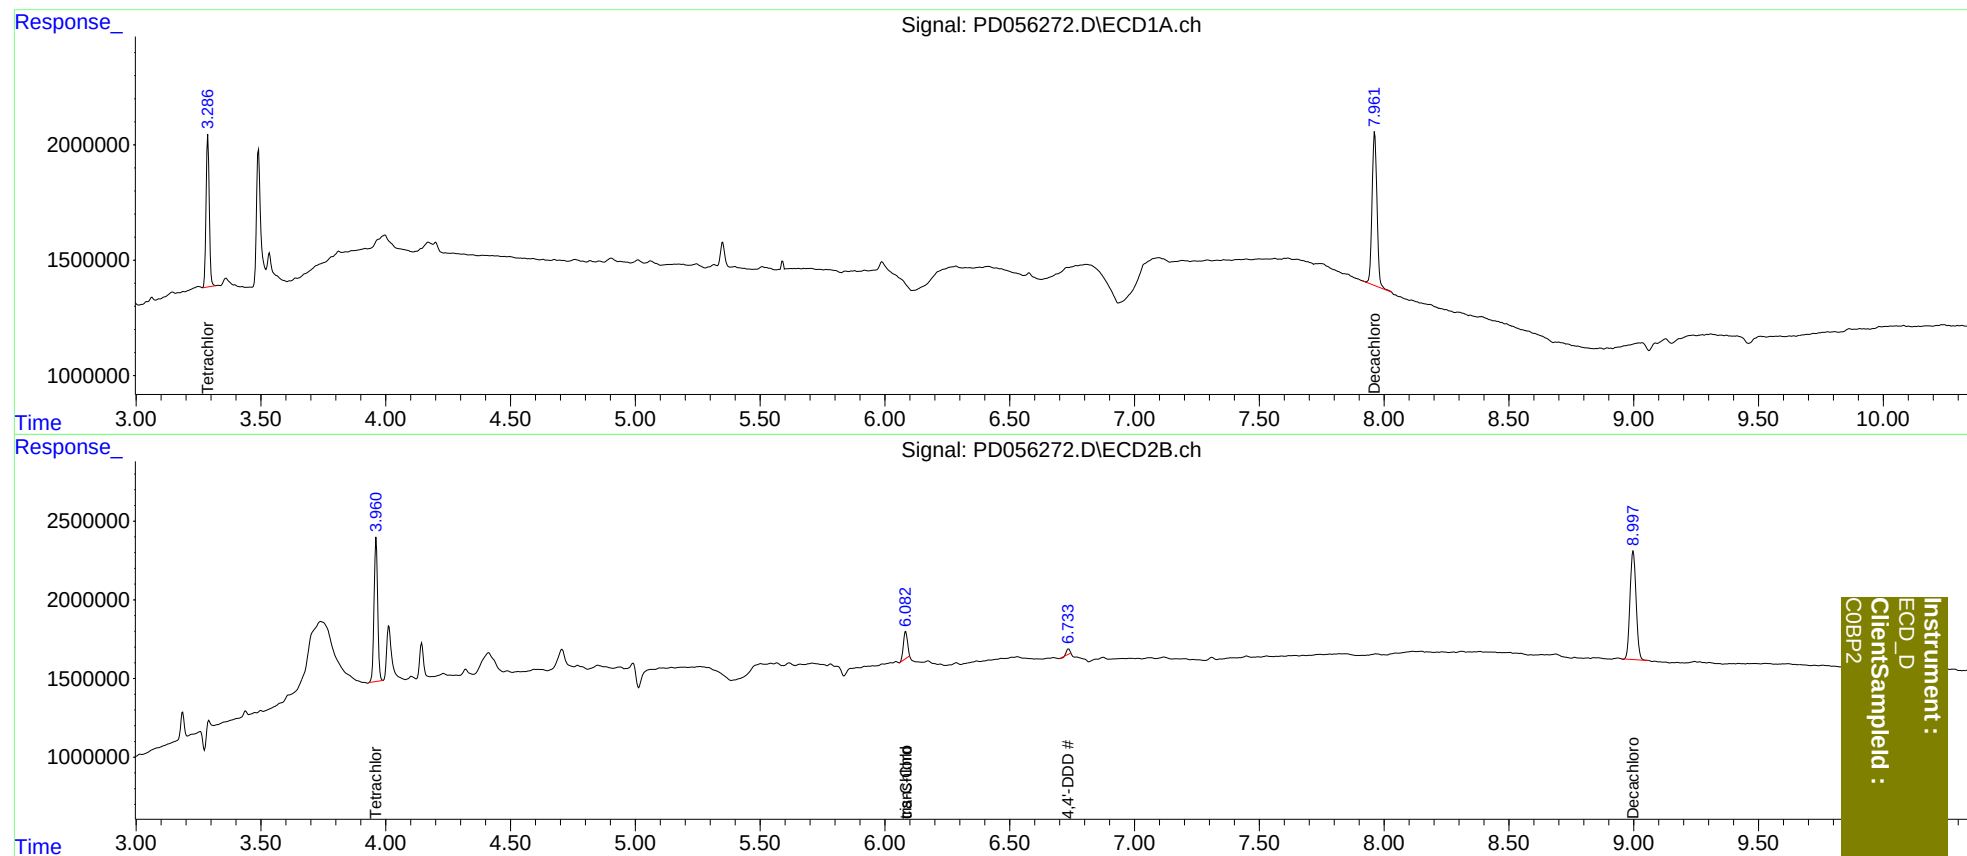


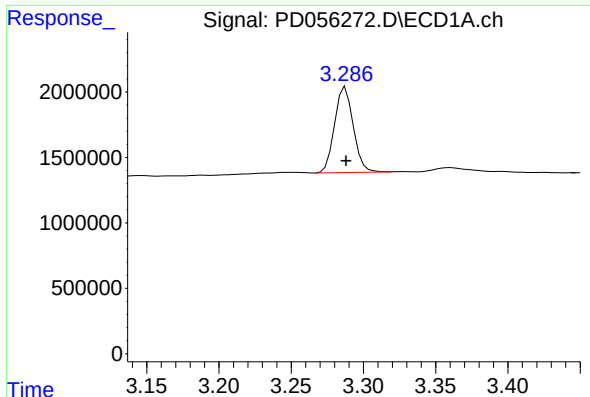

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: 0.000 min
Response: 5873032
Conc: 7.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BP2

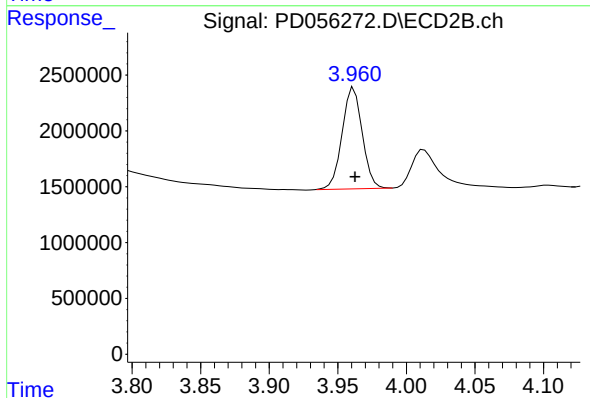


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 9277178
Conc: 7.72 ng/ml

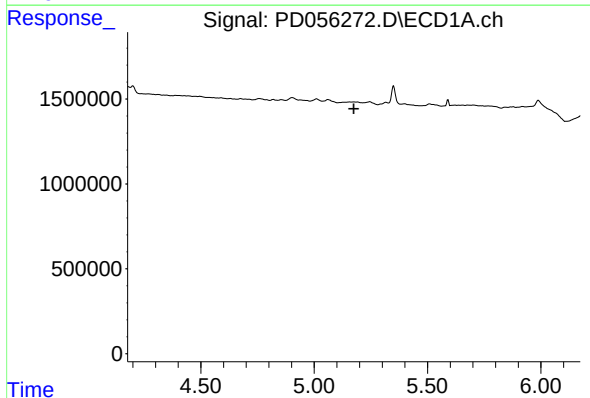


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.175 min
Response: 0
Conc: N.D.

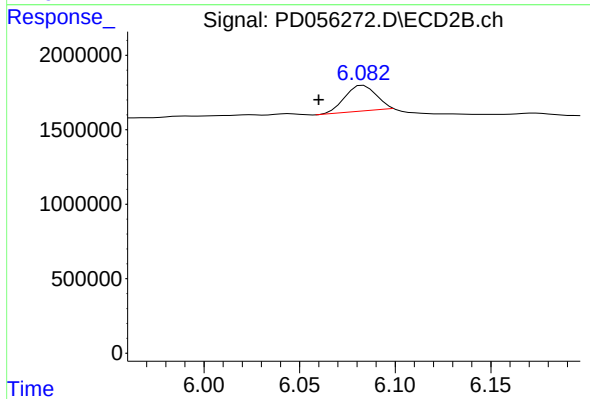

#10 trans-Chlordane


R.T.: 6.083 min
Delta R.T.: 0.024 min
Response: 2002567
Conc: 1.21 ng/ml

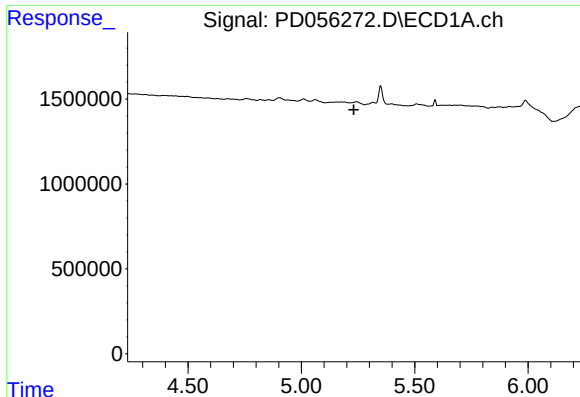

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.232 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BP2

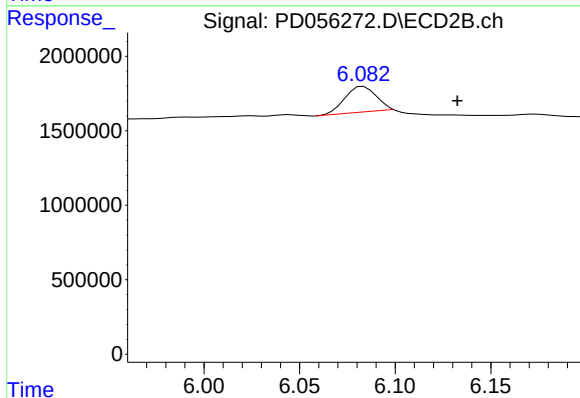


#11 cis-Chlordane

R.T.: 6.083 min
Delta R.T.: -0.049 min
Response: 2002567
Conc: 1.24 ng/ml

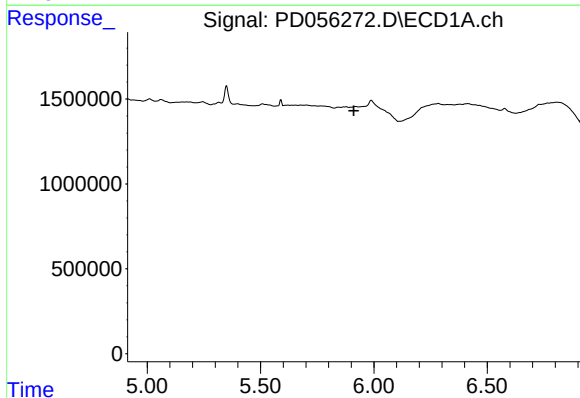


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.912 min
Response: 0
Conc: N.D.

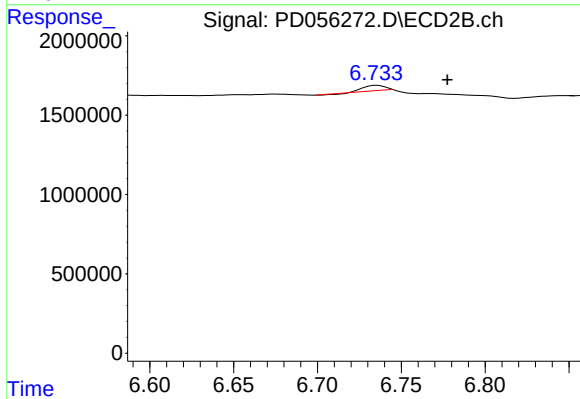

#16 4,4'-DDD


R.T.: 6.736 min
Delta R.T.: -0.042 min
Response: 309650
Conc: 0.26 ng/ml

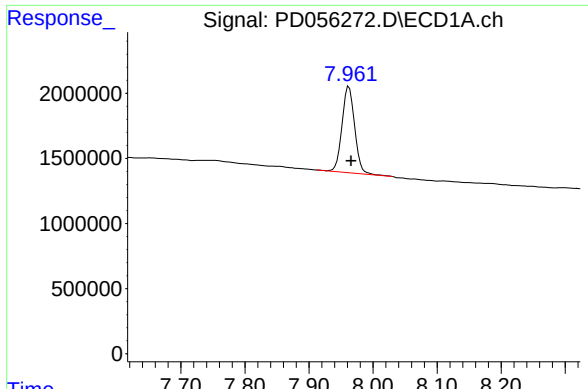

#27 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: -0.003 min
Response: 9044422
Conc: 10.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BP2

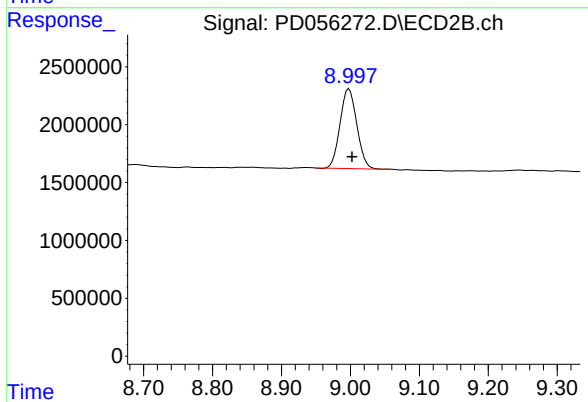

#27 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: -0.004 min
Response: 11624458
Conc: 9.66 ng/ml