

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120519\
 Data File : PD056274.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2019 12:01
 Operator : SG\AJ
 Sample : K6088-18
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BP6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 03:00:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.288	3.962	6919658	10663822	8.355	8.870
27) SA Decachlor...	7.961	8.999	13069066	16991172	14.473	14.122
Target Compounds						
10) B trans-Chl...	0.000	5.990f	0	1336414	N.D.	0.808
16) A 4,4'-DDD	0.000	6.736f	0	123777	N.D.	0.105


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120519\
Data File : PD056274.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2019 12:01
Operator : SG\AJ
Sample : K6088-18
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 03:00:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

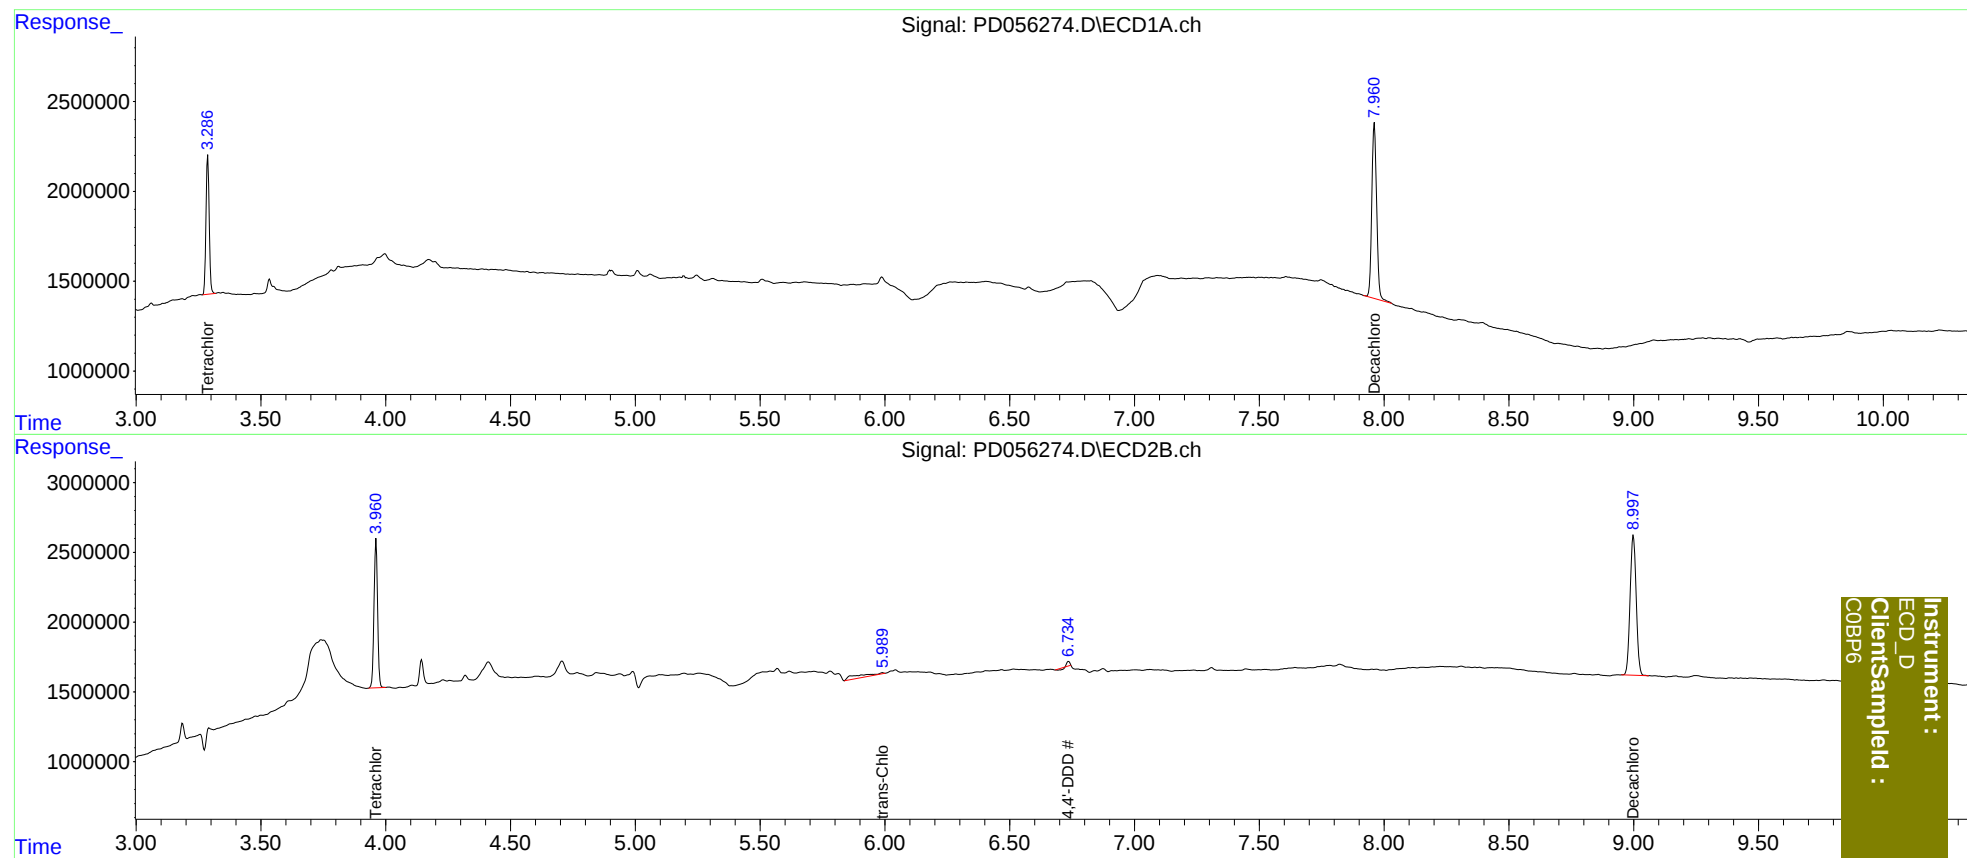


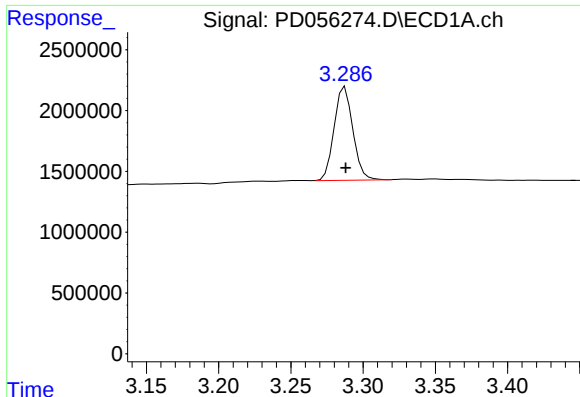

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: 0.000 min
Response: 6919658
Conc: 8.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BP6

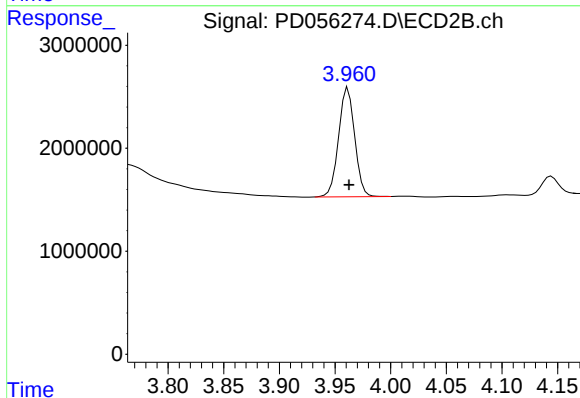


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 10663822
Conc: 8.87 ng/ml

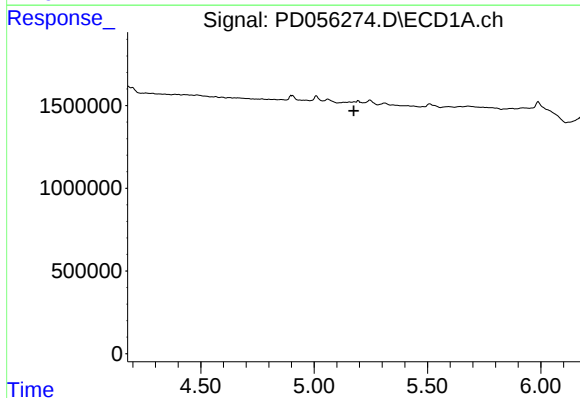


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.175 min
Response: 0
Conc: N.D.

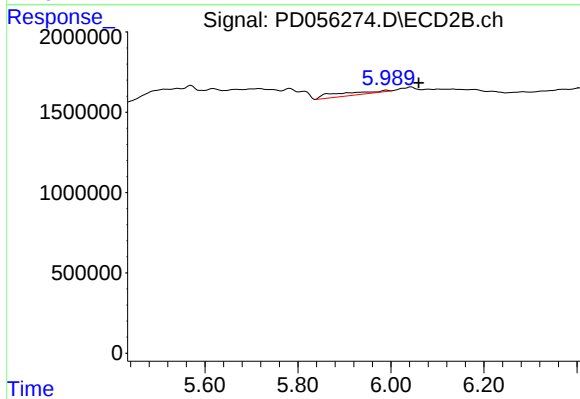

#10 trans-Chlordane


R.T.: 5.990 min
Delta R.T.: -0.070 min
Response: 1336414
Conc: 0.81 ng/ml

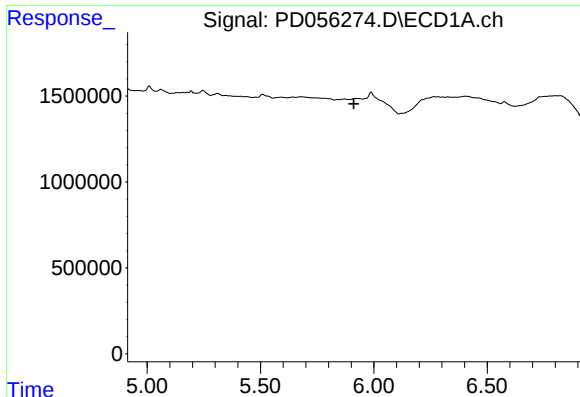

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.912 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BP6

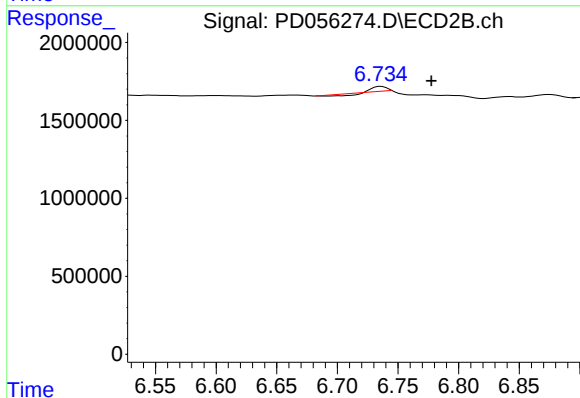


#16 4,4'-DDD

R.T.: 6.736 min
Delta R.T.: -0.041 min
Response: 123777
Conc: 0.11 ng/ml

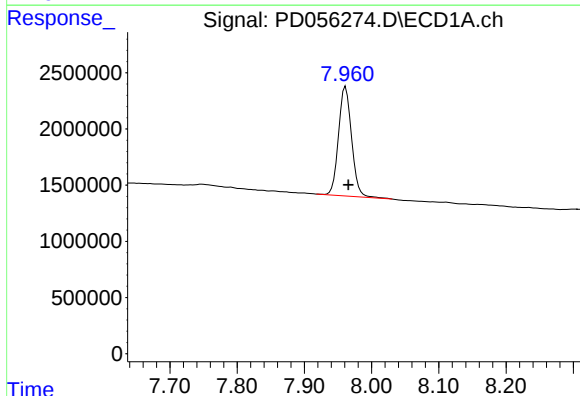

#27 Decachlorobiphenyl

R.T.: 7.961 min
Delta R.T.: -0.004 min
Response: 13069066
Conc: 14.47 ng/ml

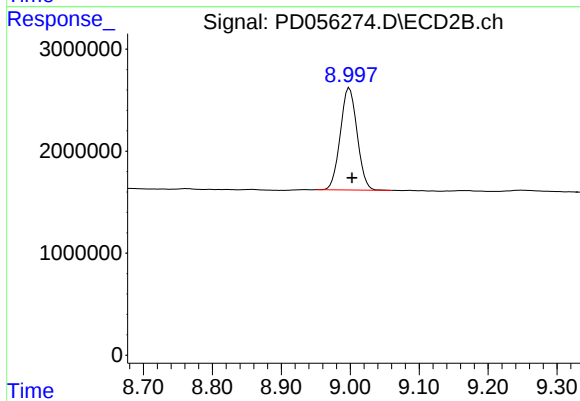

#27 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: -0.004 min
Response: 16991172
Conc: 14.12 ng/ml