

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120519\
 Data File : PD056285.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2019 14:35
 Operator : SG\AJ
 Sample : K6089-13
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BR1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 03:02:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.962	11451729	16727873	13.827	13.914
2)	SA Decachlor...	7.963	8.999	18509909	24295792	20.499	20.194
Target Compounds							
10)	B trans-Chl...	0.000	6.044	0	2441623	N.D.	1.477
16)	A 4,4'-DDD	0.000	6.779	0	1090891	N.D.	0.927
19)	B Endosulfa...	0.000	7.233	0	2311372	N.D.	1.729
20)	A Methoxychlor	6.737f	0.000	6868503	0	20.266	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120519\
Data File : PD056285.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2019 14:35
Operator : SG\AJ
Sample : K6089-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 03:02:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

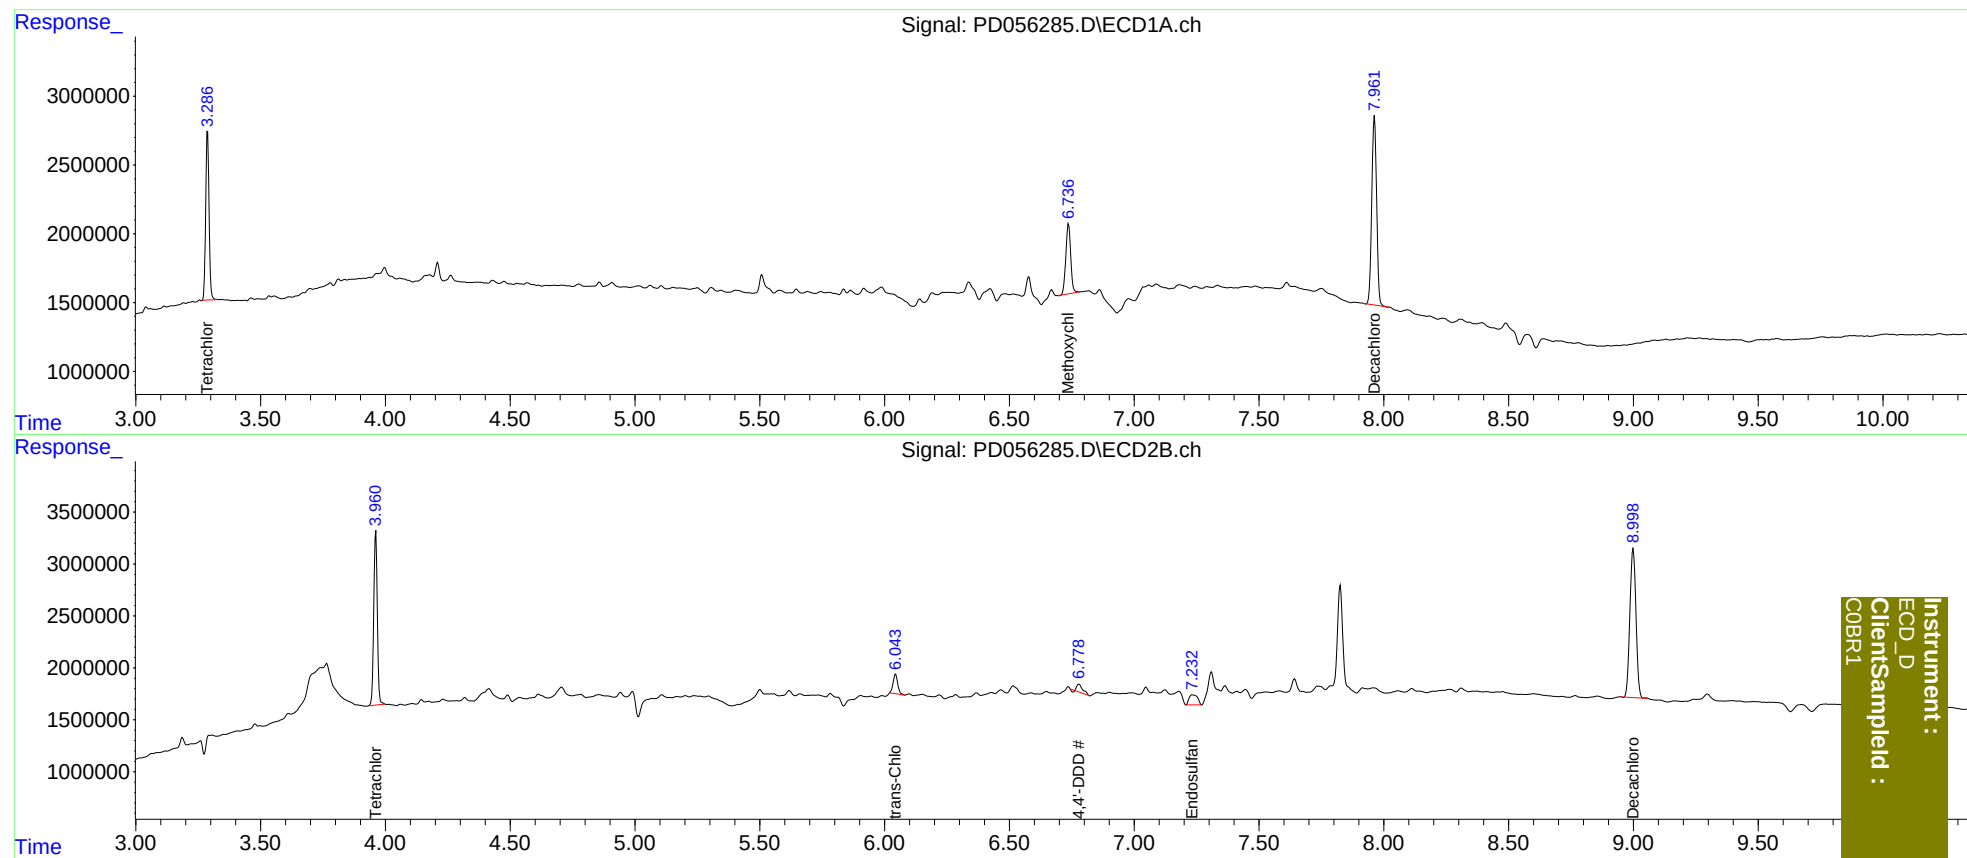


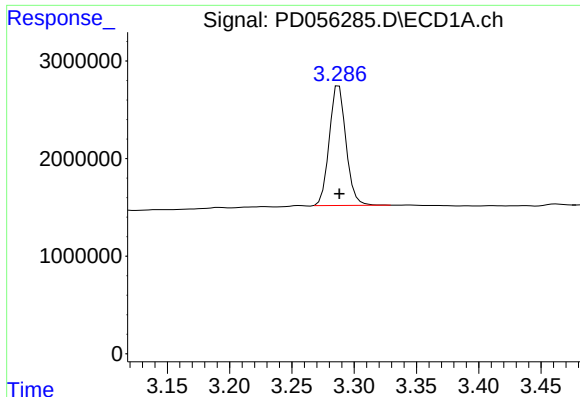

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: 0.000 min
Response: 11451729
Conc: 13.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BR1

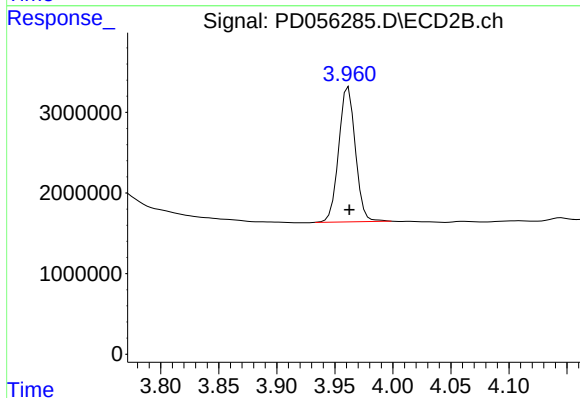


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 16727873
Conc: 13.91 ng/ml

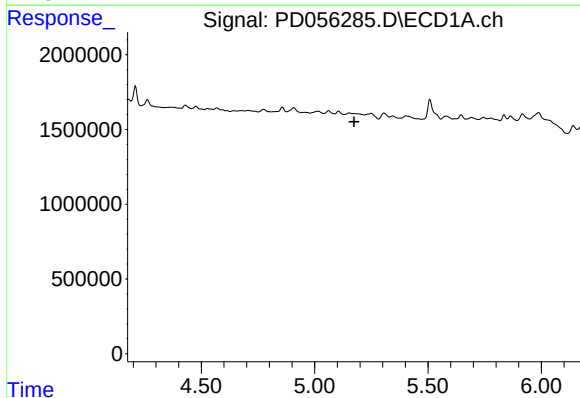


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.175 min
Response: 0
Conc: N.D.

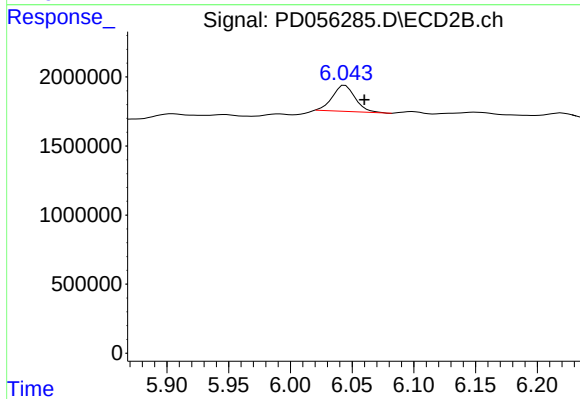

#10 trans-Chlordane


R.T.: 6.044 min
Delta R.T.: -0.016 min
Response: 2441623
Conc: 1.48 ng/ml

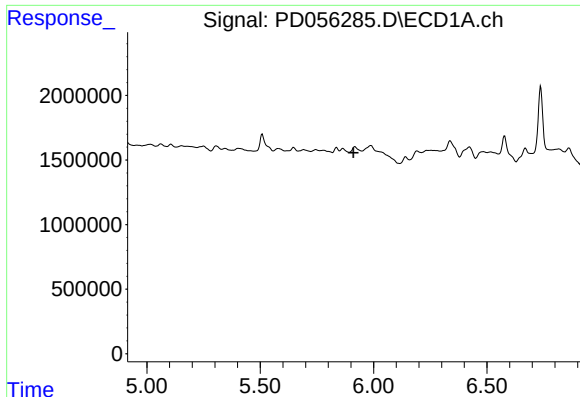

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.912 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BR1

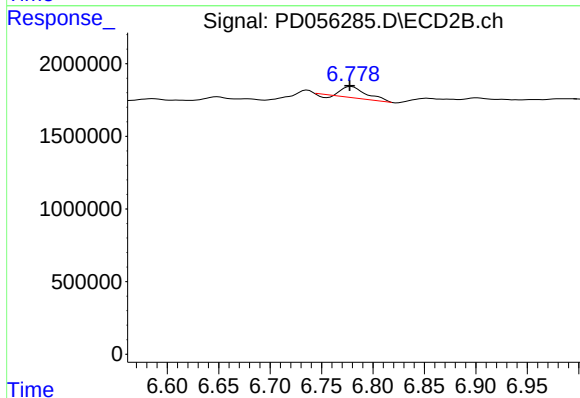


#16 4,4'-DDD

R.T.: 6.779 min
Delta R.T.: 0.002 min
Response: 1090891
Conc: 0.93 ng/ml

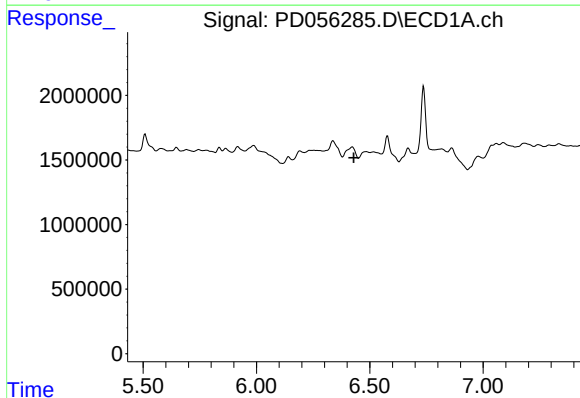


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.430 min
Response: 0
Conc: N.D.

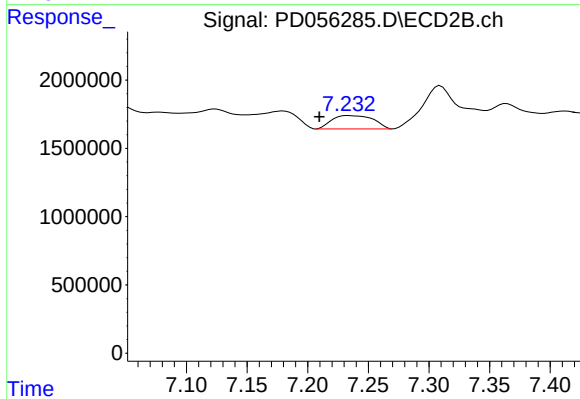

#19 Endosulfan Sulfate


R.T.: 7.233 min
Delta R.T.: 0.023 min
Response: 2311372
Conc: 1.73 ng/ml

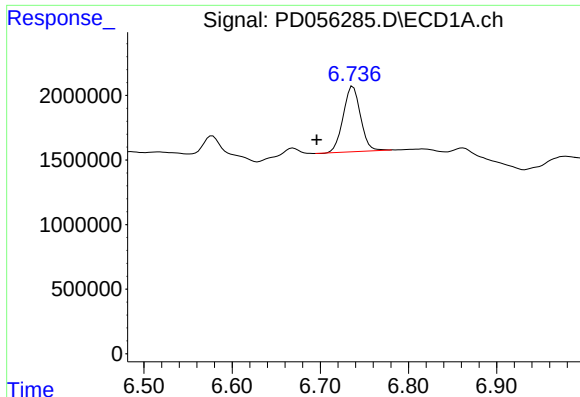

#20 Methoxychlor


R.T.: 6.737 min
Delta R.T.: 0.041 min
Response: 6868503
Conc: 20.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BR1

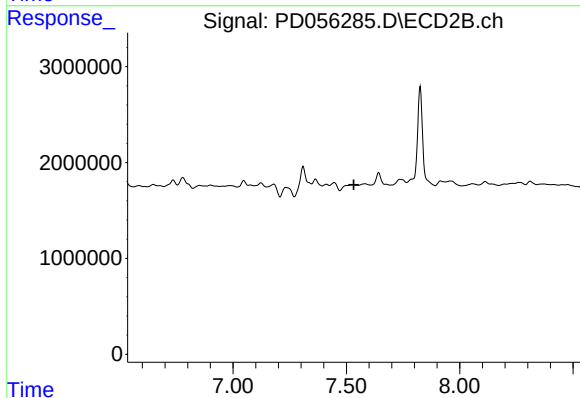


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.533 min
Response: 0
Conc: N.D.

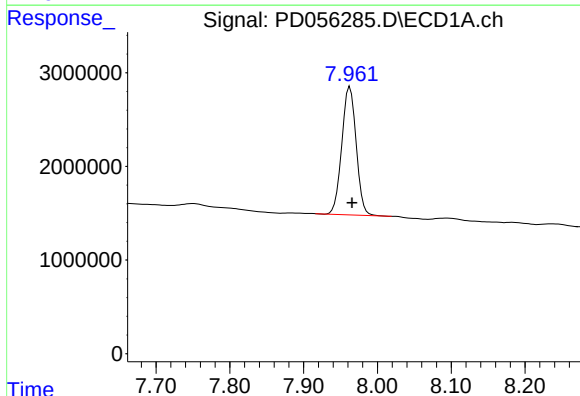

#27 Decachlorobiphenyl

R.T.: 7.963 min
Delta R.T.: -0.003 min
Response: 18509909
Conc: 20.50 ng/ml

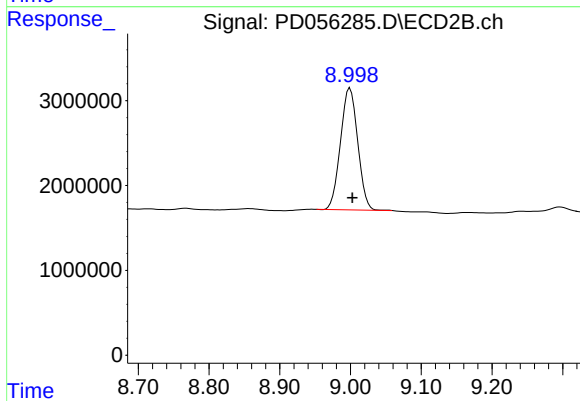

#27 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: -0.003 min
Response: 24295792
Conc: 20.19 ng/ml