

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120519\
 Data File : PD056293.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2019 16:40
 Operator : SG\AJ
 Sample : K6089-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BP9

Manual Integrations
 APPROVED

Ankita
 12/6/2019 4:13:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 05:42:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.292	3.961	12588136	15896923	15.199m	13.223
27) SA Decachlor...	7.968	9.000	48591496	26621758	53.813	22.127m#
Target Compounds						
3) MA gamma-BHC...	4.002	4.610	3636659	4466416	3.239m	2.768m
14) MA Endrin	5.785	6.649	811183	795490	0.971m	0.629m#
16) A 4,4'-DDD	5.921	6.771	3156666	4813443	4.435m	4.090m
19) B Endosulfa...	6.422	7.207	5140980	3480710	5.919	2.603m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120519\
Data File : PD056293.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2019 16:40
Operator : SG\AJ
Sample : K6089-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 05:42:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

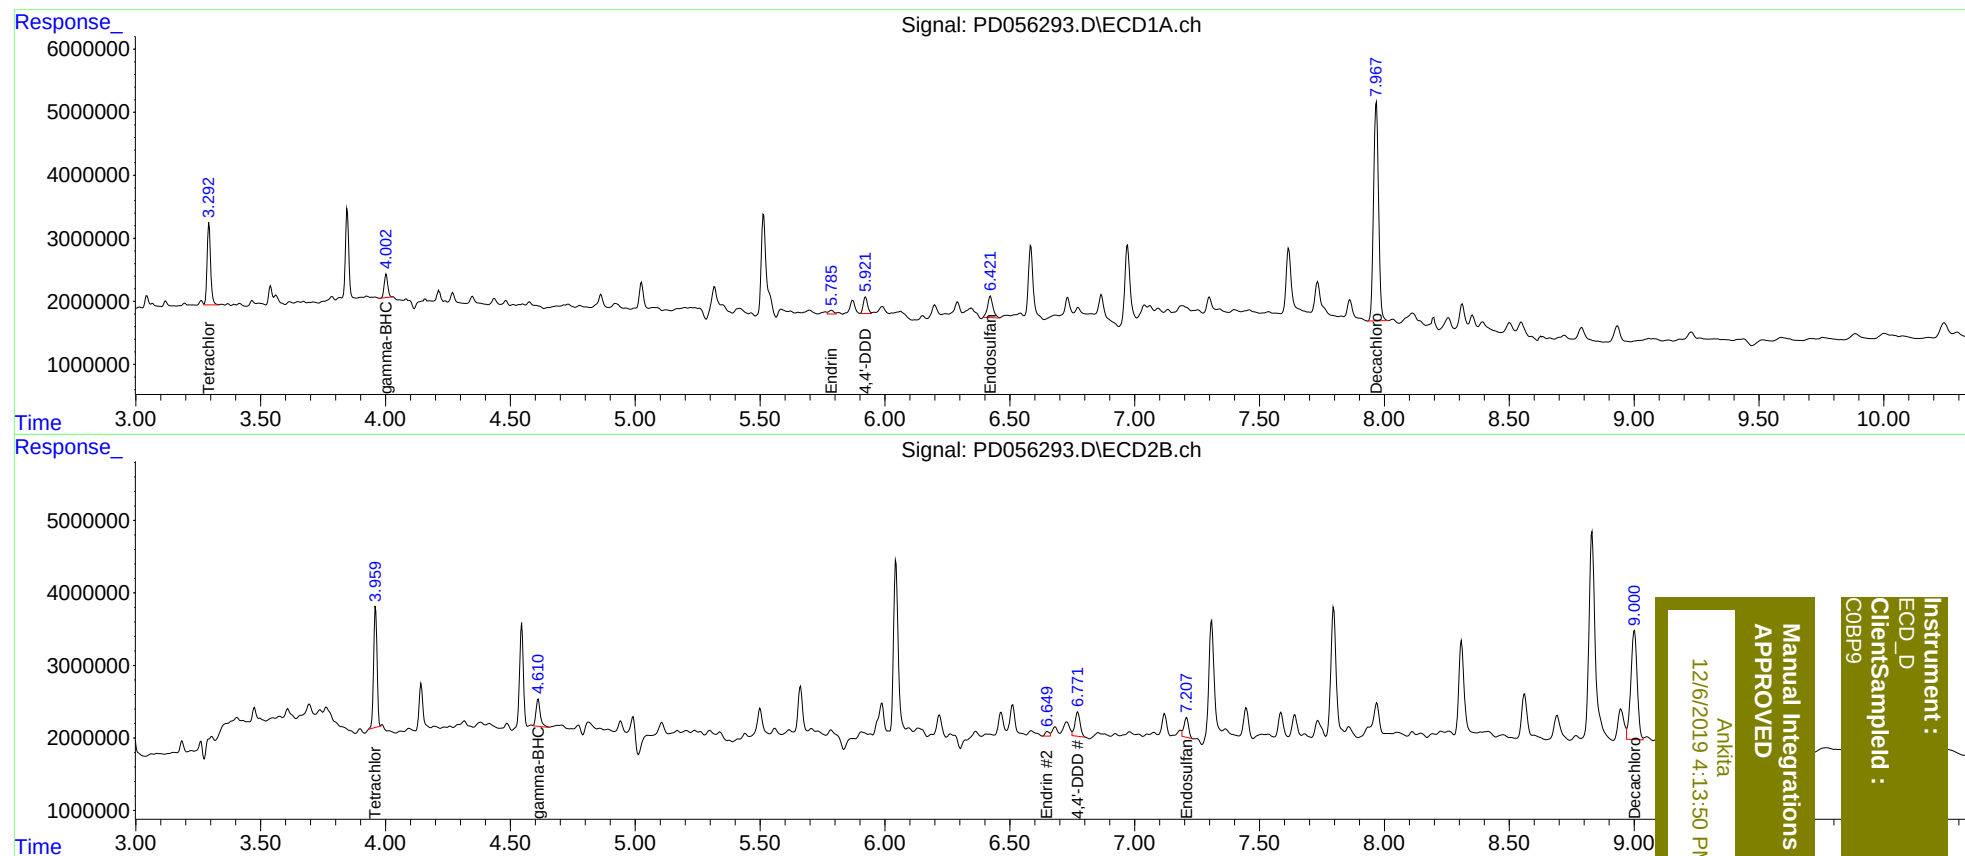

12/6/2019 4:13:50 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sampled :
C0BP9