

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120519\
 Data File : PD056296.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2019 17:22
 Operator : SG\AJ
 Sample : K6089-07
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BQ5

Manual Integrations
 APPROVED

Ankita
 12/6/2019 4:13:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 06:07:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.962	10543937	11585034	12.731	9.636
27)	SA Decachlor...	7.961	8.997	15624319	16925901	17.303	14.068m
Target Compounds							
3)	MA gamma-BHC...	3.995	4.611	3625634	3673306	3.229	2.276m#
12)	B 4,4'-DDE	5.398	6.286	11920778	15151748	11.799	9.650
14)	MA Endrin	5.778	6.648	1632338	1136099	1.953m	0.898m#
16)	A 4,4'-DDD	5.913	6.773	5110281	6111097	7.181m	5.193 #
17)	MA 4,4'-DDT	6.145	7.074	5261406	7815505	7.477	6.611

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120519\
Data File : PD056296.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2019 17:22
Operator : SG\AJ
Sample : K6089-07
Misc :
ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 06:07:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

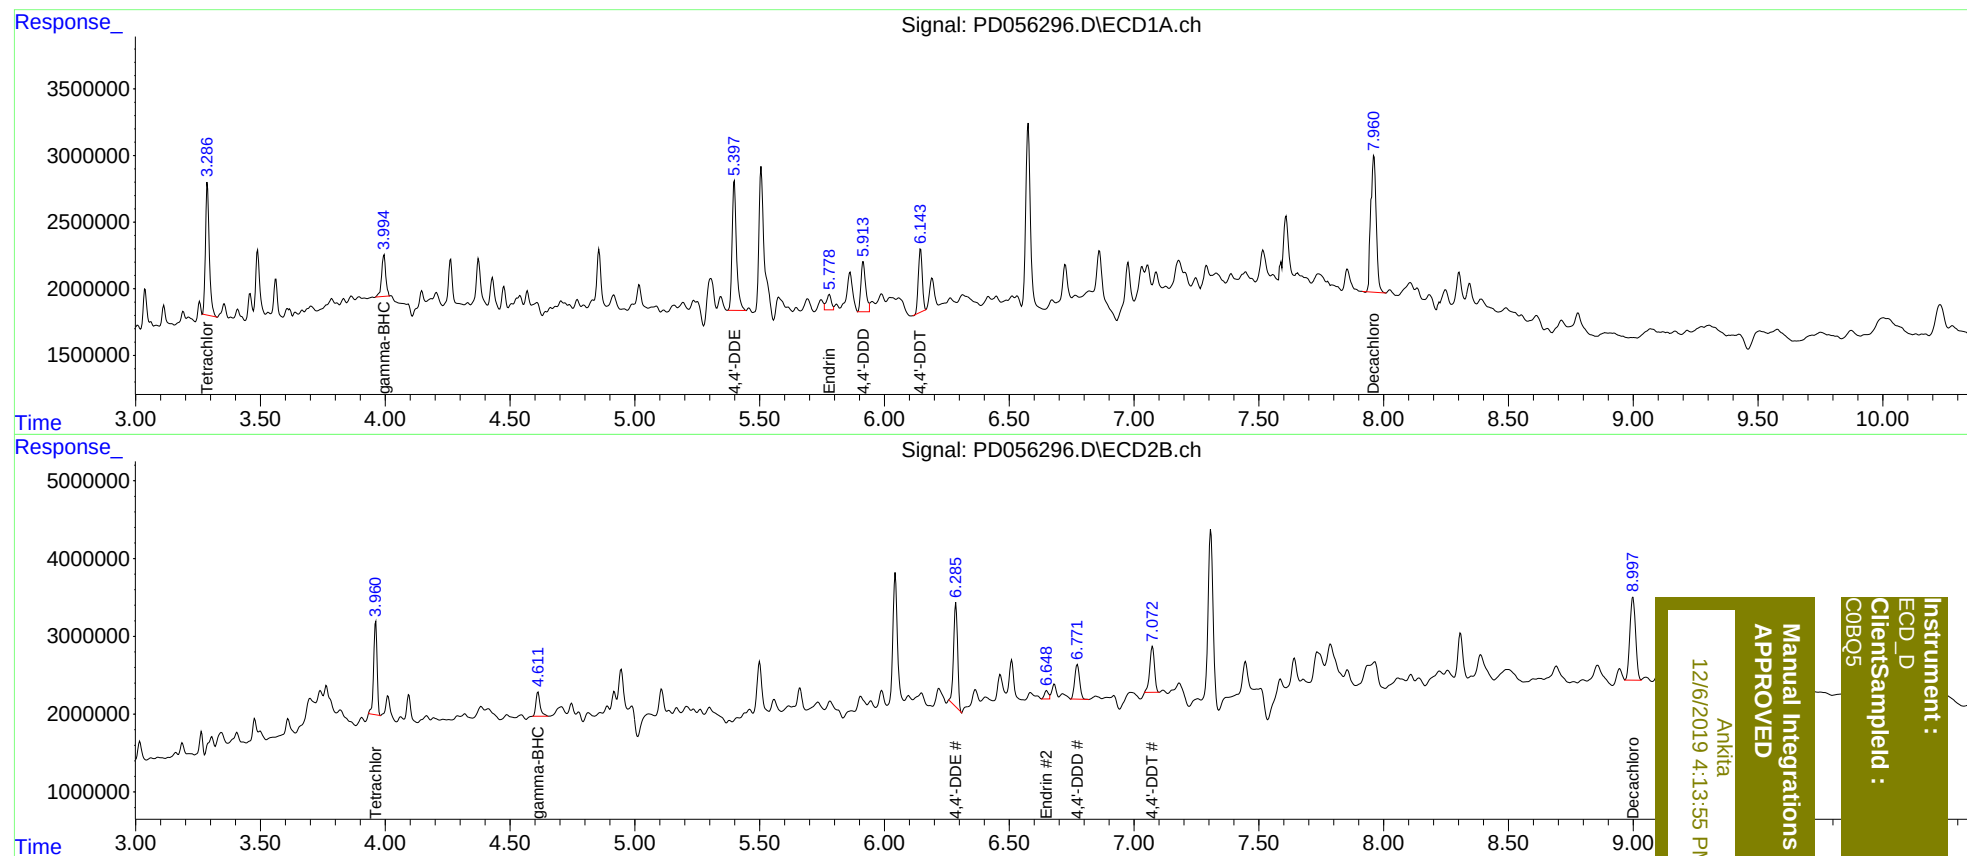

12/6/2019 4:13:55 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sampled :
C0B05