

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120519\
 Data File : PD056298.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2019 17:50
 Operator : SG\AJ
 Sample : K6089-12
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BR0

Manual Integrations
 APPROVED

Ankita
 12/6/2019 4:13:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 03:05:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.288	3.962	11220664	12330269	13.548	10.256
27) SA Decachlor...	7.962	8.997	18234851	23218445	20.194	19.298m
Target Compounds						
3) MA gamma-BHC...	3.996	4.611	5295392	5763559	4.716	3.571m
12) B 4,4'-DDE	5.400	6.284	4560240	4798600	4.514	3.056 #
14) MA Endrin	5.777	6.649	1547855	1640146	1.852m	1.296m#
16) A 4,4'-DDD	5.914	6.772	4954625	7841013	6.962m	6.663
17) MA 4,4'-DDT	6.143	7.074	3416323	4491449	4.855m	3.799

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120519\
Data File : PD056298.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2019 17:50
Operator : SG\AJ
Sample : K6089-12
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 03:05:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

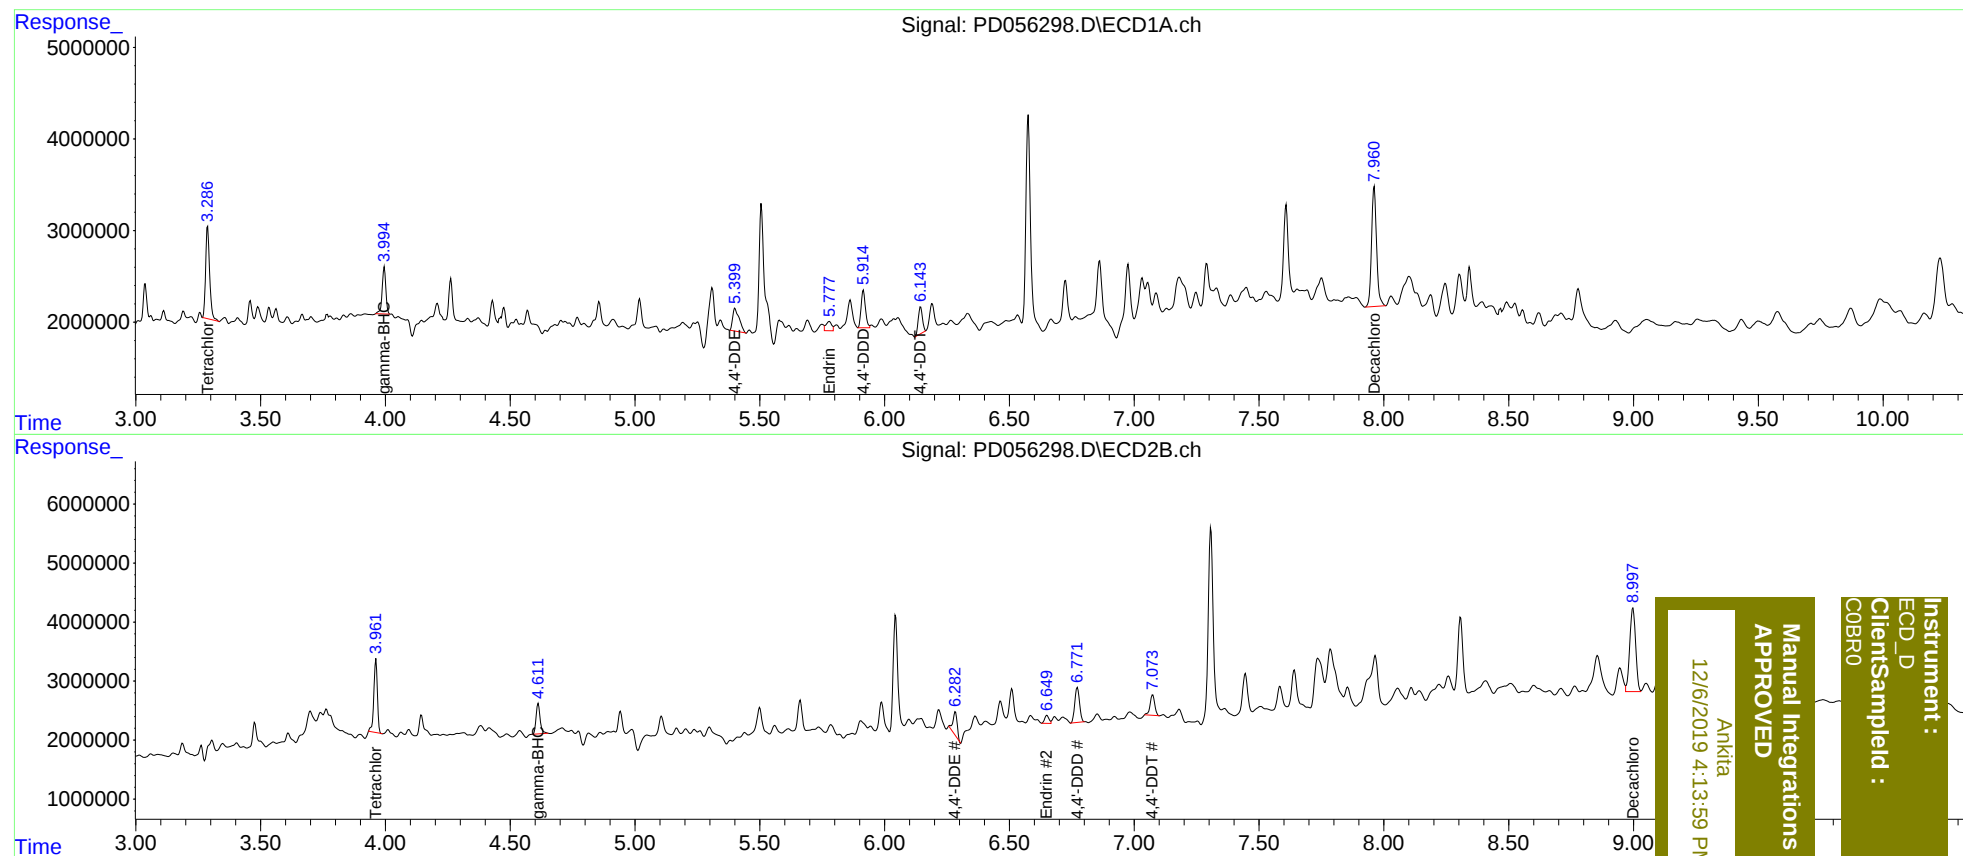

12/6/2019 4:13:59 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sampled :
COBR0