

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120519\
 Data File : PD056282.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2019 13:53
 Operator : SG\AJ
 Sample : K6089-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BQ4

Manual Integrations
 APPROVED

Ankita
 12/6/2019 4:13:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 04:38:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.286	3.962	10609112	12078923	12.810m	10.047
27) SA Decachlor...	7.962	8.997	14973189	20829982	16.582	17.313m
Target Compounds						
3) MA gamma-BHC...	3.995	4.612	1763905	1506470	1.571m	0.933m#
12) B 4,4'-DDE	5.400	6.285	703178	1242386	0.696m	0.791m
16) A 4,4'-DDD	5.915	6.771	1651991	2118612	2.321m	1.800m
17) MA 4,4'-DDT	6.144	7.072	570813	1682318	0.811m	1.423m#
19) B Endosulfa...	6.414	7.206	1609677	815279	1.853m	0.610m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120519\
Data File : PD056282.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2019 13:53
Operator : SG\AJ
Sample : K6089-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 04:38:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

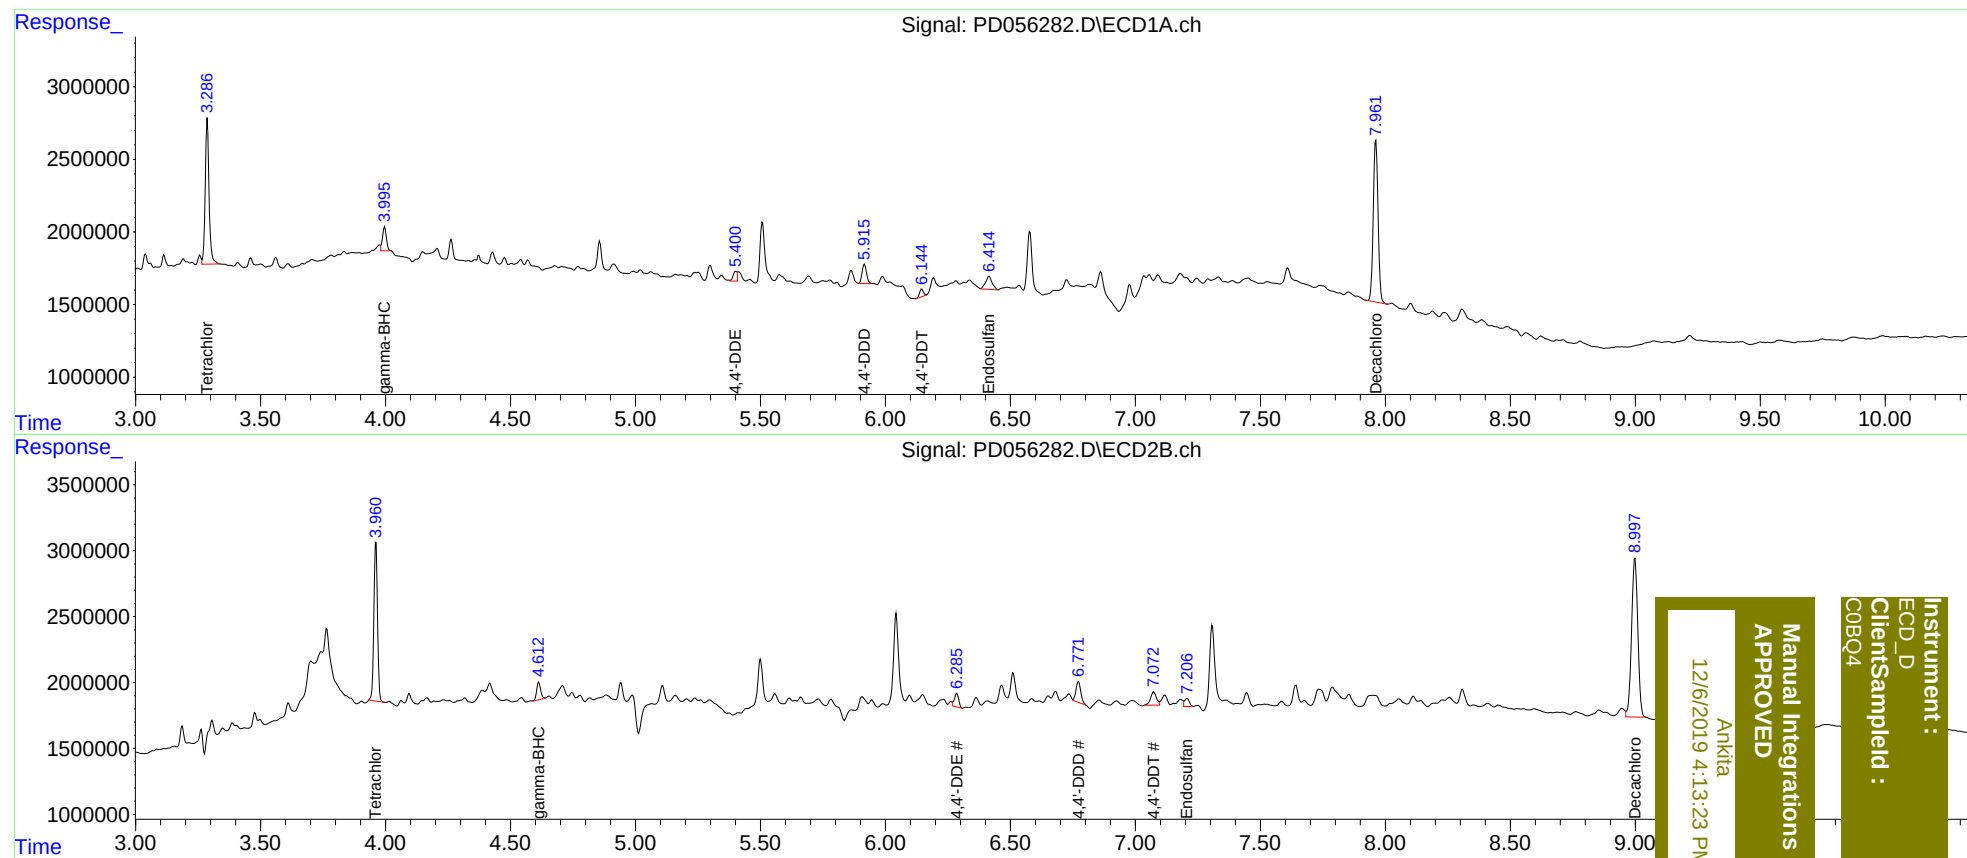

12/6/2019 4:13:23 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSampled :
C0BQ4