

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120519\
 Data File : PD056302.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2019 18:46
 Operator : SG\AJ
 Sample : K6089-17MSD
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BR3MSD

Manual Integrations
 APPROVED

Ankita
 12/6/2019 4:14:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 03:06:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.962	16785173	17594644	20.267	14.635 #
27)	SA Decachlor...	7.959	8.996	30916206	49858958	34.238m	41.440m
Target Compounds							
3)	MA gamma-BHC...	3.990	4.630	68699807	88473681	61.179	54.822m
4)	MA Heptachlor	4.275	5.136	60619436	83917038	60.143	51.489m
5)	MB Aldrin	4.514	5.441	52556424	76617311	48.395	46.627
13)	MA Dieldrin	5.521	6.436	147.6E6	154.1E6	145.271	98.071 #
14)	MA Endrin	5.775	6.653	92120353	125.6E6	110.232	99.272
15)	B Endosulfa...	6.055	6.851	7213490	4876688	7.573	3.328 #
16)	A 4,4'-DDD	5.912	6.771	10059482	22242996	14.135m	18.902 #
17)	MA 4,4'-DDT	6.145	7.073	68918908	119.0E6	97.946	100.658

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120519\
Data File : PD056302.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2019 18:46
Operator : SG\AJ
Sample : K6089-17MSD
Misc :
ALS Vial : 39 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 03:06:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

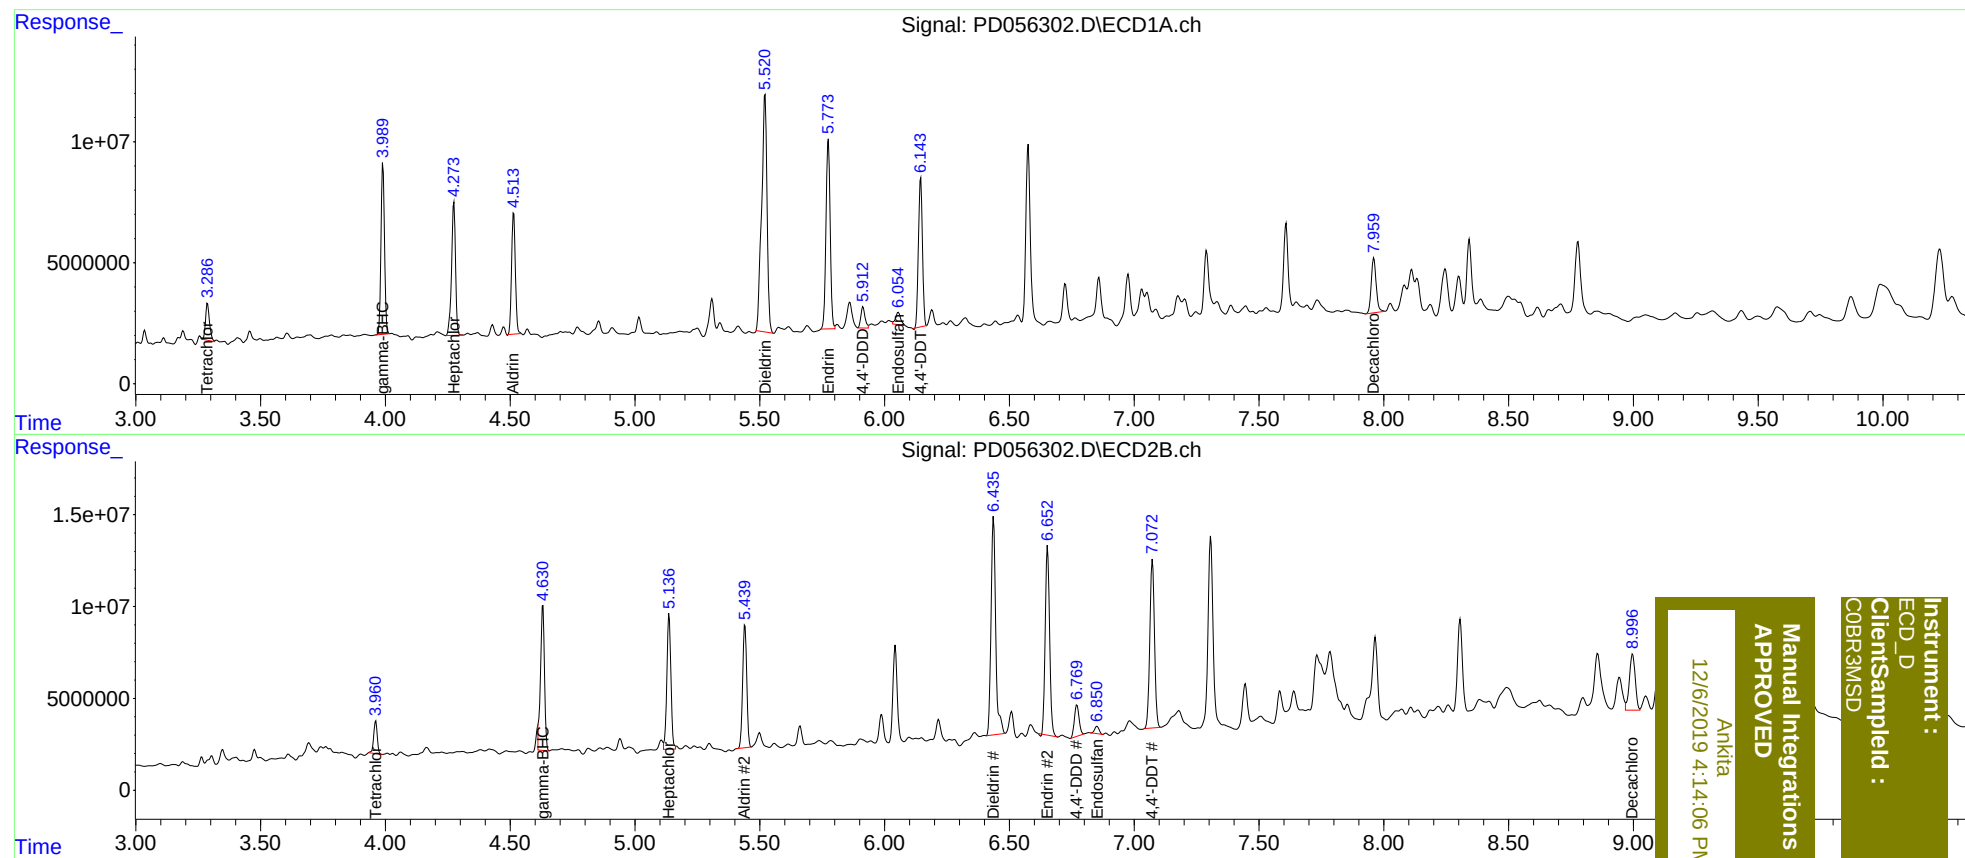

12/6/2019 4:14:06 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sampled :
COBR3M/MSD