

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120523\
 Data File : PD079921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2023 14:09
 Operator : AR\AJ
 Sample : TOXAPH401
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 14:21:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 05 14:17:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.800	69008560	110.8E6	39.219	39.314
27)	SA Decachlor...	9.114	7.943	178.5E6	232.6E6	77.964	77.972
Target Compounds							
22)	Toxaphene-1	5.887	5.031	26353576	68062046	3887.649	3915.360
23)	Toxaphene-2	6.478	5.356	78415530	70674526	3955.380	3940.854
24)	Toxaphene-3	7.096	6.630	234.4E6	256.4E6	3986.072	4048.972
25)	Toxaphene-4	7.189	6.754	174.0E6	342.9E6	3995.151	4003.237
26)	Toxaphene-5	7.610	7.070	133.7E6	145.1E6	4017.352	4028.581

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120523\
Data File : PD079921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2023 14:09
Operator : AR\AJ
Sample : TOXAPH401
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 14:21:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 05 14:17:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

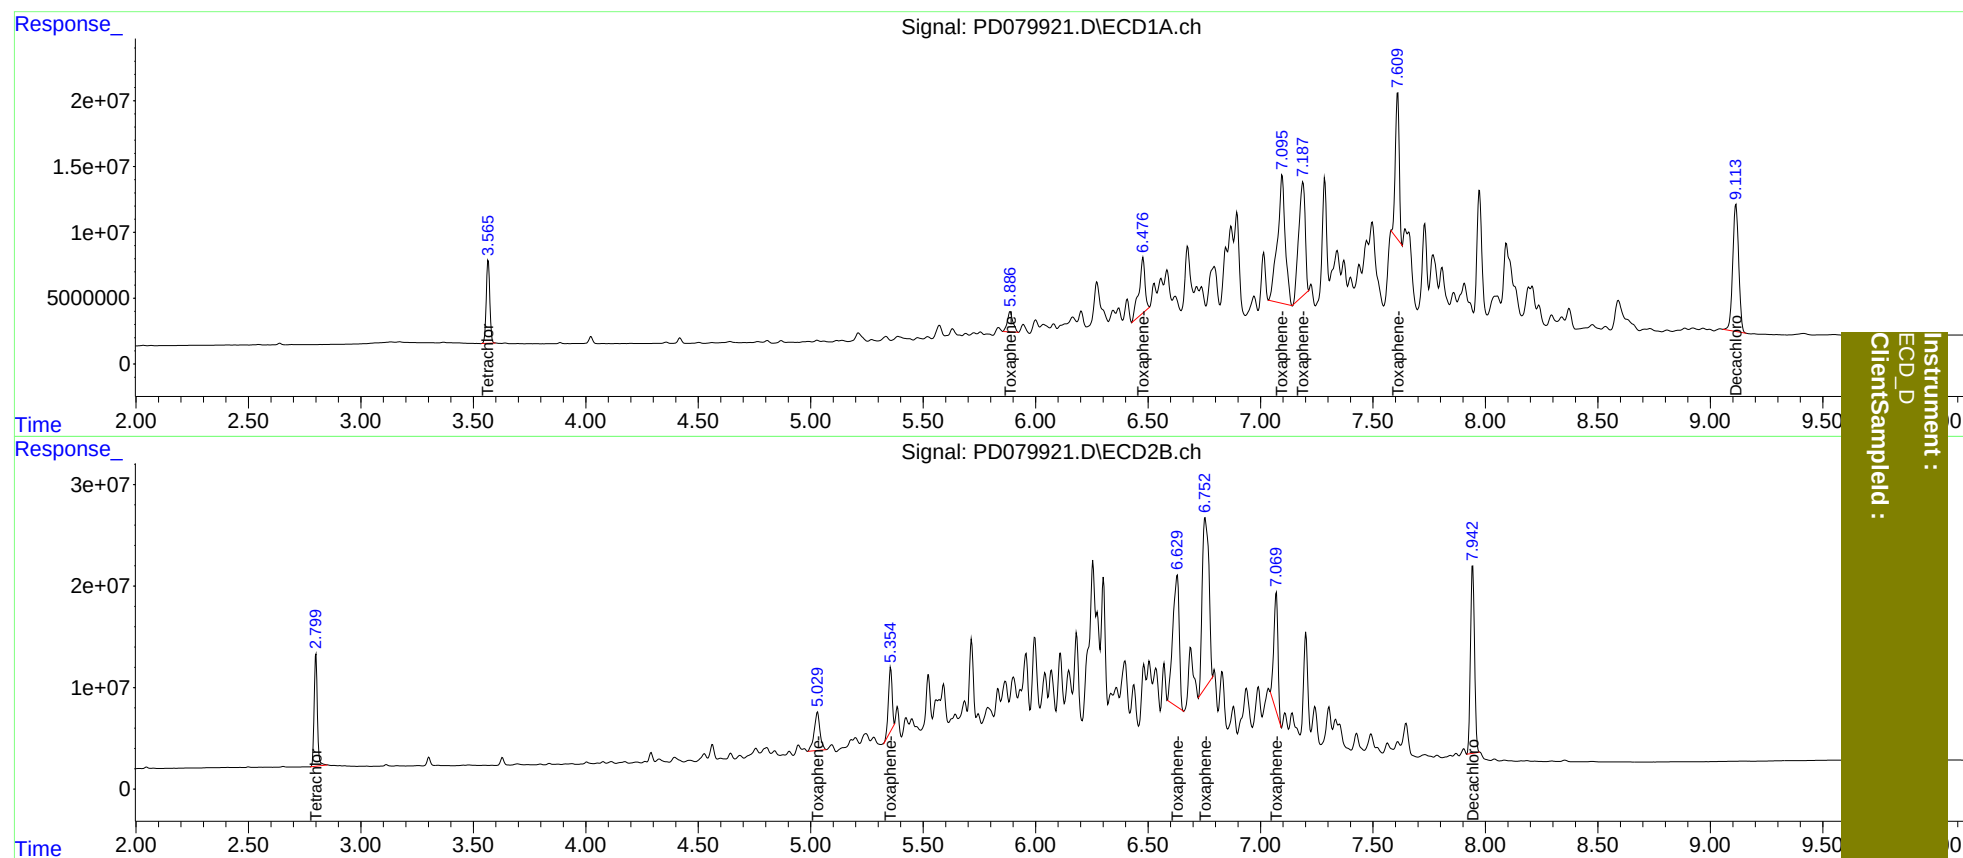

Instrument :
ECD_D
ClientSampled :
0