

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120523\
 Data File : PD079935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2023 17:16
 Operator : AR\AJ
 Sample : 05607-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 20:42:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 05 17:09:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	2.795	0	121594	N.D.	<MDL
27)	SA Decachlor...	0.000	7.938	0	237434	N.D.	<MDL
Target Compounds							
2)	A alpha-BHC	0.000	3.262f	0	101049	N.D.	<MDL
7)	B delta-BHC	0.000	4.182	0	494959	N.D.	0.135
9)	A Endosulfan I	0.000	5.113	0	116828	N.D.	<MDL
11)	B cis-Chlor...	0.000	5.113f	0	116828	N.D.	<MDL
14)	MA Endrin	0.000	5.683	0	54652	N.D.	<MDL
15)	B Endosulfa...	0.000	5.919f	0	1497845	N.D.	0.548
18)	B Endrin al...	0.000	6.151	0	352224	N.D.	0.166
21)	B Endrin ke...	0.000	6.831f	0	240794	N.D.	<MDL

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120523\
Data File : PD079935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2023 17:16
Operator : AR\AJ
Sample : 05607-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 20:42:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 05 17:09:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

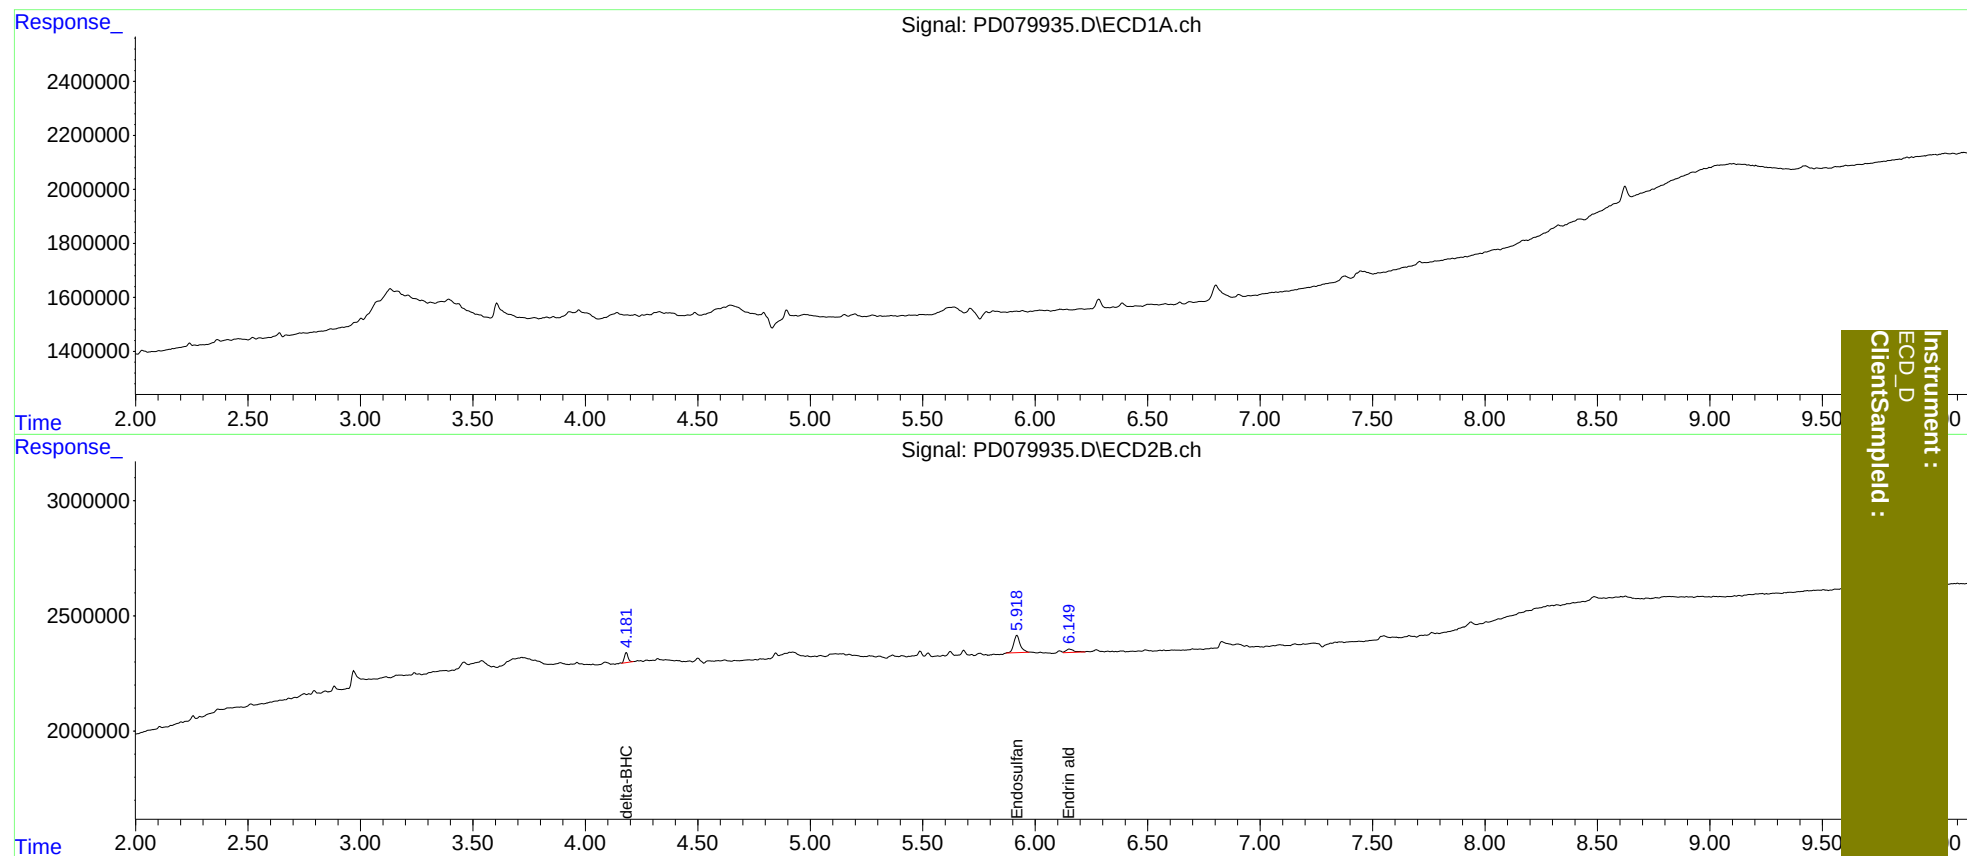


Instrument :
ECD_D
ClientSampled :
0

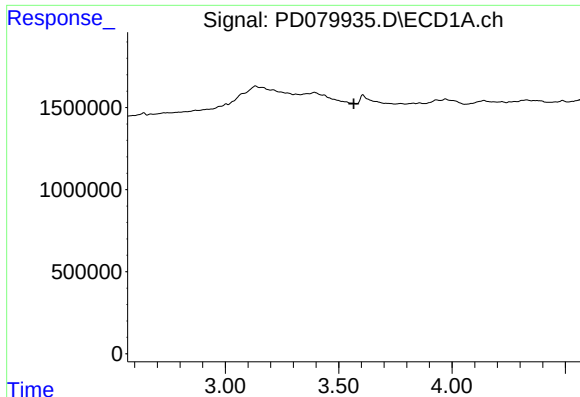

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.567 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

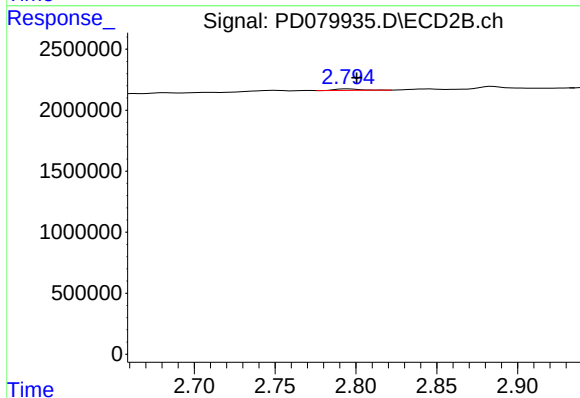


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: -0.005 min
Response: 121594
Conc: N.D.

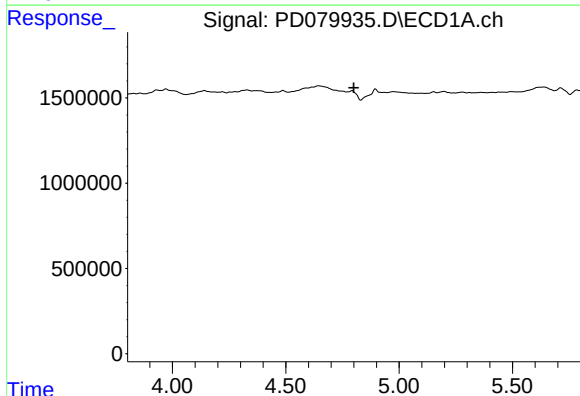


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.800 min
Response: 0
Conc: N.D.

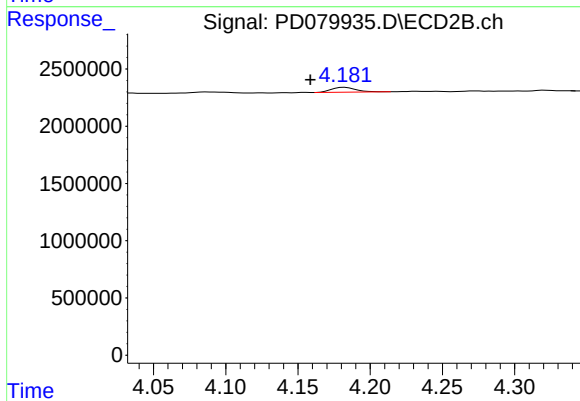

#7 delta-BHC


R.T.: 4.182 min
Delta R.T.: 0.024 min
Response: 494959
Conc: 0.13 ng/ml

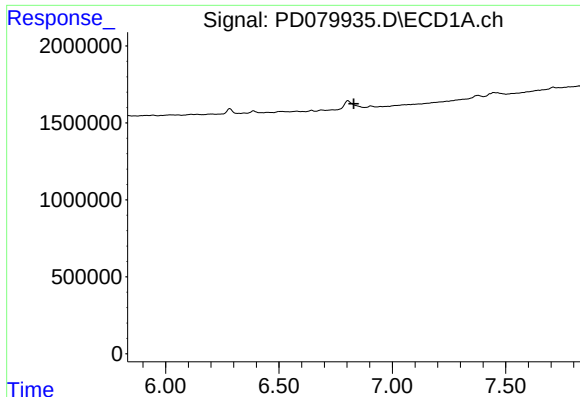

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.830 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

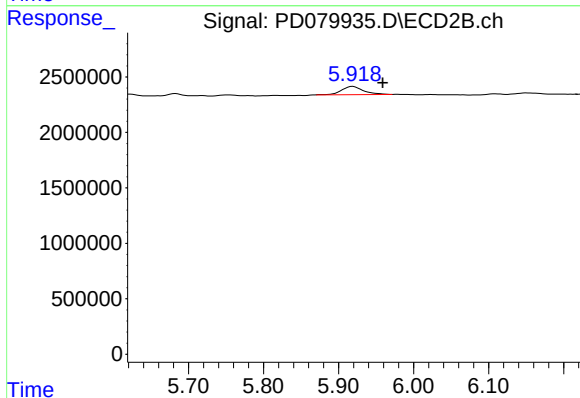


#15 Endosulfan II

R.T.: 5.919 min
Delta R.T.: -0.040 min
Response: 1497845
Conc: 0.55 ng/ml

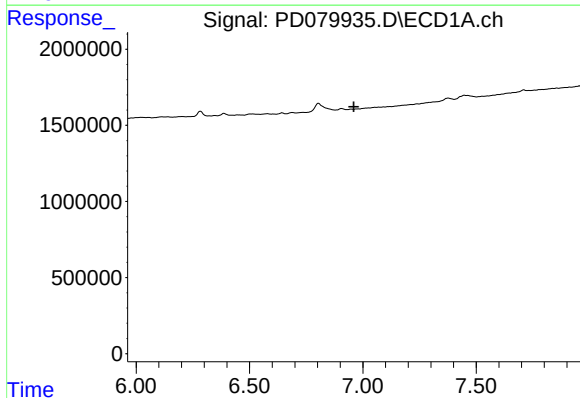


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.960 min
Response: 0
Conc: N.D.

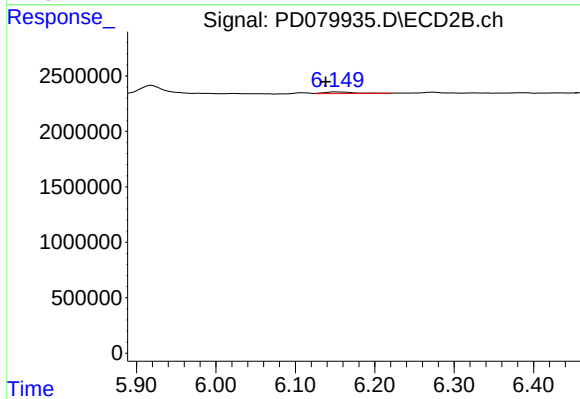

#18 Endrin aldehyde


R.T.: 6.151 min
Delta R.T.: 0.013 min
Response: 352224
Conc: 0.17 ng/ml

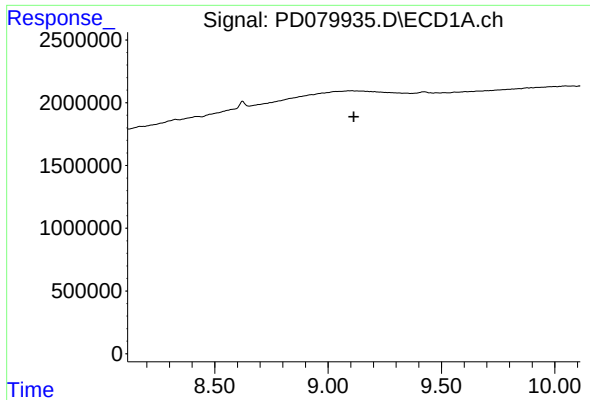

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

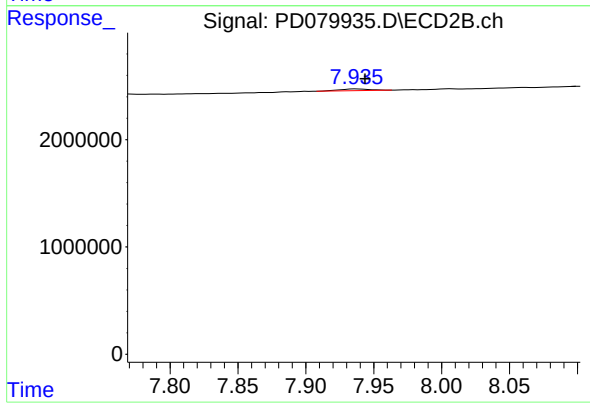

#27 Decachlorobiphenyl

R.T.: 7.938 min
Delta R.T.: -0.006 min
Response: 237434
Conc: N.D.