

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120619\
 Data File : PD056322.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 09:18
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 22:32:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
Target Compounds						
8) B Heptachlo...	0.000	5.818	0	30686714	N.D.	19.807
12) B 4,4'-DDE	5.432	6.355f	7464665	1423355	7.389	0.907 #
14) MA Endrin	0.000	6.652	0	12103228	N.D.	9.563
16) A 4,4'-DDD	0.000	6.722f	0	13306015	N.D.	11.307
17) MA 4,4'-DDT	0.000	7.068	0	2573472	N.D.	2.177
18) B Endrin al...	0.000	6.984	0	2626515	N.D.	2.160
19) B Endosulfa...	0.000	7.206	0	904057	N.D.	0.676
22) Toxaphene-1	5.432	6.355	7464665	1423355	828.502	126.780 #
23) Toxaphene-2	0.000	6.652	0	12103228	N.D.	877.023
24) Toxaphene-3	0.000	7.068	0	2573472	N.D.	130.823
25) Toxaphene-4	0.000	7.135	0	355684	N.D.	6.442


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120619\
Data File : PD056322.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 09:18
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 22:32:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

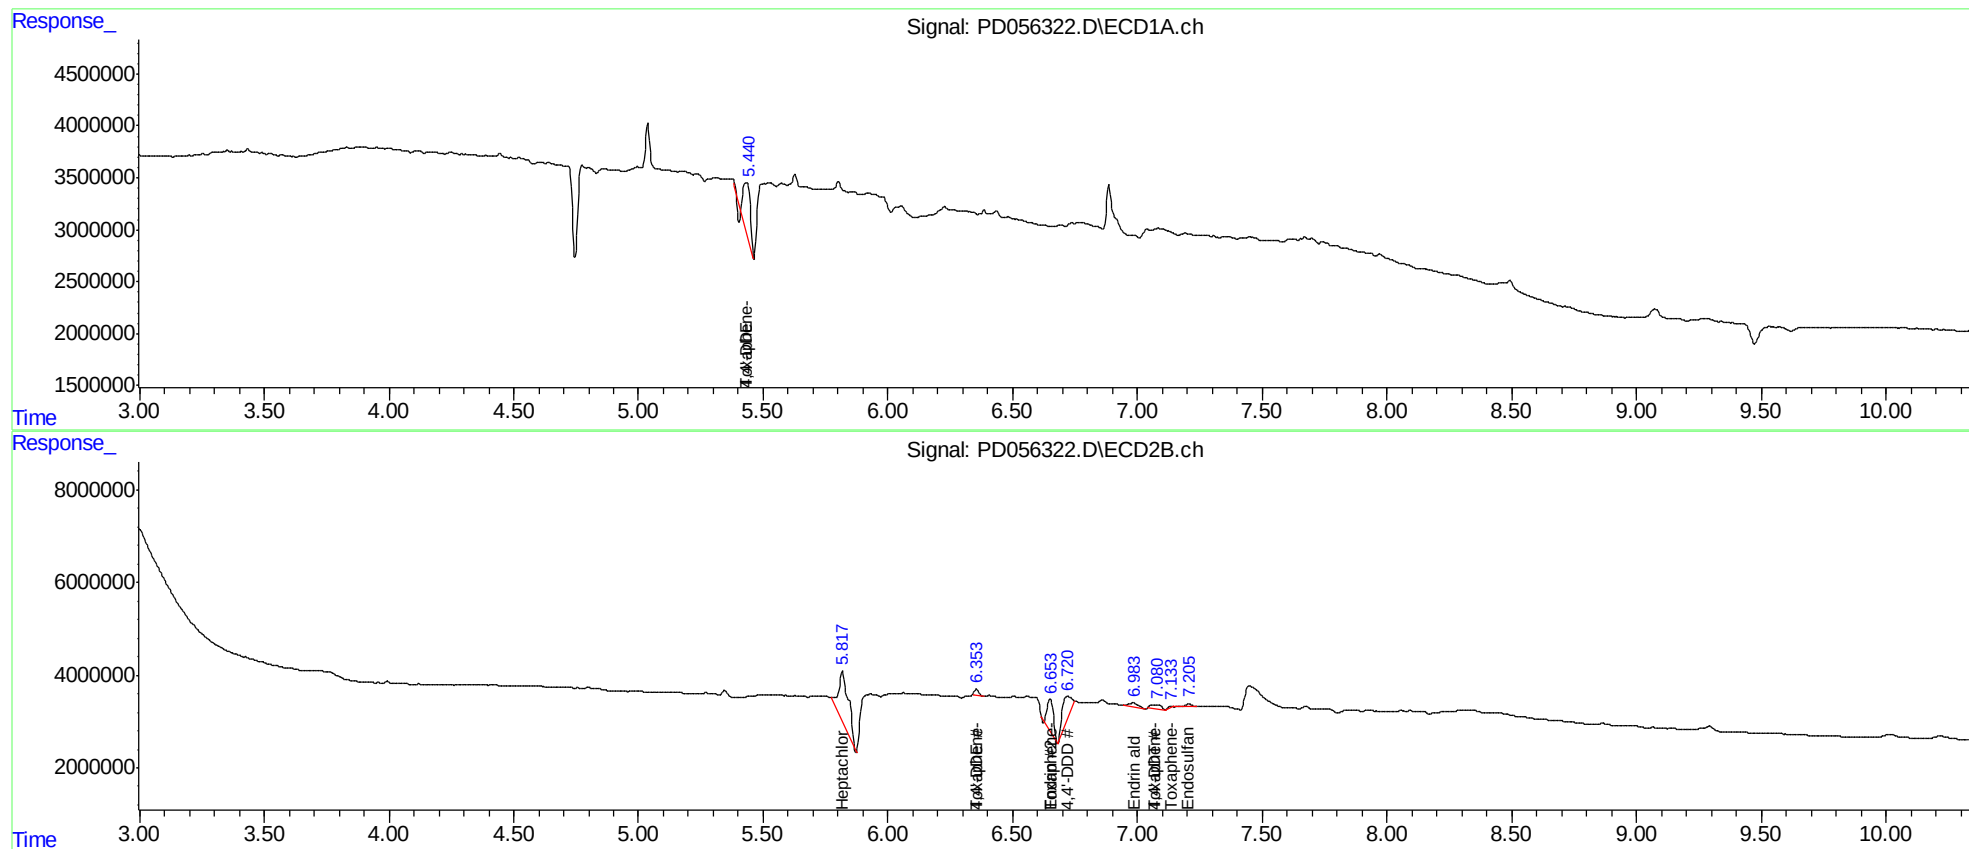


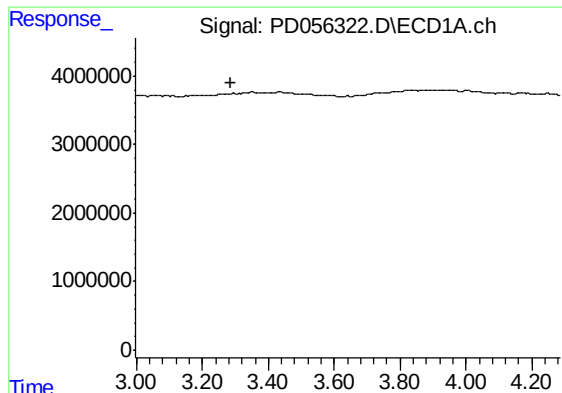

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.288 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

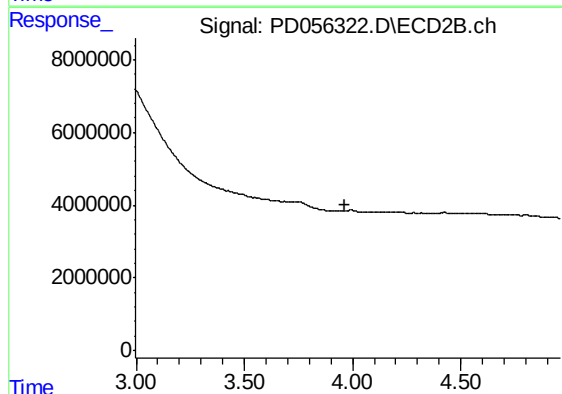


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.963 min
Response: 0
Conc: N.D.

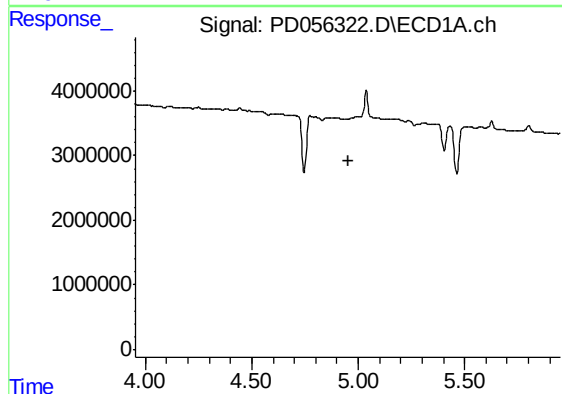


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

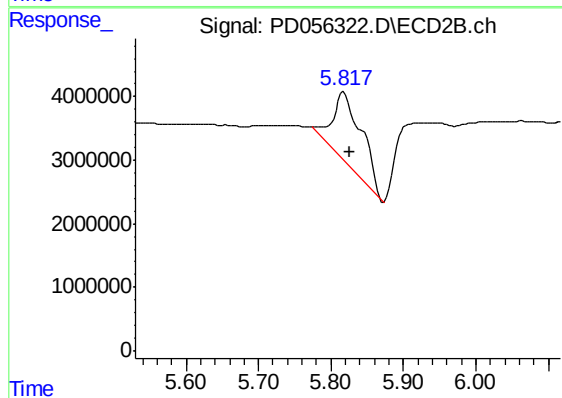

#8 Heptachlor epoxide


R.T.: 5.818 min
Delta R.T.: -0.009 min
Response: 30686714
Conc: 19.81 ng/ml

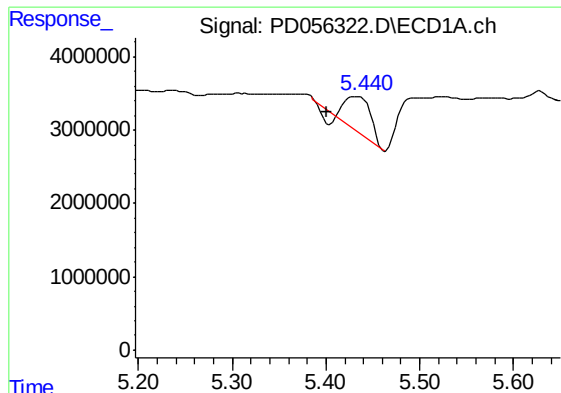

#12 4,4'-DDE


R.T.: 5.432 min
Delta R.T.: 0.031 min
Response: 7464665
Conc: 7.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

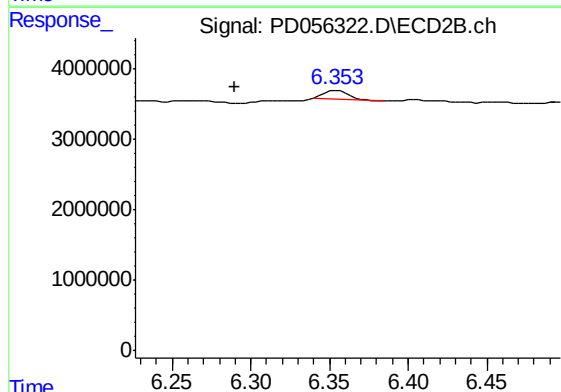


#12 4,4'-DDE

R.T.: 6.355 min
Delta R.T.: 0.065 min
Response: 1423355
Conc: 0.91 ng/ml

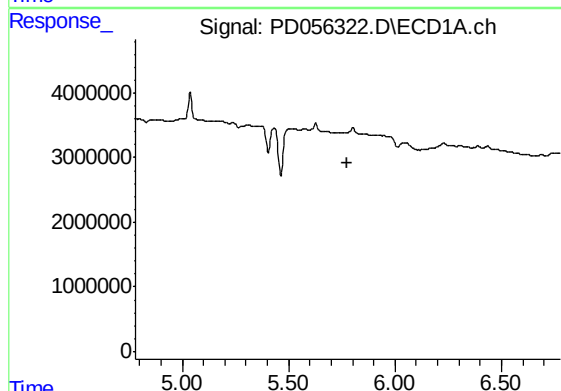


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.778 min
Response: 0
Conc: N.D.

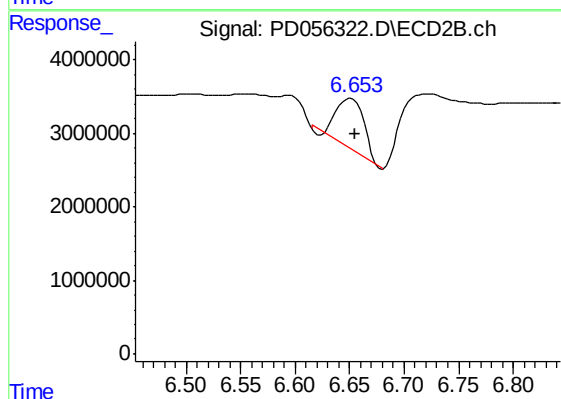

#14 Endrin


R.T.: 6.652 min
Delta R.T.: -0.004 min
Response: 12103228
Conc: 9.56 ng/ml

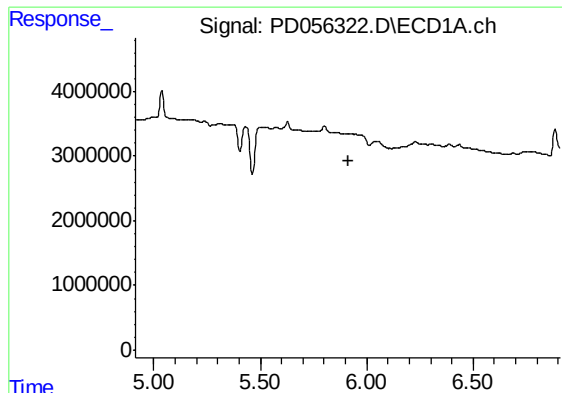

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 5.912 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

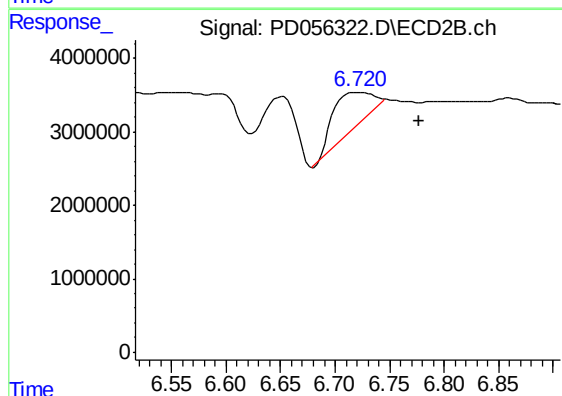


#16 4,4'-DDD

R.T.: 6.722 min
Delta R.T.: -0.055 min
Response: 13306015
Conc: 11.31 ng/ml

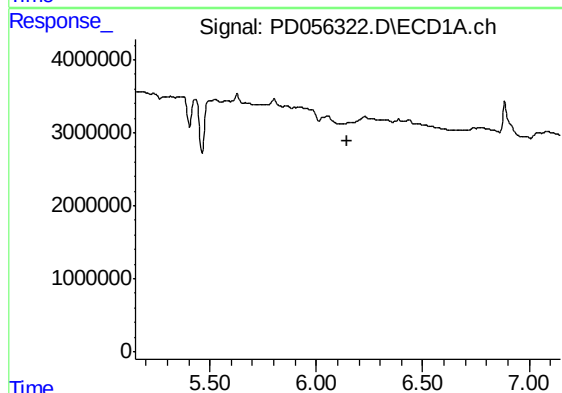


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.147 min
Response: 0
Conc: N.D.

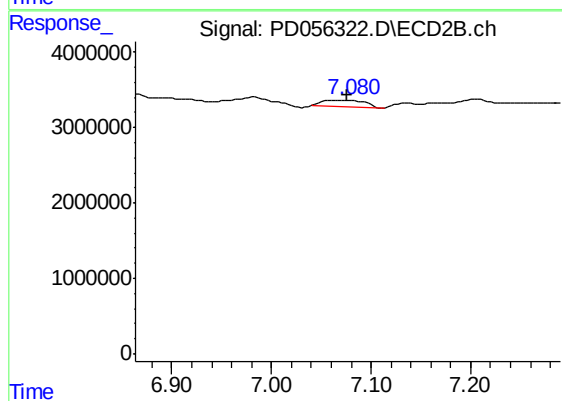

#17 4,4'-DDT


R.T.: 7.068 min
Delta R.T.: -0.008 min
Response: 2573472
Conc: 2.18 ng/ml

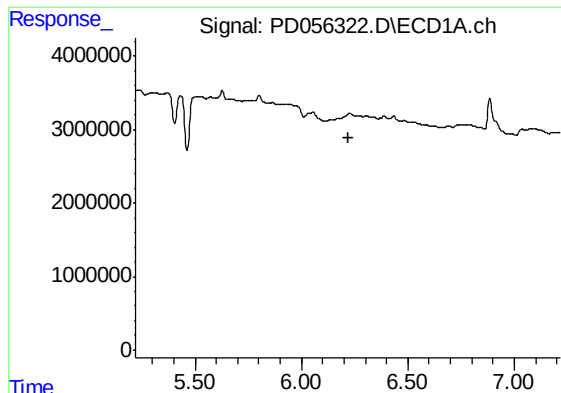

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

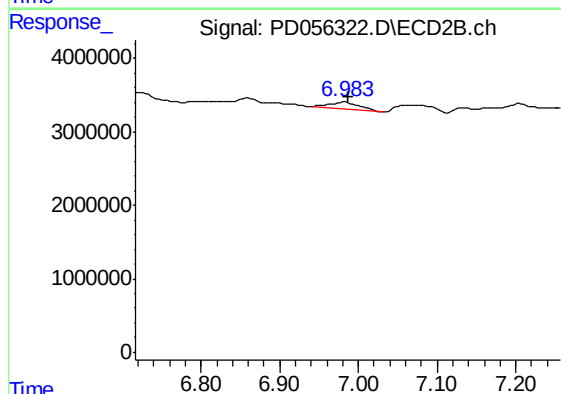


#18 Endrin aldehyde

R.T.: 6.984 min
Delta R.T.: -0.003 min
Response: 2626515
Conc: 2.16 ng/ml

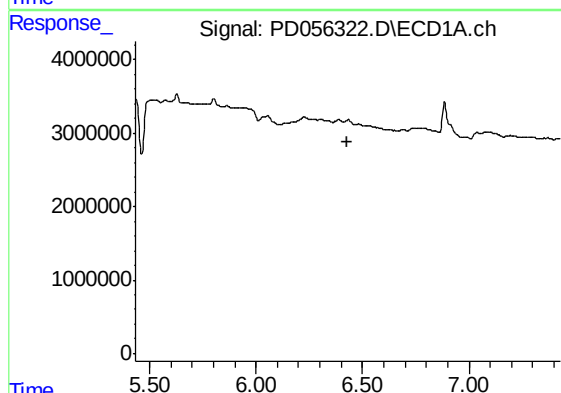


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.430 min
Response: 0
Conc: N.D.

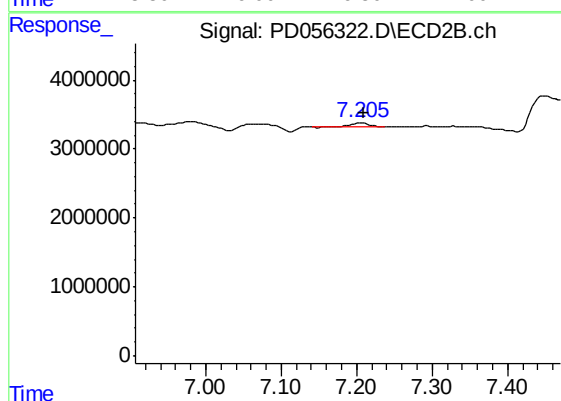

#19 Endosulfan Sulfate


R.T.: 7.206 min
Delta R.T.: -0.004 min
Response: 904057
Conc: 0.68 ng/ml

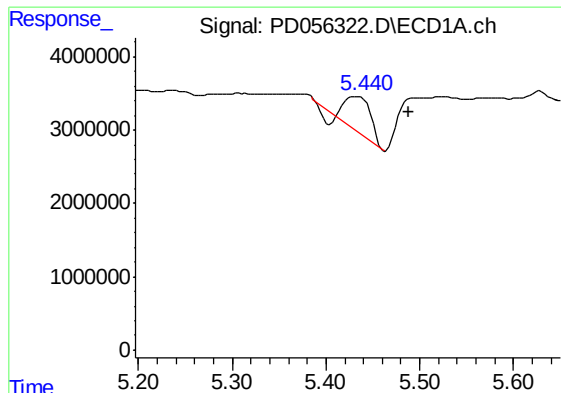

#22 Toxaphene-1


R.T.: 5.432 min
Delta R.T.: -0.057 min
Response: 7464665
Conc: 828.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

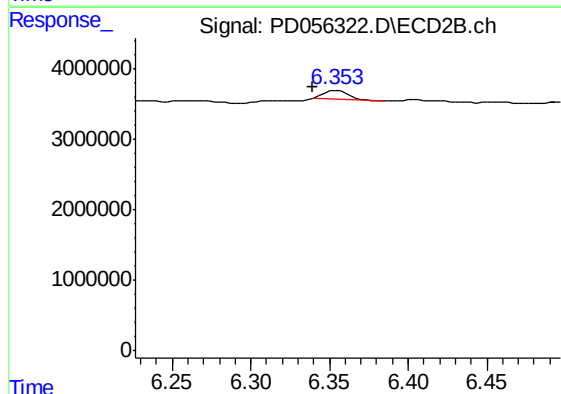


#22 Toxaphene-1

R.T.: 6.355 min
Delta R.T.: 0.016 min
Response: 1423355
Conc: 126.78 ng/ml

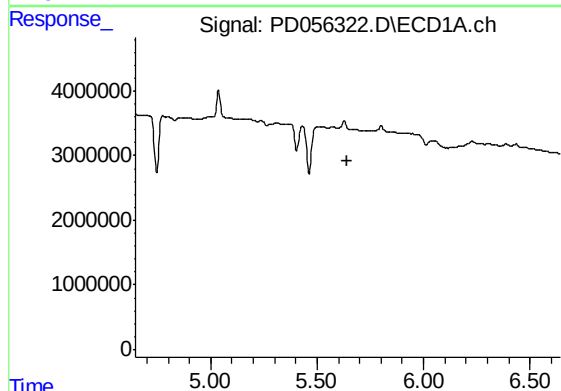


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 5.644 min
Response: 0
Conc: N.D.

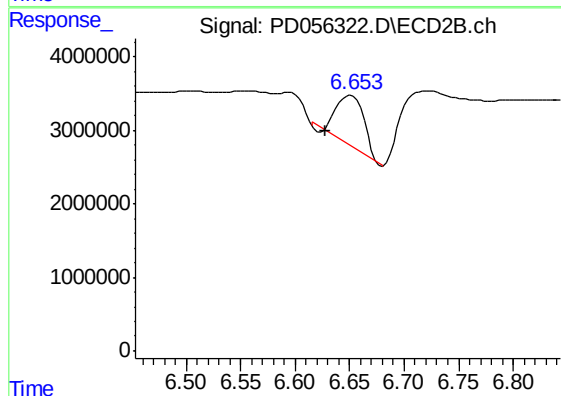

#23 Toxaphene-2


R.T.: 6.652 min
Delta R.T.: 0.023 min
Response: 12103228
Conc: 877.02 ng/ml

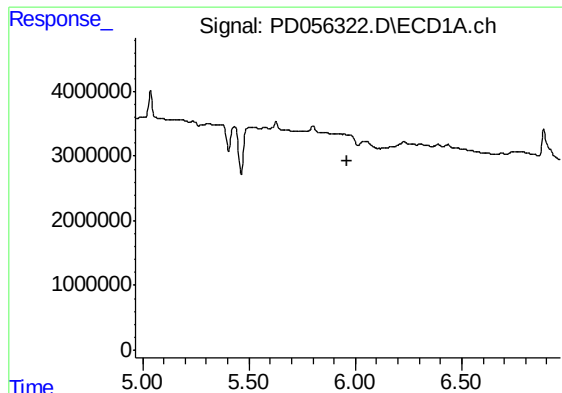

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 5.965 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

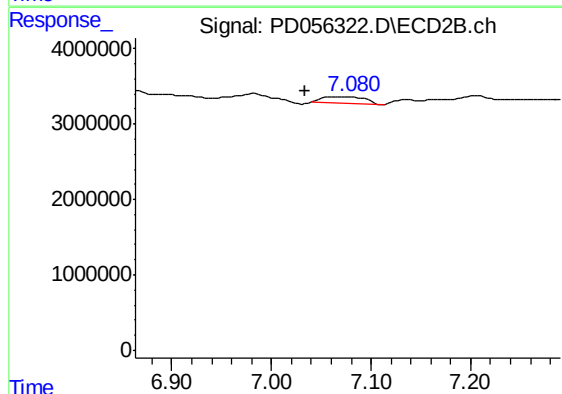


#24 Toxaphene-3

R.T.: 7.068 min
Delta R.T.: 0.035 min
Response: 2573472
Conc: 130.82 ng/ml

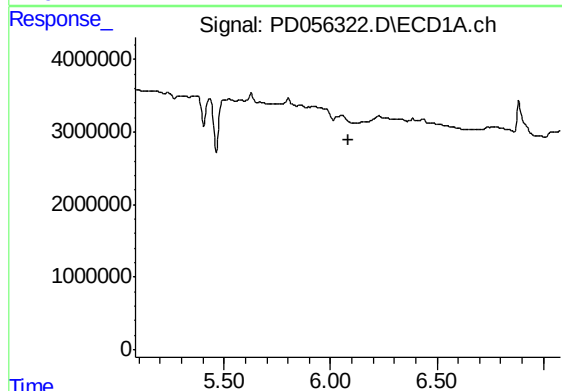


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T.: 6.082 min
Response: 0
Conc: N.D.

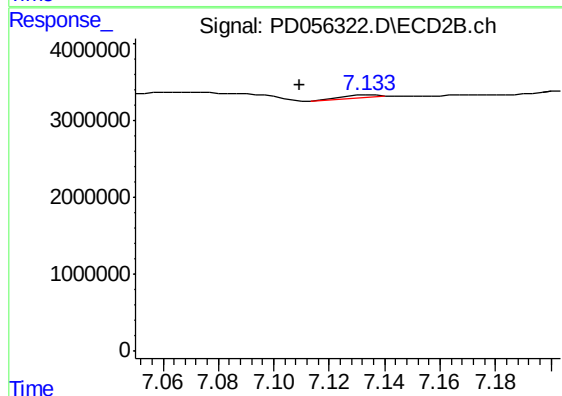

#25 Toxaphene-4


R.T.: 7.135 min
Delta R.T.: 0.026 min
Response: 355684
Conc: 6.44 ng/ml

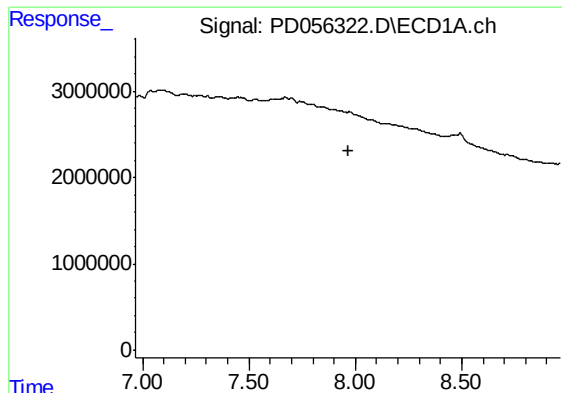

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.965 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

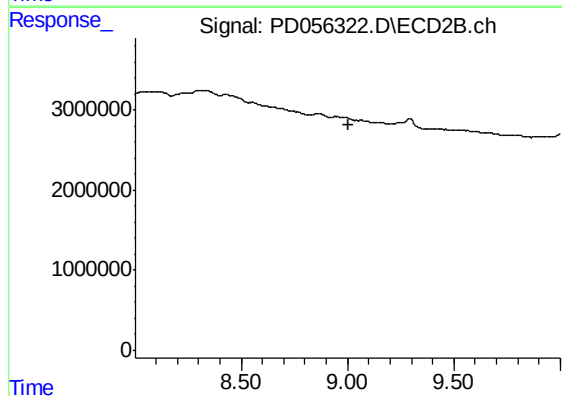

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.002 min
Response: 0
Conc: N.D.