

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120619\
 Data File : PD056323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 09:32
 Operator : SG\AJ
 Sample : PIBLK50
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK50

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 22:32:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.961	18250317	27474001	22.036	22.852
27)	SA Decachlor...	7.963	8.996	37463363	47735300	41.489	39.675
Target Compounds							
6)	B beta-BHC	0.000	4.847f	0	795854	N.D.	0.966
16)	A 4,4'-DDD	0.000	6.735f	0	515620	N.D.	0.438


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120619\
Data File : PD056323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 09:32
Operator : SG\AJ
Sample : PIBLK50
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK50

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 22:32:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

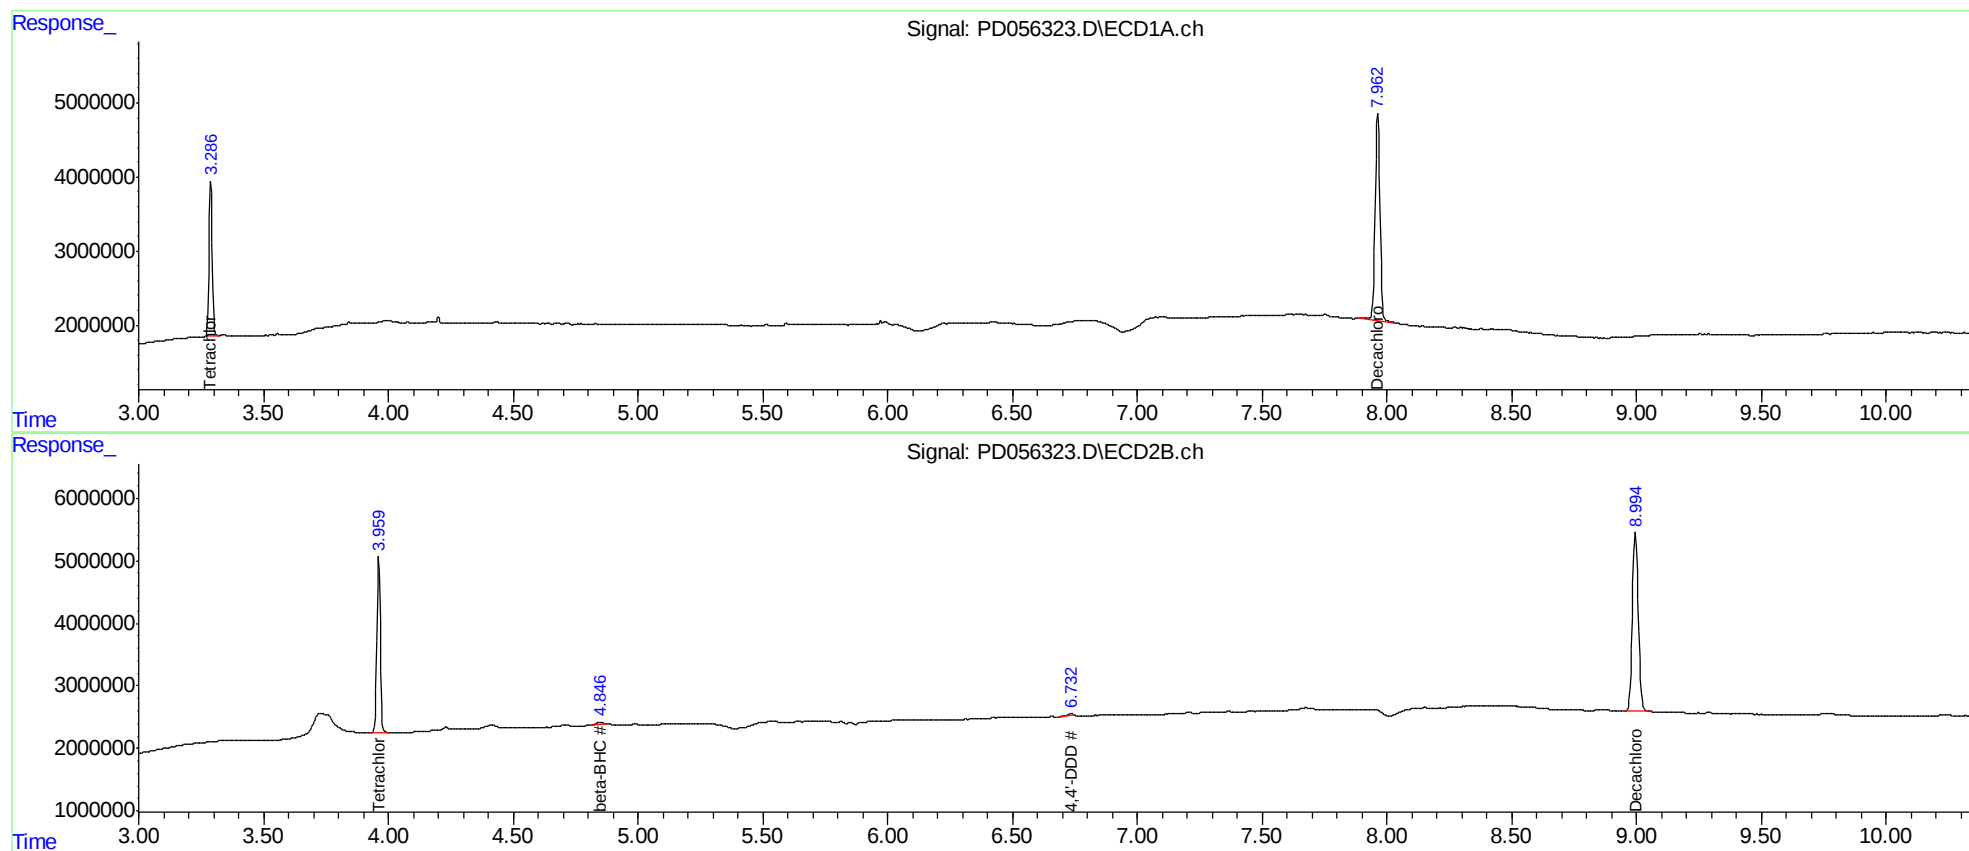


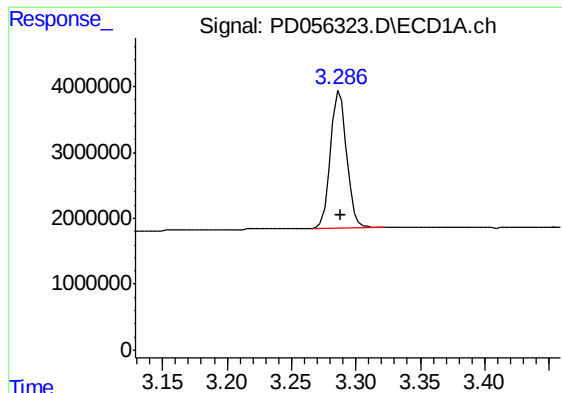

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: 0.000 min
Response: 18250317
Conc: 22.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK50

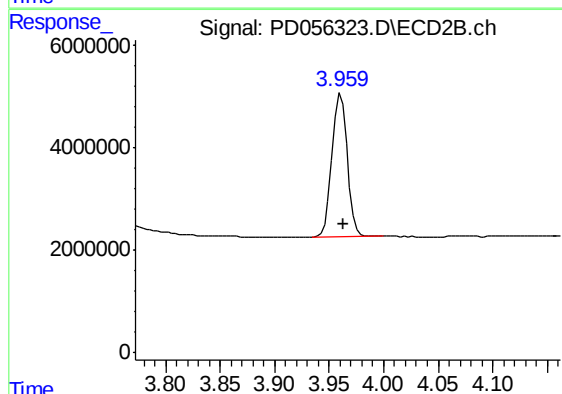


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.002 min
Response: 27474001
Conc: 22.85 ng/ml

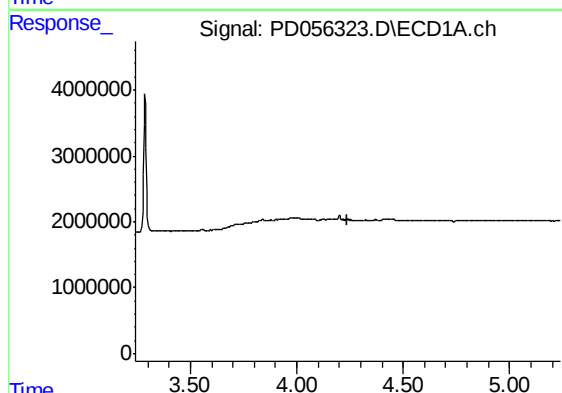


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.240 min
Response: 0
Conc: N.D.

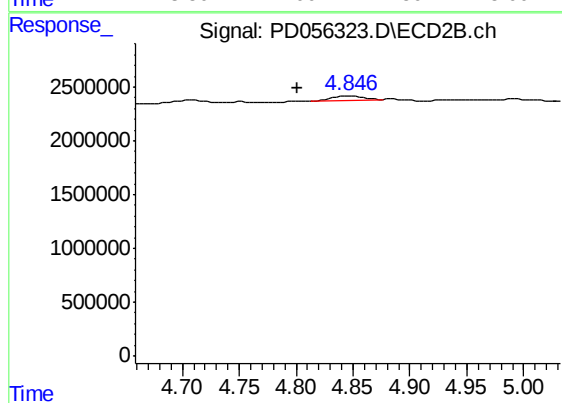

#6 beta-BHC


R.T.: 4.847 min
Delta R.T.: 0.047 min
Response: 795854
Conc: 0.97 ng/ml

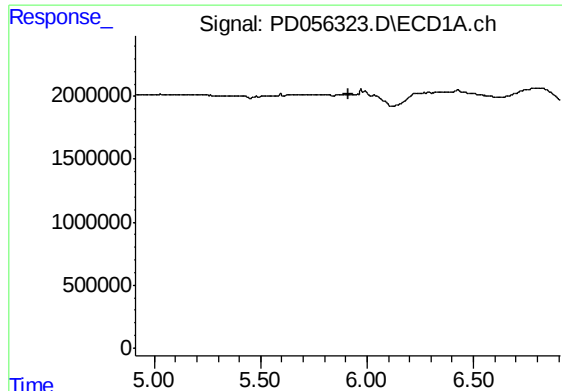

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.912 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK50

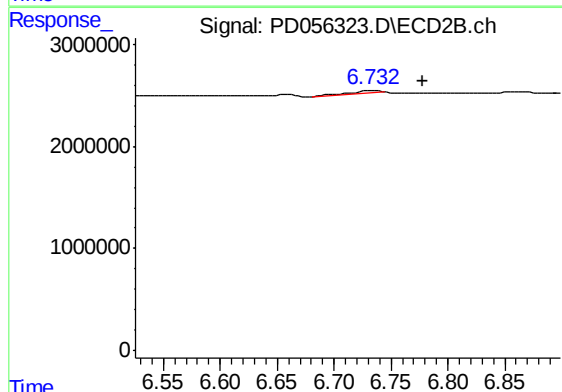


#16 4,4'-DDD

R.T.: 6.735 min
Delta R.T.: -0.042 min
Response: 515620
Conc: 0.44 ng/ml

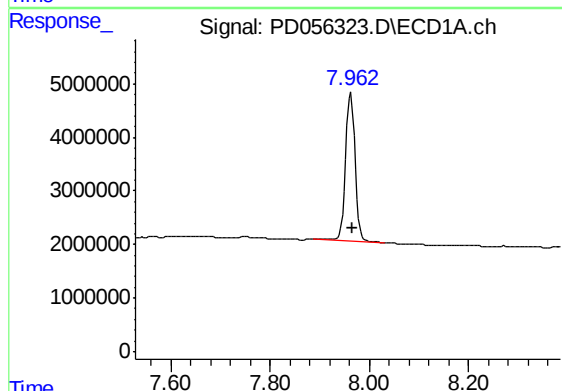

#27 Decachlorobiphenyl

R.T.: 7.963 min
Delta R.T.: -0.002 min
Response: 37463363
Conc: 41.49 ng/ml

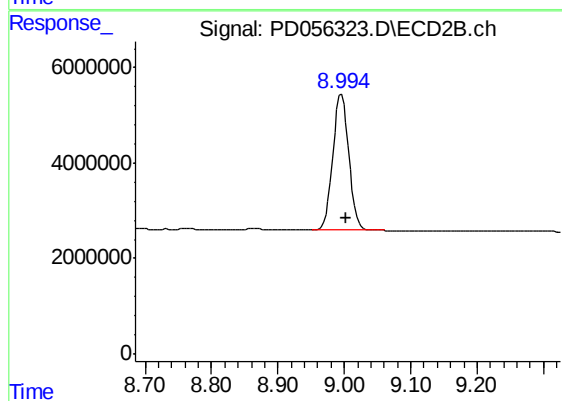

#27 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: -0.007 min
Response: 47735300
Conc: 39.68 ng/ml