

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120622\
 Data File : PD073297.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2022 11:45
 Operator : AR\AJ
 Sample : INDA388
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3244

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 20:38:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.698	3.457	49626477	1559.9E6	20.695	23.879
27)	SA Decachlor...	7.823	8.905	108.1E6	614.3E6	47.356	41.513
Target Compounds							
2)	A alpha-BHC	3.200	3.921	78347193	2065.7E6	21.408	23.687
3)	MA gamma-BHC...	3.530	4.255	73809778	1601.0E6	22.241	23.596
4)	MA Heptachlor	3.862	4.821	74678836	1097.1E6	22.354	23.892
9)	A Endosulfan I	5.014	5.975	62301756	709.4E6	22.046	24.387
13)	MA Dieldrin	5.280	6.252	138.0E6	1452.5E6	45.052	48.186
14)	MA Endrin	5.557	6.483	117.9E6	1100.5E6	43.477	44.614
16)	A 4,4'-DDD	5.703	6.618	109.0E6	1107.6E6	45.238	48.327
17)	MA 4,4'-DDT	5.952	6.925	101.8E6	973.2E6	45.493	45.314
20)	A Methoxychlor	6.535	7.405	284.9E6	2129.3E6	227.510	228.210


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120622\
Data File : PD073297.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2022 11:45
Operator : AR\AJ
Sample : INDA388
Misc :
ALS Vial : 6 Sample Multiplier: 1


Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 20:38:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
Qlast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm
Signal #2 Phase: ZB-MR1

Signal: PD073297.D\ECD1A.ch

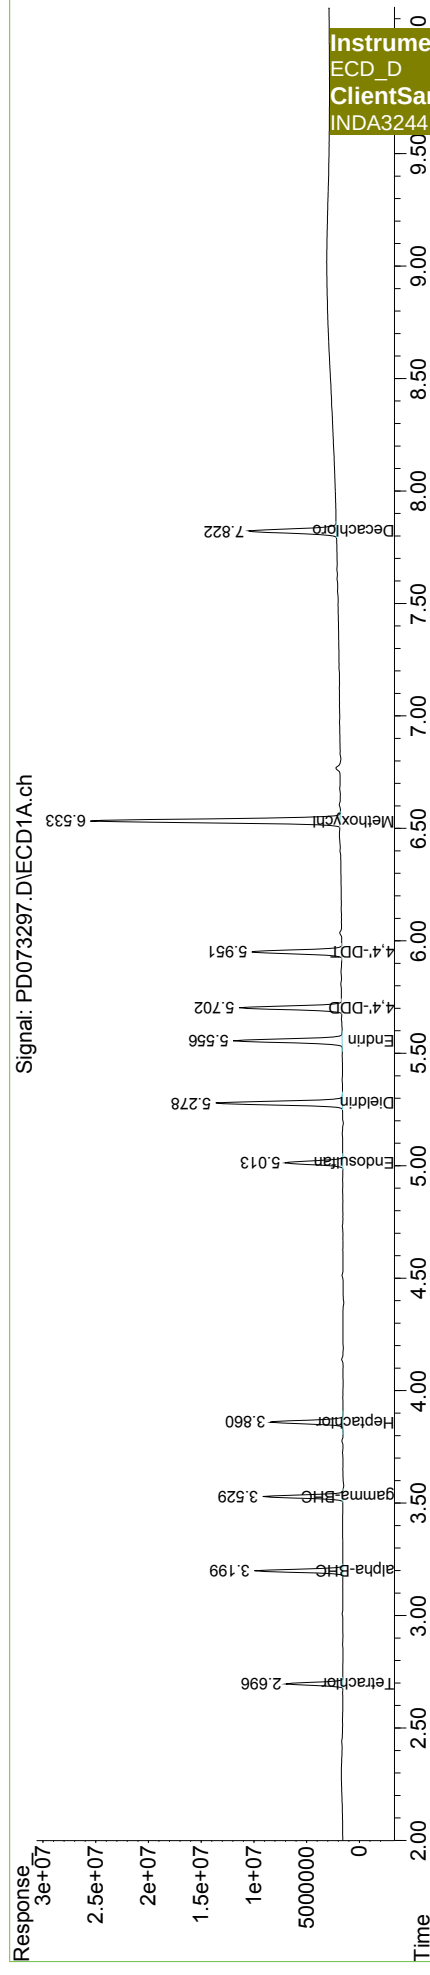

Signal: PD073297.D\ECD2B.ch

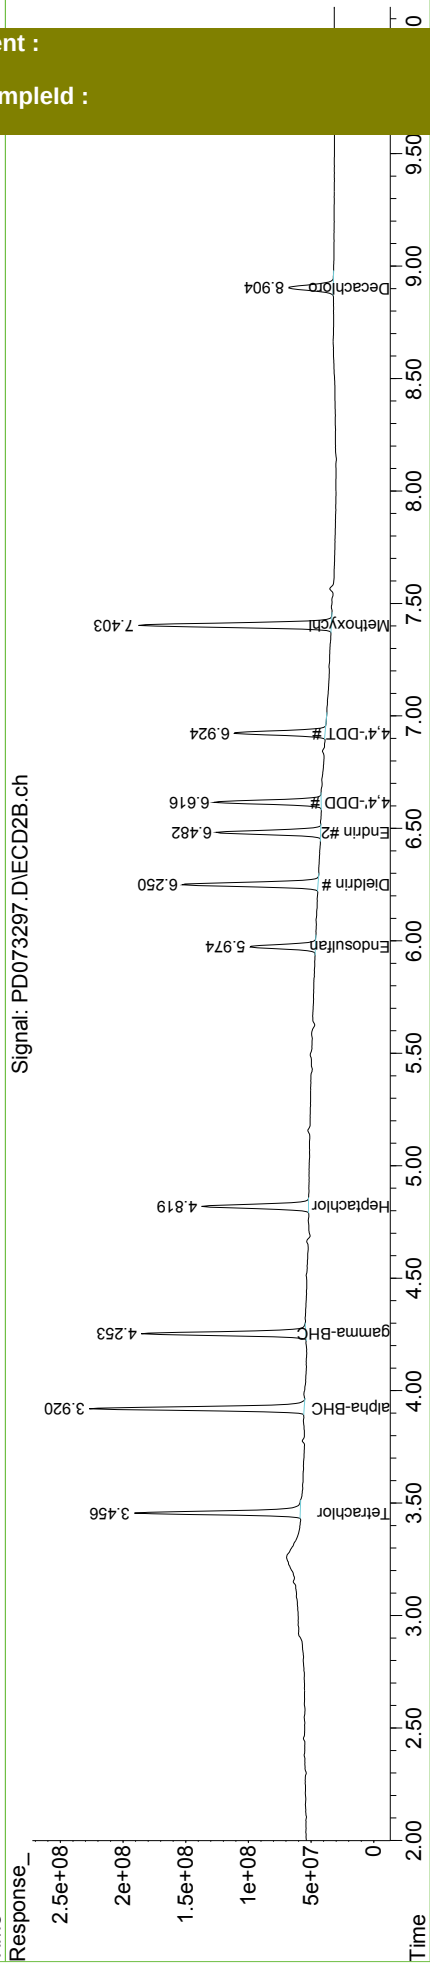

Instrument :
ECD_D
ClientSampleId :
INDA3244