



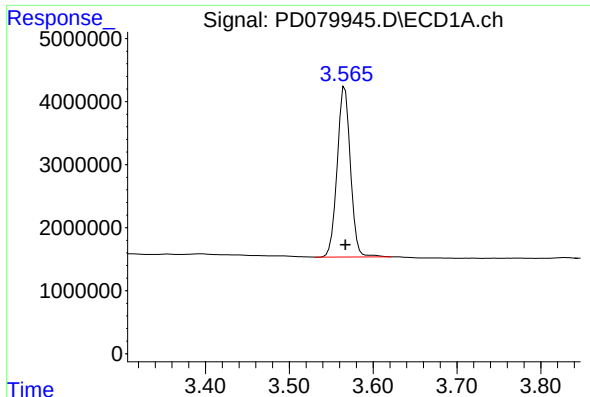

#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 29684095
Conc: 19.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

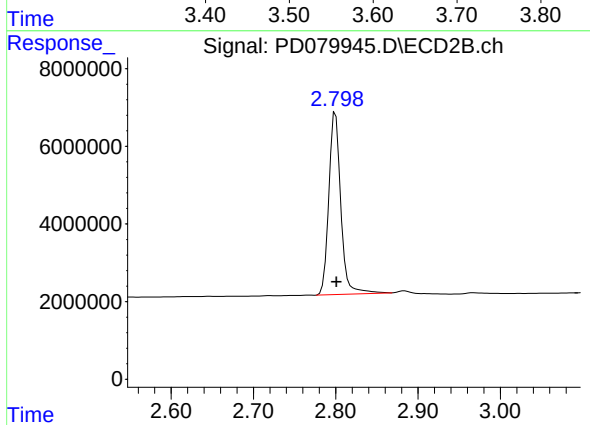

#1 Tetrachloro-m-xylene

R.T.: 2.800 min
Delta R.T.: 0.000 min
Response: 47689035
Conc: 18.97 ng/ml