

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120623\
 Data File : PD079951.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2023 12:59
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 13:50:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 06 13:47:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.800	142.9E6	285.0E6	98.720	99.508
28)	SA Decachlor...	9.114	7.944	182.7E6	261.4E6	97.300	97.884
Target Compounds							
23)	Chlordane-1	4.735	3.801	73115035	96419680	986.031	988.035
24)	Chlordane-2	5.265	4.377	70120036	107.7E6	960.018	969.698
25)	Chlordane-3	5.977	5.007	306.7E6	324.1E6	1000.400	1000.733
26)	Chlordane-4	6.059	5.071	361.9E6	298.7E6	997.129	997.627
27)	Chlordane-5	6.911	5.965	65890514	114.3E6	983.152	987.215



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120623\
Data File : PD079951.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2023 12:59
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 13:50:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
Quant Title : GC Extractables
QLast Update : Wed Dec 06 13:47:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

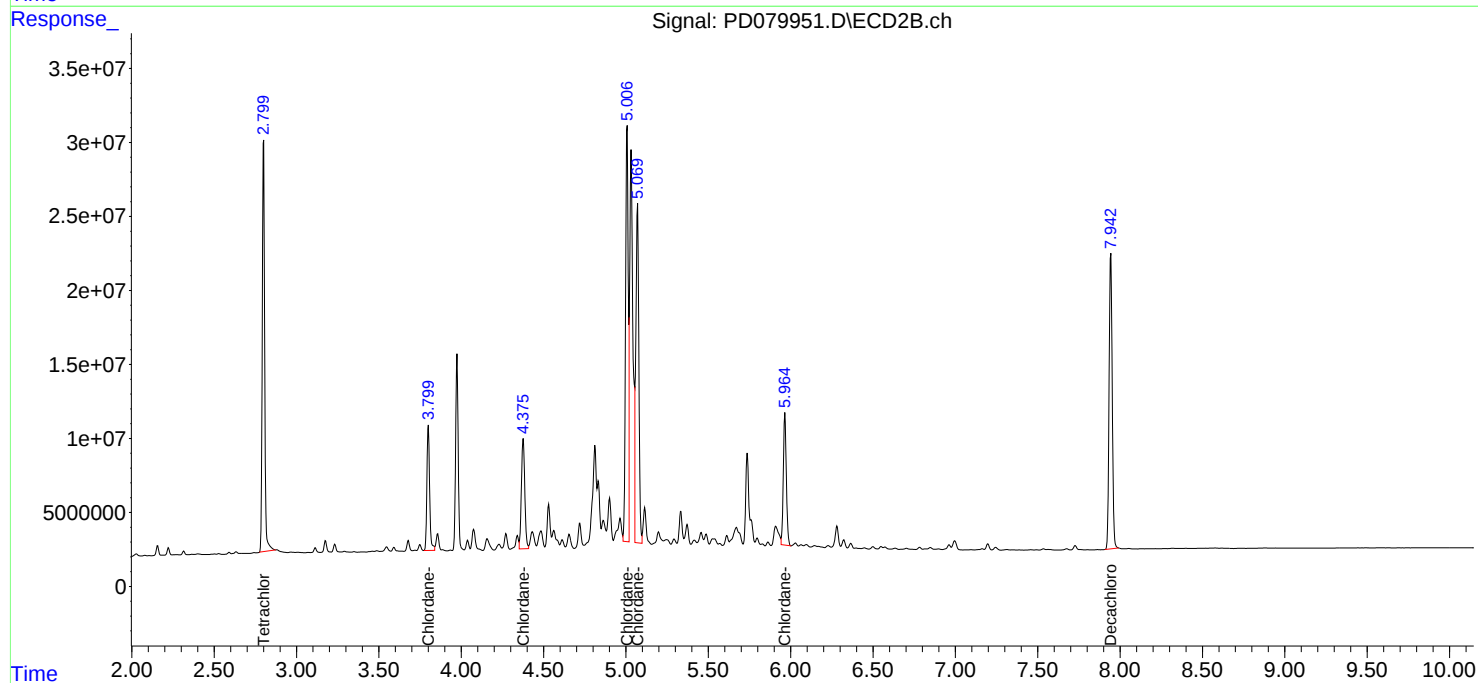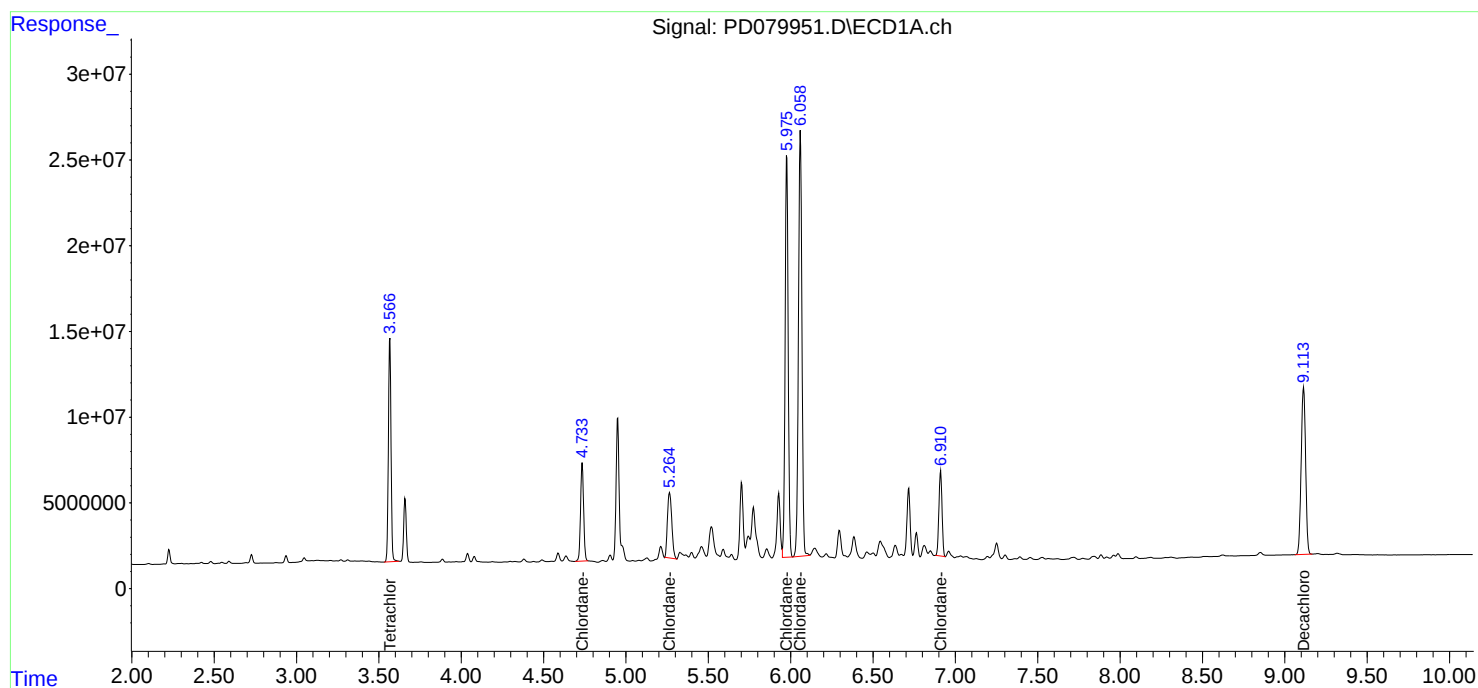


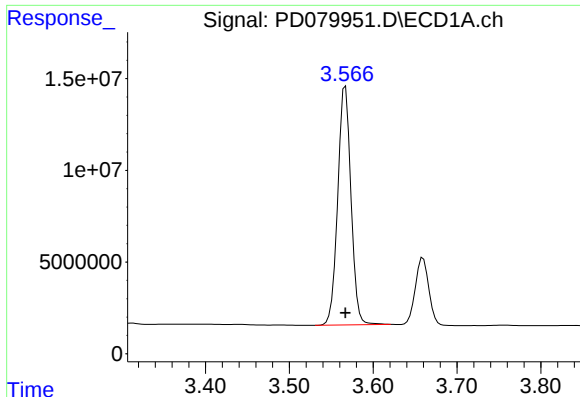

#1 Tetrachloro-m-xylene


R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 142933669
Conc: 98.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

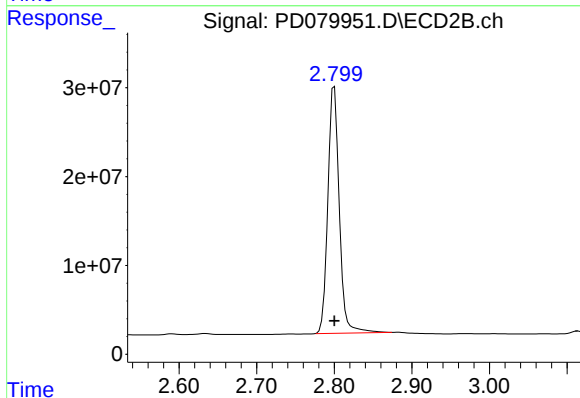


#1 Tetrachloro-m-xylene

R.T.: 2.800 min
Delta R.T.: 0.000 min
Response: 285044079
Conc: 99.51 ng/ml

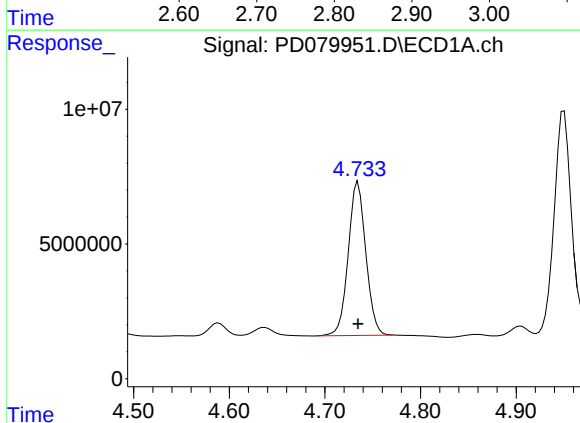


#23 Chlordane-1

R.T.: 4.735 min
Delta R.T.: 0.000 min
Response: 73115035
Conc: 986.03 ng/ml

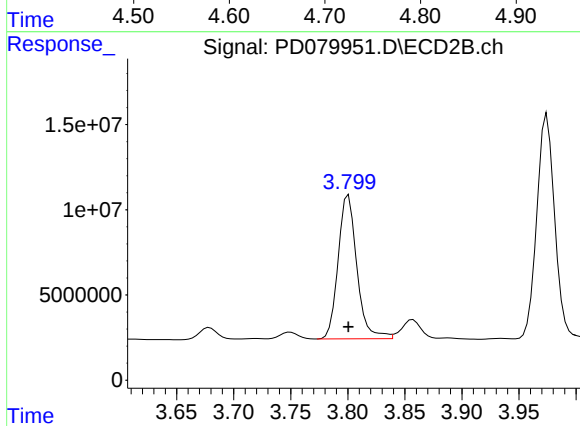

#23 Chlordane-1


R.T.: 3.801 min
Delta R.T.: 0.000 min
Response: 96419680
Conc: 988.04 ng/ml

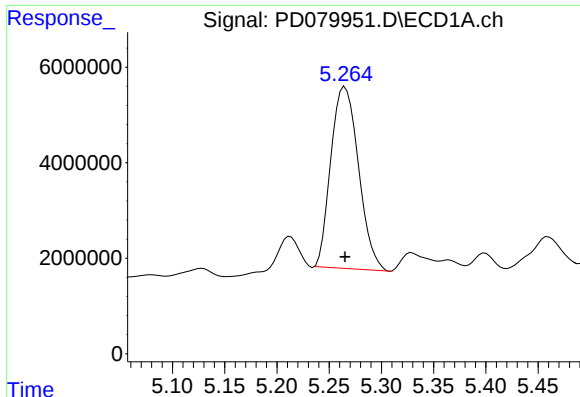

#24 Chlordane-2


R.T.: 5.265 min
Delta R.T.: 0.000 min
Response: 70120036
Conc: 960.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

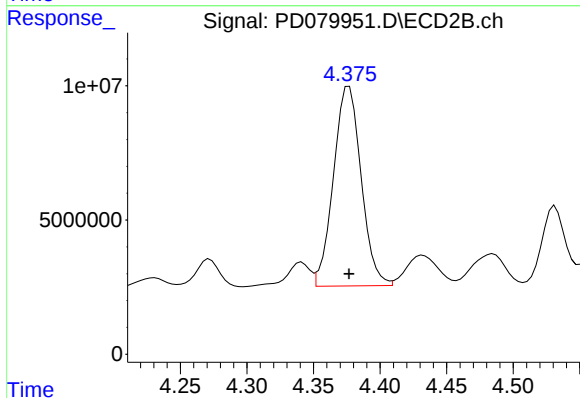


#24 Chlordane-2

R.T.: 4.377 min
Delta R.T.: 0.000 min
Response: 107650013
Conc: 969.70 ng/ml

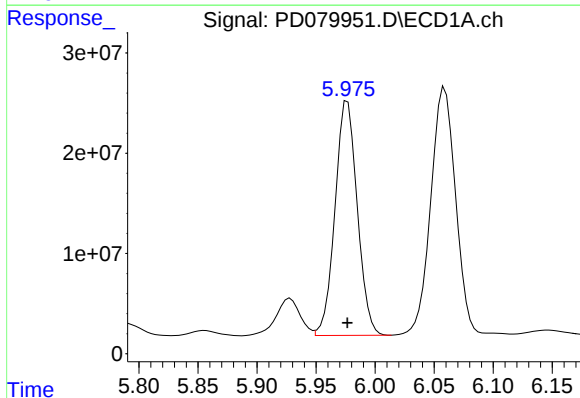


#25 Chlordane-3

R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 306650490
Conc: 1000.40 ng/ml

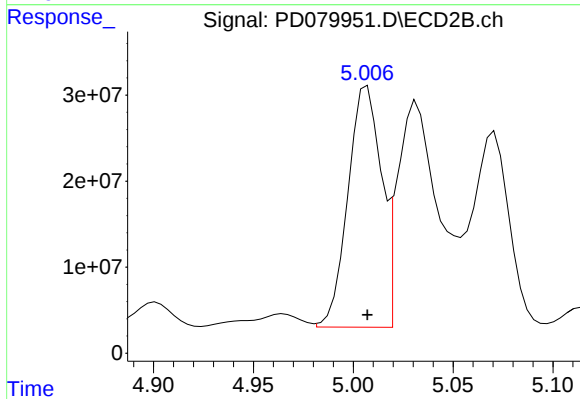

#25 Chlordane-3


R.T.: 5.007 min
Delta R.T.: 0.000 min
Response: 324058065
Conc: 1000.73 ng/ml

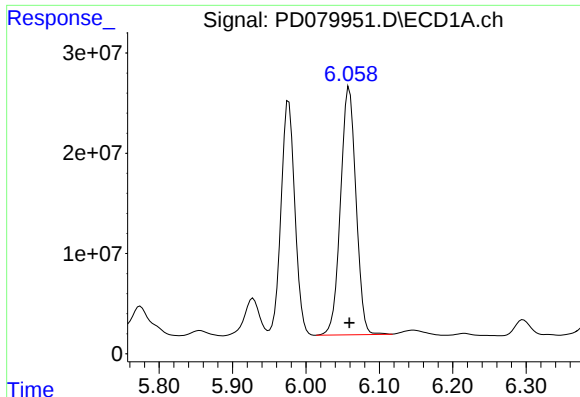

#26 Chlordane-4


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 361917667
Conc: 997.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

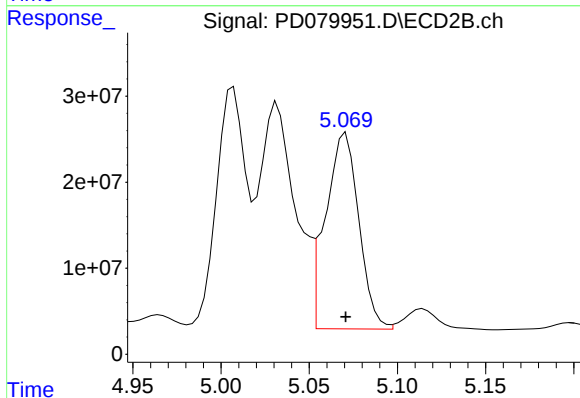


#26 Chlordane-4

R.T.: 5.071 min
Delta R.T.: 0.000 min
Response: 298745846
Conc: 997.63 ng/ml

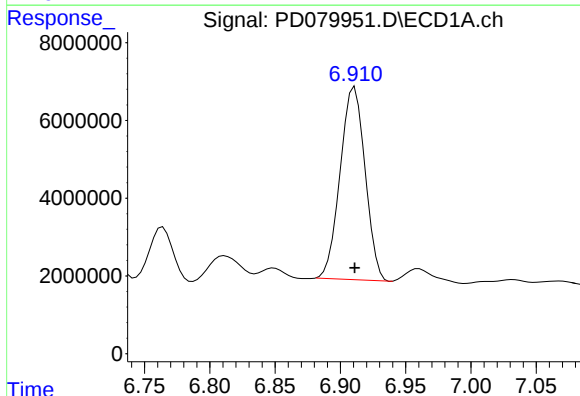


#27 Chlordane-5

R.T.: 6.911 min
Delta R.T.: 0.000 min
Response: 65890514
Conc: 983.15 ng/ml

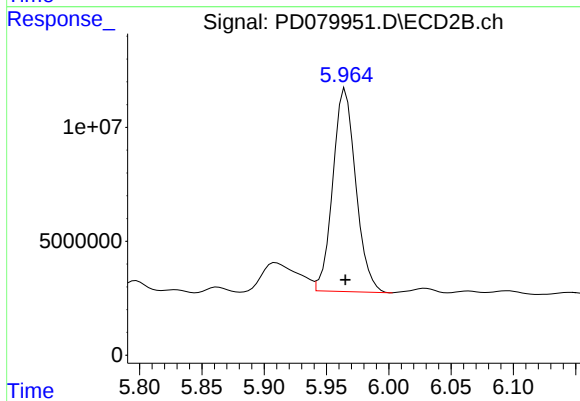

#27 Chlordane-5


R.T.: 5.965 min
Delta R.T.: 0.000 min
Response: 114323406
Conc: 987.21 ng/ml

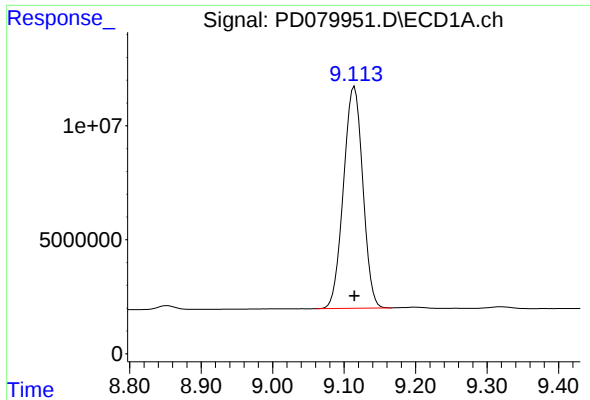

#28 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: 0.000 min
Response: 182741064
Conc: 97.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

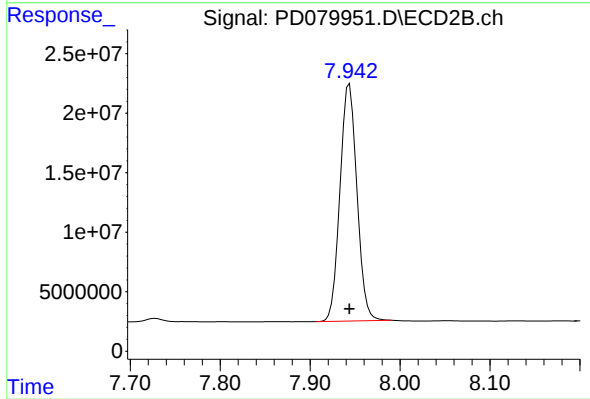

#28 Decachlorobiphenyl

R.T.: 7.944 min
Delta R.T.: 0.000 min
Response: 261398720
Conc: 97.88 ng/ml