

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120623\
 Data File : PD079952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2023 13:12
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 13:52:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 06 13:47:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.801	107.8E6	215.0E6	74.632	75.048
28)	SA Decachlor...	9.113	7.944	140.0E6	199.4E6	74.691	74.790
Target Compounds							
23)	Chlordane-1	4.735	3.800	55439954	72760840	748.441	747.059
24)	Chlordane-2	5.265	4.377	54177833	82386073	744.481	744.731
25)	Chlordane-3	5.977	5.007	230.0E6	243.4E6	750.191	751.178
26)	Chlordane-4	6.059	5.071	272.8E6	221.0E6	751.096	741.988
27)	Chlordane-5	6.911	5.966	50248862	86029135	749.842	745.242



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120623\
Data File : PD079952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2023 13:12
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 13:52:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
Quant Title : GC Extractables
QLast Update : Wed Dec 06 13:47:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

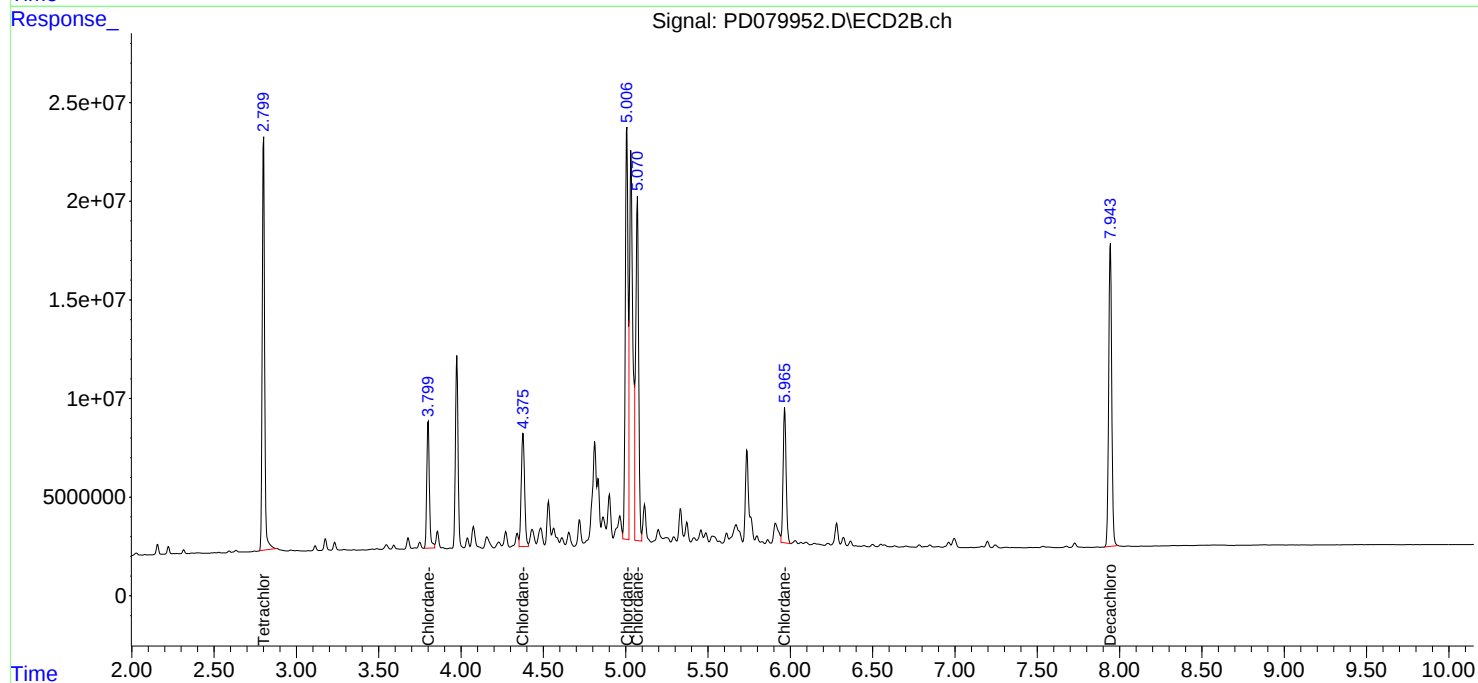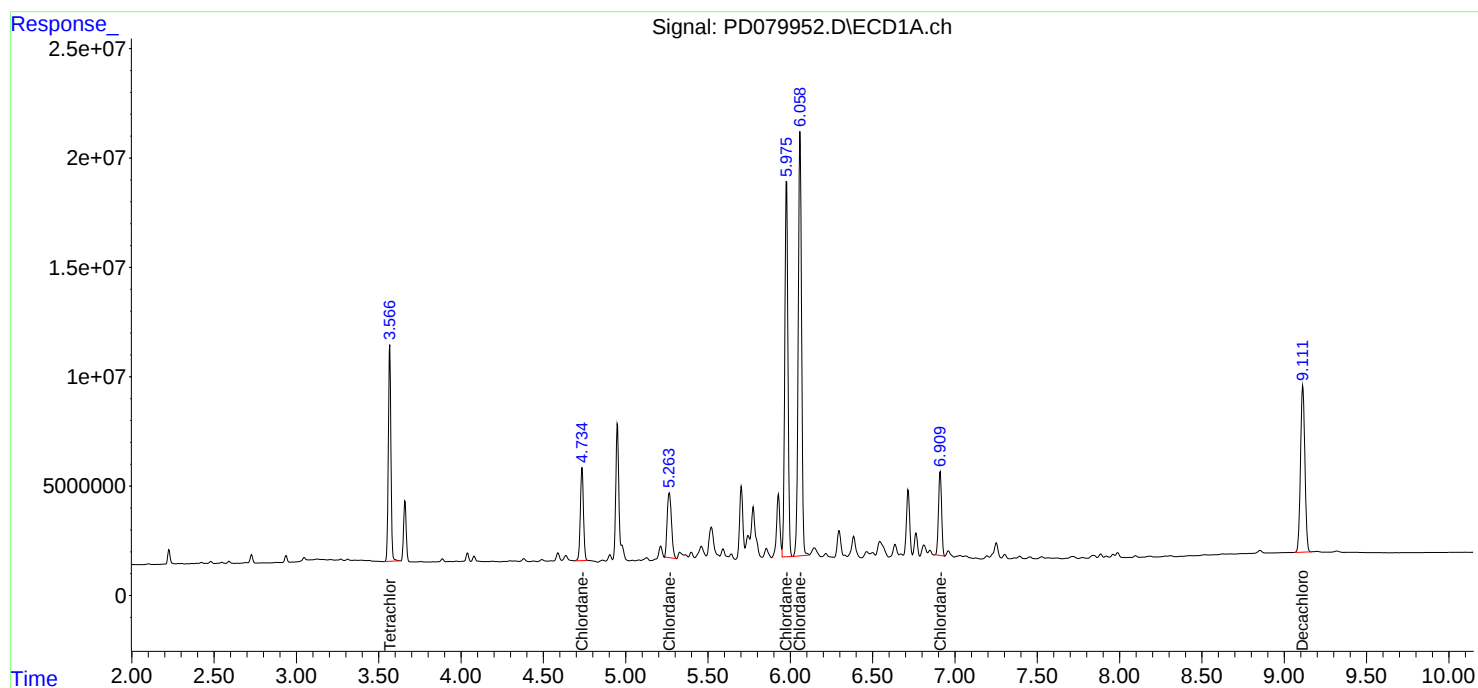


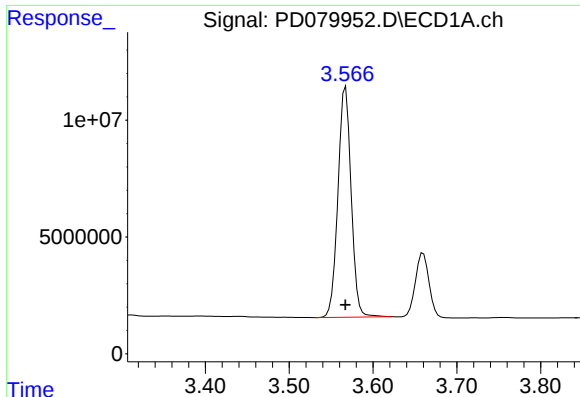

#1 Tetrachloro-m-xylene


R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 107793177
Conc: 74.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

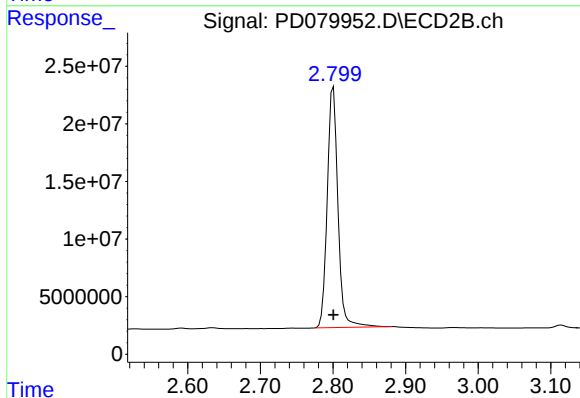


#1 Tetrachloro-m-xylene

R.T.: 2.801 min
Delta R.T.: 0.000 min
Response: 215046803
Conc: 75.05 ng/ml

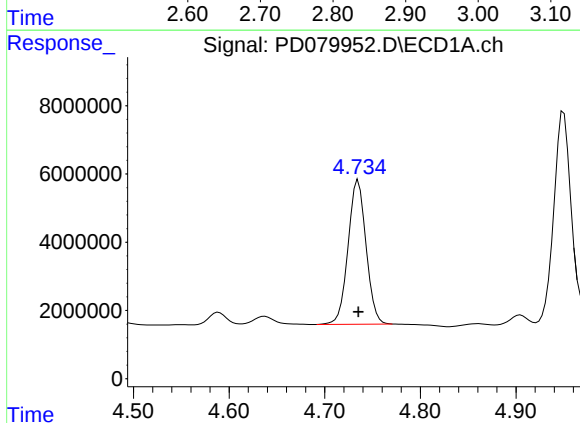


#23 Chlordane-1

R.T.: 4.735 min
Delta R.T.: 0.000 min
Response: 55439954
Conc: 748.44 ng/ml

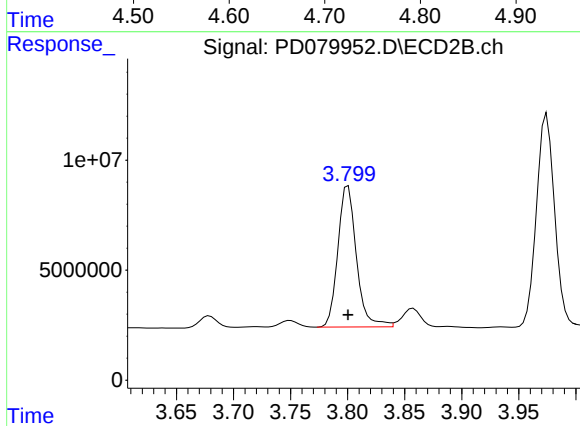

#23 Chlordane-1


R.T.: 3.800 min
Delta R.T.: 0.000 min
Response: 72760840
Conc: 747.06 ng/ml

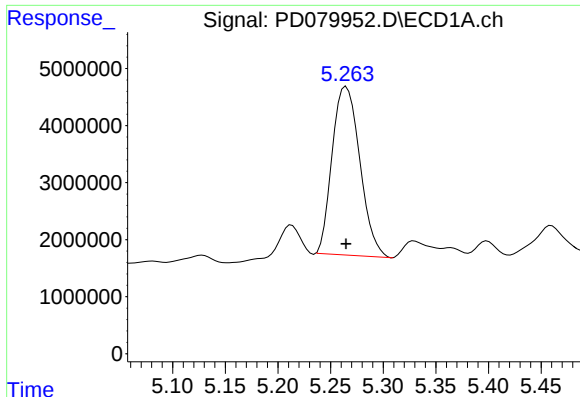

#24 Chlordane-2


R.T.: 5.265 min
Delta R.T.: 0.000 min
Response: 54177833
Conc: 744.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

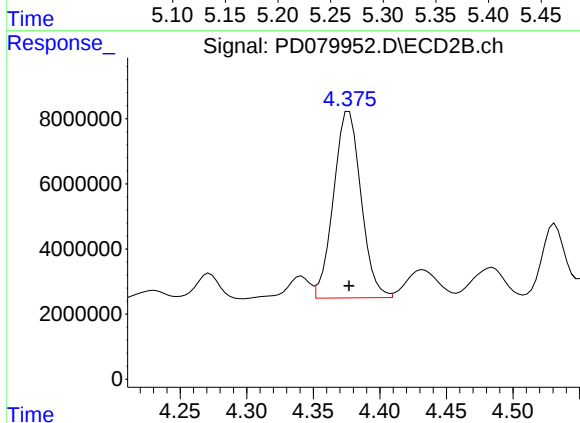


#24 Chlordane-2

R.T.: 4.377 min
Delta R.T.: 0.000 min
Response: 82386073
Conc: 744.73 ng/ml

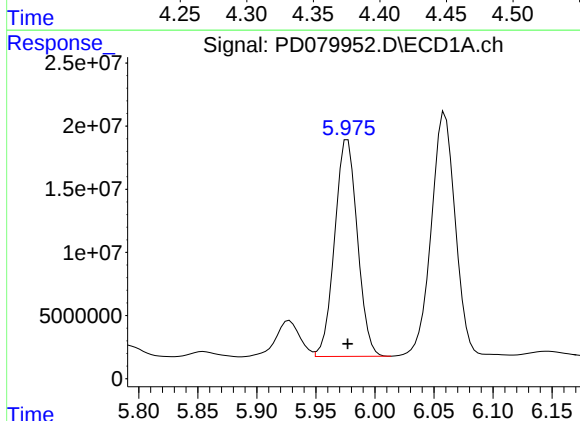


#25 Chlordane-3

R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 229983962
Conc: 750.19 ng/ml

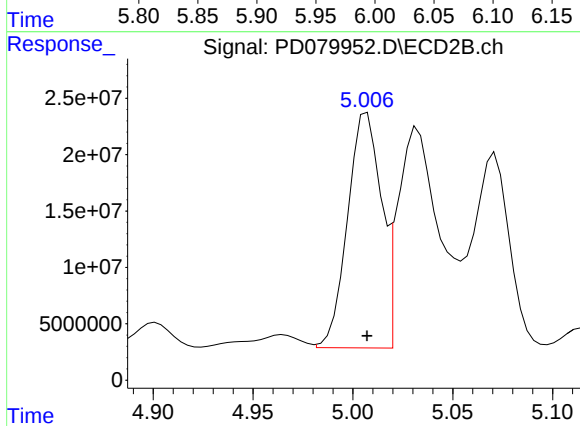

#25 Chlordane-3


R.T.: 5.007 min
Delta R.T.: 0.000 min
Response: 243438335
Conc: 751.18 ng/ml

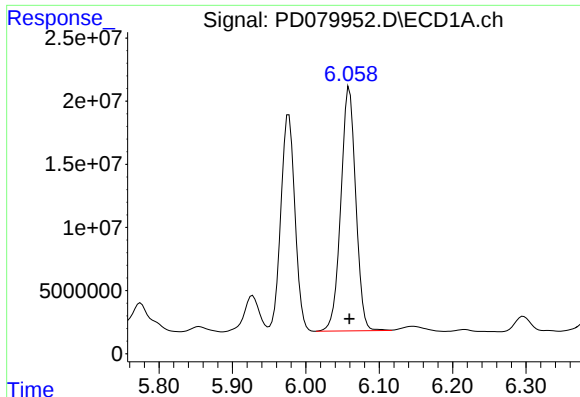

#26 Chlordane-4


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 272816631
Conc: 751.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

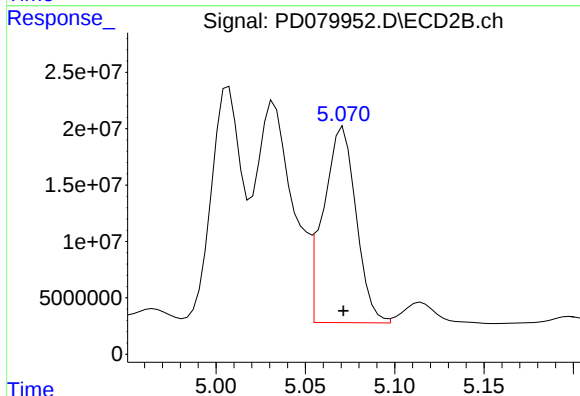


#26 Chlordane-4

R.T.: 5.071 min
Delta R.T.: 0.000 min
Response: 221012680
Conc: 741.99 ng/ml

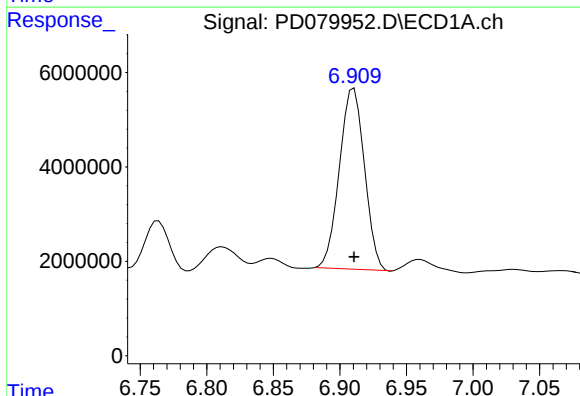


#27 Chlordane-5

R.T.: 6.911 min
Delta R.T.: 0.000 min
Response: 50248862
Conc: 749.84 ng/ml

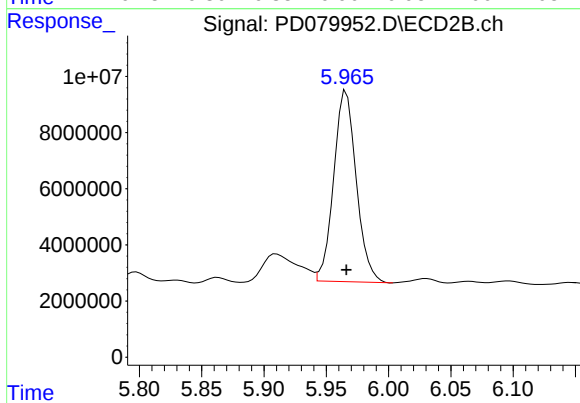

#27 Chlordane-5


R.T.: 5.966 min
Delta R.T.: 0.000 min
Response: 86029135
Conc: 745.24 ng/ml

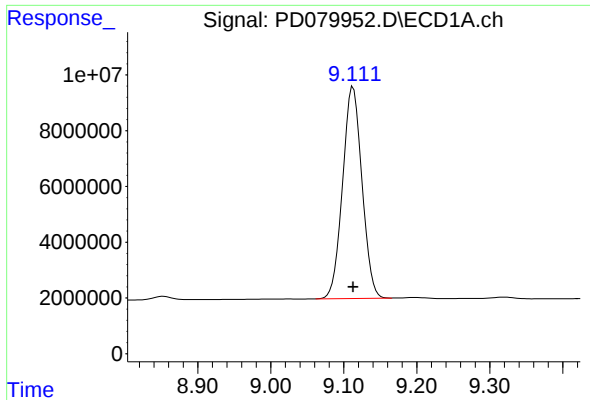

#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 139989195
Conc: 74.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

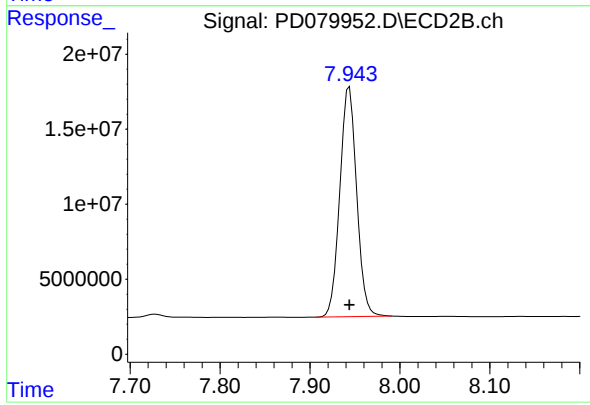

#28 Decachlorobiphenyl

R.T.: 7.944 min
Delta R.T.: 0.000 min
Response: 199446164
Conc: 74.79 ng/ml