

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120623\
 Data File : PD079953.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2023 13:26
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 13:47:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 06 13:47:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.800	73320629	143.9E6	50.000	50.000
28)	SA Decachlor...	9.113	7.944	96440757	136.3E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.734	3.800	37593357	49377447	500.000	500.000
24)	Chlordane-2	5.264	4.377	37980302	57188969	500.000	500.000
25)	Chlordane-3	5.976	5.007	153.2E6	161.8E6	500.000	500.000
26)	Chlordane-4	6.059	5.071	182.0E6	150.1E6	500.000	500.000
27)	Chlordane-5	6.910	5.966	34074385	58642302	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120623\
Data File : PD079953.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2023 13:26
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 13:47:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
Quant Title : GC Extractables
QLast Update : Wed Dec 06 13:47:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

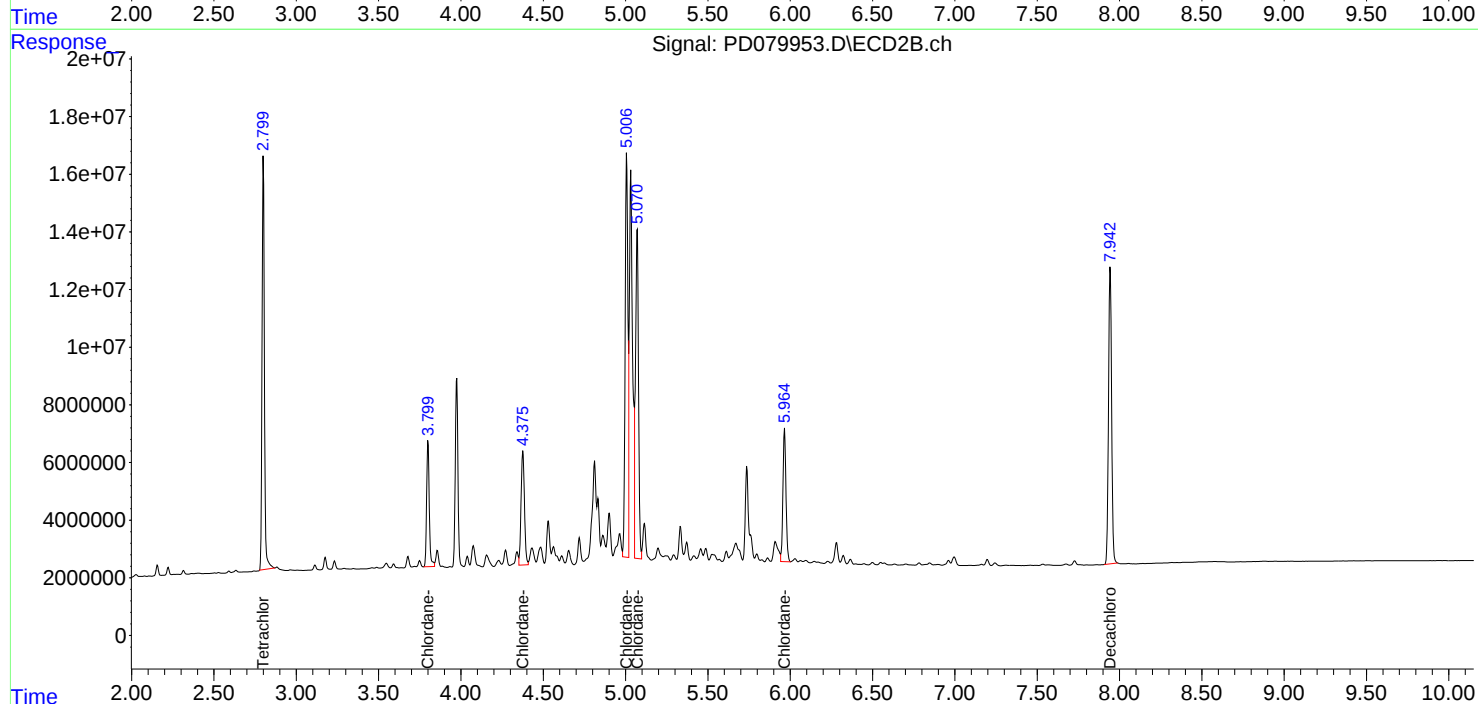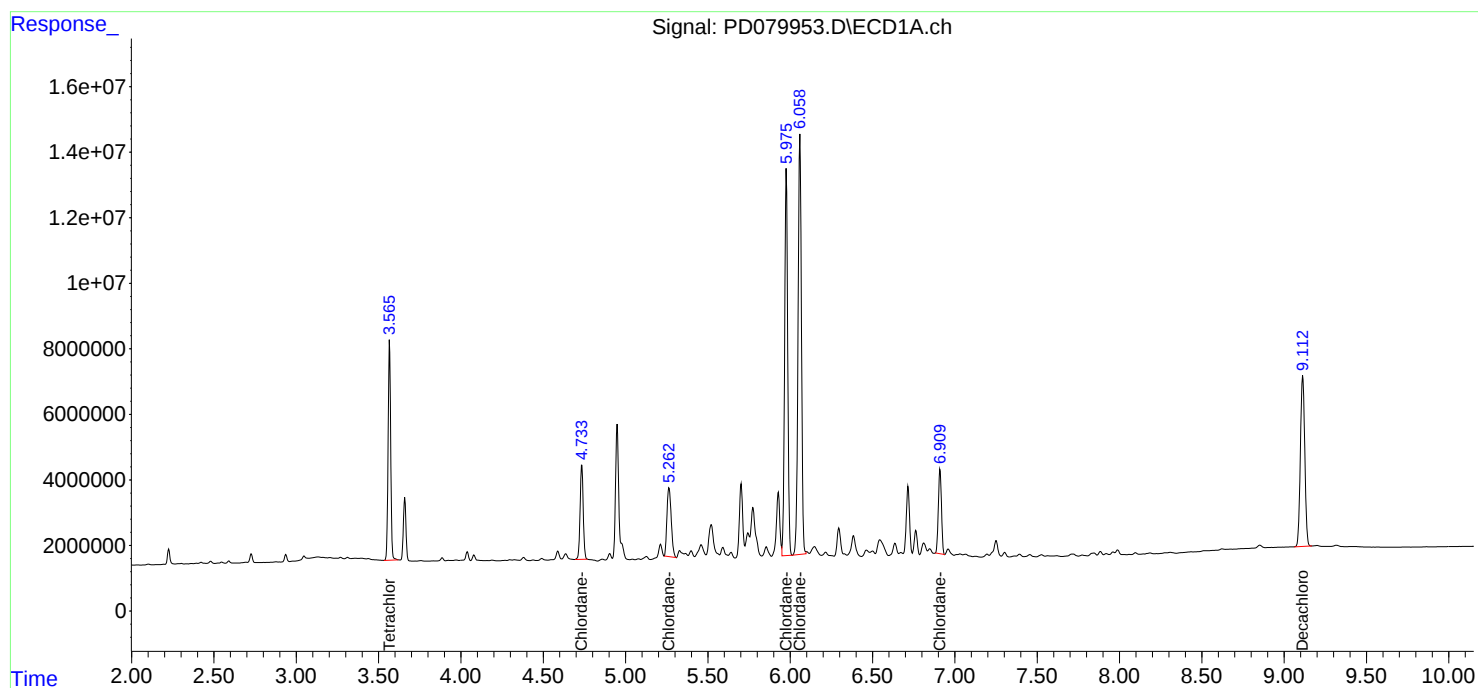


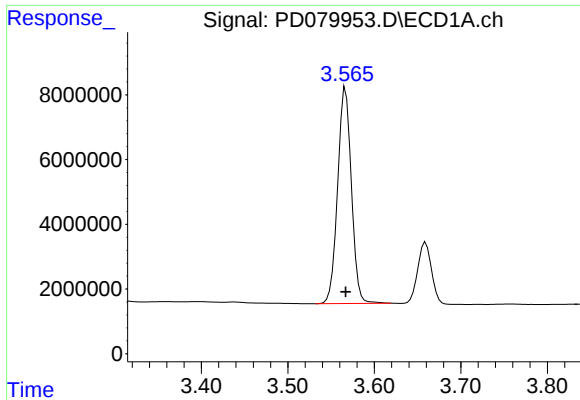

#1 Tetrachloro-m-xylene


R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 73320629
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

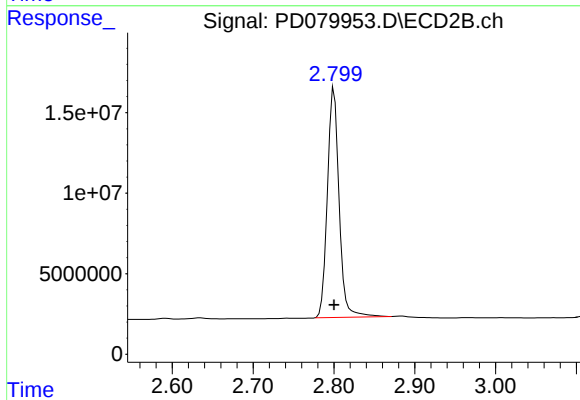


#1 Tetrachloro-m-xylene

R.T.: 2.800 min
Delta R.T.: 0.000 min
Response: 143932180
Conc: 50.00 ng/ml

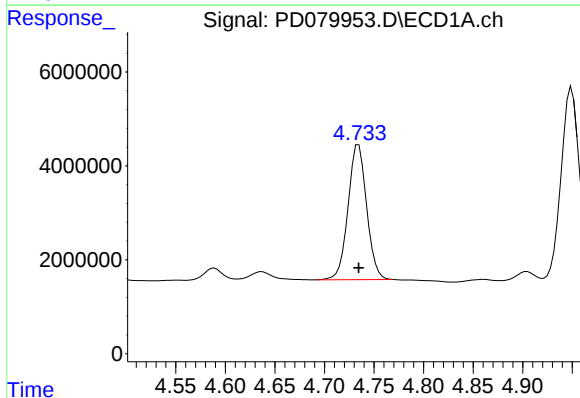


#23 Chlordane-1

R.T.: 4.734 min
Delta R.T.: 0.000 min
Response: 37593357
Conc: 500.00 ng/ml

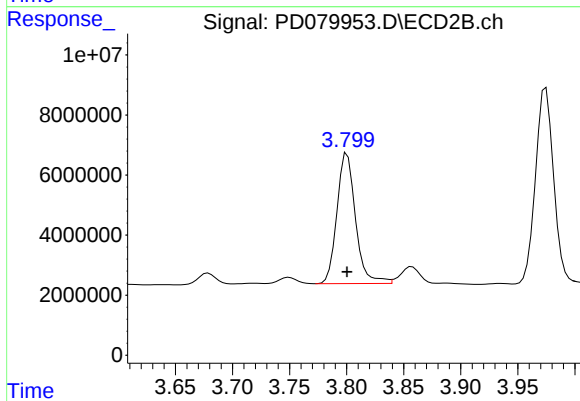

#23 Chlordane-1


R.T.: 3.800 min
Delta R.T.: 0.000 min
Response: 49377447
Conc: 500.00 ng/ml

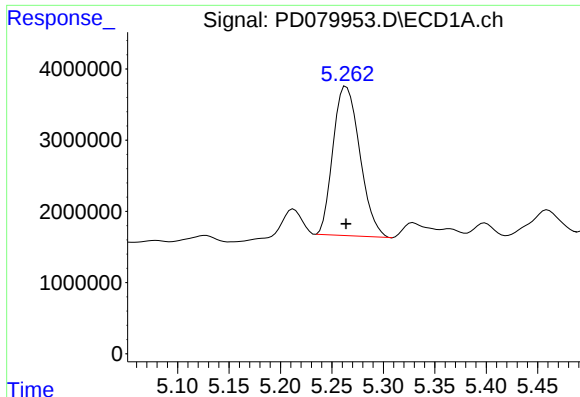

#24 Chlordane-2


R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 37980302
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

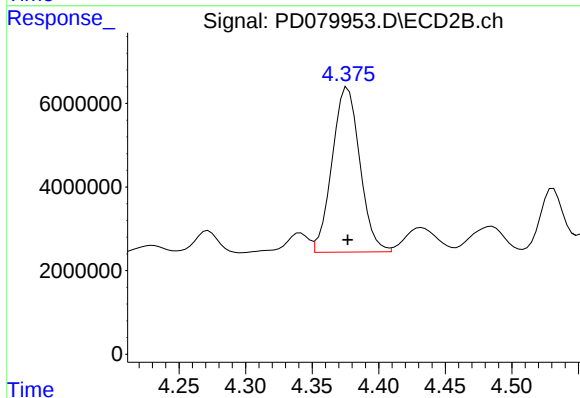


#24 Chlordane-2

R.T.: 4.377 min
Delta R.T.: 0.000 min
Response: 57188969
Conc: 500.00 ng/ml

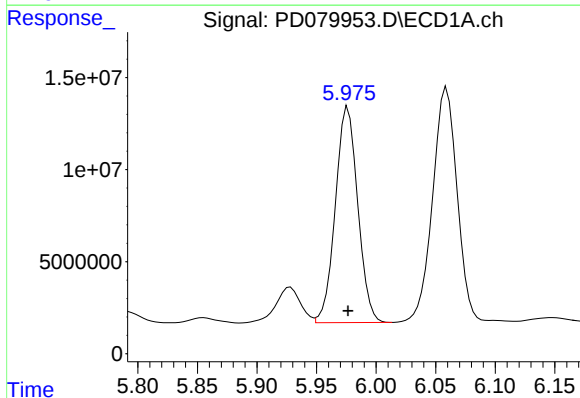


#25 Chlordane-3

R.T.: 5.976 min
Delta R.T.: 0.000 min
Response: 153202765
Conc: 500.00 ng/ml

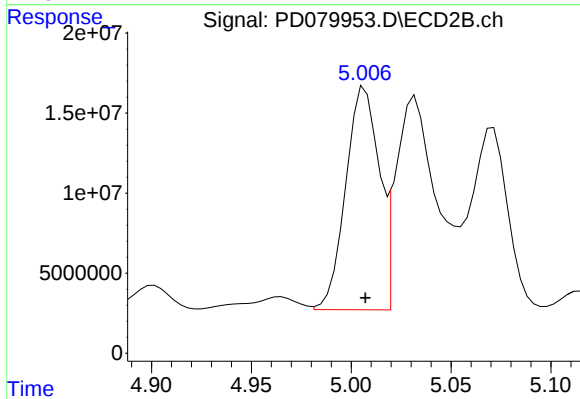

#25 Chlordane-3


R.T.: 5.007 min
Delta R.T.: 0.000 min
Response: 161791666
Conc: 500.00 ng/ml

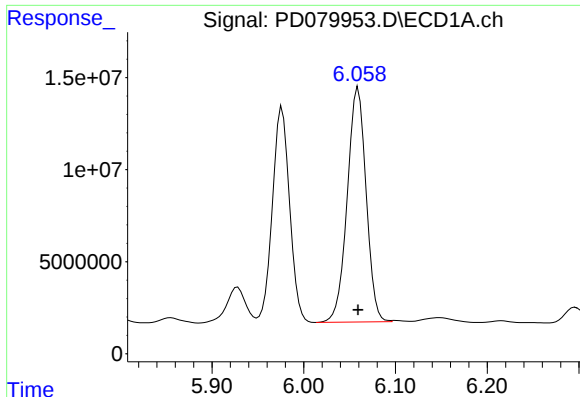

#26 Chlordane-4


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 18200796
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

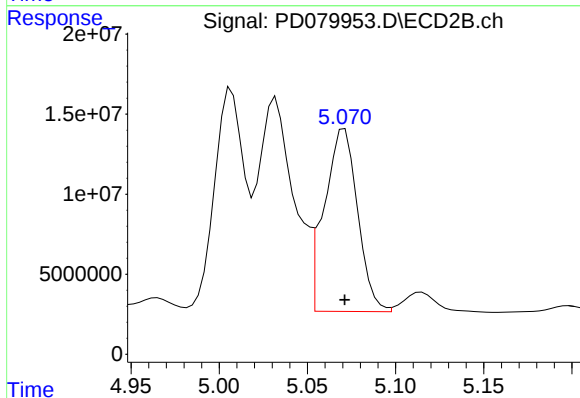


#26 Chlordane-4

R.T.: 5.071 min
Delta R.T.: 0.000 min
Response: 150083411
Conc: 500.00 ng/ml

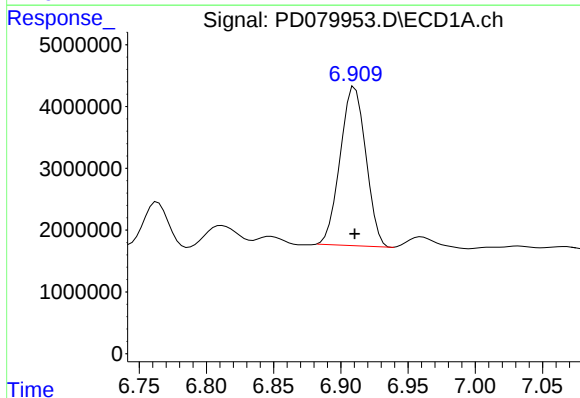


#27 Chlordane-5

R.T.: 6.910 min
Delta R.T.: 0.000 min
Response: 34074385
Conc: 500.00 ng/ml

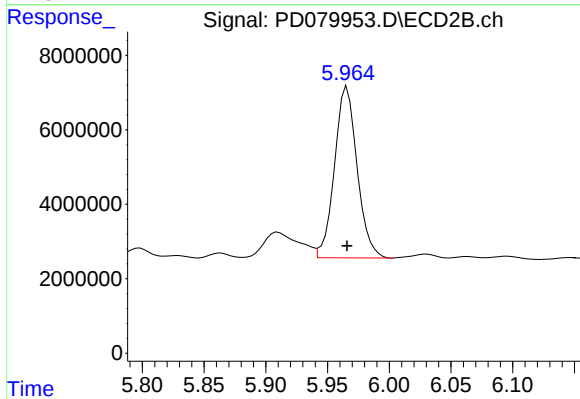

#27 Chlordane-5


R.T.: 5.966 min
Delta R.T.: 0.000 min
Response: 58642302
Conc: 500.00 ng/ml

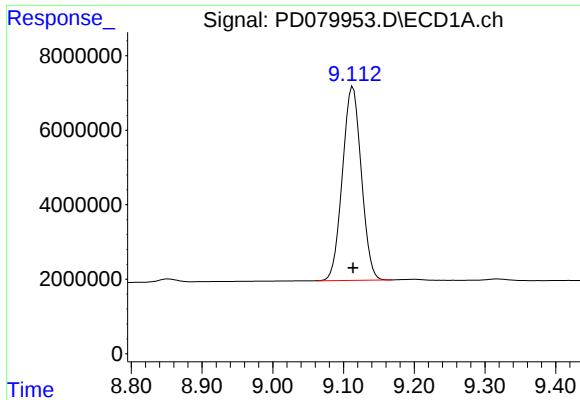

#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 96440757
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

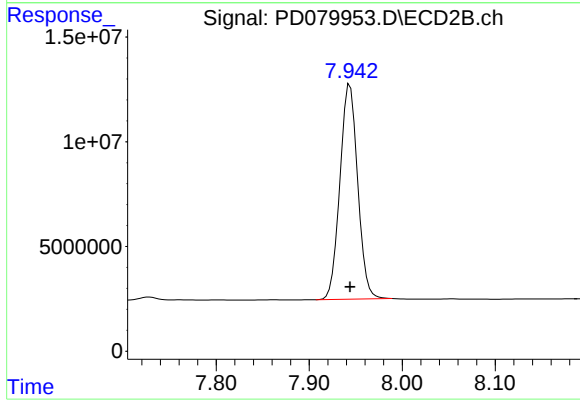

#28 Decachlorobiphenyl

R.T.: 7.944 min
Delta R.T.: 0.000 min
Response: 136349639
Conc: 50.00 ng/ml