

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR120623\
 Data File : PR064595.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2023 11:58
 Operator : AJ\MA
 Sample : 05607-13
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCB-GPC-BLANK-SPIKE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 21:44:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR112023CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 21 05:53:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.041f	0	129381	N.D.	0.023 #
Target Compounds							
3)	L1 AR-1016-1	4.948	4.156	157832	375532	0.866	1.968 #
4)	L1 AR-1016-2	4.959	4.191	403760	294762	1.506	1.111 #
5)	L1 AR-1016-3	4.959f	4.360	403760	441993	2.418	3.097 #
6)	L1 AR-1016-4	5.125	4.414	682316	230772	4.999	2.160 #
7)	L1 AR-1016-5	5.489f	4.626	918978	561978	6.939	3.913 #
8)	L2 AR-1221-1	3.986f	3.239	567167	38968	8.174	0.607 #
9)	L2 AR-1221-2	3.986	3.323	567167	76901	11.987	1.734 #
10)	L2 AR-1221-3	0.000	3.408	0	249779	N.D.	1.634 #
11)	L3 AR-1232-1	0.000	3.408	0	249779	N.D.	1.982 #
12)	L3 AR-1232-2	4.648	4.191	520682	294762	8.155	2.427 #
13)	L3 AR-1232-3	4.959	4.360	403760	441993	3.386	6.922 #
14)	L3 AR-1232-4	5.125	4.434	682316	240600	11.539	4.191 #
15)	L3 AR-1232-5	5.173f	4.626	86251	561978	1.952	9.001 #
16)	L4 AR-1242-1	4.948	4.156	157832	375532	1.030	2.311 #
17)	L4 AR-1242-2	4.959	4.191	403760	294762	1.801	1.321 #
18)	L4 AR-1242-3	4.959f	4.360	403760	441993	2.868	3.682 #
19)	L4 AR-1242-4	5.125	4.434	682316	240600	5.937	2.101 #
20)	L4 AR-1242-5	5.916	5.037	2710117	3610936	23.516	24.359
21)	L5 AR-1248-1	4.948	4.156	157832	375532	1.336	3.041 #
22)	L5 AR-1248-2	5.173f	4.414	86251	230772	0.528	1.409 #
23)	L5 AR-1248-3	5.489f	4.434	918978	240600	4.870	1.401 #
24)	L5 AR-1248-4	5.860	4.626	3611425	561978	17.666	2.705 #
25)	L5 AR-1248-5	5.916	5.037	2710117	3610936	13.387	17.442 #
26)	L6 AR-1254-1	5.860	5.037	3611425	3610936	17.785	11.661 #
27)	L6 AR-1254-2	0.000	5.175	0	1851971	N.D.	6.897 #
28)	L6 AR-1254-3	6.484	5.585	250859	3556903	0.799	8.387 #
29)	L6 AR-1254-4	6.842	5.853	507287	968187	2.350	3.665 #
30)	L6 AR-1254-5	7.264	6.308	583146	477883	2.495	1.265 #
31)	L7 AR-1260-1	6.676	5.745	106245	1468173	0.444	5.023 #
32)	L7 AR-1260-2	6.973	5.962	335738	376225	1.228	1.073
33)	L7 AR-1260-3	7.365	6.126	371229	2102121	1.868	6.241 #
34)	L7 AR-1260-4	7.585	6.624	29288	99722	0.133	0.371 #
35)	L7 AR-1260-5	7.942	6.893	1454984	1341232	3.505	2.129 #
36)	L8 AR-1262-1	7.365	6.380	371229	540601	1.290	1.393
37)	L8 AR-1262-2	7.942	6.893	1454984	1341232	3.137	1.930 #
38)	L8 AR-1262-3	8.265	7.235	356502	137269	1.155	0.552 #
39)	L8 AR-1262-4	8.347	7.279	66946	432259	0.290	0.856 #
40)	L8 AR-1262-5	9.026f	7.883f	801261	1597599	5.090	7.066 #
41)	L9 AR-1268-1	8.265	7.235	356502	137269	0.673	0.191 #
42)	L9 AR-1268-2	8.347	7.279	66946	432259	0.143	0.603 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR120623\
 Data File : PR064595.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2023 11:58
 Operator : AJ\MA
 Sample : 05607-13
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCB-GPC-BLANK-SPIKE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 21:44:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR112023CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 21 05:53:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	8.543	7.544f	469281	890693	1.145	1.456 #
44) L9	AR-1268-4	9.026	7.883f	801261	1597599	4.716	6.370 #
45) L9	AR-1268-5	0.000	8.121	0	299892	N.D.	0.165 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR120623\
Data File : PR064595.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2023 11:58
Operator : AJ\MA
Sample : 05607-13
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 21:44:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR112023CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 21 05:53:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

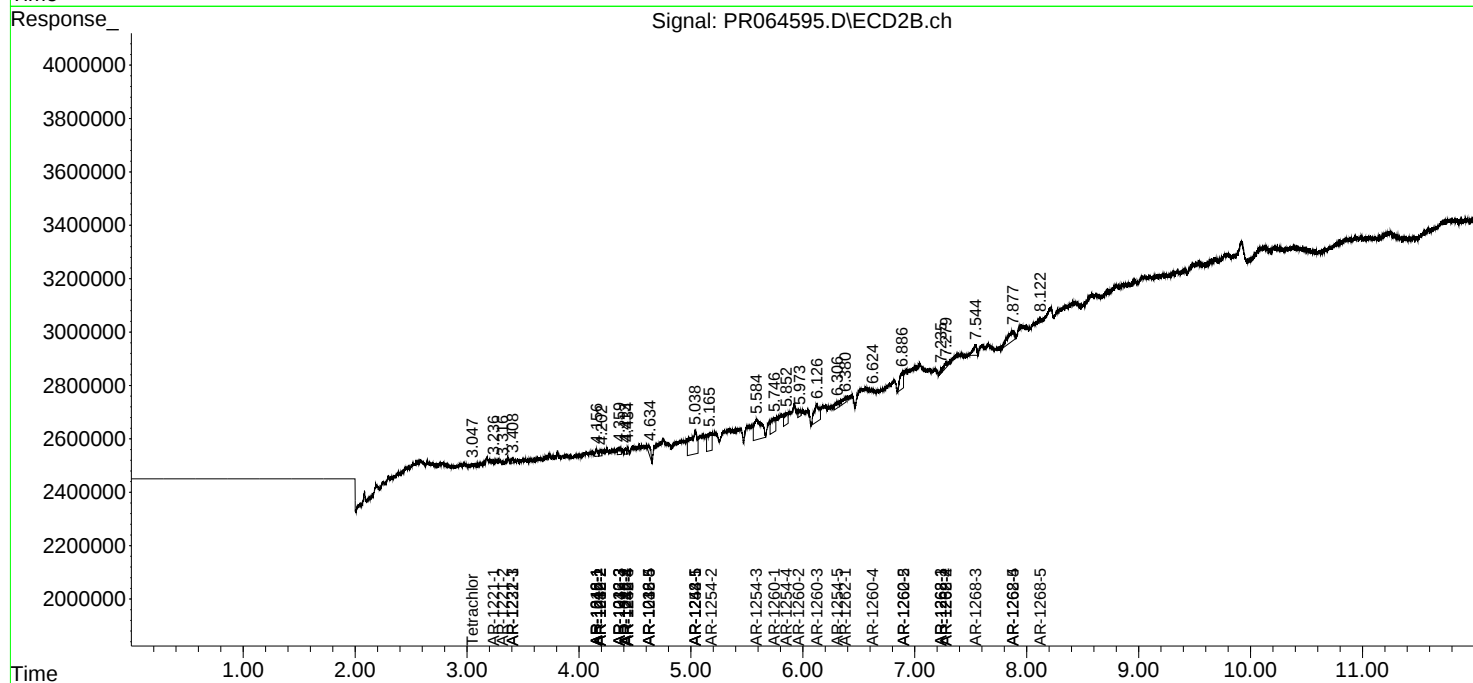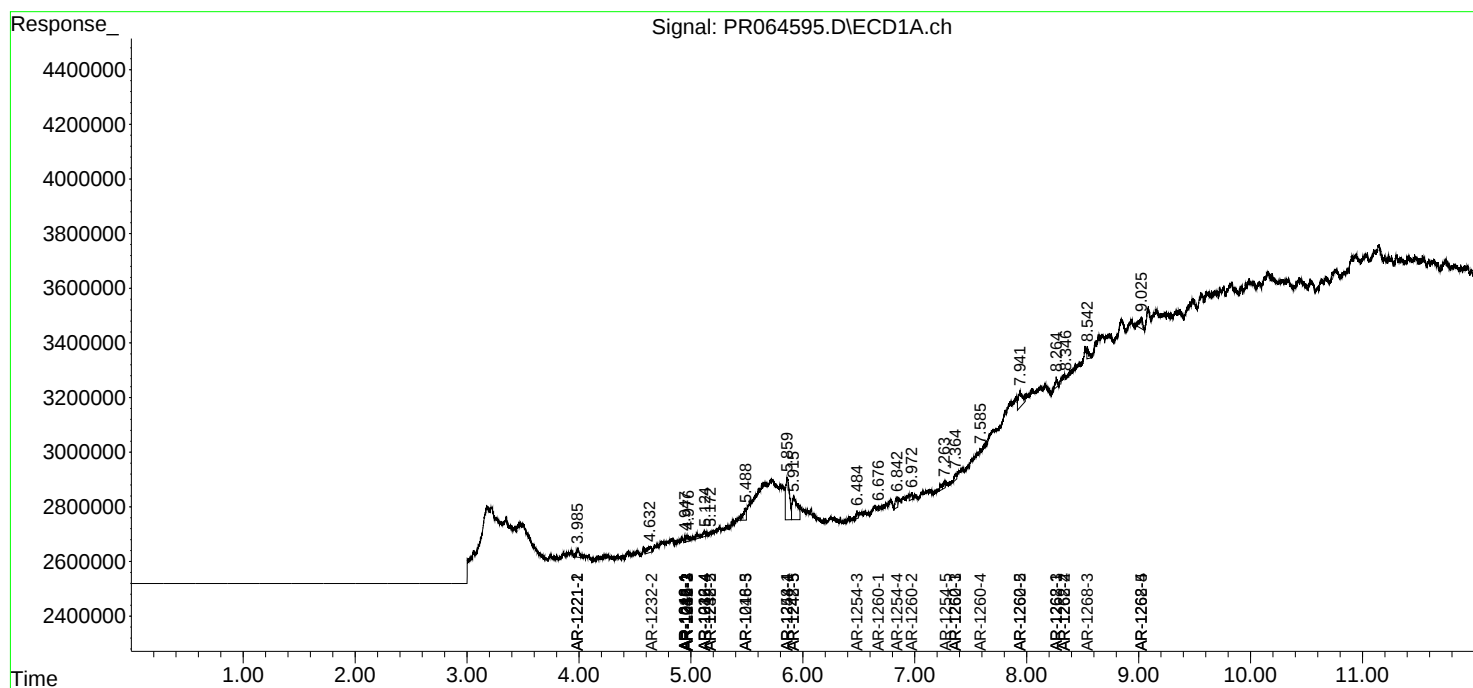


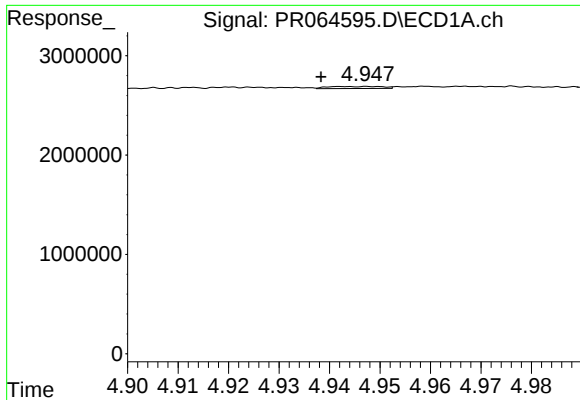

#3 AR-1016-1


R.T.: 4.948 min
Delta R.T.: 0.009 min
Response: 157832
Conc: 0.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

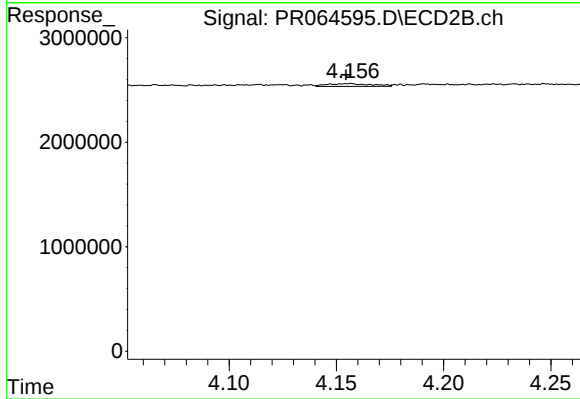


#3 AR-1016-1

R.T.: 4.156 min
Delta R.T.: 0.002 min
Response: 375532
Conc: 1.97 ng/ml

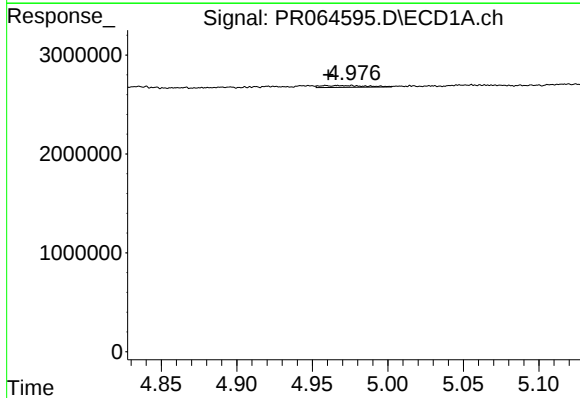


#4 AR-1016-2

R.T.: 4.959 min
Delta R.T.: -0.002 min
Response: 403760
Conc: 1.51 ng/ml

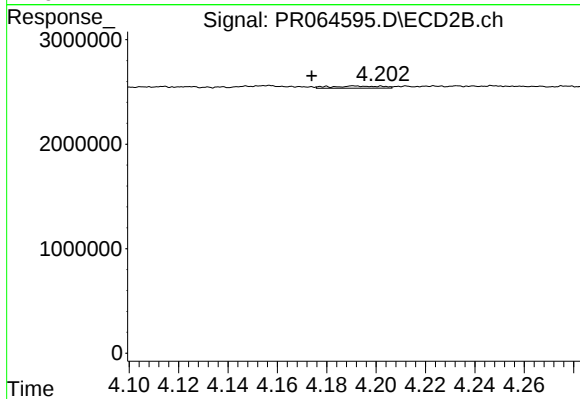

#4 AR-1016-2


R.T.: 4.191 min
Delta R.T.: 0.017 min
Response: 294762
Conc: 1.11 ng/ml

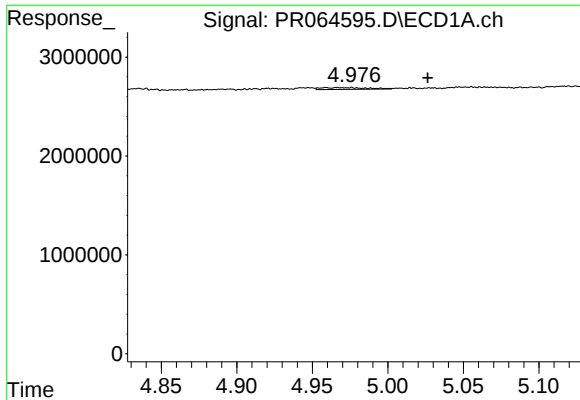

#5 AR-1016-3


R.T.: 4.959 min
Delta R.T.: -0.067 min
Response: 403760
Conc: 2.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

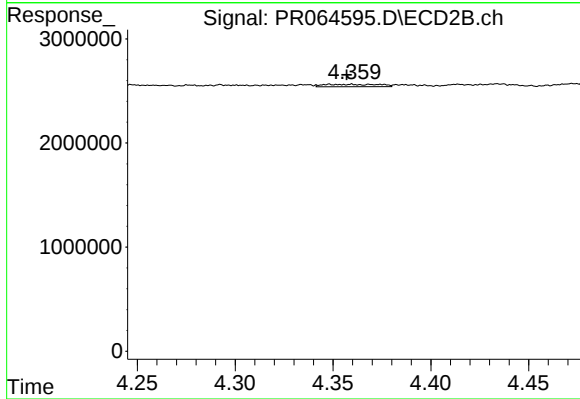


#5 AR-1016-3

R.T.: 4.360 min
Delta R.T.: 0.003 min
Response: 441993
Conc: 3.10 ng/ml

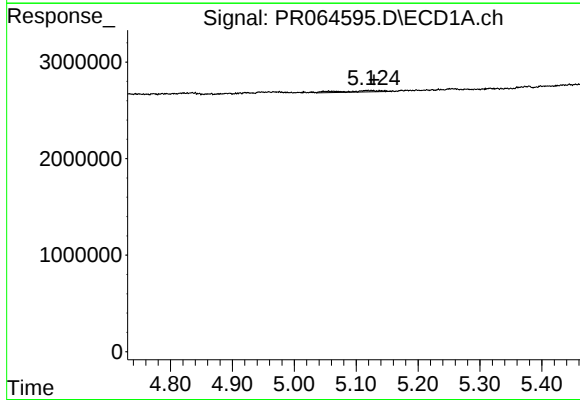


#6 AR-1016-4

R.T.: 5.125 min
Delta R.T.: -0.004 min
Response: 682316
Conc: 5.00 ng/ml

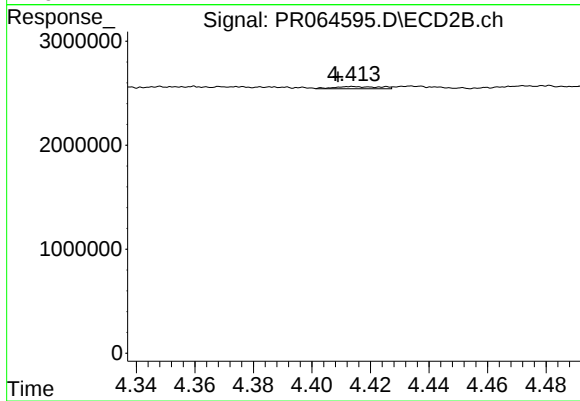

#6 AR-1016-4


R.T.: 4.414 min
Delta R.T.: 0.005 min
Response: 230772
Conc: 2.16 ng/ml

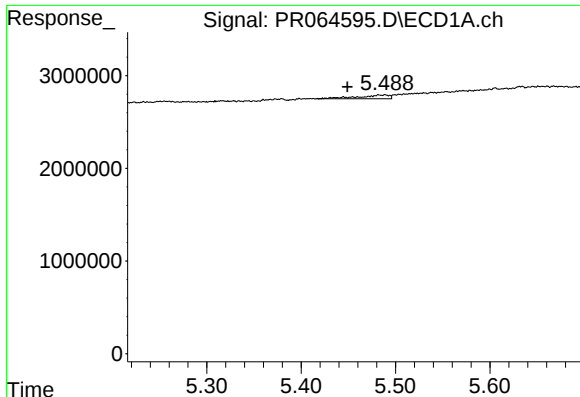

#7 AR-1016-5


R.T.: 5.489 min
Delta R.T.: 0.040 min
Response: 918978
Conc: 6.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

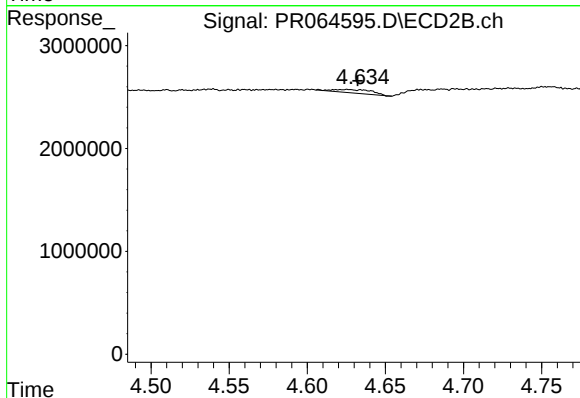


#7 AR-1016-5

R.T.: 4.626 min
Delta R.T.: -0.007 min
Response: 561978
Conc: 3.91 ng/ml

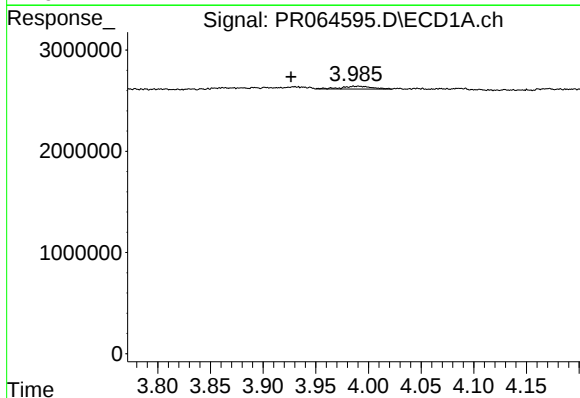


#8 AR-1221-1

R.T.: 3.986 min
Delta R.T.: 0.060 min
Response: 567167
Conc: 8.17 ng/ml

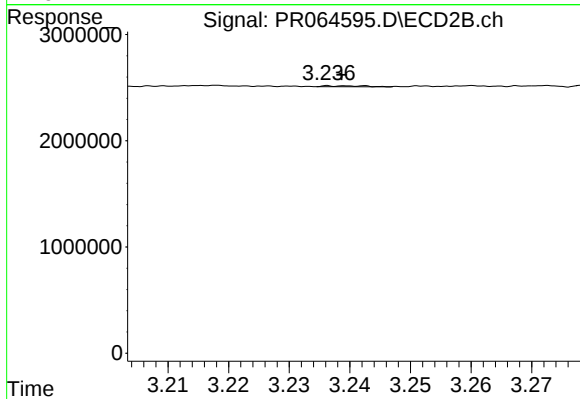

#8 AR-1221-1


R.T.: 3.239 min
Delta R.T.: 0.000 min
Response: 38968
Conc: 0.61 ng/ml

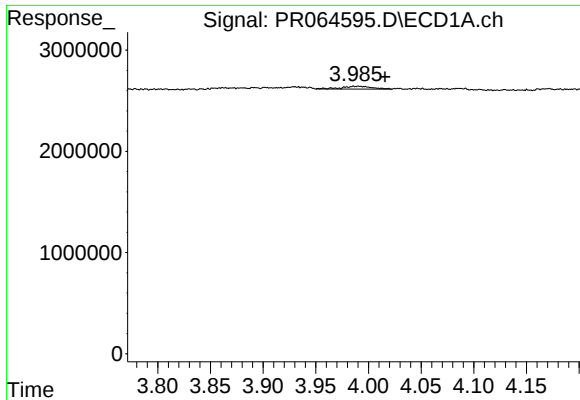

#9 AR-1221-2


R.T.: 3.986 min
Delta R.T.: -0.030 min
Response: 567167
Conc: 11.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

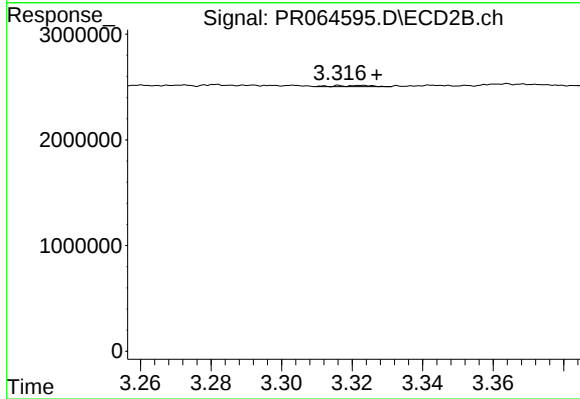


#9 AR-1221-2

R.T.: 3.323 min
Delta R.T.: -0.004 min
Response: 76901
Conc: 1.73 ng/ml

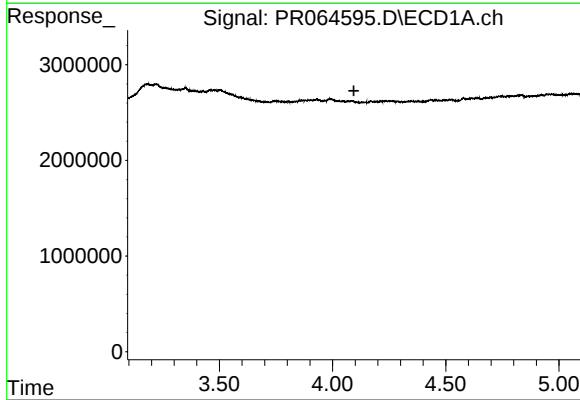


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.094 min
Response: 0
Conc: N.D.

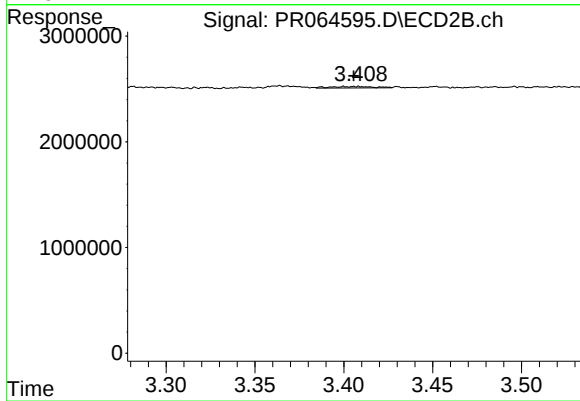

#10 AR-1221-3


R.T.: 3.408 min
Delta R.T.: 0.002 min
Response: 249779
Conc: 1.63 ng/ml

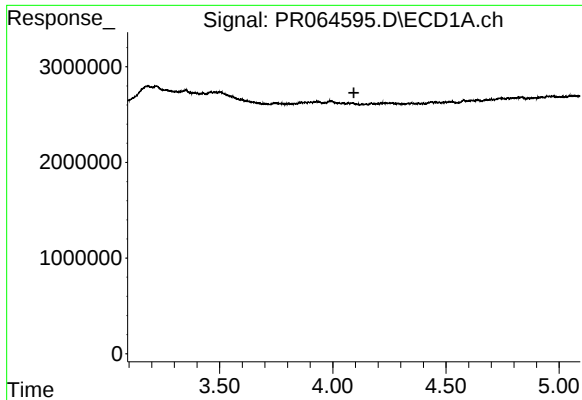

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.093 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

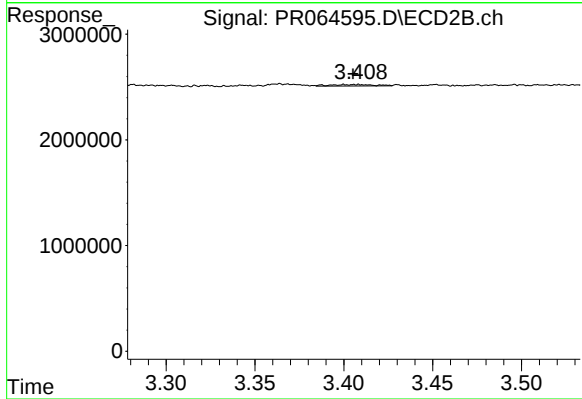


#11 AR-1232-1

R.T.: 3.408 min
Delta R.T.: 0.003 min
Response: 249779
Conc: 1.98 ng/ml

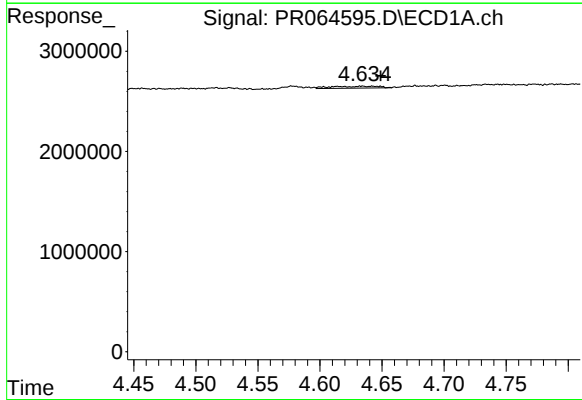


#12 AR-1232-2

R.T.: 4.648 min
Delta R.T.: 0.000 min
Response: 520682
Conc: 8.15 ng/ml

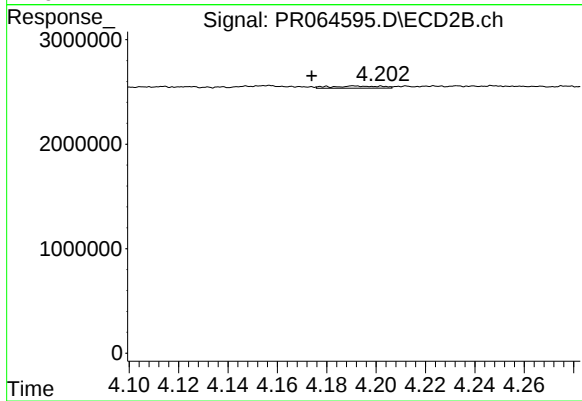

#12 AR-1232-2


R.T.: 4.191 min
Delta R.T.: 0.017 min
Response: 294762
Conc: 2.43 ng/ml

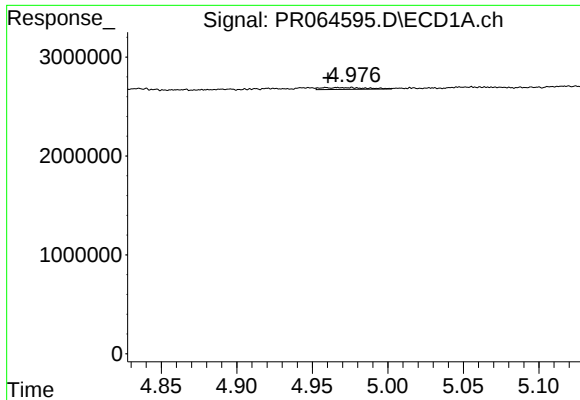

#13 AR-1232-3


R.T.: 4.959 min
Delta R.T.: -0.001 min
Response: 403760
Conc: 3.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

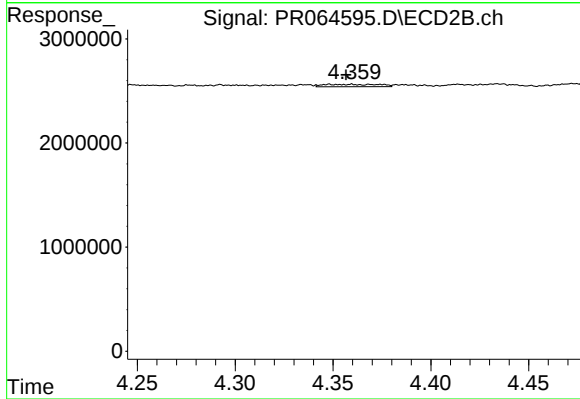


#13 AR-1232-3

R.T.: 4.360 min
Delta R.T.: 0.003 min
Response: 441993
Conc: 6.92 ng/ml

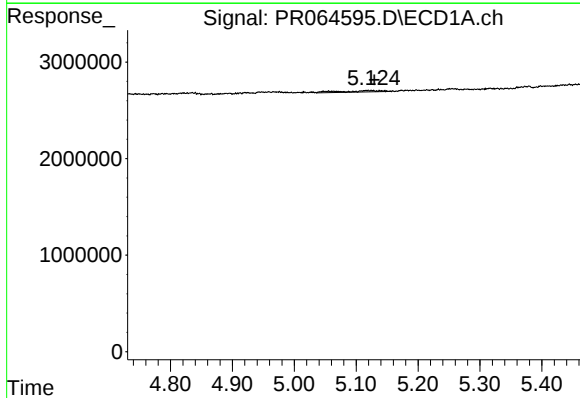


#14 AR-1232-4

R.T.: 5.125 min
Delta R.T.: -0.005 min
Response: 682316
Conc: 11.54 ng/ml

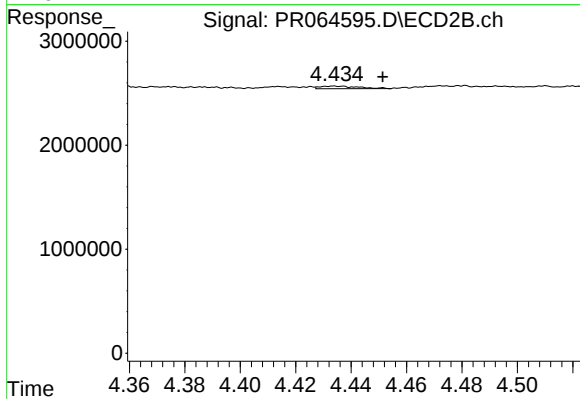

#14 AR-1232-4


R.T.: 4.434 min
Delta R.T.: -0.017 min
Response: 240600
Conc: 4.19 ng/ml

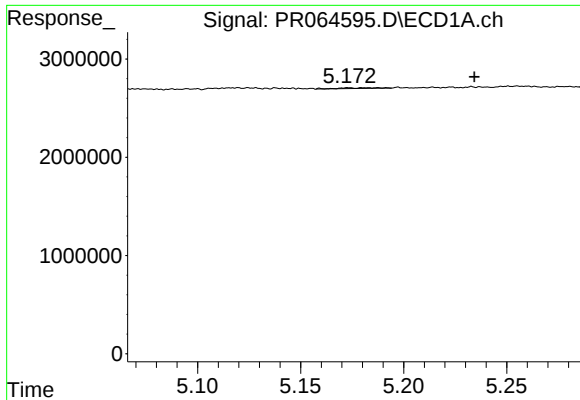

#15 AR-1232-5


R.T.: 5.173 min
Delta R.T.: -0.061 min
Response: 86251
Conc: 1.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

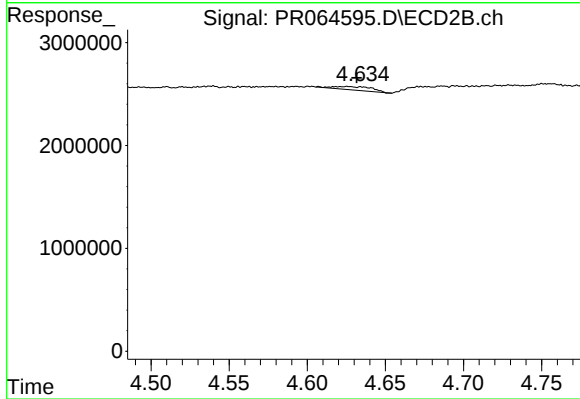


#15 AR-1232-5

R.T.: 4.626 min
Delta R.T.: -0.006 min
Response: 561978
Conc: 9.00 ng/ml

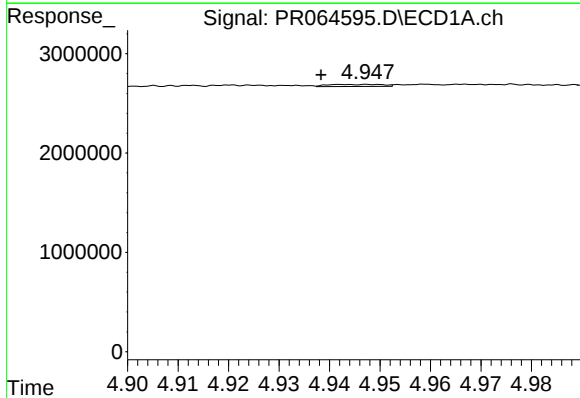


#16 AR-1242-1

R.T.: 4.948 min
Delta R.T.: 0.009 min
Response: 157832
Conc: 1.03 ng/ml

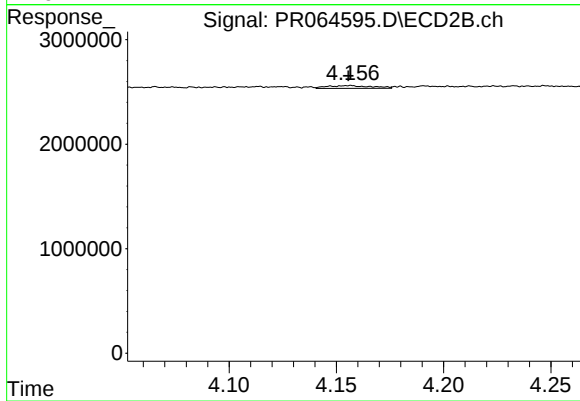

#16 AR-1242-1


R.T.: 4.156 min
Delta R.T.: 0.000 min
Response: 375532
Conc: 2.31 ng/ml

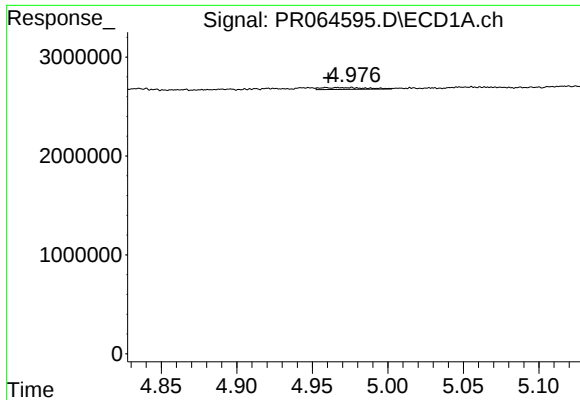

#17 AR-1242-2


R.T.: 4.959 min
Delta R.T.: -0.002 min
Response: 403760
Conc: 1.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

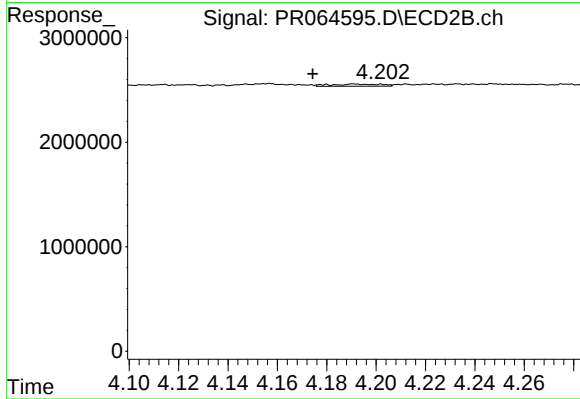


#17 AR-1242-2

R.T.: 4.191 min
Delta R.T.: 0.017 min
Response: 294762
Conc: 1.32 ng/ml

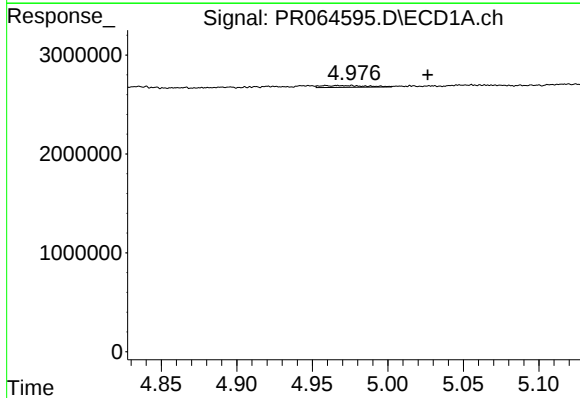


#18 AR-1242-3

R.T.: 4.959 min
Delta R.T.: -0.067 min
Response: 403760
Conc: 2.87 ng/ml

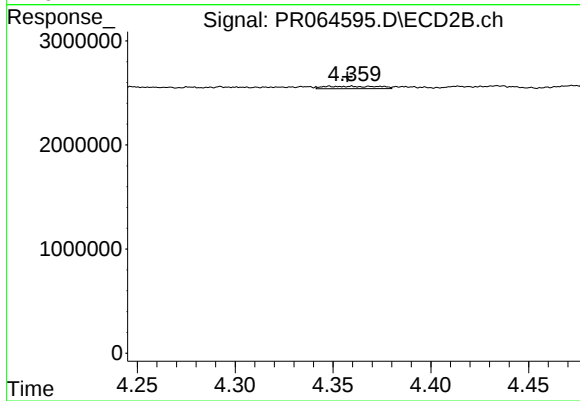

#18 AR-1242-3


R.T.: 4.360 min
Delta R.T.: 0.002 min
Response: 441993
Conc: 3.68 ng/ml

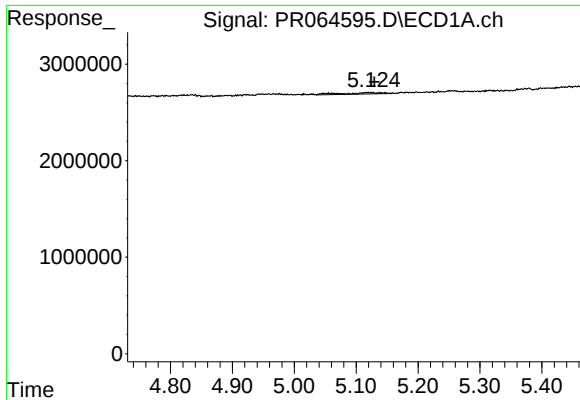

#19 AR-1242-4


R.T.: 5.125 min
Delta R.T.: -0.005 min
Response: 682316
Conc: 5.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

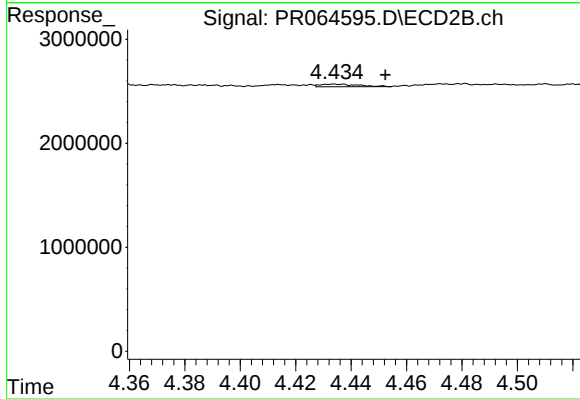


#19 AR-1242-4

R.T.: 4.434 min
Delta R.T.: -0.018 min
Response: 240600
Conc: 2.10 ng/ml

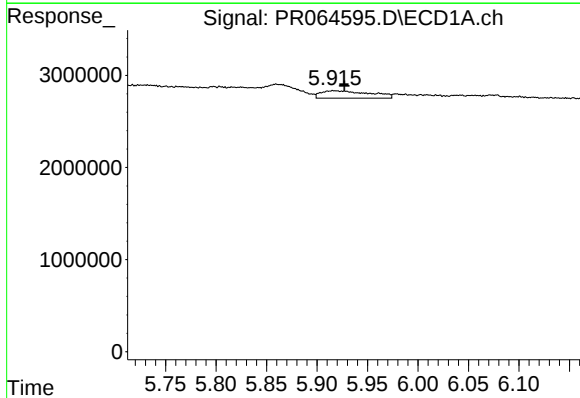


#20 AR-1242-5

R.T.: 5.916 min
Delta R.T.: -0.011 min
Response: 2710117
Conc: 23.52 ng/ml

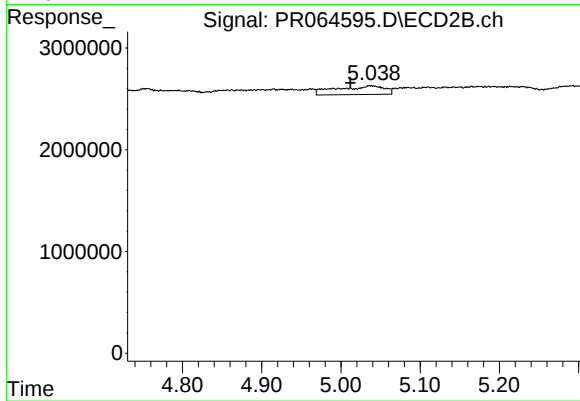

#20 AR-1242-5


R.T.: 5.037 min
Delta R.T.: 0.025 min
Response: 3610936
Conc: 24.36 ng/ml

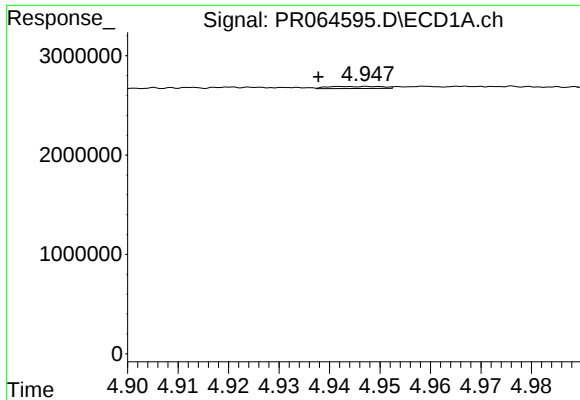

#21 AR-1248-1


R.T.: 4.948 min
Delta R.T.: 0.010 min
Response: 157832
Conc: 1.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

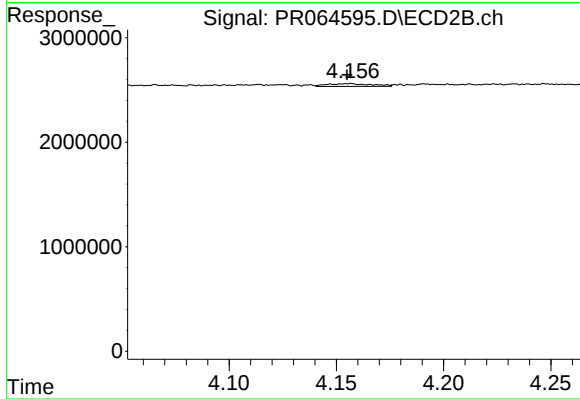


#21 AR-1248-1

R.T.: 4.156 min
Delta R.T.: 0.001 min
Response: 375532
Conc: 3.04 ng/ml

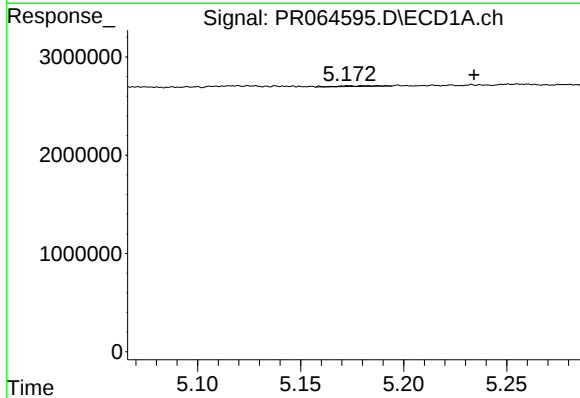


#22 AR-1248-2

R.T.: 5.173 min
Delta R.T.: -0.061 min
Response: 86251
Conc: 0.53 ng/ml

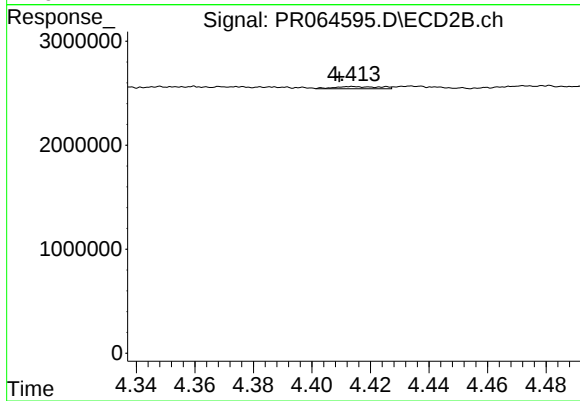

#22 AR-1248-2


R.T.: 4.414 min
Delta R.T.: 0.005 min
Response: 230772
Conc: 1.41 ng/ml

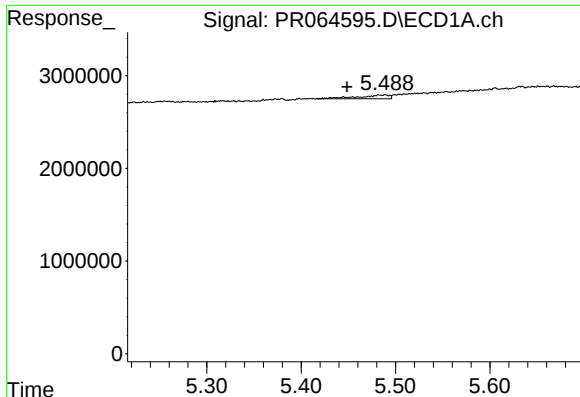

#23 AR-1248-3


R.T.: 5.489 min
Delta R.T.: 0.040 min
Response: 918978
Conc: 4.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

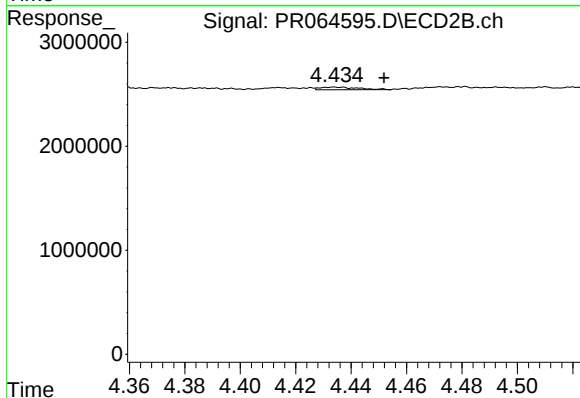


#23 AR-1248-3

R.T.: 4.434 min
Delta R.T.: -0.018 min
Response: 240600
Conc: 1.40 ng/ml

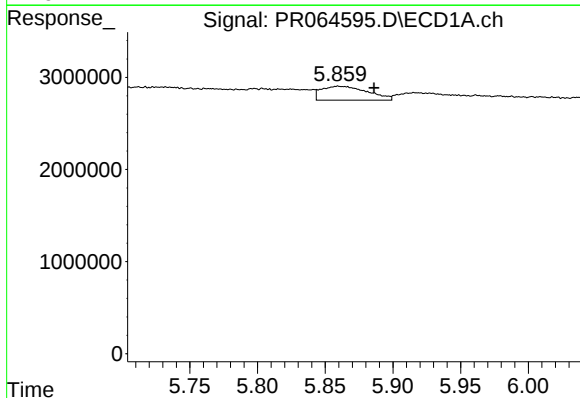


#24 AR-1248-4

R.T.: 5.860 min
Delta R.T.: -0.027 min
Response: 3611425
Conc: 17.67 ng/ml

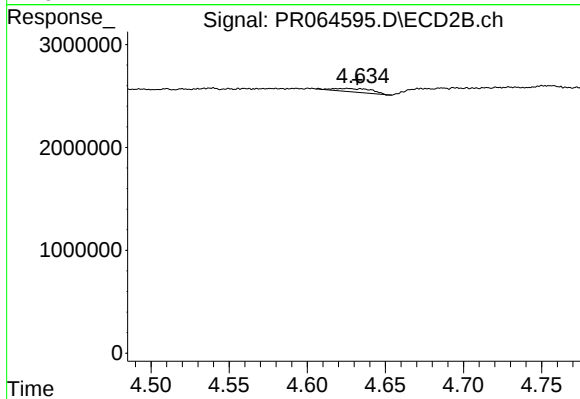

#24 AR-1248-4


R.T.: 4.626 min
Delta R.T.: -0.006 min
Response: 561978
Conc: 2.71 ng/ml

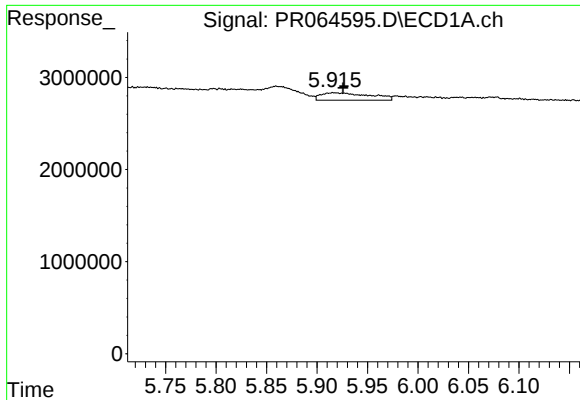

#25 AR-1248-5


R.T.: 5.916 min
Delta R.T.: -0.010 min
Response: 2710117
Conc: 13.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

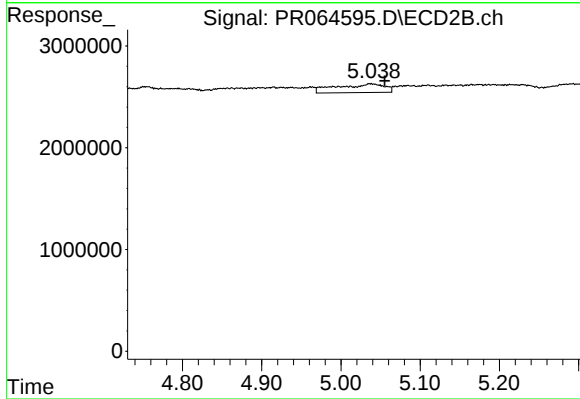


#25 AR-1248-5

R.T.: 5.037 min
Delta R.T.: -0.019 min
Response: 3610936
Conc: 17.44 ng/ml

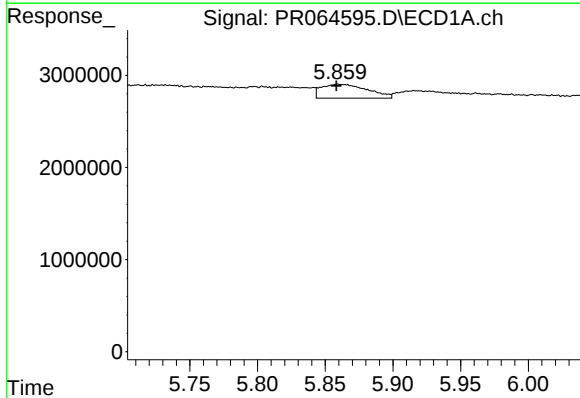


#26 AR-1254-1

R.T.: 5.860 min
Delta R.T.: 0.001 min
Response: 3611425
Conc: 17.78 ng/ml

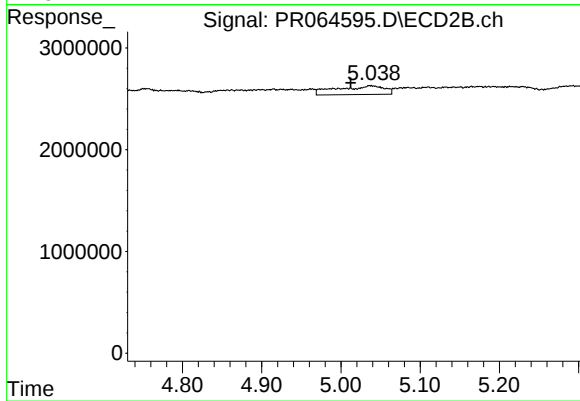

#26 AR-1254-1


R.T.: 5.037 min
Delta R.T.: 0.024 min
Response: 3610936
Conc: 11.66 ng/ml

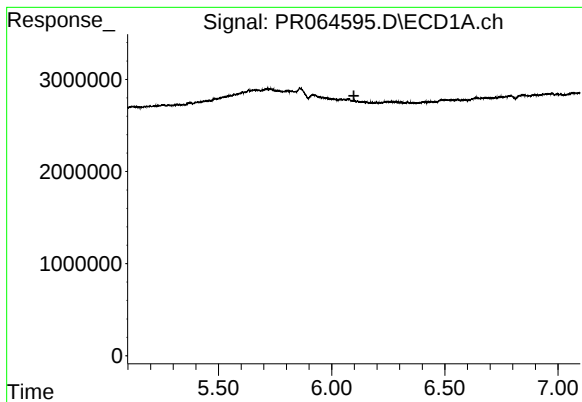

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.098 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

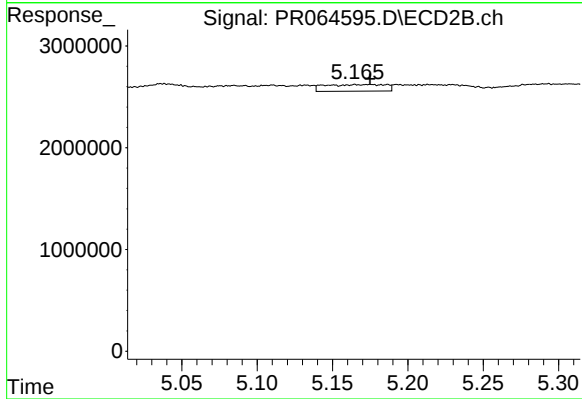


#27 AR-1254-2

R.T.: 5.175 min
Delta R.T.: 0.000 min
Response: 1851971
Conc: 6.90 ng/ml

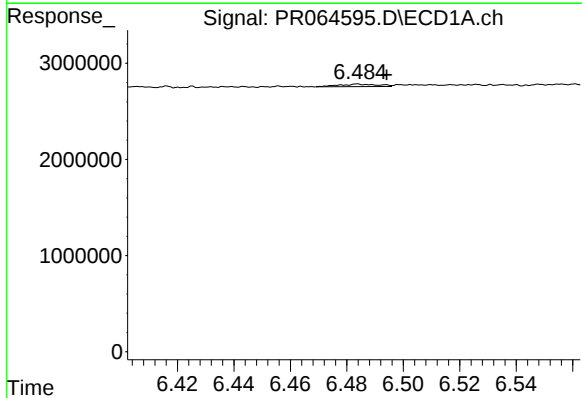


#28 AR-1254-3

R.T.: 6.484 min
Delta R.T.: -0.010 min
Response: 250859
Conc: 0.80 ng/ml

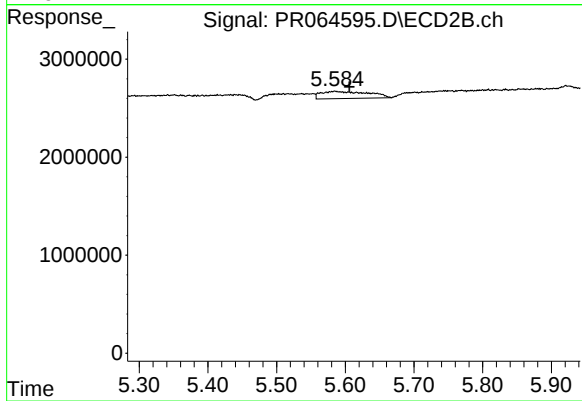

#28 AR-1254-3


R.T.: 5.585 min
Delta R.T.: -0.021 min
Response: 3556903
Conc: 8.39 ng/ml

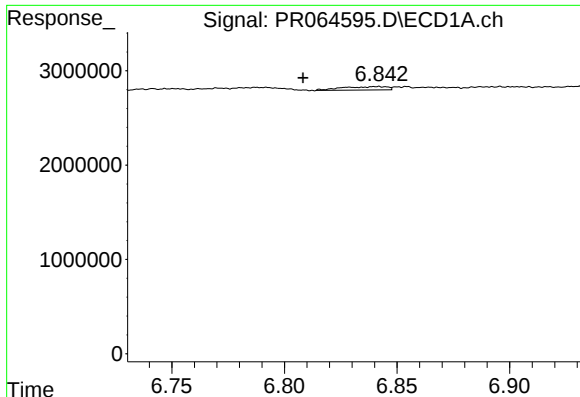

#29 AR-1254-4


R.T.: 6.842 min
Delta R.T.: 0.033 min
Response: 507287
Conc: 2.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

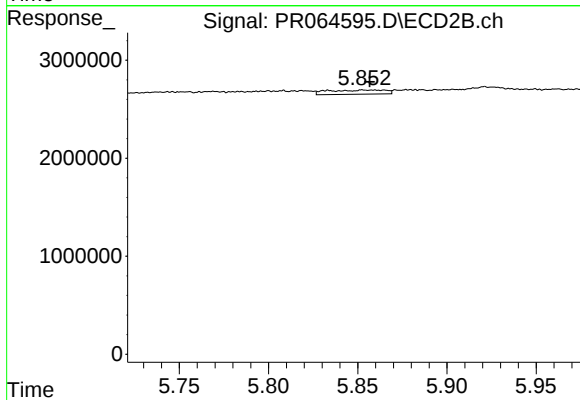


#29 AR-1254-4

R.T.: 5.853 min
Delta R.T.: -0.004 min
Response: 968187
Conc: 3.67 ng/ml

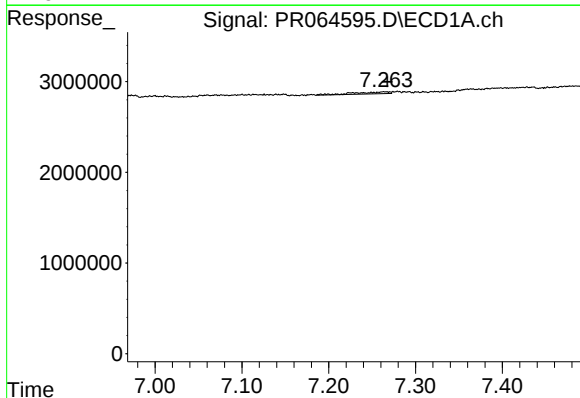


#30 AR-1254-5

R.T.: 7.264 min
Delta R.T.: -0.004 min
Response: 583146
Conc: 2.50 ng/ml

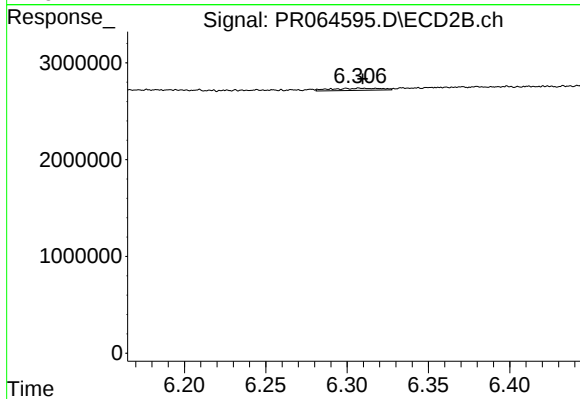

#30 AR-1254-5


R.T.: 6.308 min
Delta R.T.: -0.002 min
Response: 477883
Conc: 1.27 ng/ml

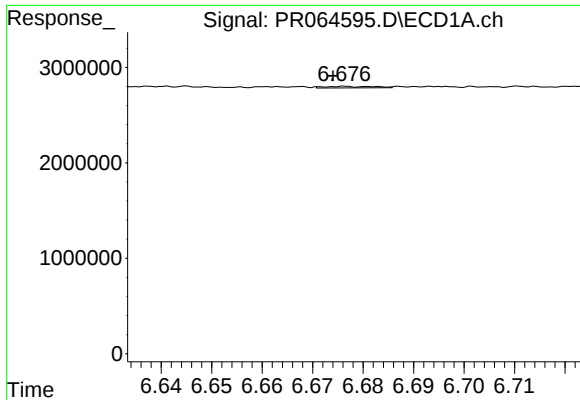

#31 AR-1260-1


R.T.: 6.676 min
Delta R.T.: 0.002 min
Response: 106245
Conc: 0.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

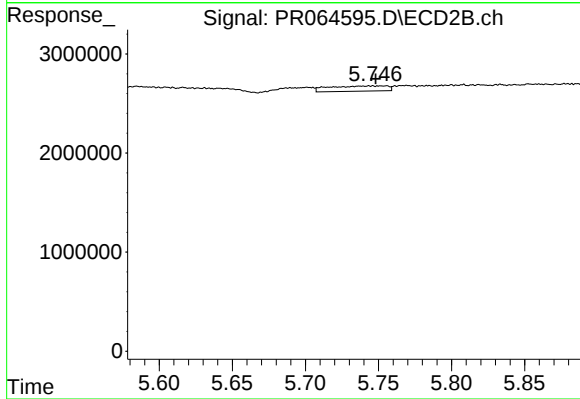


#31 AR-1260-1

R.T.: 5.745 min
Delta R.T.: -0.003 min
Response: 1468173
Conc: 5.02 ng/ml

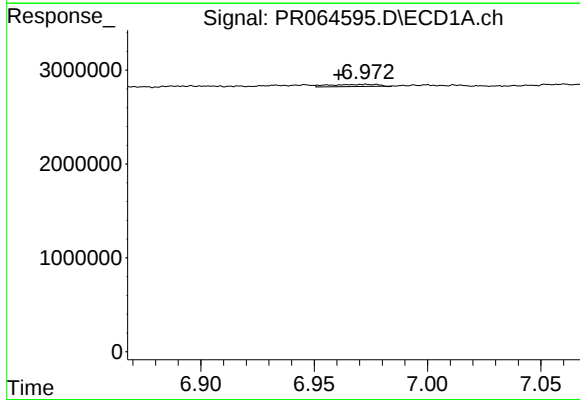


#32 AR-1260-2

R.T.: 6.973 min
Delta R.T.: 0.012 min
Response: 335738
Conc: 1.23 ng/ml

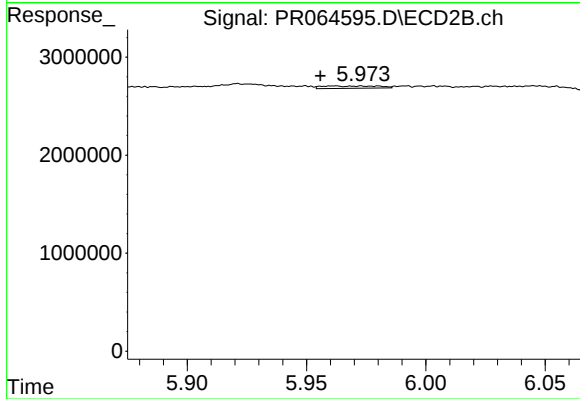

#32 AR-1260-2


R.T.: 5.962 min
Delta R.T.: 0.006 min
Response: 376225
Conc: 1.07 ng/ml

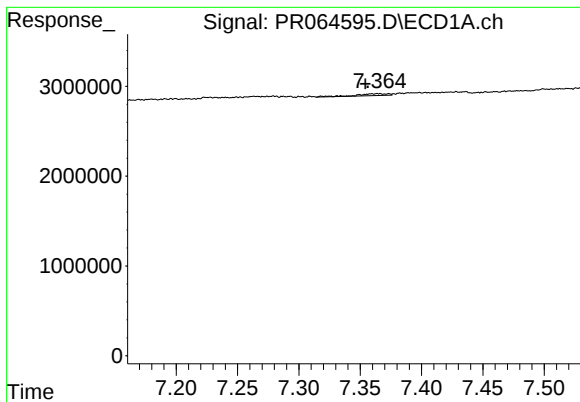

#33 AR-1260-3


R.T.: 7.365 min
Delta R.T.: 0.010 min
Response: 371229
Conc: 1.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

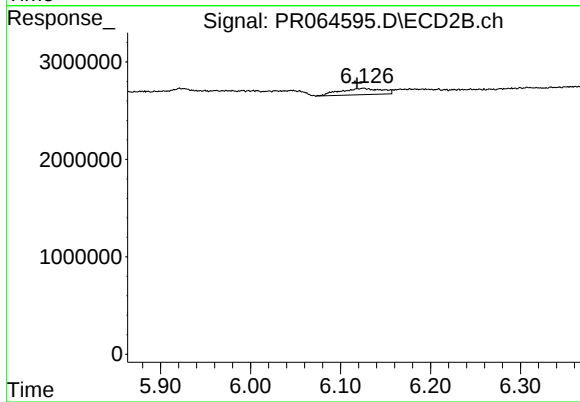


#33 AR-1260-3

R.T.: 6.126 min
Delta R.T.: 0.007 min
Response: 2102121
Conc: 6.24 ng/ml

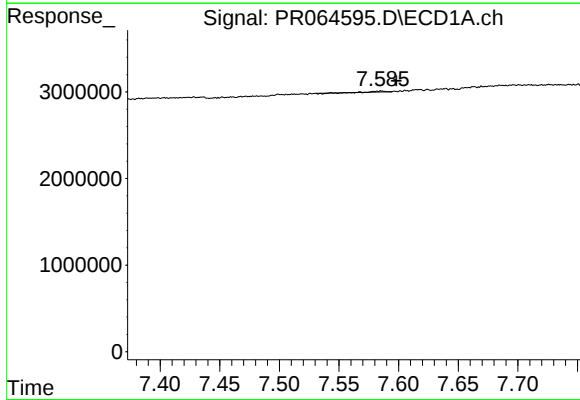


#34 AR-1260-4

R.T.: 7.585 min
Delta R.T.: -0.013 min
Response: 29288
Conc: 0.13 ng/ml

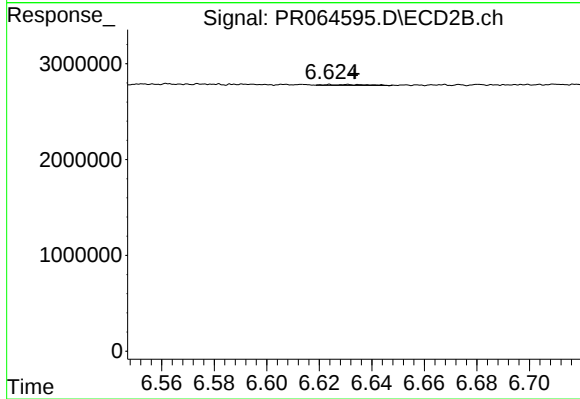

#34 AR-1260-4


R.T.: 6.624 min
Delta R.T.: -0.009 min
Response: 99722
Conc: 0.37 ng/ml

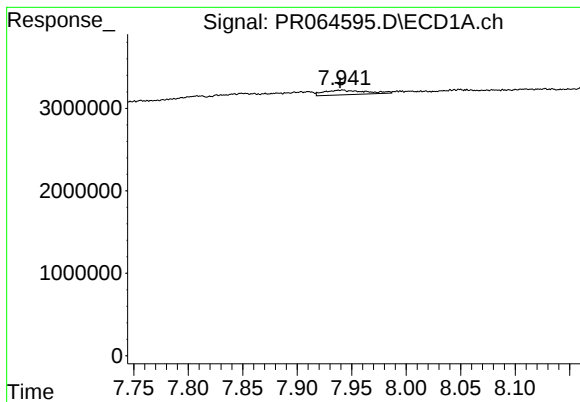

#35 AR-1260-5


R.T.: 7.942 min
Delta R.T.: 0.002 min
Response: 1454984
Conc: 3.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

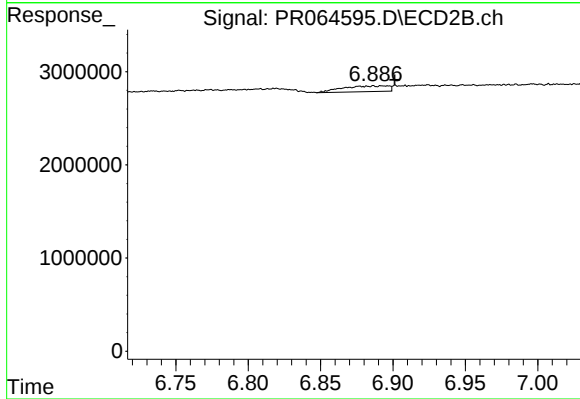


#35 AR-1260-5

R.T.: 6.893 min
Delta R.T.: -0.008 min
Response: 1341232
Conc: 2.13 ng/ml

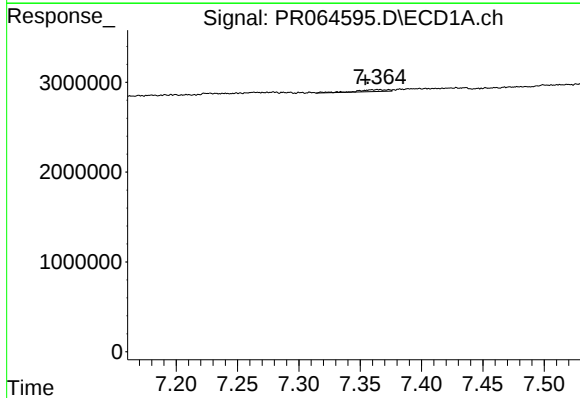


#36 AR-1262-1

R.T.: 7.365 min
Delta R.T.: 0.010 min
Response: 371229
Conc: 1.29 ng/ml

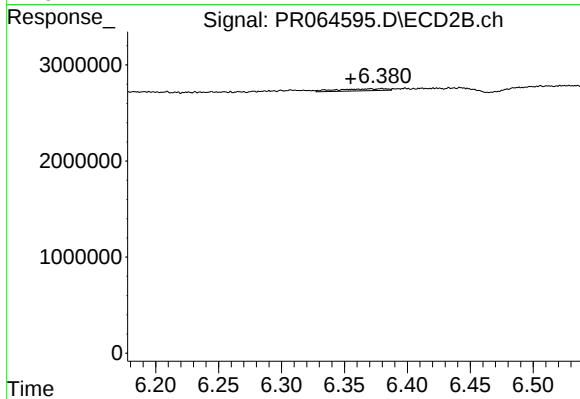

#36 AR-1262-1


R.T.: 6.380 min
Delta R.T.: 0.025 min
Response: 540601
Conc: 1.39 ng/ml

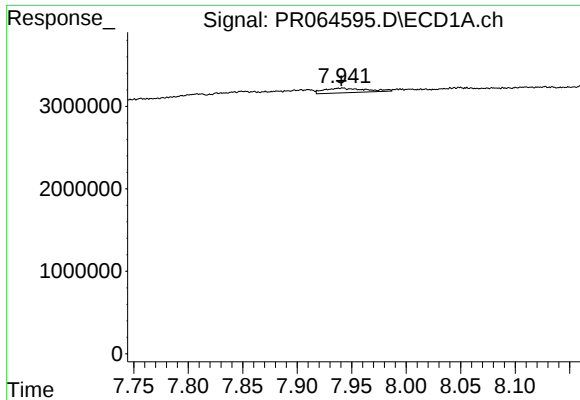

#37 AR-1262-2


R.T.: 7.942 min
Delta R.T.: 0.001 min
Response: 1454984
Conc: 3.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

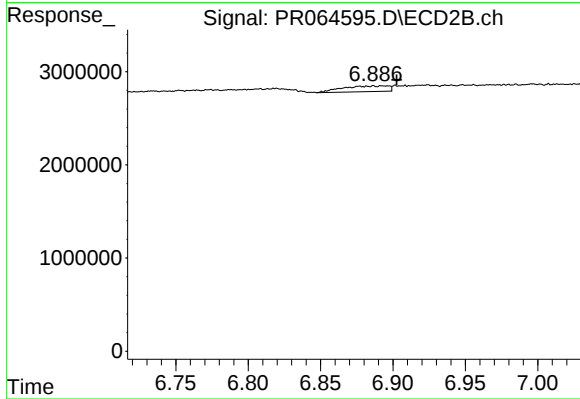


#37 AR-1262-2

R.T.: 6.893 min
Delta R.T.: -0.010 min
Response: 1341232
Conc: 1.93 ng/ml

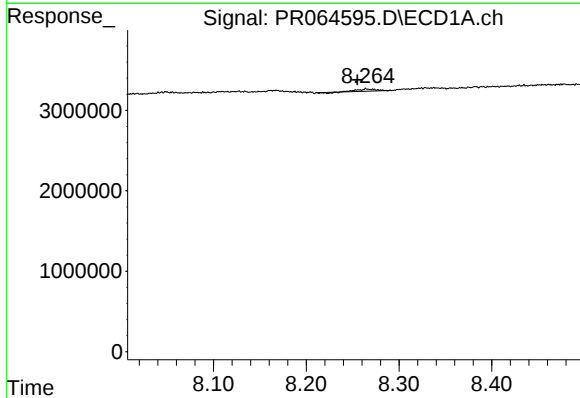


#38 AR-1262-3

R.T.: 8.265 min
Delta R.T.: 0.009 min
Response: 356502
Conc: 1.16 ng/ml

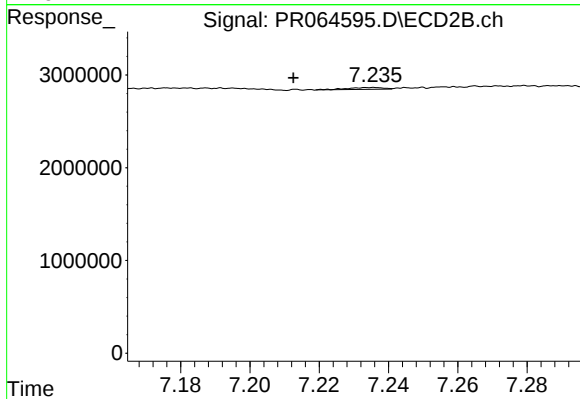

#38 AR-1262-3


R.T.: 7.235 min
Delta R.T.: 0.023 min
Response: 137269
Conc: 0.55 ng/ml

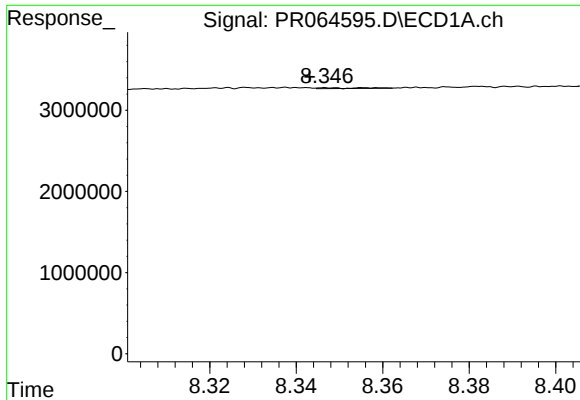

#39 AR-1262-4


R.T.: 8.347 min
Delta R.T.: 0.004 min
Response: 66946
Conc: 0.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

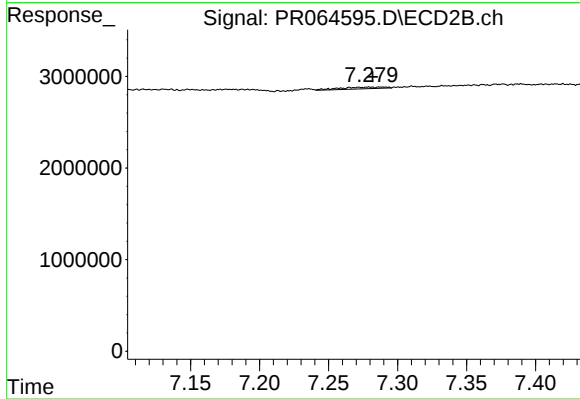


#39 AR-1262-4

R.T.: 7.279 min
Delta R.T.: -0.003 min
Response: 432259
Conc: 0.86 ng/ml

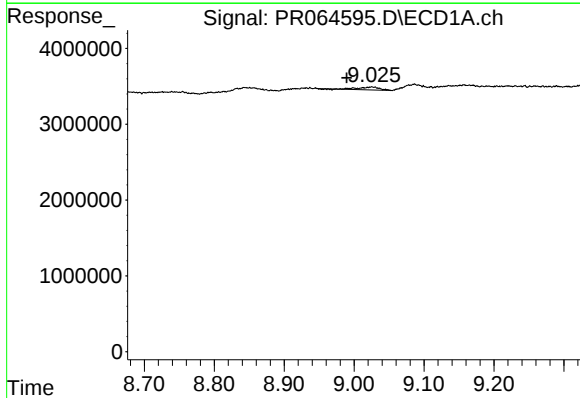


#40 AR-1262-5

R.T.: 9.026 min
Delta R.T.: 0.036 min
Response: 801261
Conc: 5.09 ng/ml

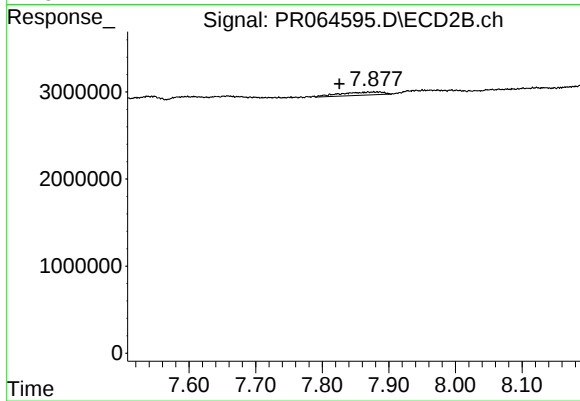

#40 AR-1262-5


R.T.: 7.883 min
Delta R.T.: 0.057 min
Response: 1597599
Conc: 7.07 ng/ml

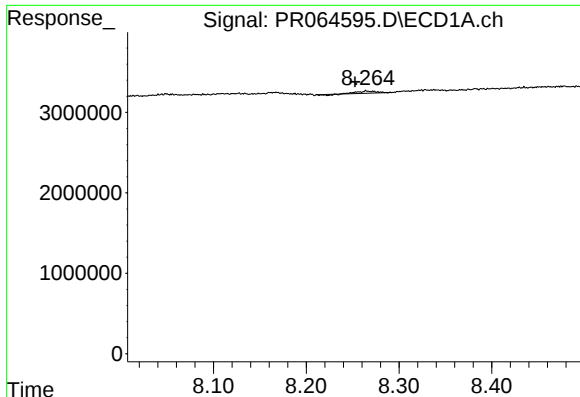

#41 AR-1268-1


R.T.: 8.265 min
Delta R.T.: 0.012 min
Response: 356502
Conc: 0.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

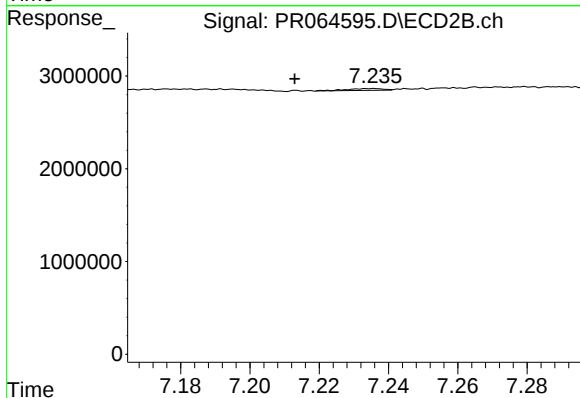


#41 AR-1268-1

R.T.: 7.235 min
Delta R.T.: 0.022 min
Response: 137269
Conc: 0.19 ng/ml

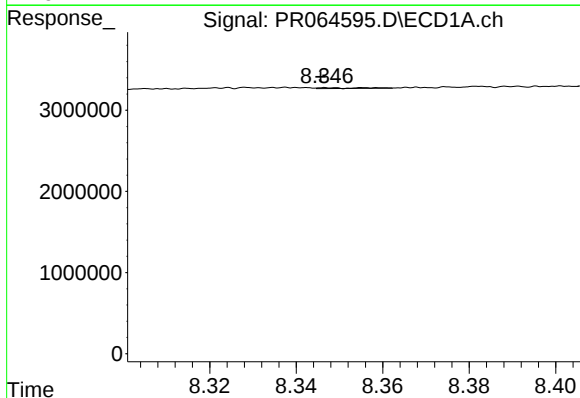


#42 AR-1268-2

R.T.: 8.347 min
Delta R.T.: 0.001 min
Response: 66946
Conc: 0.14 ng/ml

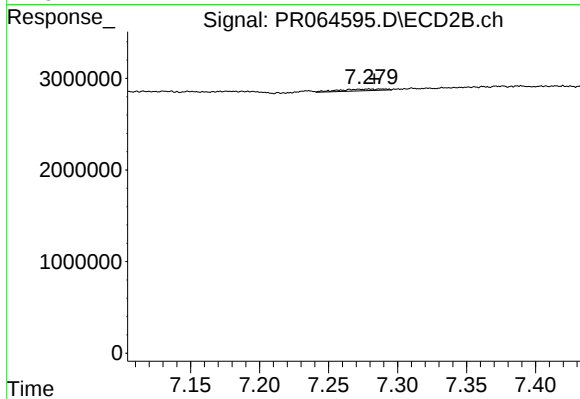

#42 AR-1268-2


R.T.: 7.279 min
Delta R.T.: -0.004 min
Response: 432259
Conc: 0.60 ng/ml

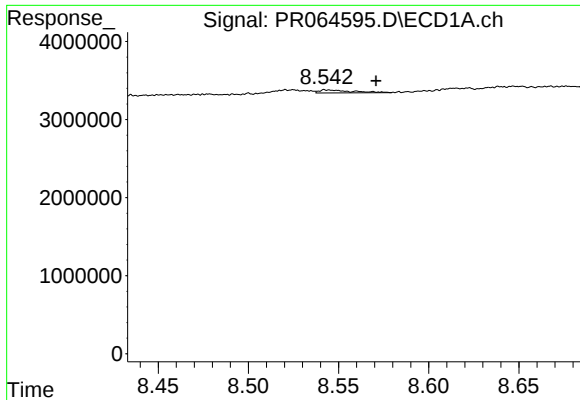

#43 AR-1268-3


R.T.: 8.543 min
Delta R.T.: -0.028 min
Response: 469281
Conc: 1.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

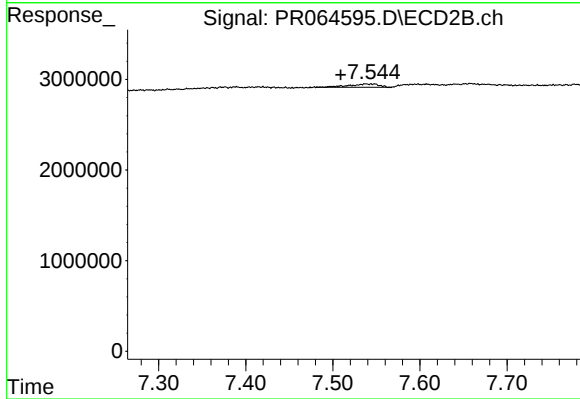


#43 AR-1268-3

R.T.: 7.544 min
Delta R.T.: 0.035 min
Response: 890693
Conc: 1.46 ng/ml

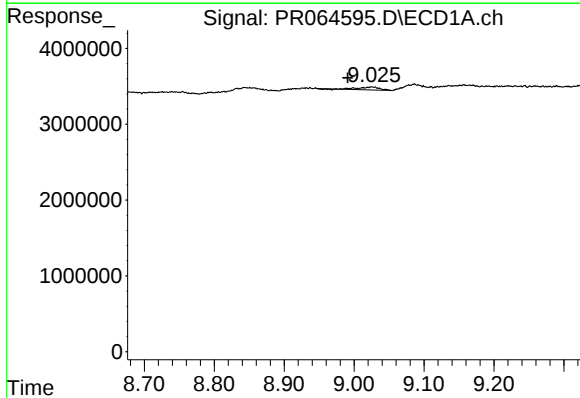


#44 AR-1268-4

R.T.: 9.026 min
Delta R.T.: 0.035 min
Response: 801261
Conc: 4.72 ng/ml

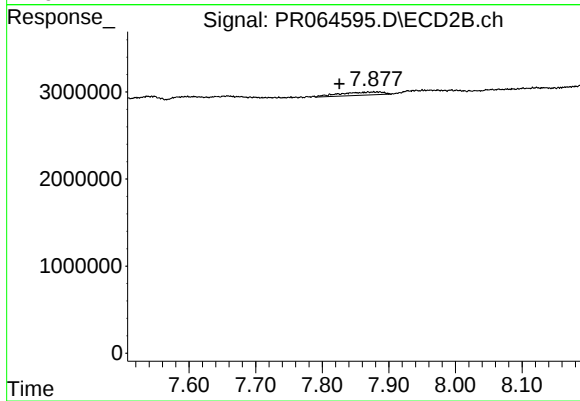

#44 AR-1268-4


R.T.: 7.883 min
Delta R.T.: 0.057 min
Response: 1597599
Conc: 6.37 ng/ml

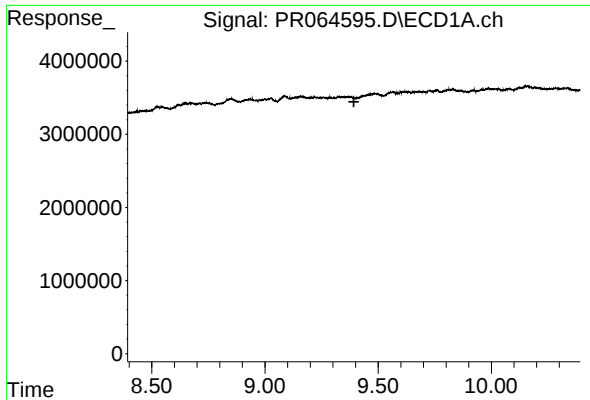

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.393 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PCB-GPC-BLANK-SPIKE

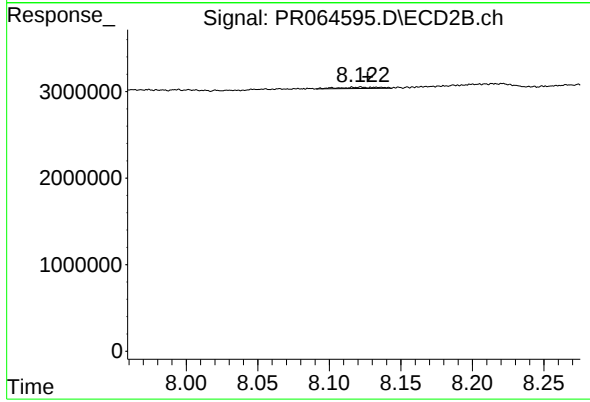

#45 AR-1268-5

R.T.: 8.121 min
Delta R.T.: -0.006 min
Response: 299892
Conc: 0.16 ng/ml