

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120623\
 Data File : PD079945.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2023 11:39
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 14:18:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 06 14:11:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.800	29684095	47689035	19.695	18.971
28)	SA Decachlor...	9.114	7.943	40367565	55215901	19.943	19.588
Target Compounds							
9)	A Endosulfan I	6.106	5.126	21193637	29430627	10.307	9.748
10)	B gamma-Chl...	5.975	5.006	22901846	32332822	10.520	10.030
12)	B 4,4'-DDE	6.226	5.259	39663958	58562309	19.781	19.428
13)	MA Dieldrin	6.382	5.391	42781774	63119600	19.608	19.277
19)	B Endosulfa...	7.194	6.360	37955045	52602103	20.017	19.620
20)	A Methoxychlor	7.533	6.639	92495803	138.4E6	93.582	94.650
21)	B Endrin ke...	7.681	6.867	41329820	60973816	19.961	19.510



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120623\
Data File : PD079945.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2023 11:39
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 14:18:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
Quant Title : GC Extractables
QLast Update : Wed Dec 06 14:11:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

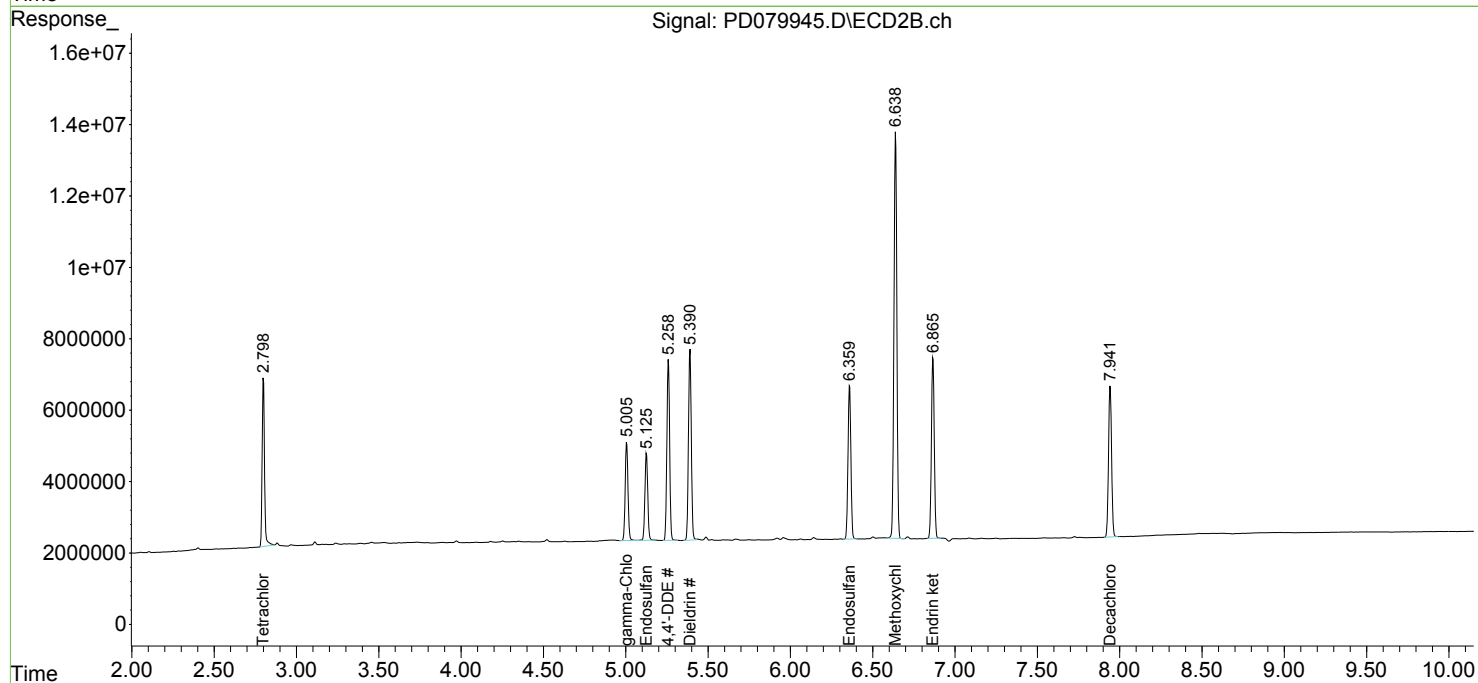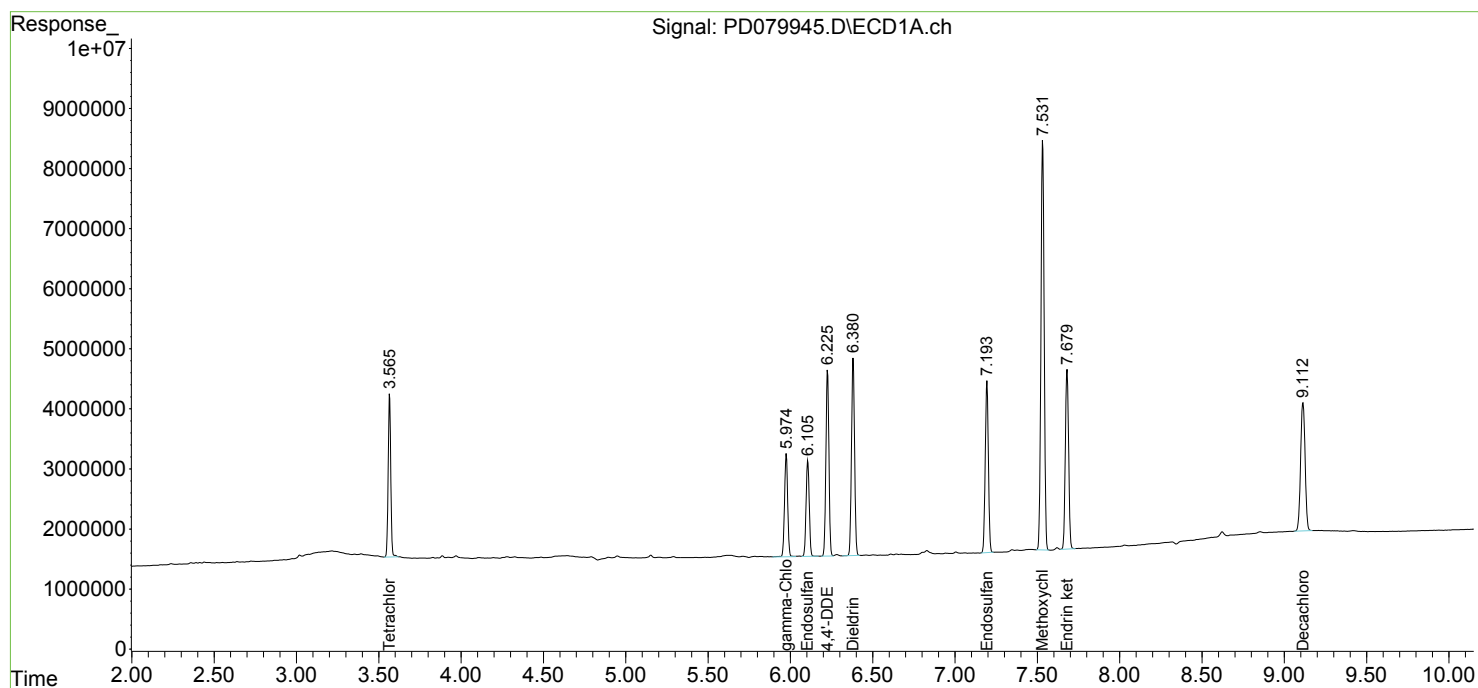


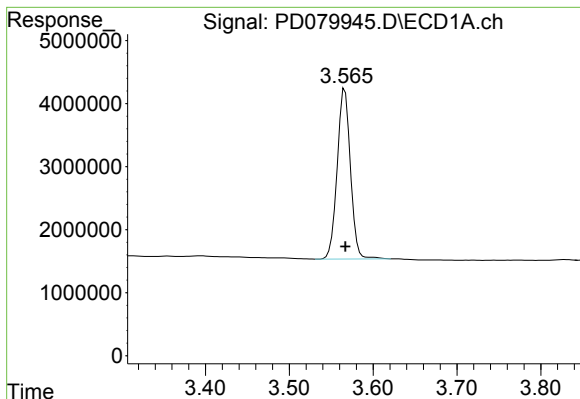

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 29684095
Conc: 19.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

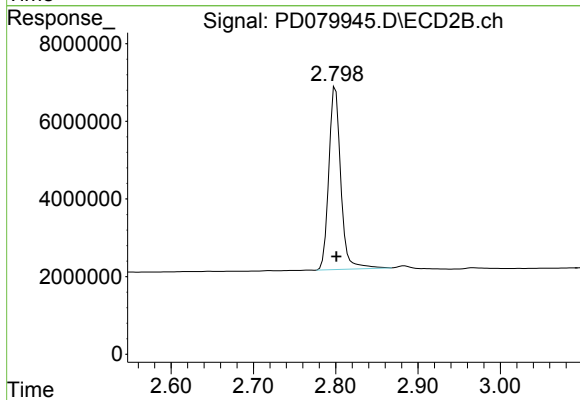


#1 Tetrachloro-m-xylene

R.T.: 2.800 min
Delta R.T.: 0.000 min
Response: 47689035
Conc: 18.97 ng/ml

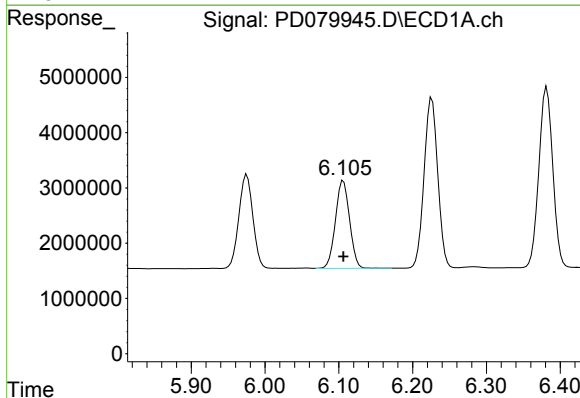


#9 Endosulfan I

R.T.: 6.106 min
Delta R.T.: 0.000 min
Response: 21193637
Conc: 10.31 ng/ml

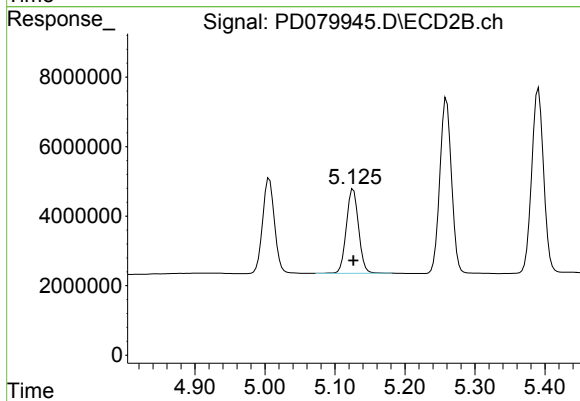

#9 Endosulfan I


R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 29430627
Conc: 9.75 ng/ml

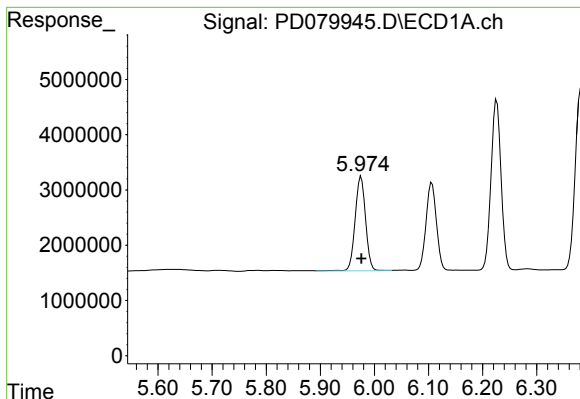

#10 gamma-Chlordane


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 22901846
Conc: 10.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

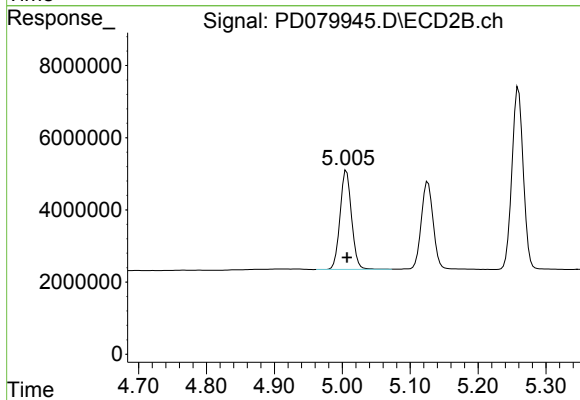


#10 gamma-Chlordane

R.T.: 5.006 min
Delta R.T.: 0.000 min
Response: 32332822
Conc: 10.03 ng/ml

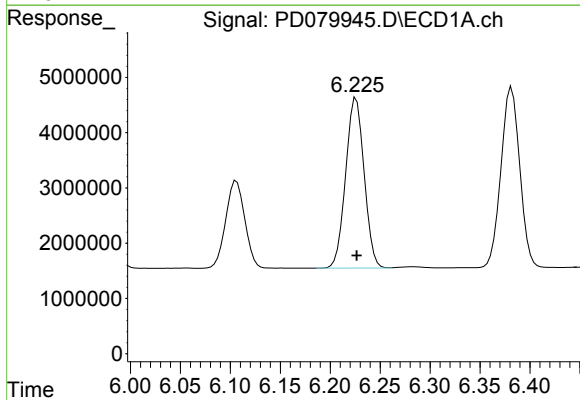


#12 4,4'-DDE

R.T.: 6.226 min
Delta R.T.: 0.000 min
Response: 39663958
Conc: 19.78 ng/ml

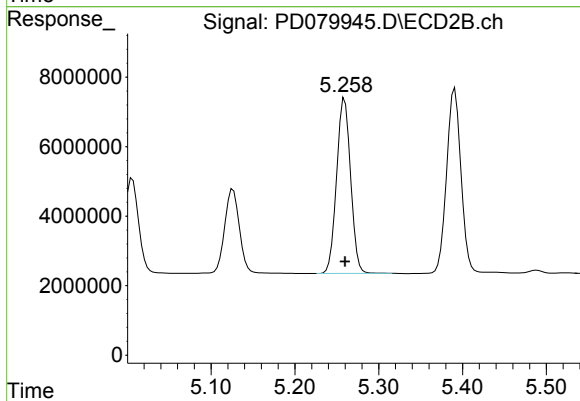

#12 4,4'-DDE


R.T.: 5.259 min
Delta R.T.: 0.000 min
Response: 58562309
Conc: 19.43 ng/ml

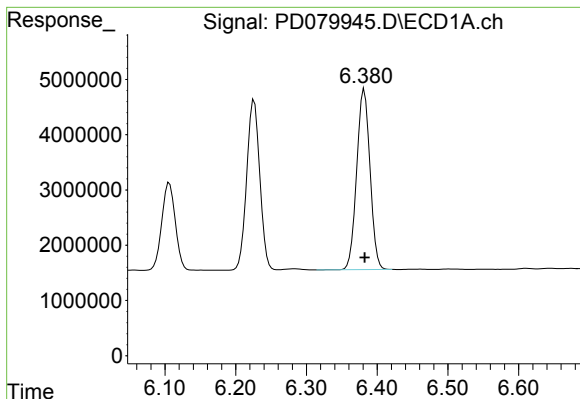

#13 Dieldrin


R.T.: 6.382 min
Delta R.T.: 0.000 min
Response: 42781774
Conc: 19.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

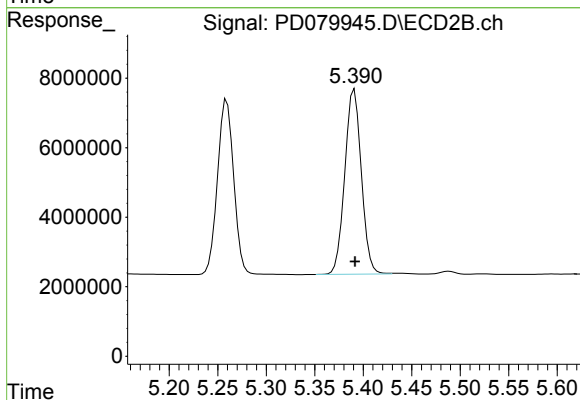


#13 Dieldrin

R.T.: 5.391 min
Delta R.T.: 0.000 min
Response: 63119600
Conc: 19.28 ng/ml

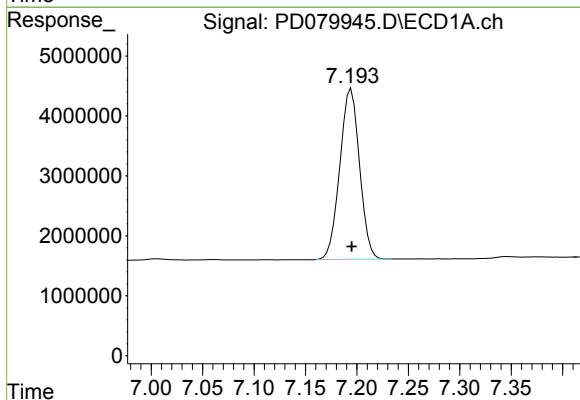


#19 Endosulfan Sulfate

R.T.: 7.194 min
Delta R.T.: 0.000 min
Response: 37955045
Conc: 20.02 ng/ml

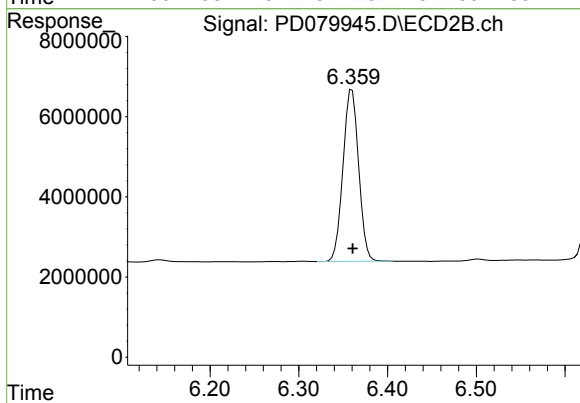

#19 Endosulfan Sulfate


R.T.: 6.360 min
Delta R.T.: 0.000 min
Response: 52602103
Conc: 19.62 ng/ml

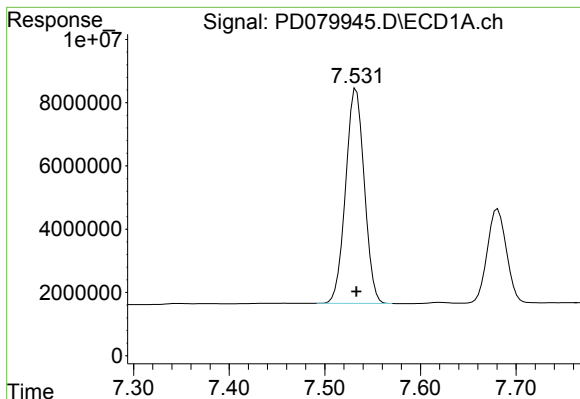

#20 Methoxychlor


R.T.: 7.533 min
Delta R.T.: 0.000 min
Response: 92495803
Conc: 93.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

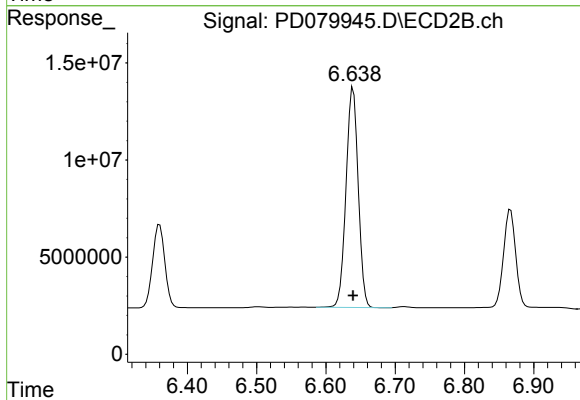


#20 Methoxychlor

R.T.: 6.639 min
Delta R.T.: 0.000 min
Response: 138408126
Conc: 94.65 ng/ml

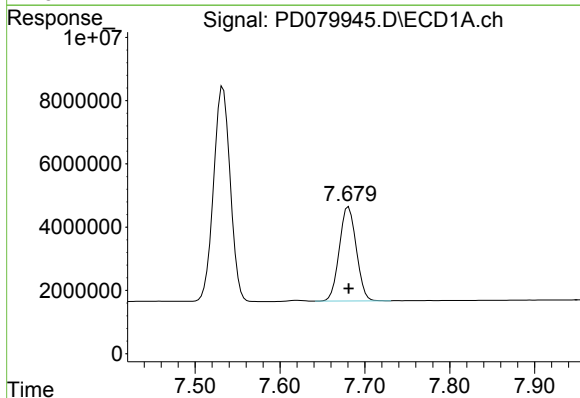


#21 Endrin ketone

R.T.: 7.681 min
Delta R.T.: 0.000 min
Response: 41329820
Conc: 19.96 ng/ml

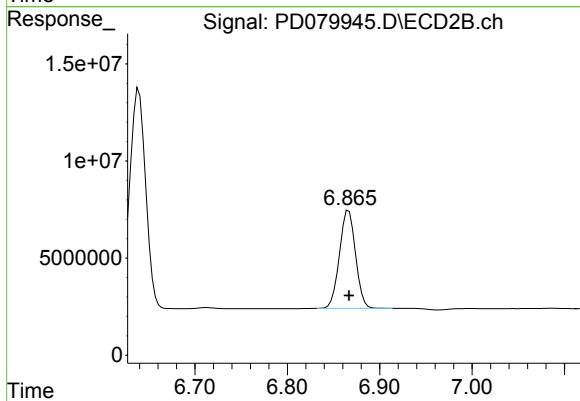

#21 Endrin ketone


R.T.: 6.867 min
Delta R.T.: 0.000 min
Response: 60973816
Conc: 19.51 ng/ml

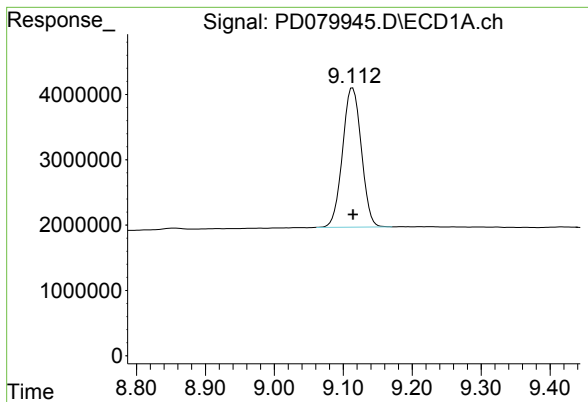

#28 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: 0.000 min
Response: 40367565
Conc: 19.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

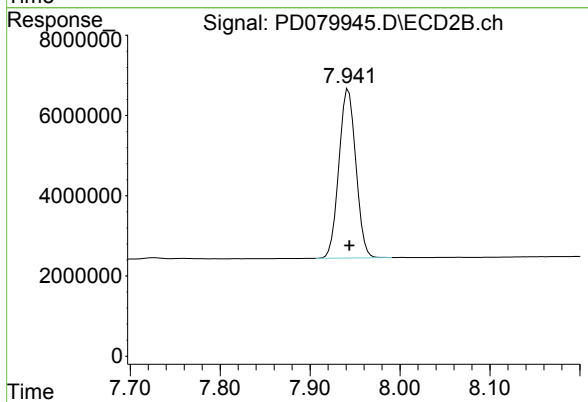

#28 Decachlorobiphenyl

R.T.: 7.943 min
Delta R.T.: -0.001 min
Response: 55215901
Conc: 19.59 ng/ml