

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120623\
 Data File : PD079982.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2023 19:52
 Operator : AR\AJ
 Sample : 05620-01 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 OILY-WATER-TOTE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/07/2023
 Supervised By :Ankita Jodhani 12/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 21:50:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 06 14:11:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.564	2.795	1263066	2795082	0.838m	1.112m#
2) SA Decachlor...	9.112	7.936	604471	6345731	0.299m	2.251 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120623\
Data File : PD079982.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2023 19:52
Operator : AR\AJ
Sample : 05620-01 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
OILY-WATER-TOTE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/07/2023
Supervised By :Ankita Jodhani 12/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 21:50:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
Quant Title : GC Extractables
QLast Update : Wed Dec 06 14:11:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

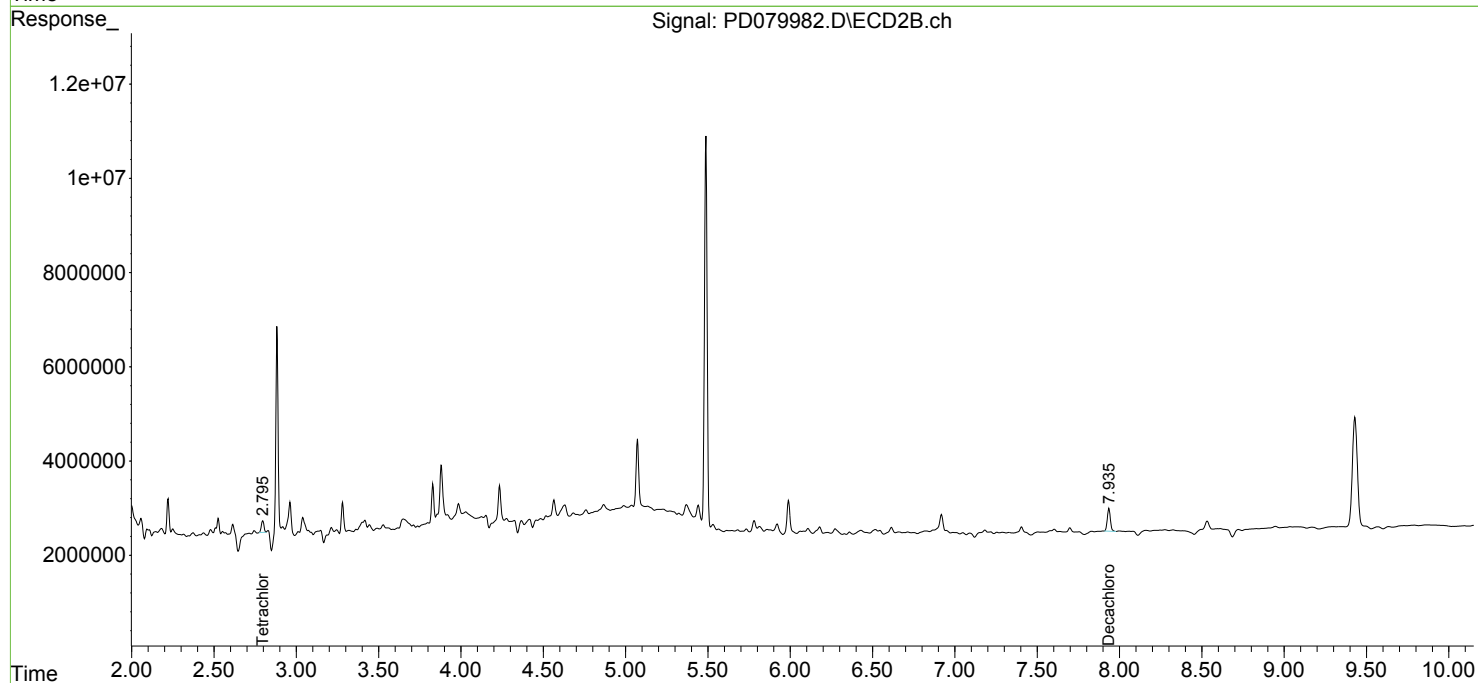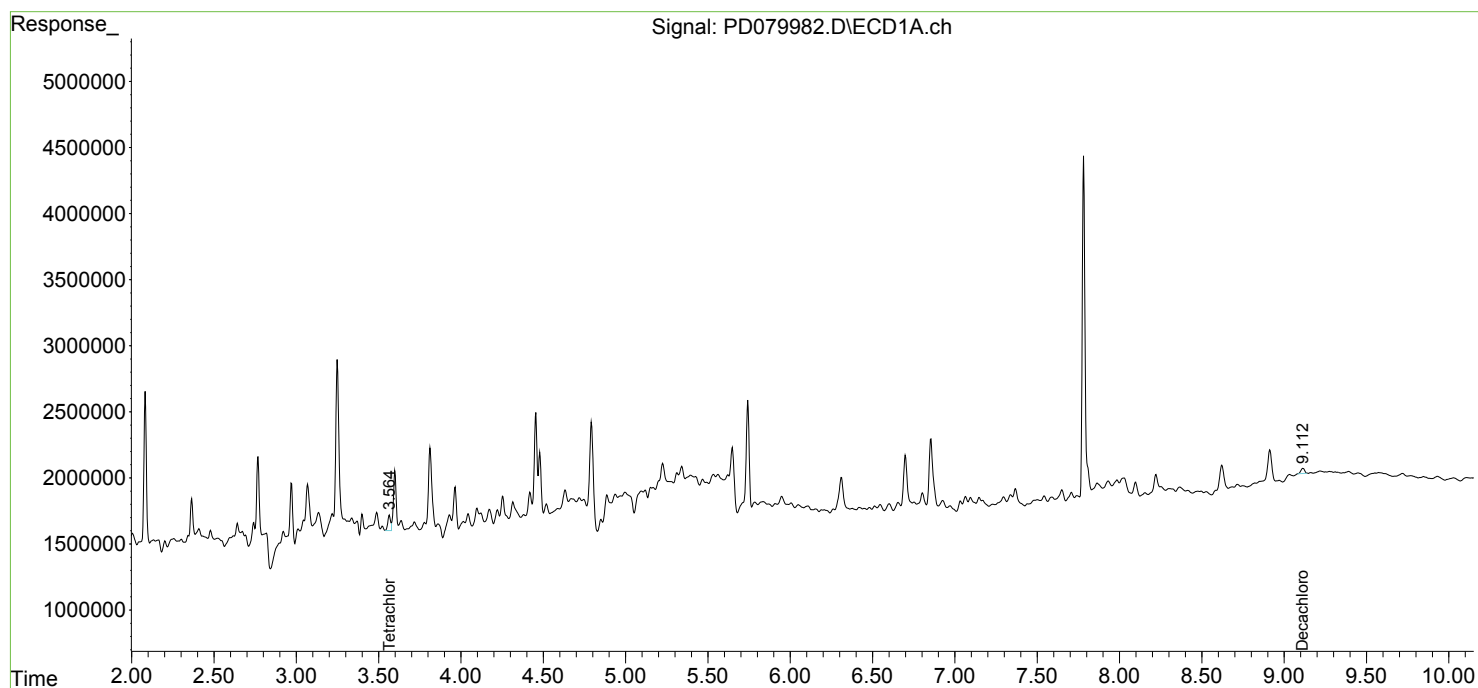

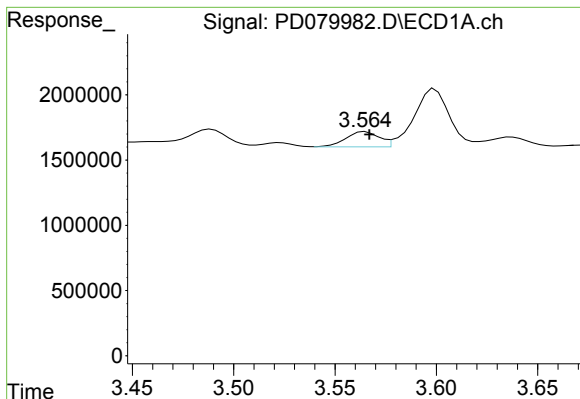


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: -0.003 min
Response: 1263066
Conc: 0.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
OILY-WATER-TOTE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/07/2023
Supervised By :Ankita Jodhani 12/07/2023

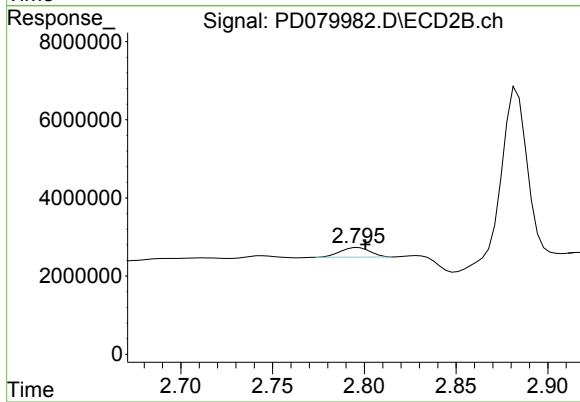


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: -0.005 min
Response: 2795082
Conc: 1.11 ng/ml m

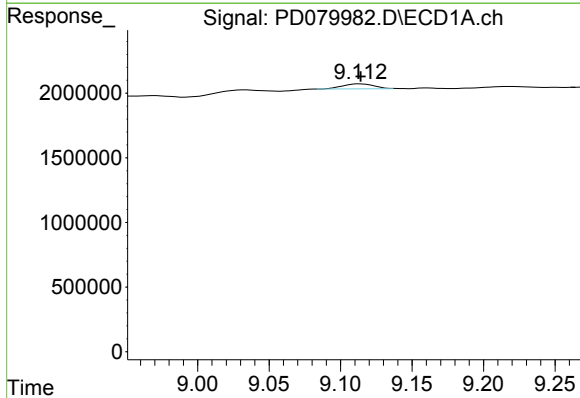

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: -0.002 min
Response: 604471
Conc: 0.30 ng/ml m

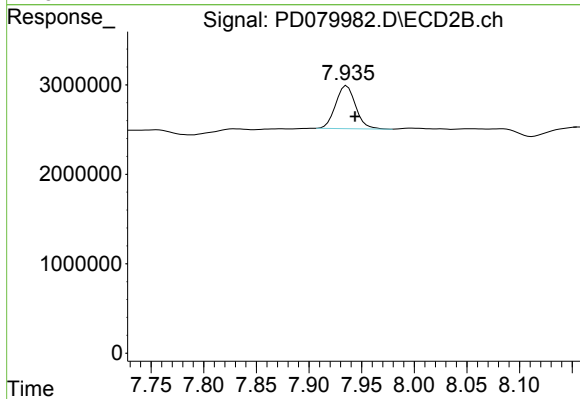

#28 Decachlorobiphenyl

R.T.: 7.936 min
Delta R.T.: -0.008 min
Response: 6345731
Conc: 2.25 ng/ml