

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120623\
 Data File : PD079985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2023 20:32
 Operator : AR\AJ
 Sample : 05629-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 VNJ-216

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/07/2023
 Supervised By :Ankita Jodhani 12/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 21:51:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 06 14:11:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.566	2.800	15396189	33937057	10.215m	13.500 #
2) SA Decachlor...	9.112	7.943	28322912	37227405	13.992m	13.206

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120623\
Data File : PD079985.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2023 20:32
Operator : AR\AJ
Sample : 05629-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
VNJ-216


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/07/2023
Supervised By :Ankita Jodhani 12/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 21:51:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
Quant Title : GC Extractables
QLast Update : Wed Dec 06 14:11:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

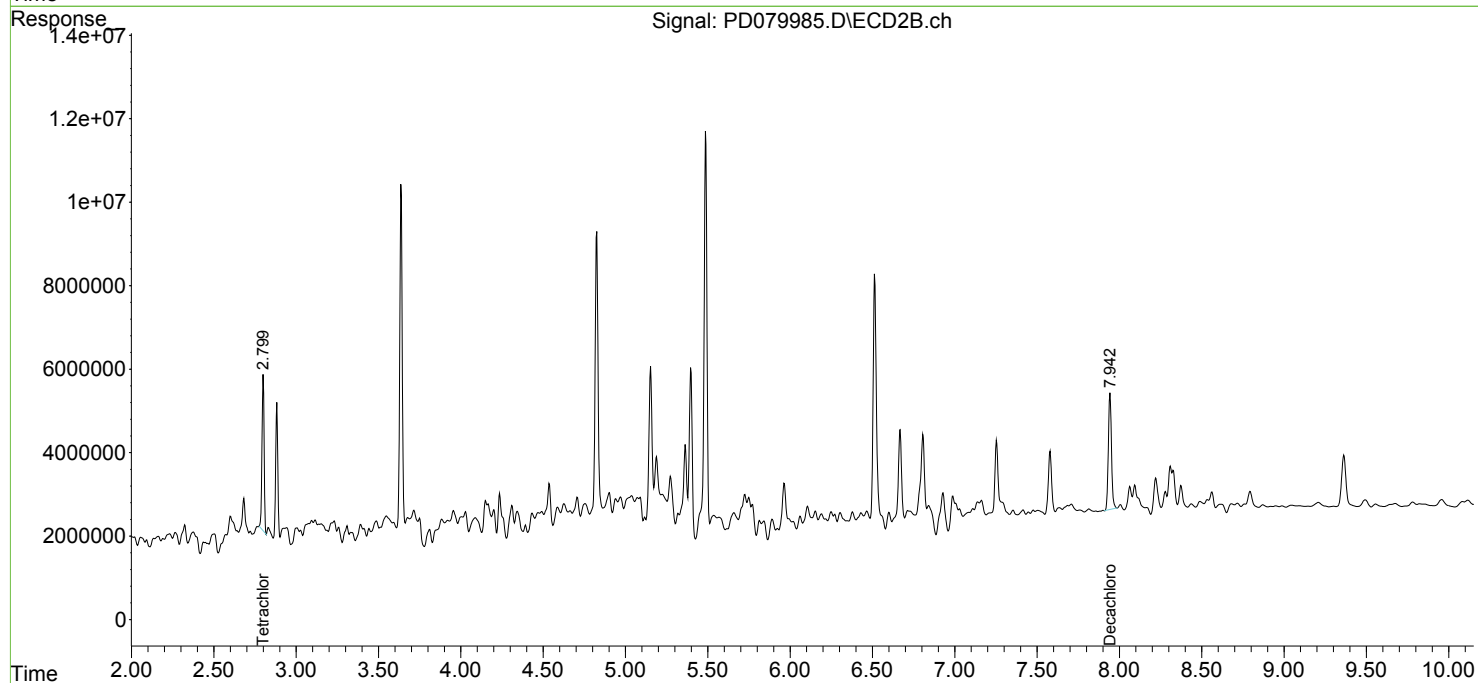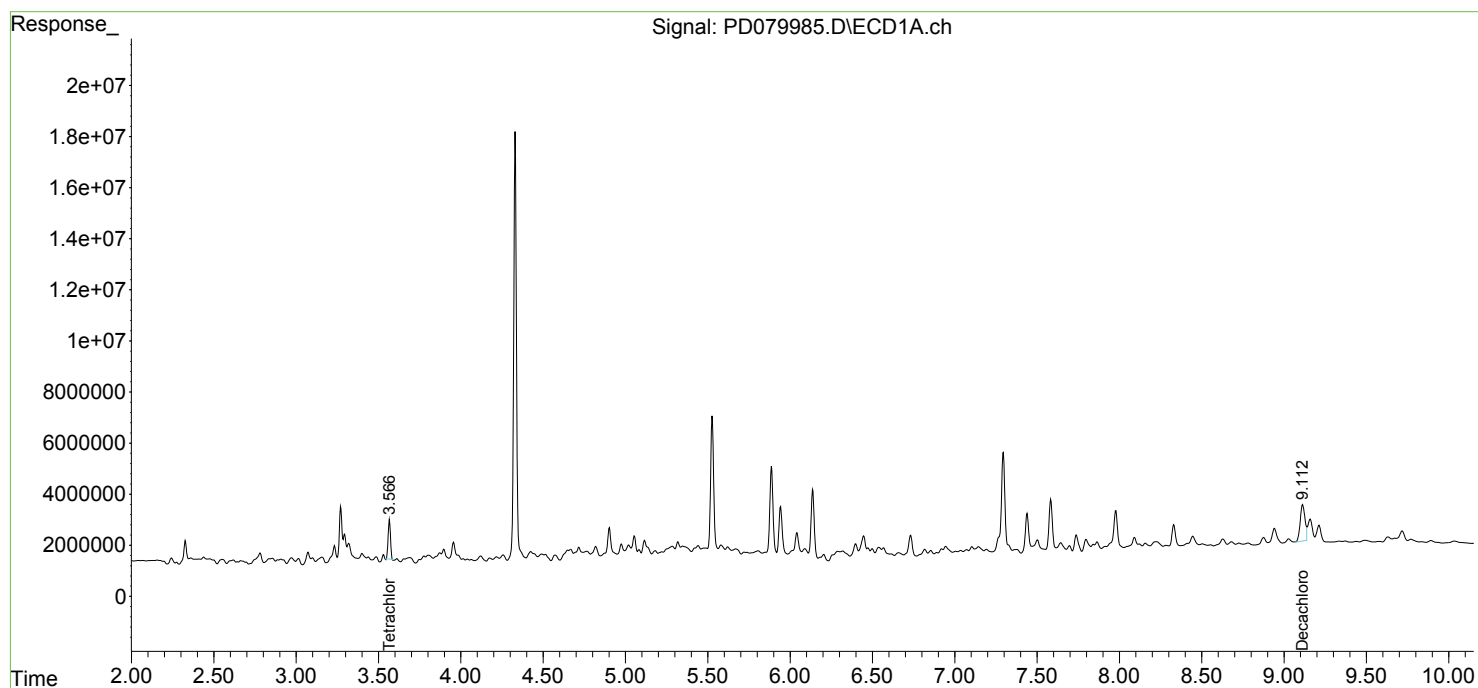

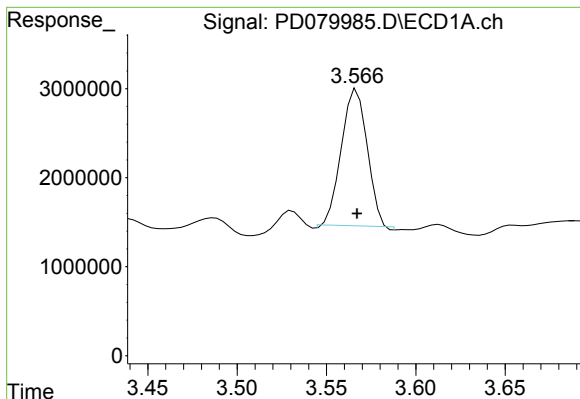


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.001 min
Response: 15396189
Conc: 10.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
VNJ-216


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/07/2023
Supervised By :Ankita Jodhani 12/07/2023

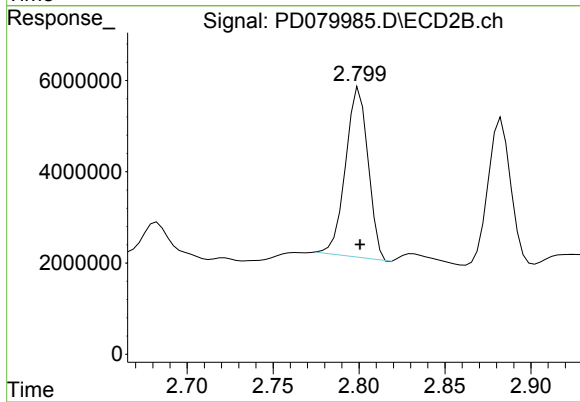


#1 Tetrachloro-m-xylene

R.T.: 2.800 min
Delta R.T.: 0.000 min
Response: 33937057
Conc: 13.50 ng/ml

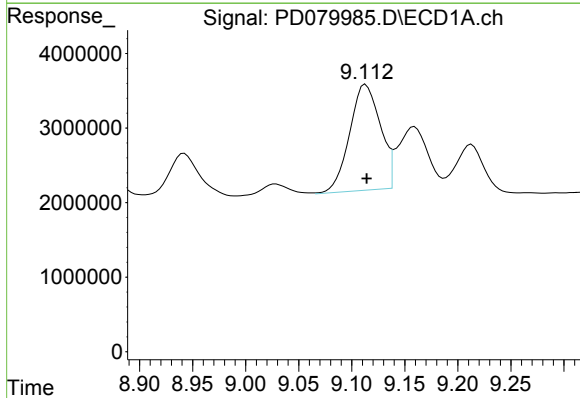

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: -0.002 min
Response: 28322912
Conc: 13.99 ng/ml m

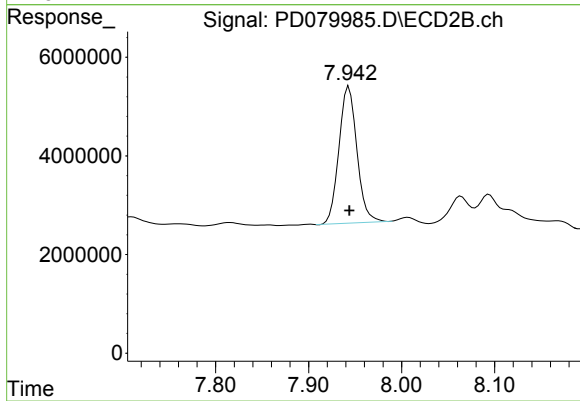

#28 Decachlorobiphenyl

R.T.: 7.943 min
Delta R.T.: 0.000 min
Response: 37227405
Conc: 13.21 ng/ml