

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120723\
 Data File : PD079994.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Dec 2023 09:02
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 20:40:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 06 14:11:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	0.000	2.795	0	109822	N.D.	0.044 #
Target Compounds						
4) MA Heptachlor	4.949	0.000	329462	0	0.134	N.D. #
8) B Heptachlo...	5.715	0.000	1959517	0	0.890	N.D. #
10) B gamma-Chl...	5.985	0.000	168743	0	0.078	N.D. #
14) MA Endrin	0.000	5.683f	0	326260	N.D.	0.116 #
15) B Endosulfa...	6.831	0.000	652652	0	0.343	N.D. #
21) B Endrin ke...	7.712f	0.000	140308	0	0.068	N.D. #
22) Mirex	8.173f	0.000	346713	0	0.212	N.D. #
25) Chlordane-3	5.985	0.000	168743	0	0.559	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120723\
Data File : PD079994.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Dec 2023 09:02
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 20:40:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
Quant Title : GC Extractables
QLast Update : Wed Dec 06 14:11:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

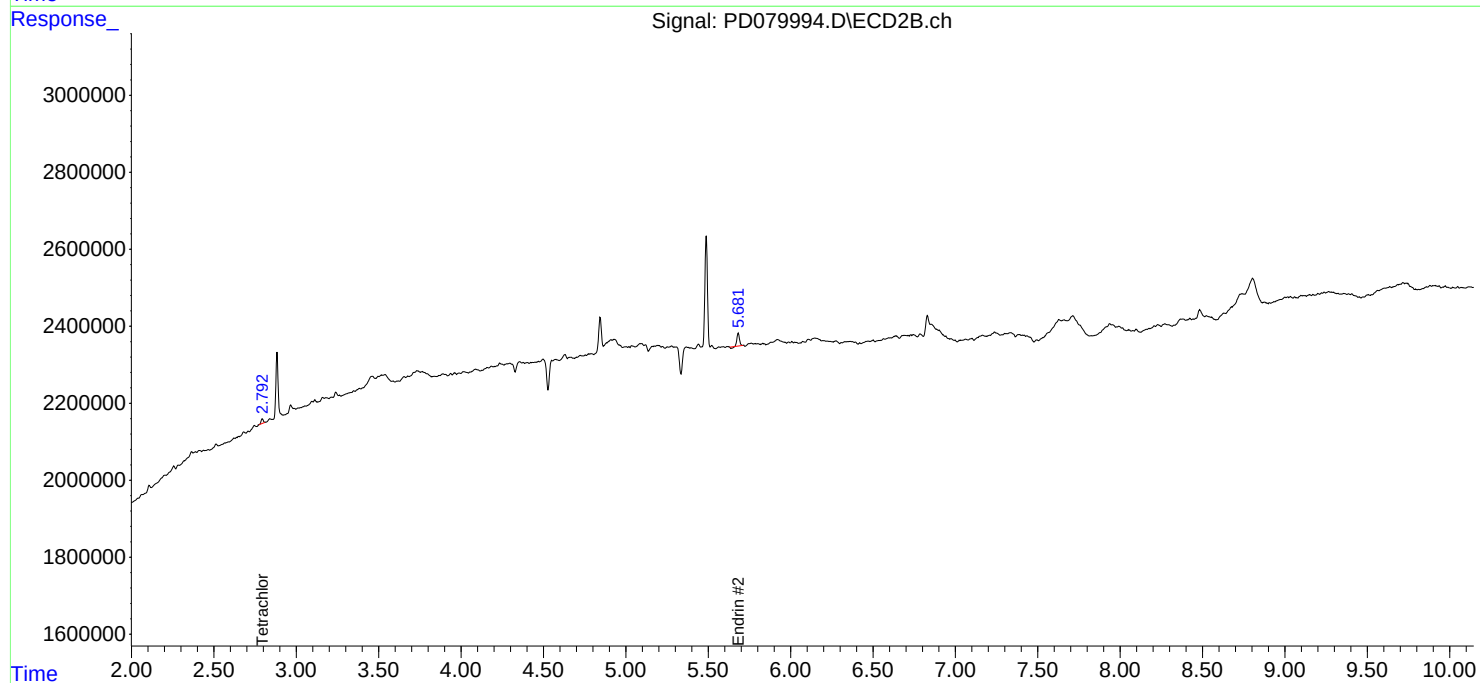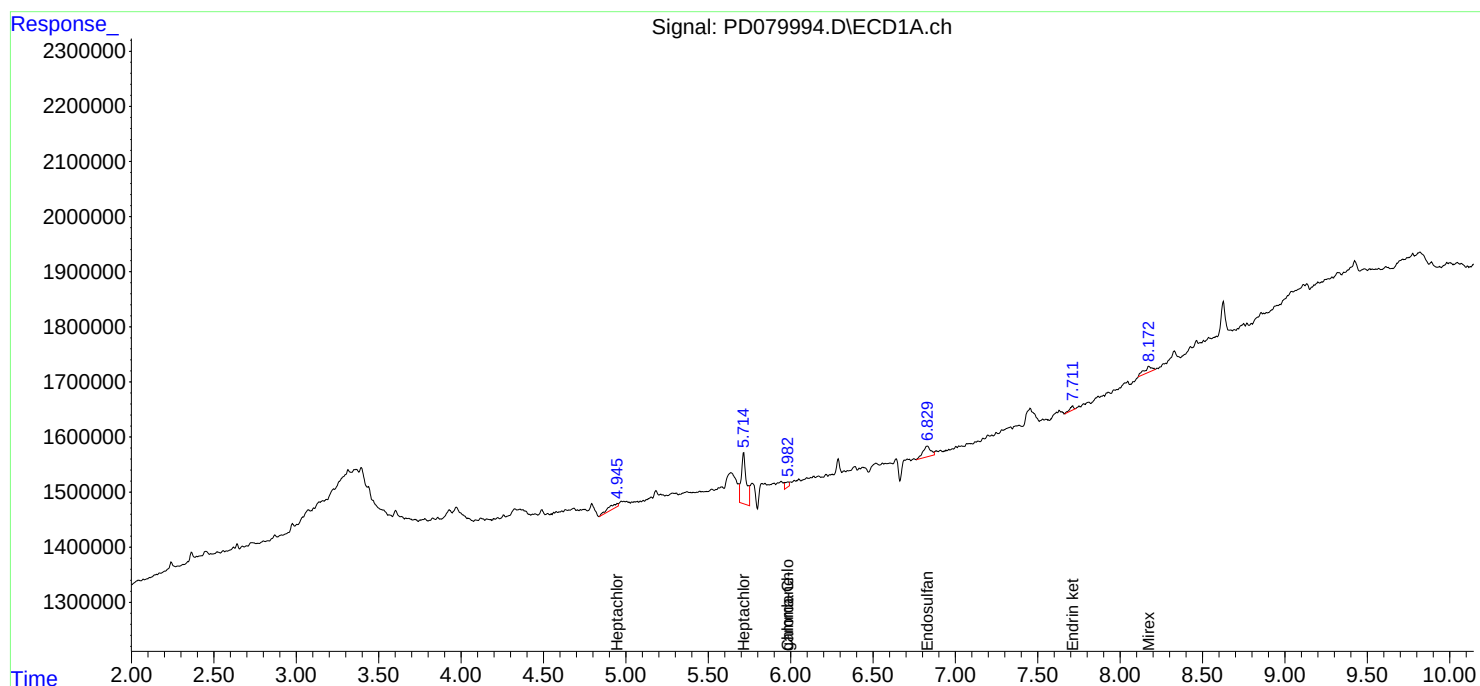


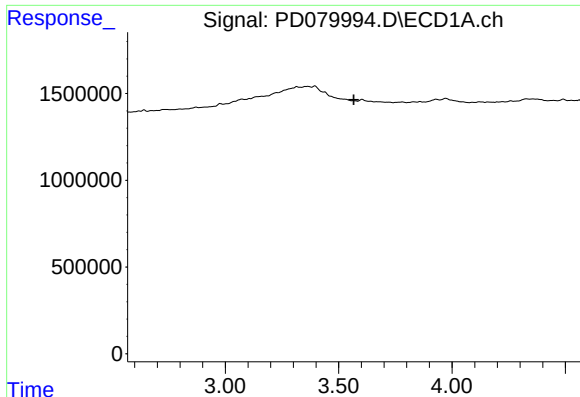

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.567 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

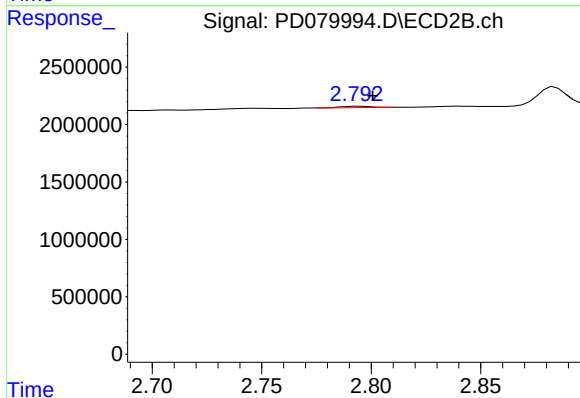


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: -0.006 min
Response: 109822
Conc: 0.04 ng/ml

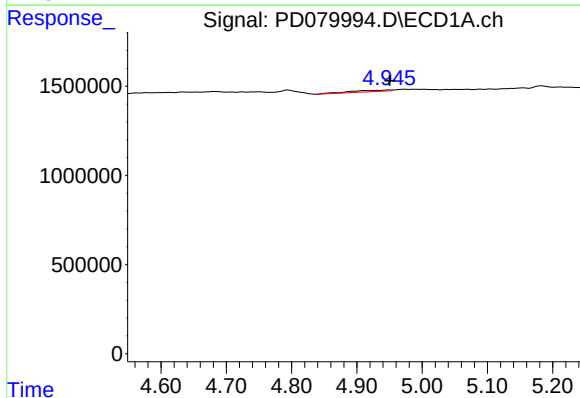


#4 Heptachlor

R.T.: 4.949 min
Delta R.T.: -0.002 min
Response: 329462
Conc: 0.13 ng/ml

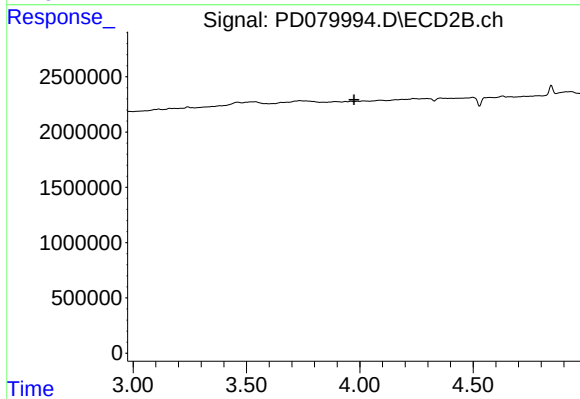

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 3.975 min
Response: 0
Conc: N.D.

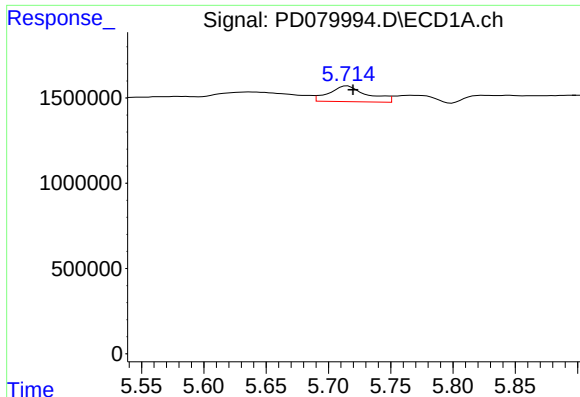

#8 Heptachlor epoxide


R.T.: 5.715 min
Delta R.T.: -0.004 min
Response: 1959517
Conc: 0.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

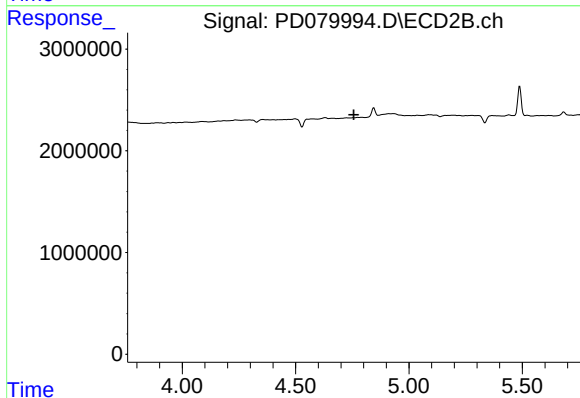


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.756 min
Response: 0
Conc: N.D.

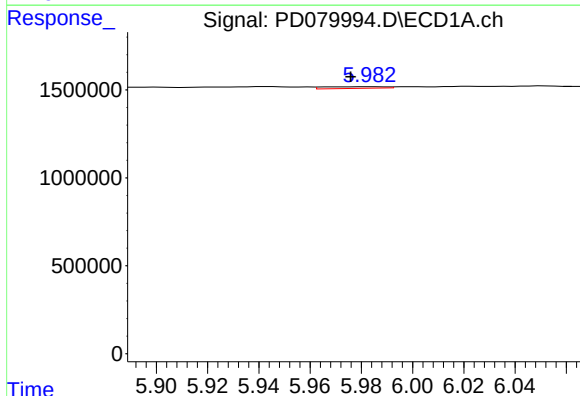


#10 gamma-Chlordane

R.T.: 5.985 min
Delta R.T.: 0.009 min
Response: 168743
Conc: 0.08 ng/ml

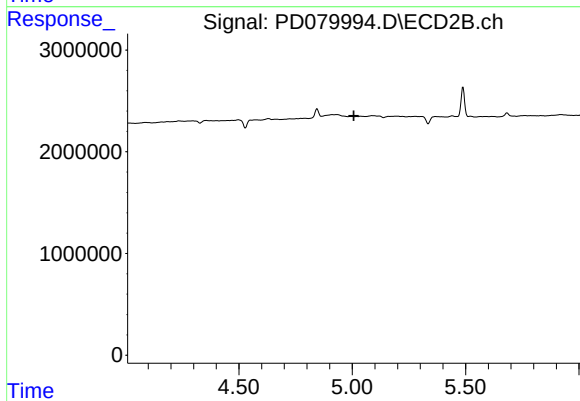

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.007 min
Response: 0
Conc: N.D.

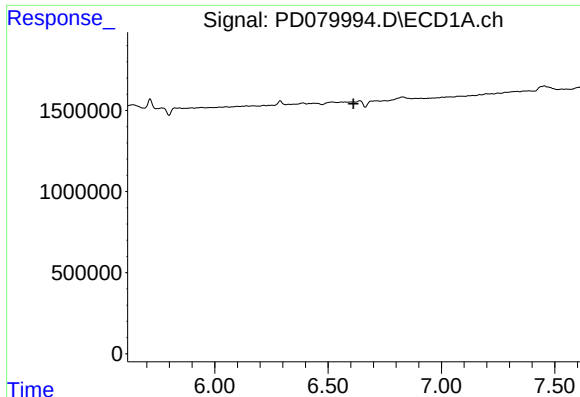

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.613 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

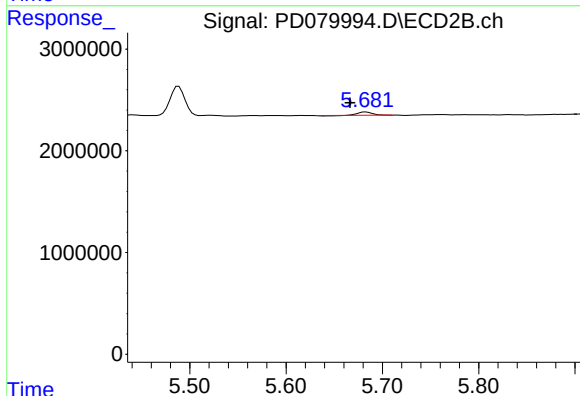


#14 Endrin

R.T.: 5.683 min
Delta R.T.: 0.016 min
Response: 326260
Conc: 0.12 ng/ml

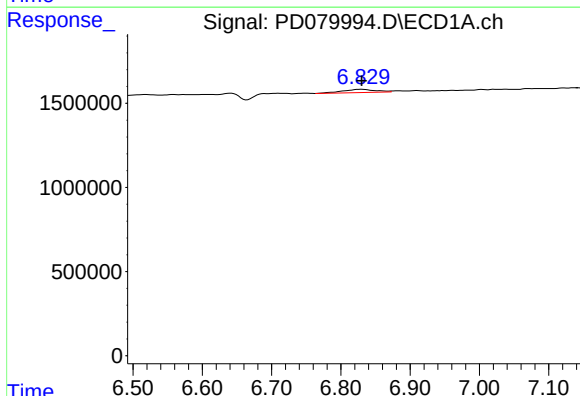


#15 Endosulfan II

R.T.: 6.831 min
Delta R.T.: 0.000 min
Response: 652652
Conc: 0.34 ng/ml

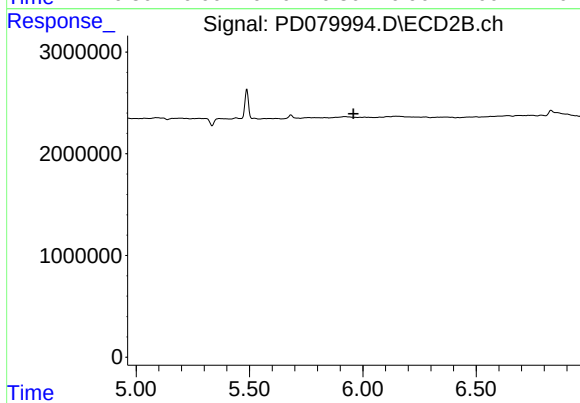

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.959 min
Response: 0
Conc: N.D.

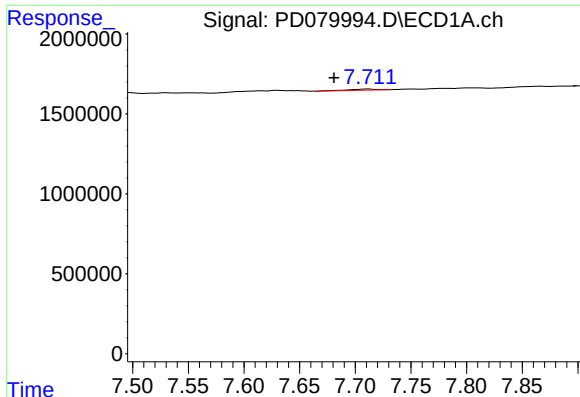

#21 Endrin ketone


R.T.: 7.712 min
Delta R.T.: 0.031 min
Response: 140308
Conc: 0.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

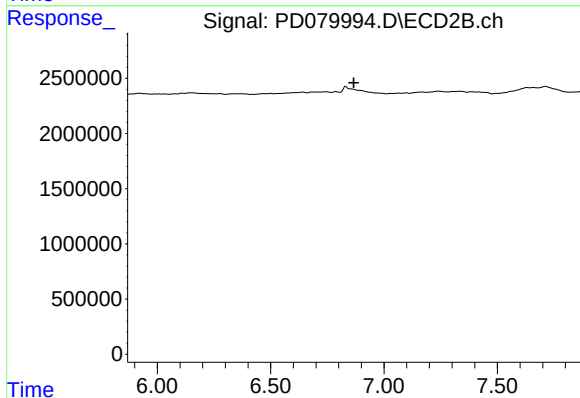


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.867 min
Response: 0
Conc: N.D.

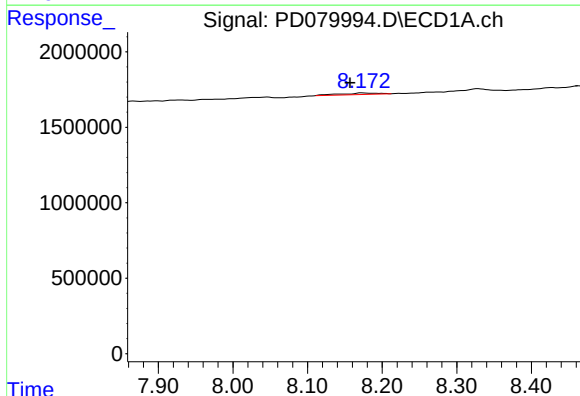


#22 Mirex

R.T.: 8.173 min
Delta R.T.: 0.016 min
Response: 346713
Conc: 0.21 ng/ml

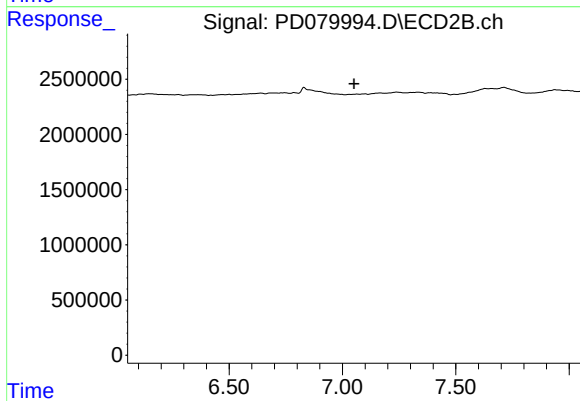

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 7.051 min
Response: 0
Conc: N.D.

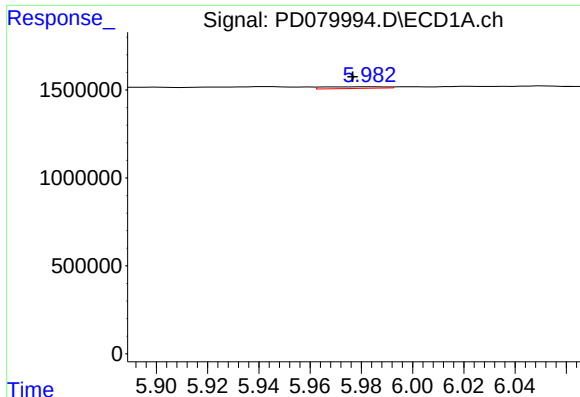

#25 Chlordane-3


R.T.: 5.985 min
Delta R.T.: 0.008 min
Response: 168743
Conc: 0.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

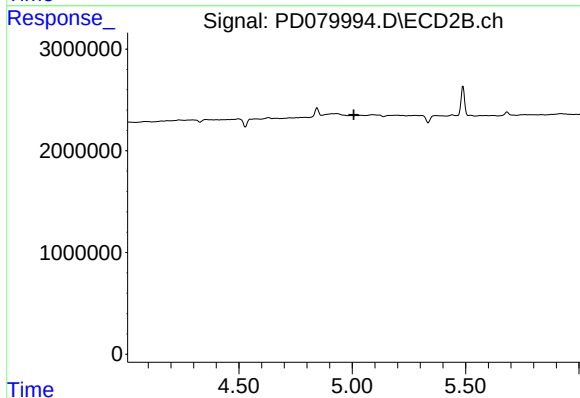


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.007 min
Response: 0
Conc: N.D.

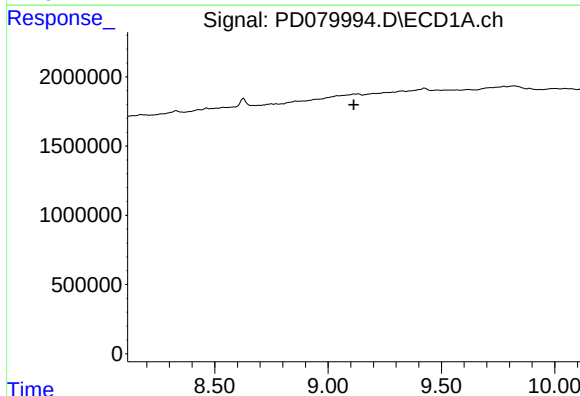

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.114 min
Response: 0
Conc: N.D.

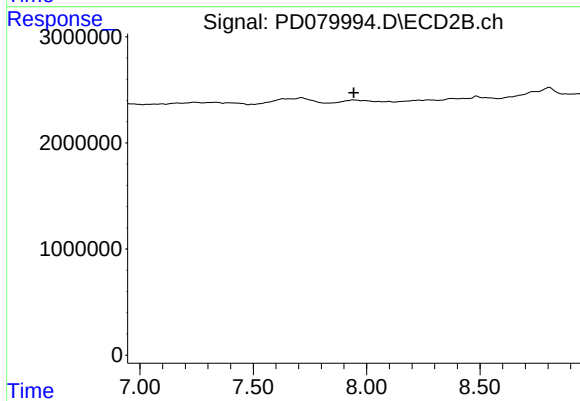

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.944 min
Response: 0
Conc: N.D.