

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120825\
 Data File : PD091487.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2025 16:31
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 17:09:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120825.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 08 17:05:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.870	178.9E6	2631.7E6	74.783	74.826
28)	SA Decachlor...	9.058	8.054	268.3E6	2211.5E6	75.174	74.014
Target Compounds							
23)	Chlordane-1	4.702	3.892	152.5E6	1059.4E6	749.442	746.916
24)	Chlordane-2	5.230	4.473	143.7E6	1106.1E6	744.651	747.574
25)	Chlordane-3	5.935	5.111	616.9E6	3599.0E6	749.785	747.637
26)	Chlordane-4	6.020	5.176	745.1E6	3004.9E6	748.397	745.298
27)	Chlordane-5	6.859	6.075	128.9E6	1326.9E6	746.892	744.508



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120825\
Data File : PD091487.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2025 16:31
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 17:09:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120825.M
Quant Title : GC Extractables
QLast Update : Mon Dec 08 17:05:17 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

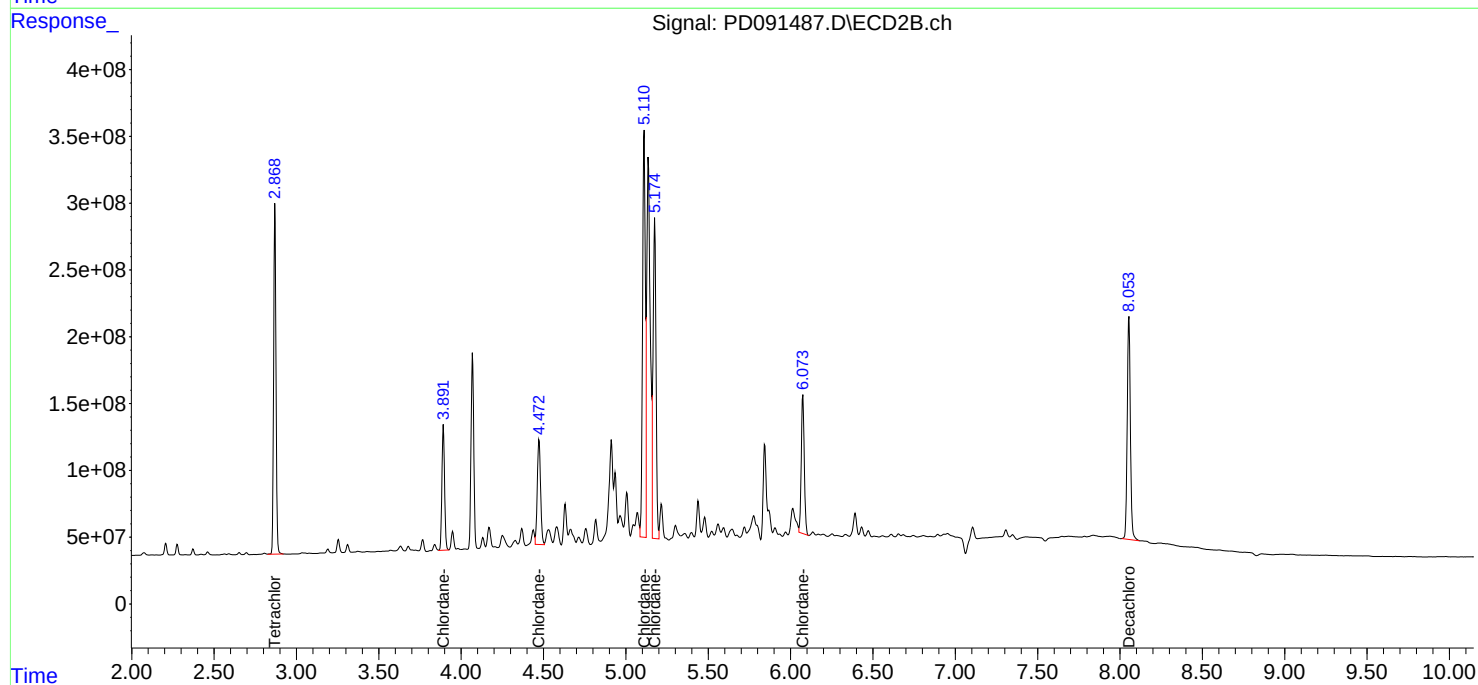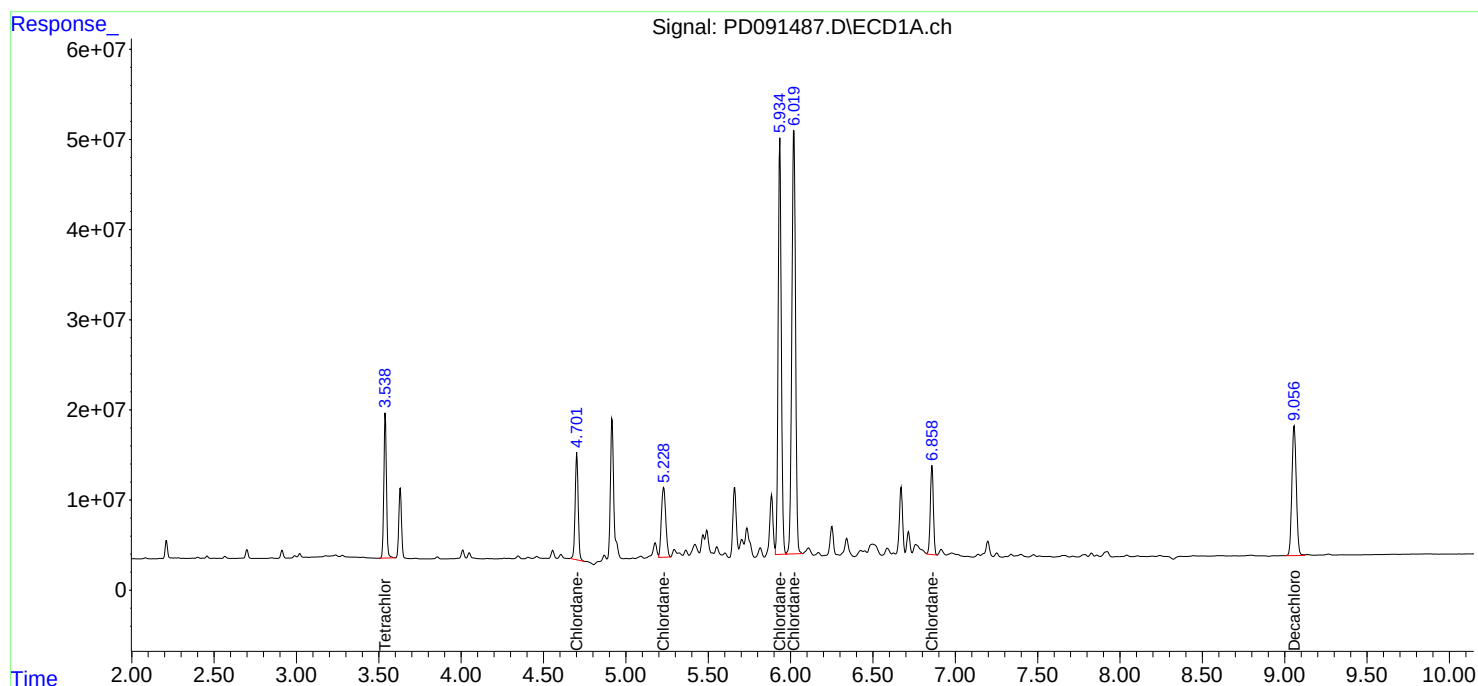


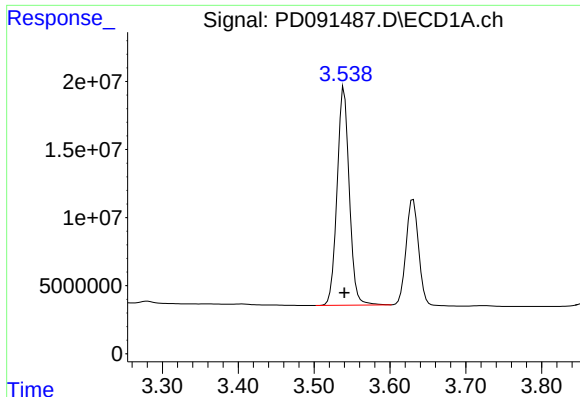

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 178923730
Conc: 74.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

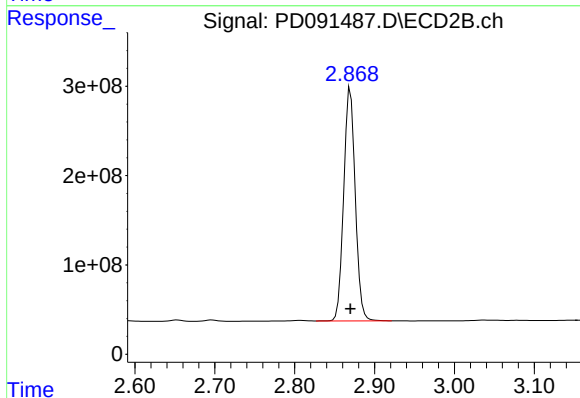


#1 Tetrachloro-m-xylene

R.T.: 2.870 min
Delta R.T.: 0.000 min
Response: 2631678718
Conc: 74.83 ng/ml

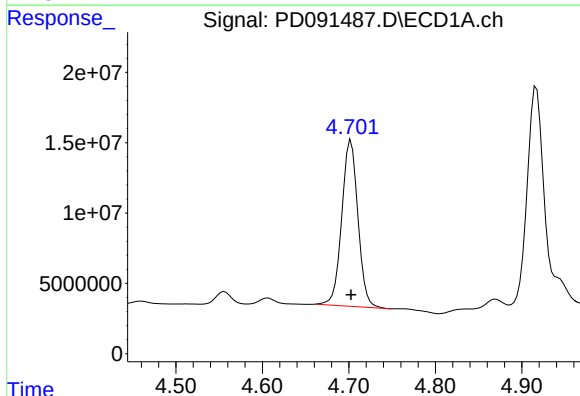


#23 Chlordane-1

R.T.: 4.702 min
Delta R.T.: 0.000 min
Response: 152492019
Conc: 749.44 ng/ml

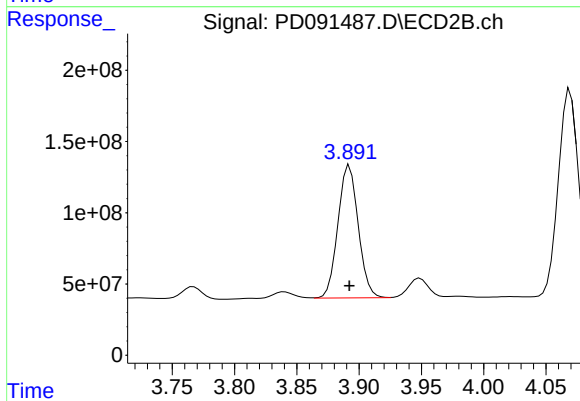

#23 Chlordane-1


R.T.: 3.892 min
Delta R.T.: 0.000 min
Response: 1059402108
Conc: 746.92 ng/ml

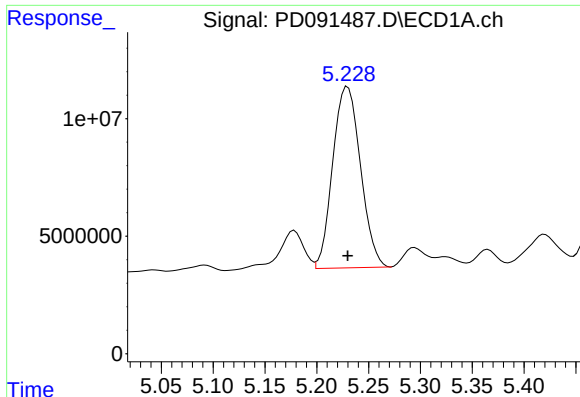

#24 Chlordane-2


R.T.: 5.230 min
Delta R.T.: 0.000 min
Response: 143663740
Conc: 744.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

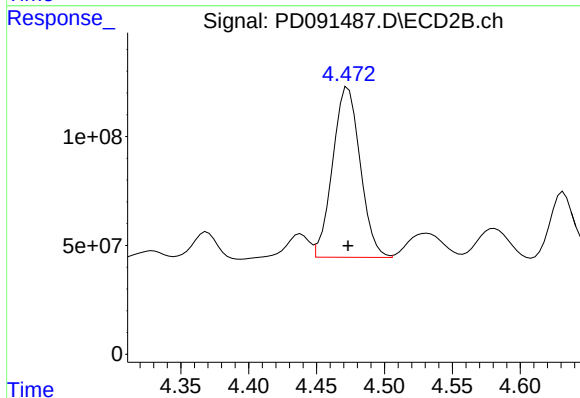


#24 Chlordane-2

R.T.: 4.473 min
Delta R.T.: 0.000 min
Response: 1106066645
Conc: 747.57 ng/ml

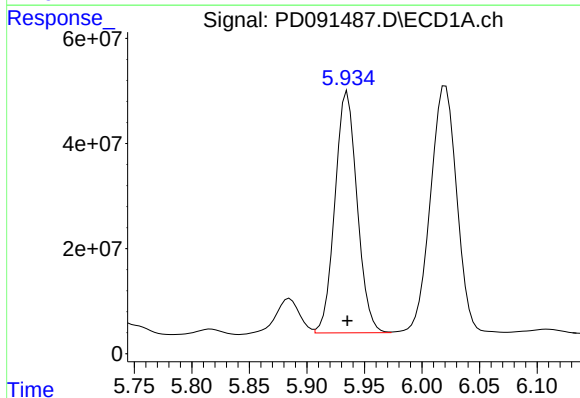


#25 Chlordane-3

R.T.: 5.935 min
Delta R.T.: 0.000 min
Response: 616919263
Conc: 749.79 ng/ml

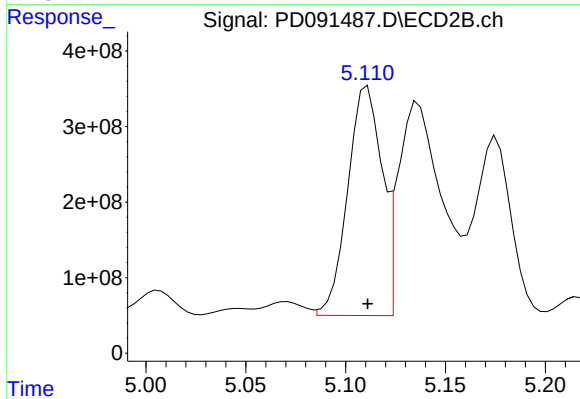

#25 Chlordane-3


R.T.: 5.111 min
Delta R.T.: 0.000 min
Response: 3598974463
Conc: 747.64 ng/ml

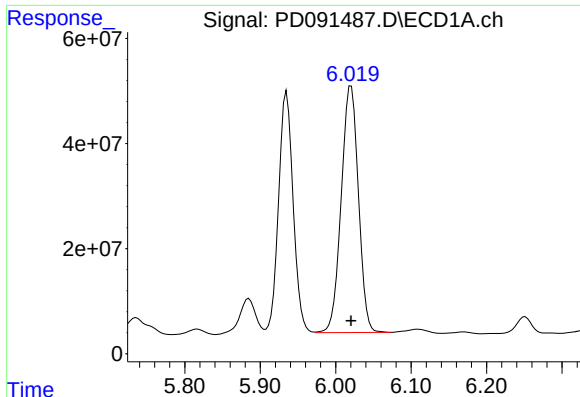

#26 Chlordane-4


R.T.: 6.020 min
Delta R.T.: 0.000 min
Response: 745066914
Conc: 748.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

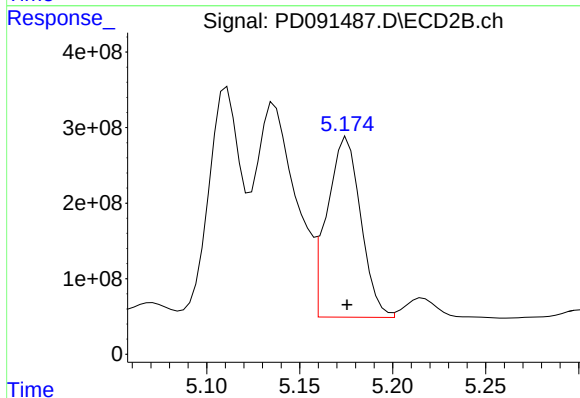


#26 Chlordane-4

R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 3004894082
Conc: 745.30 ng/ml

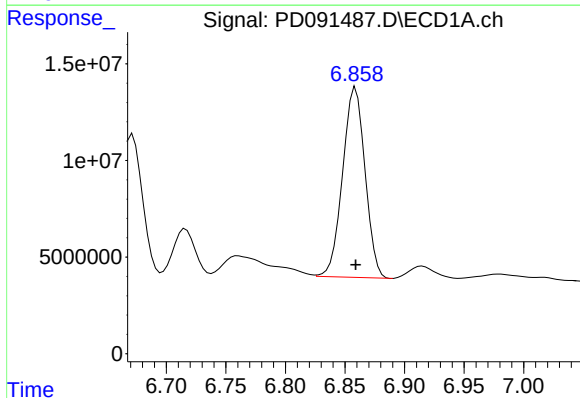


#27 Chlordane-5

R.T.: 6.859 min
Delta R.T.: 0.000 min
Response: 128947159
Conc: 746.89 ng/ml

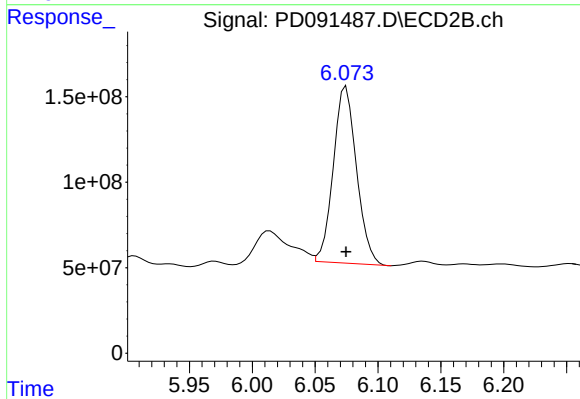

#27 Chlordane-5


R.T.: 6.075 min
Delta R.T.: 0.000 min
Response: 1326922279
Conc: 744.51 ng/ml

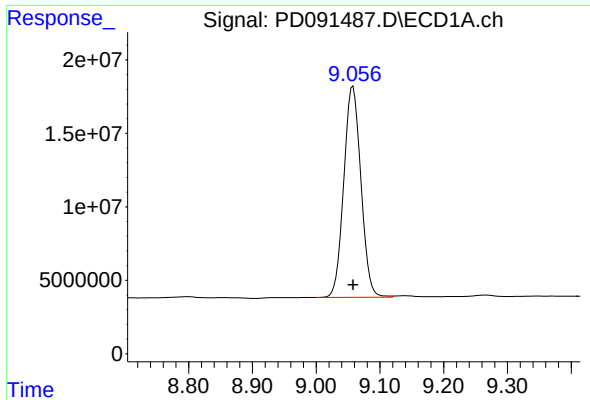

#28 Decachlorobiphenyl

R.T.: 9.058 min
Delta R.T.: 0.000 min
Response: 268298786
Conc: 75.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

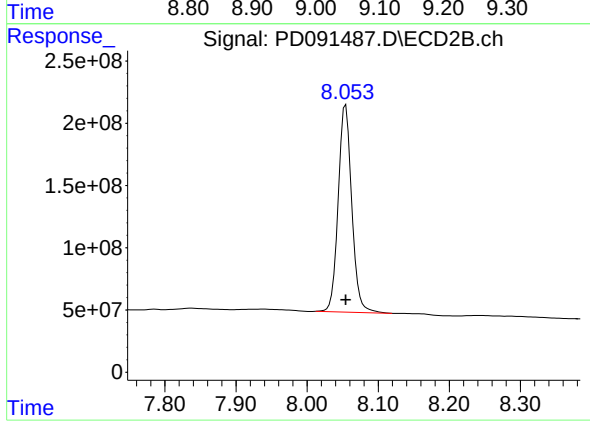

#28 Decachlorobiphenyl

R.T.: 8.054 min
Delta R.T.: 0.000 min
Response: 2211486081
Conc: 74.01 ng/ml