

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120825\
 Data File : PD091488.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2025 16:44
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 17:05:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120825.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 08 17:05:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.869	118.8E6	1745.9E6	50.000	50.000
28)	SA Decachlor...	9.057	8.054	179.2E6	1506.1E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.702	3.892	101.2E6	717.3E6	500.000	500.000
24)	Chlordane-2	5.228	4.473	97444137	753.4E6	500.000	500.000
25)	Chlordane-3	5.934	5.111	398.7E6	2414.1E6	500.000	500.000
26)	Chlordane-4	6.019	5.175	486.6E6	2038.8E6	500.000	500.000
27)	Chlordane-5	6.859	6.075	85110724	896.5E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120825\
Data File : PD091488.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2025 16:44
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 17:05:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120825.M
Quant Title : GC Extractables
QLast Update : Mon Dec 08 17:05:17 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

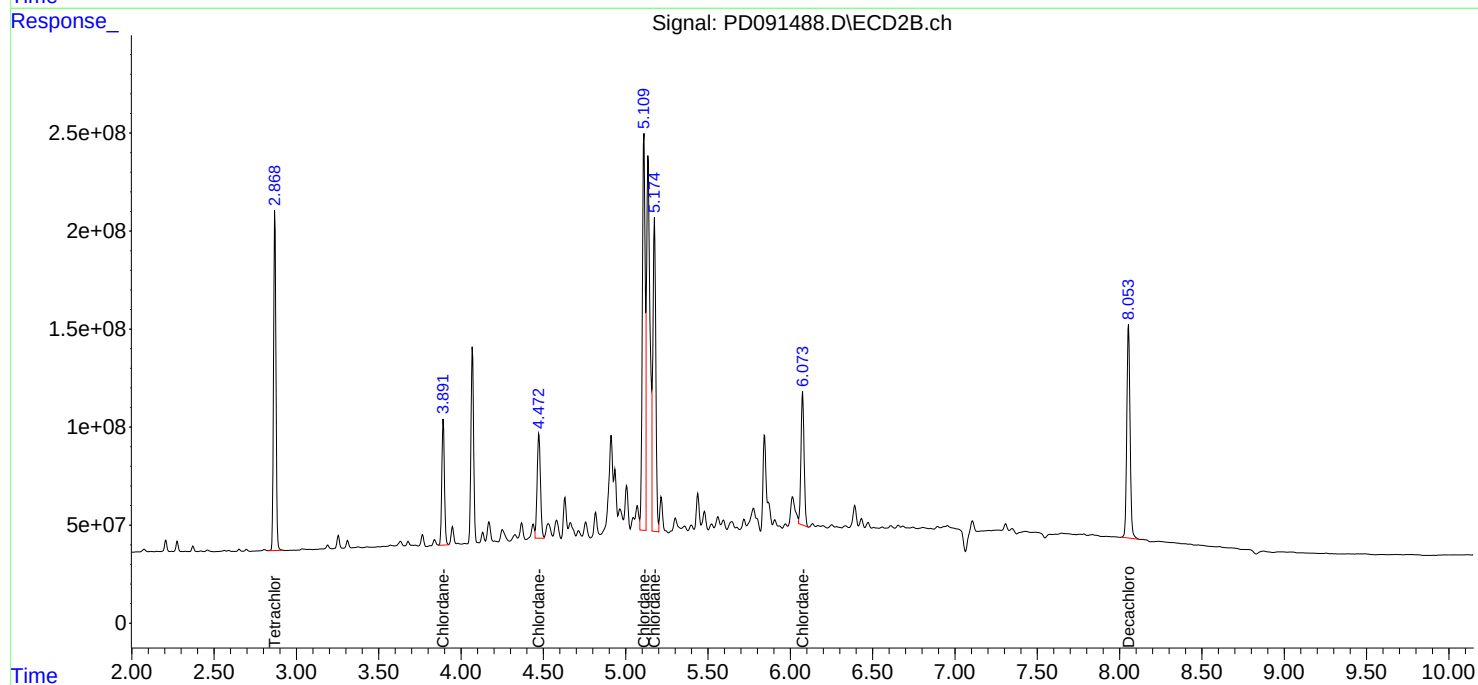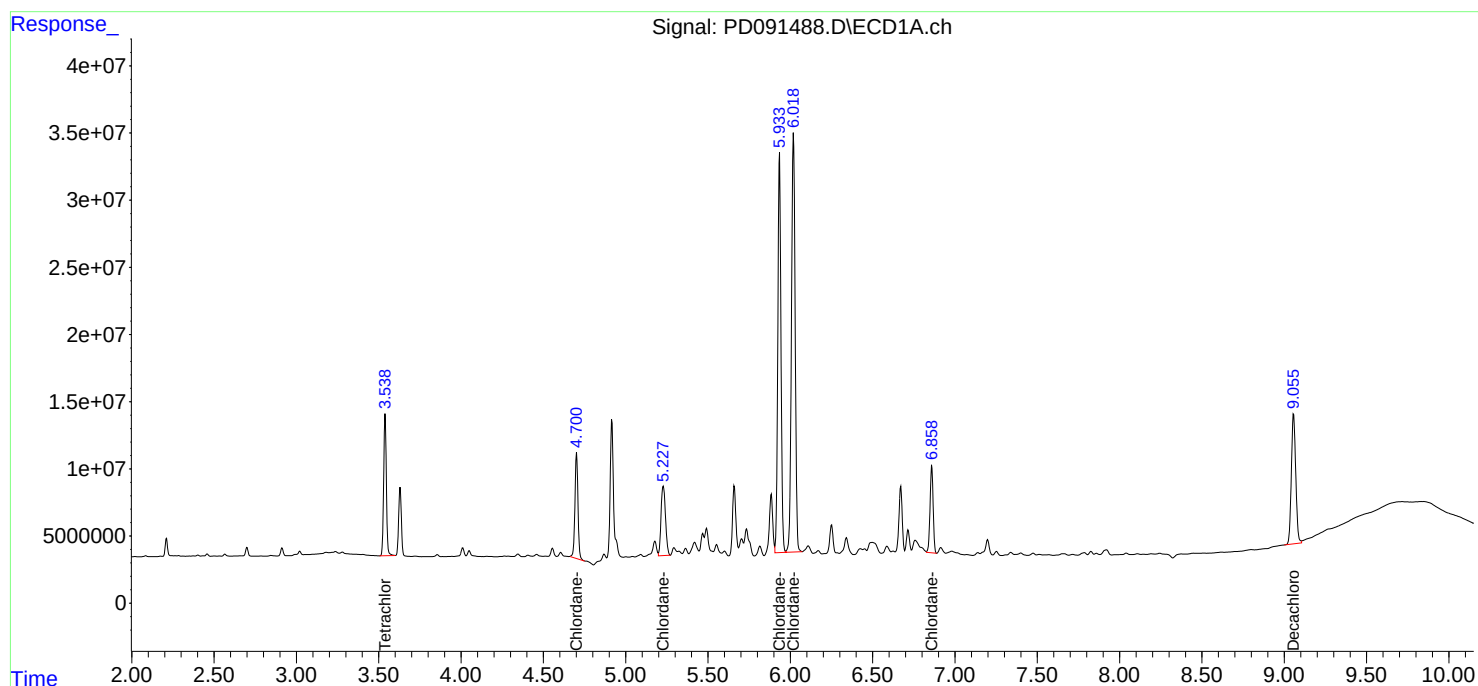


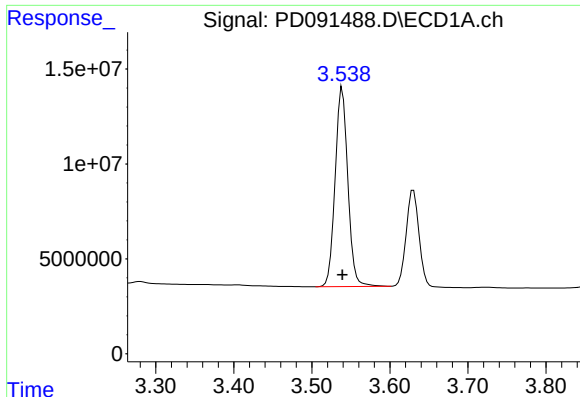

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 118801373
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

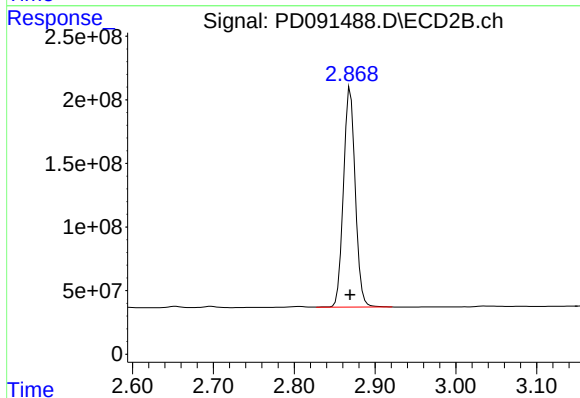


#1 Tetrachloro-m-xylene

R.T.: 2.869 min
Delta R.T.: 0.000 min
Response: 1745872302
Conc: 50.00 ng/ml

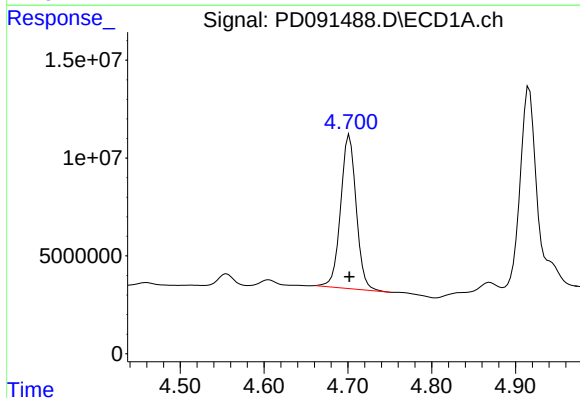


#23 Chlordane-1

R.T.: 4.702 min
Delta R.T.: 0.000 min
Response: 101155261
Conc: 500.00 ng/ml

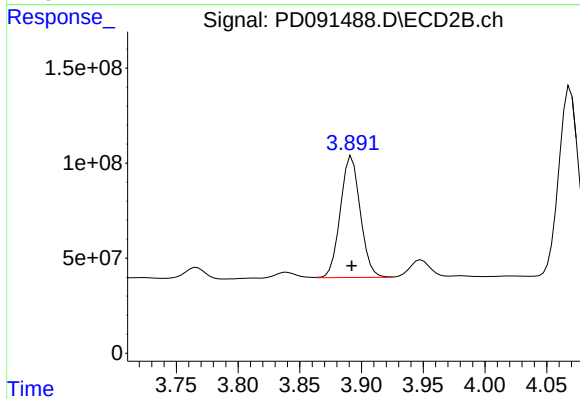

#23 Chlordane-1


R.T.: 3.892 min
Delta R.T.: 0.000 min
Response: 717297595
Conc: 500.00 ng/ml

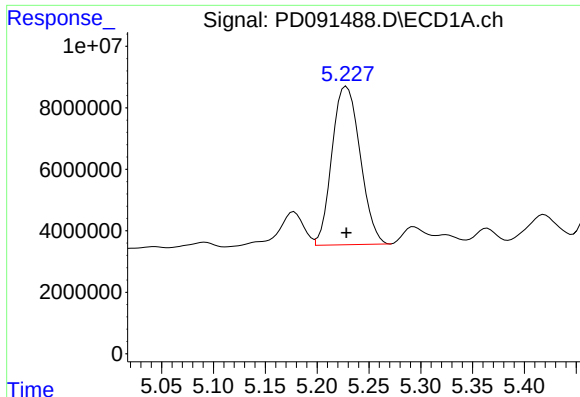

#24 Chlordane-2


R.T.: 5.228 min
Delta R.T.: 0.000 min
Response: 97444137
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

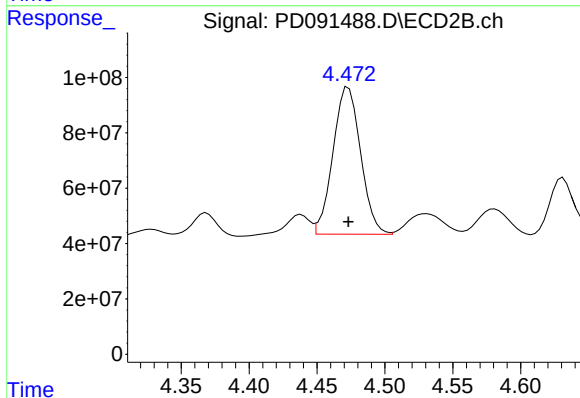


#24 Chlordane-2

R.T.: 4.473 min
Delta R.T.: 0.000 min
Response: 753362087
Conc: 500.00 ng/ml

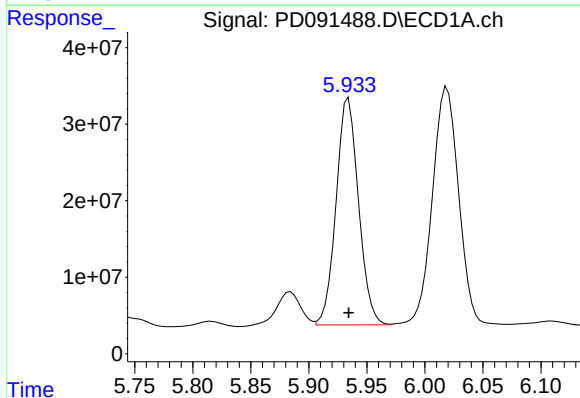


#25 Chlordane-3

R.T.: 5.934 min
Delta R.T.: 0.000 min
Response: 398704222
Conc: 500.00 ng/ml

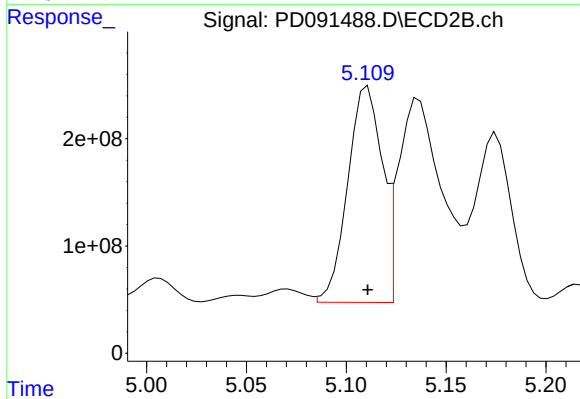

#25 Chlordane-3


R.T.: 5.111 min
Delta R.T.: 0.000 min
Response: 2414059077
Conc: 500.00 ng/ml

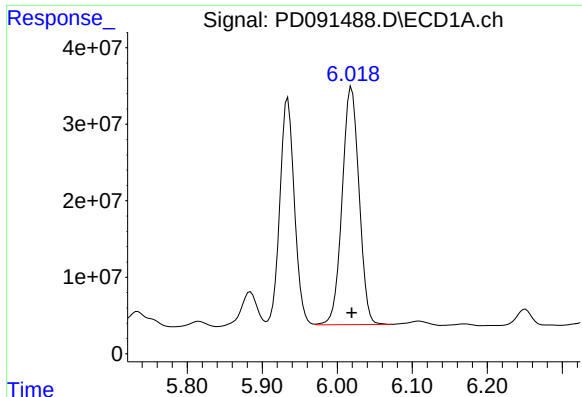

#26 Chlordane-4


R.T.: 6.019 min
Delta R.T.: 0.000 min
Response: 486624852
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

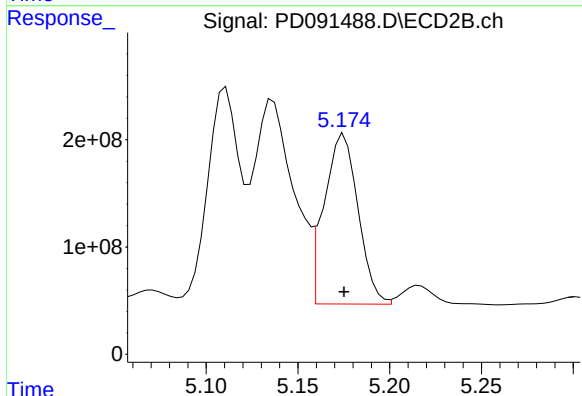


#26 Chlordane-4

R.T.: 5.175 min
Delta R.T.: 0.000 min
Response: 2038825974
Conc: 500.00 ng/ml

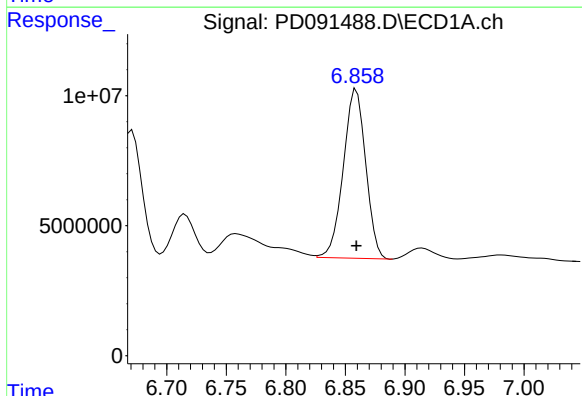


#27 Chlordane-5

R.T.: 6.859 min
Delta R.T.: 0.000 min
Response: 85110724
Conc: 500.00 ng/ml

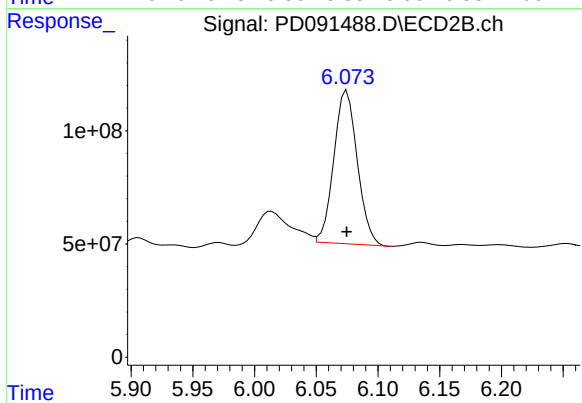

#27 Chlordane-5


R.T.: 6.075 min
Delta R.T.: 0.000 min
Response: 896532149
Conc: 500.00 ng/ml

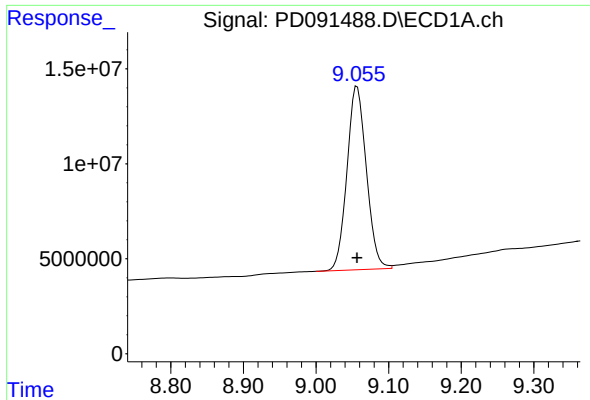

#28 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: 0.000 min
Response: 179231793
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

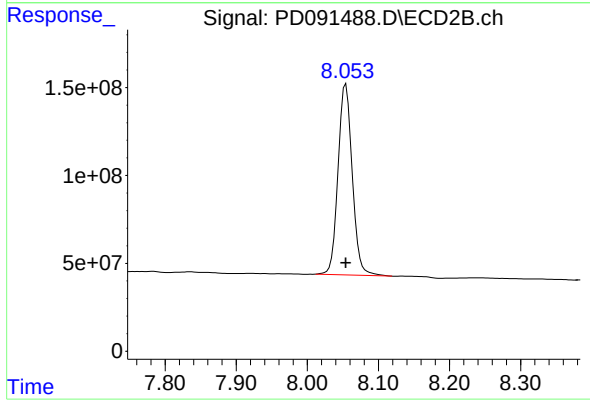

#28 Decachlorobiphenyl

R.T.: 8.054 min
Delta R.T.: 0.000 min
Response: 1506104545
Conc: 50.00 ng/ml