

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120825\
 Data File : PD091489.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2025 16:58
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 17:11:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120825.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 08 17:05:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.869	63340911	934.2E6	26.090	26.154
28)	SA Decachlor...	9.057	8.055	99065639	810.5E6	27.012	26.562
Target Compounds							
23)	Chlordane-1	4.702	3.892	53552261	393.7E6	259.763	270.120
24)	Chlordane-2	5.229	4.473	52698343	412.4E6	266.970	270.958
25)	Chlordane-3	5.935	5.110	202.9E6	1319.7E6	247.396	267.688
26)	Chlordane-4	6.019	5.175	252.0E6	1101.2E6	252.371	266.959
27)	Chlordane-5	6.859	6.074	44091591	482.9E6	254.020	265.374



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120825\
Data File : PD091489.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2025 16:58
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 17:11:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120825.M
Quant Title : GC Extractables
QLast Update : Mon Dec 08 17:05:17 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

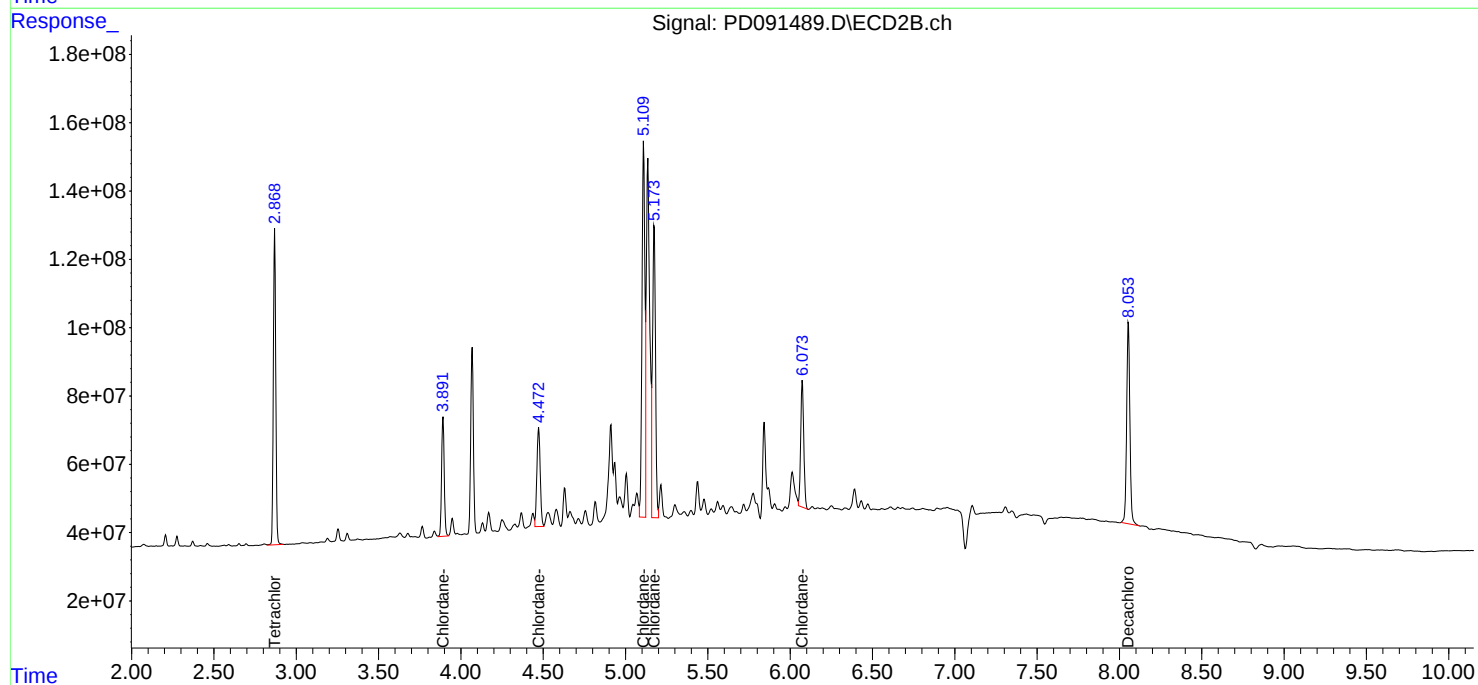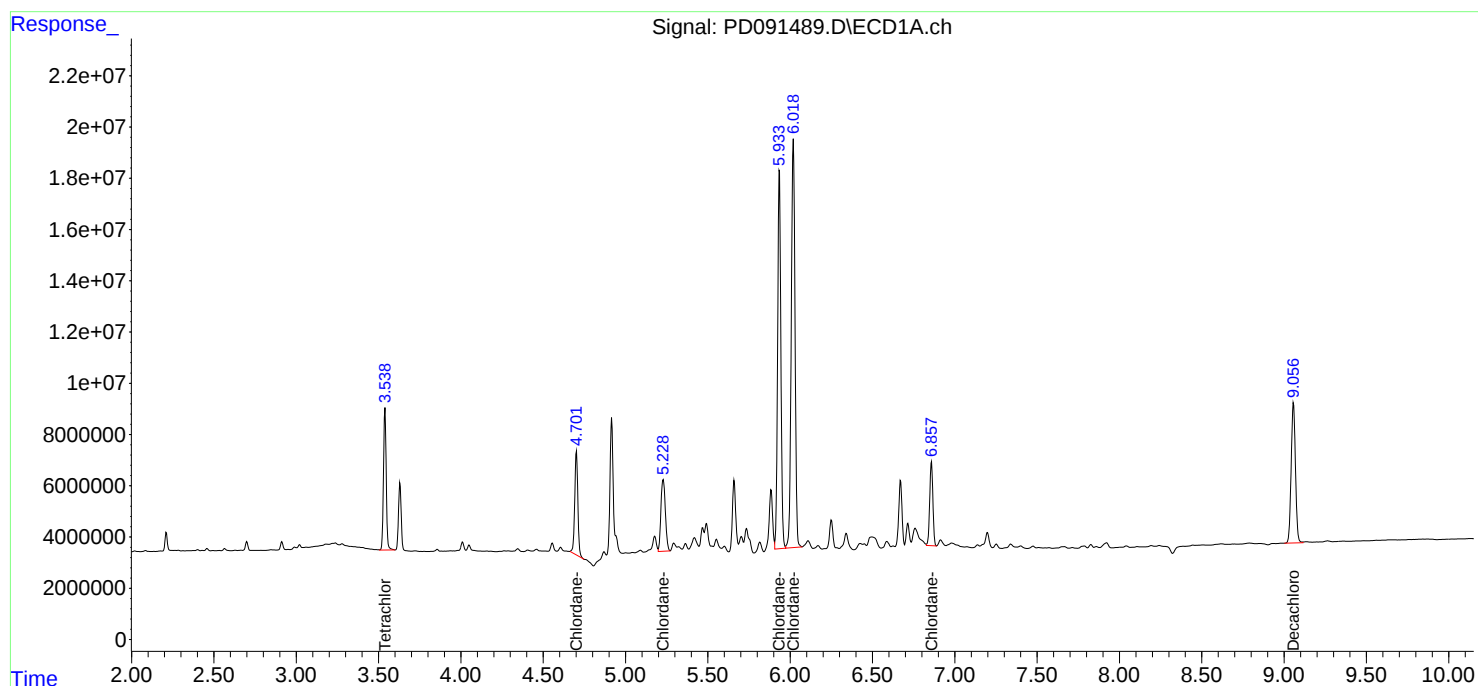


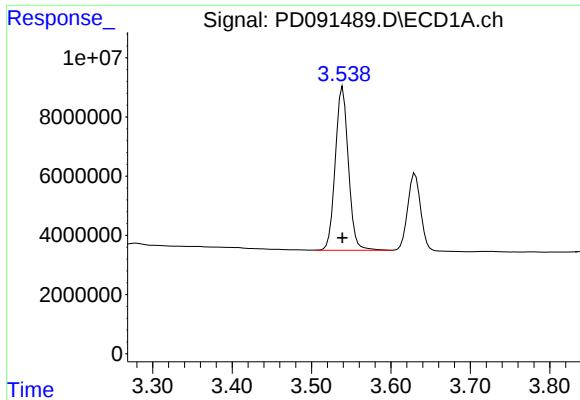

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 63340911
Conc: 26.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

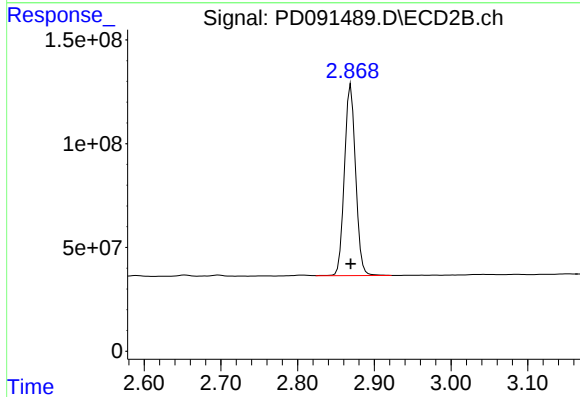


#1 Tetrachloro-m-xylene

R.T.: 2.869 min
Delta R.T.: 0.000 min
Response: 934222300
Conc: 26.15 ng/ml

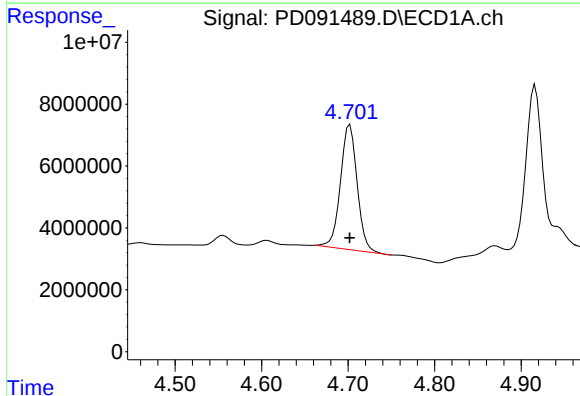


#23 Chlordane-1

R.T.: 4.702 min
Delta R.T.: 0.000 min
Response: 53552261
Conc: 259.76 ng/ml

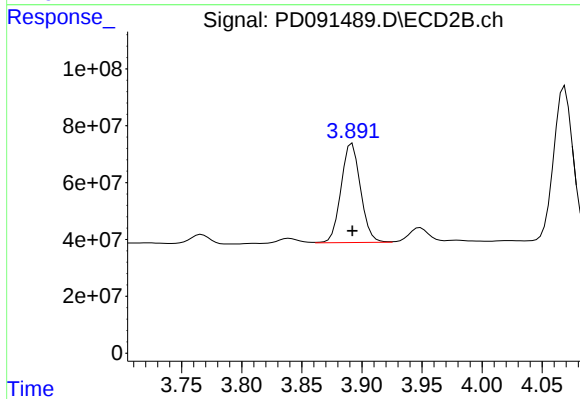

#23 Chlordane-1


R.T.: 3.892 min
Delta R.T.: 0.000 min
Response: 393691509
Conc: 270.12 ng/ml

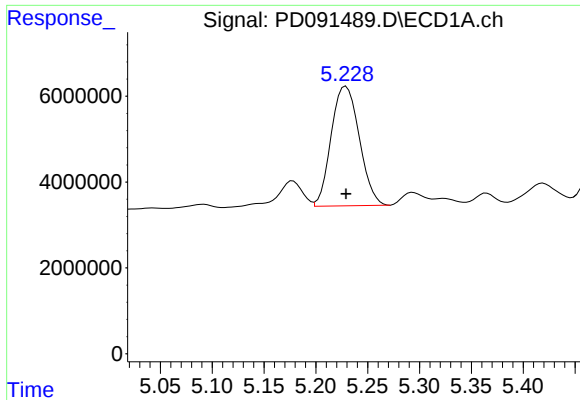

#24 Chlordane-2


R.T.: 5.229 min
Delta R.T.: 0.000 min
Response: 52698343
Conc: 266.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

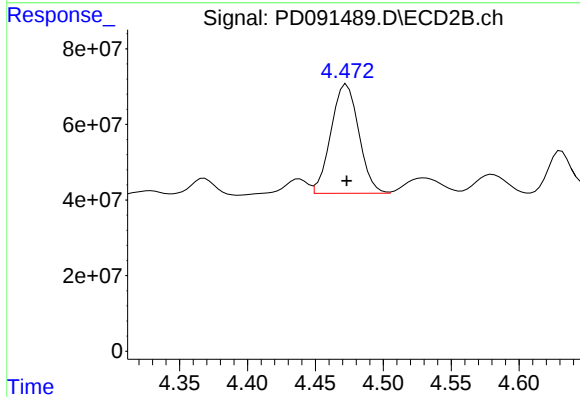


#24 Chlordane-2

R.T.: 4.473 min
Delta R.T.: 0.000 min
Response: 412417802
Conc: 270.96 ng/ml

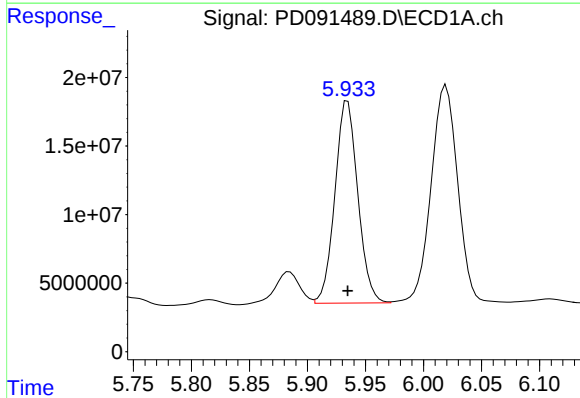


#25 Chlordane-3

R.T.: 5.935 min
Delta R.T.: 0.000 min
Response: 202852371
Conc: 247.40 ng/ml

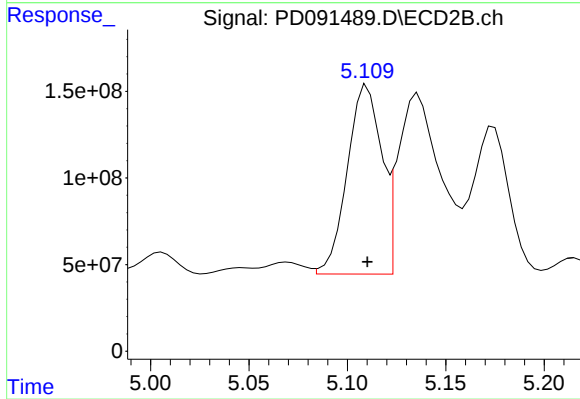

#25 Chlordane-3


R.T.: 5.110 min
Delta R.T.: 0.000 min
Response: 1319723838
Conc: 267.69 ng/ml

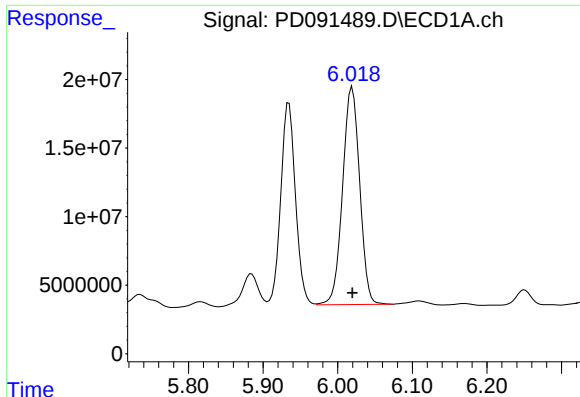

#26 Chlordane-4


R.T.: 6.019 min
Delta R.T.: 0.000 min
Response: 252045198
Conc: 252.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

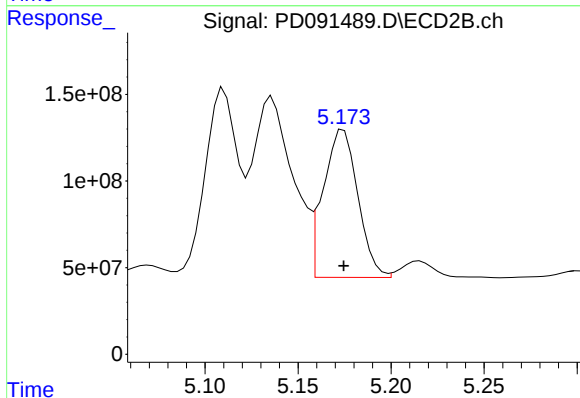


#26 Chlordane-4

R.T.: 5.175 min
Delta R.T.: 0.000 min
Response: 1101227253
Conc: 266.96 ng/ml

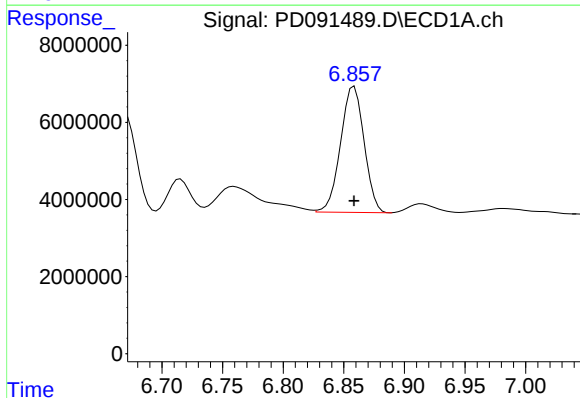


#27 Chlordane-5

R.T.: 6.859 min
Delta R.T.: 0.000 min
Response: 44091591
Conc: 254.02 ng/ml

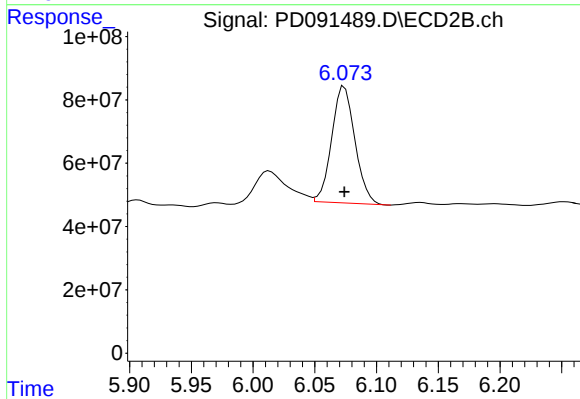

#27 Chlordane-5


R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 482868162
Conc: 265.37 ng/ml

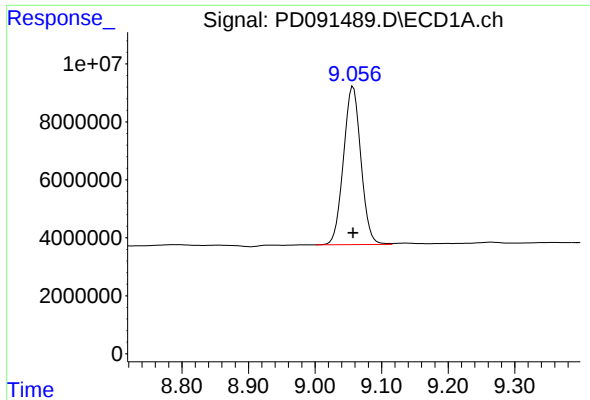

#28 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: 0.000 min
Response: 99065639
Conc: 27.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

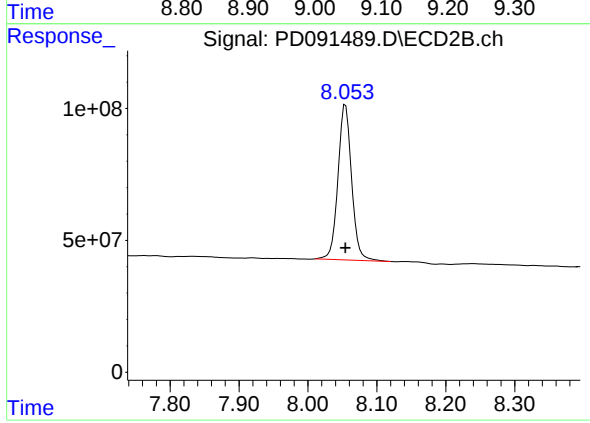

#28 Decachlorobiphenyl

R.T.: 8.055 min
Delta R.T.: 0.000 min
Response: 810512083
Conc: 26.56 ng/ml