

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120920\
 Data File : PD060664.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2020 13:00
 Operator : DD\AJ
 Sample : INDA336
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3036

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 02:36:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 04 03:58:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.505	4.023	23209320	88674637	19.866	22.544
27)	SA Decachlor...	8.296	9.110	58268617	139.0E6	39.086	42.943
Target Compounds							
2)	A alpha-BHC	3.947	4.414	33520726	130.4E6	19.905	22.099
3)	MA gamma-BHC...	4.232	4.699	32362995	122.8E6	20.064	22.909
4)	MA Heptachlor	4.539	5.211	34440604	120.1E6	20.509	22.826
9)	A Endosulfan I	5.578	6.263	29478443	95972602	20.289	22.421
13)	MA Dieldrin	5.823	6.521	64268892	207.4E6	40.469	44.407
14)	MA Endrin	6.082	6.739	55386869	171.5E6	42.807	46.536
16)	A 4,4'-DDD	6.206	6.858	51317204	159.4E6	39.939	43.271
17)	MA 4,4'-DDT	6.449	7.158	55580262	162.0E6	42.674	45.149
20)	A Methoxychlor	6.997	7.615	142.5E6	395.8E6	209.493	219.374

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD120920\
Data File : PD060664.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2020 13:00
Operator : DD\AJ
Sample : INDA336
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 02:36:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 04 03:58:39 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

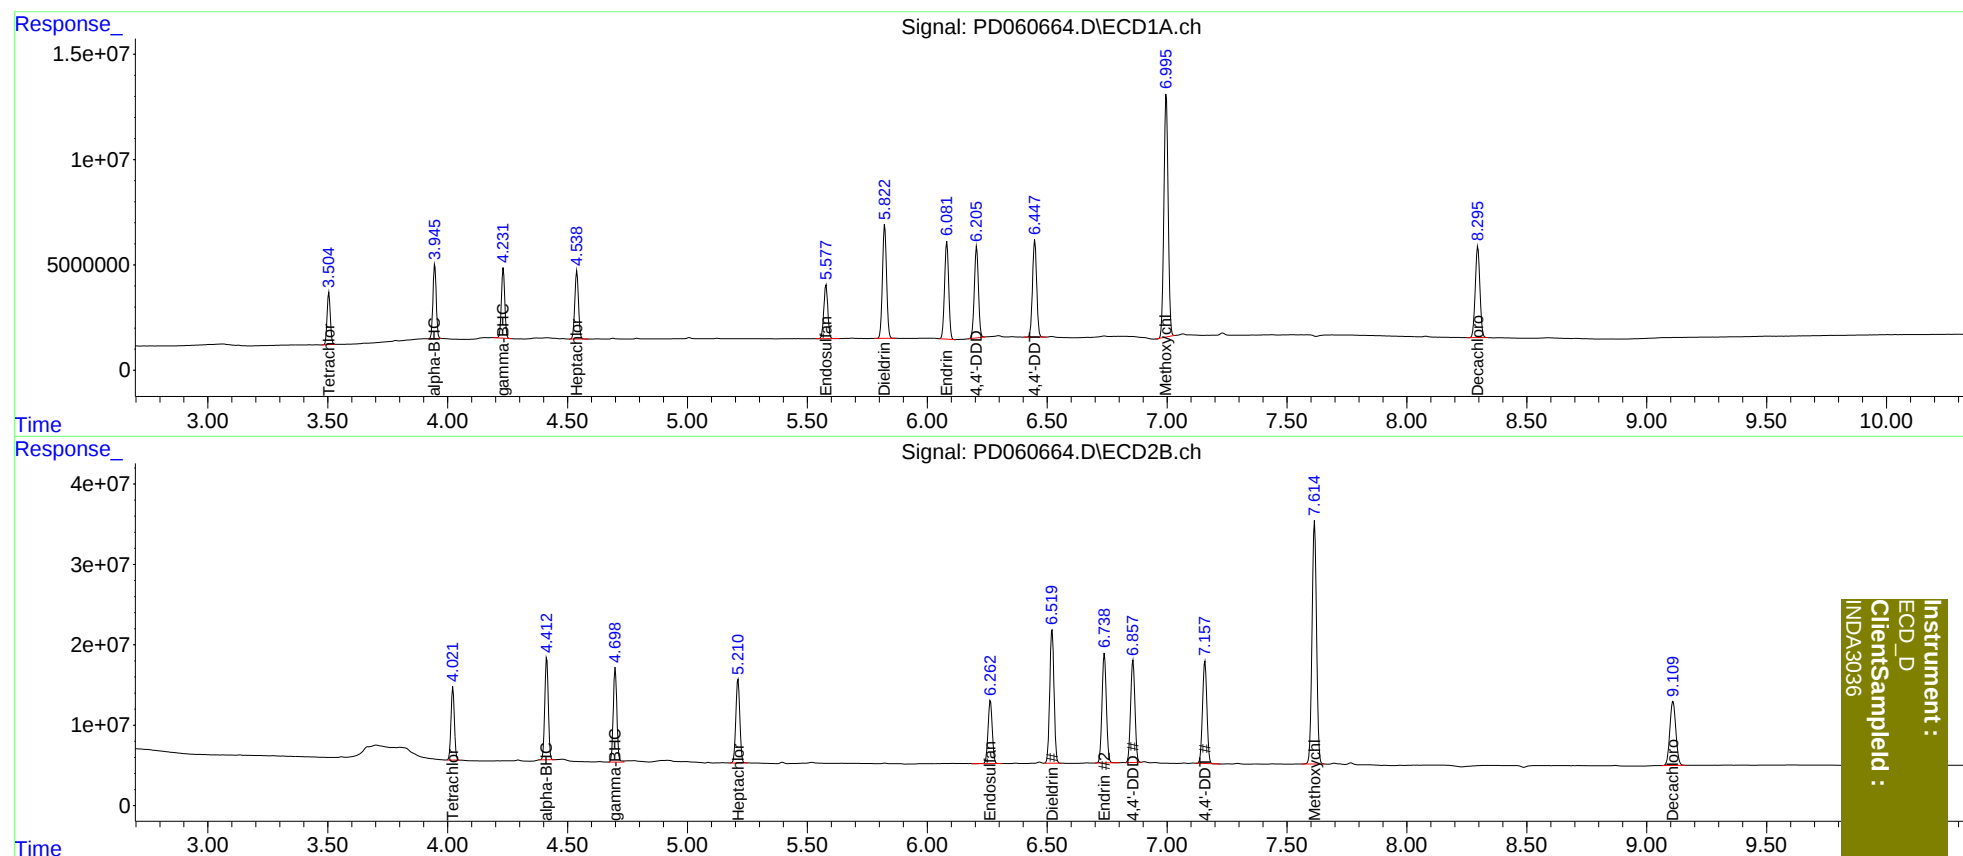

Instrument :
ECD_D
ClientSampled :
INDA3036