

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121018\
 Data File : PD050699.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Dec 2018 16:06
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 03:48:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111618.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 16 02:59:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	4.044	29864862	550.1E6	20.523	19.972
28)	SA Decachlor...	7.831	9.151	33414405	420.8E6	22.572	20.787
Target Compounds							
2)	A alpha-BHC	3.664	4.504f	1342038	197.6E6	0.572	4.657 #
3)	MA gamma-BHC...	3.922	0.000	1560925	0	0.669	N.D. #
4)	MA Heptachlor	4.132f	0.000	214500	0	0.097	N.D. #
6)	B beta-BHC	4.132	4.936f	214500	43509671	0.235	2.623 #
8)	B Heptachlo...	0.000	5.922	0	43617413	N.D.	1.372 #
12)	B 4,4'-DDE	0.000	6.465f	0	5729915	N.D.	0.195 #
14)	MA Endrin	5.678	0.000	281086	0	0.146	N.D. #
19)	B Endosulfa...	6.244f	0.000	579708	0	0.313	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121018\
Data File : PD050699.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Dec 2018 16:06
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 03:48:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111618.M
Quant Title : GC Extractables
QLast Update : Fri Nov 16 02:59:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

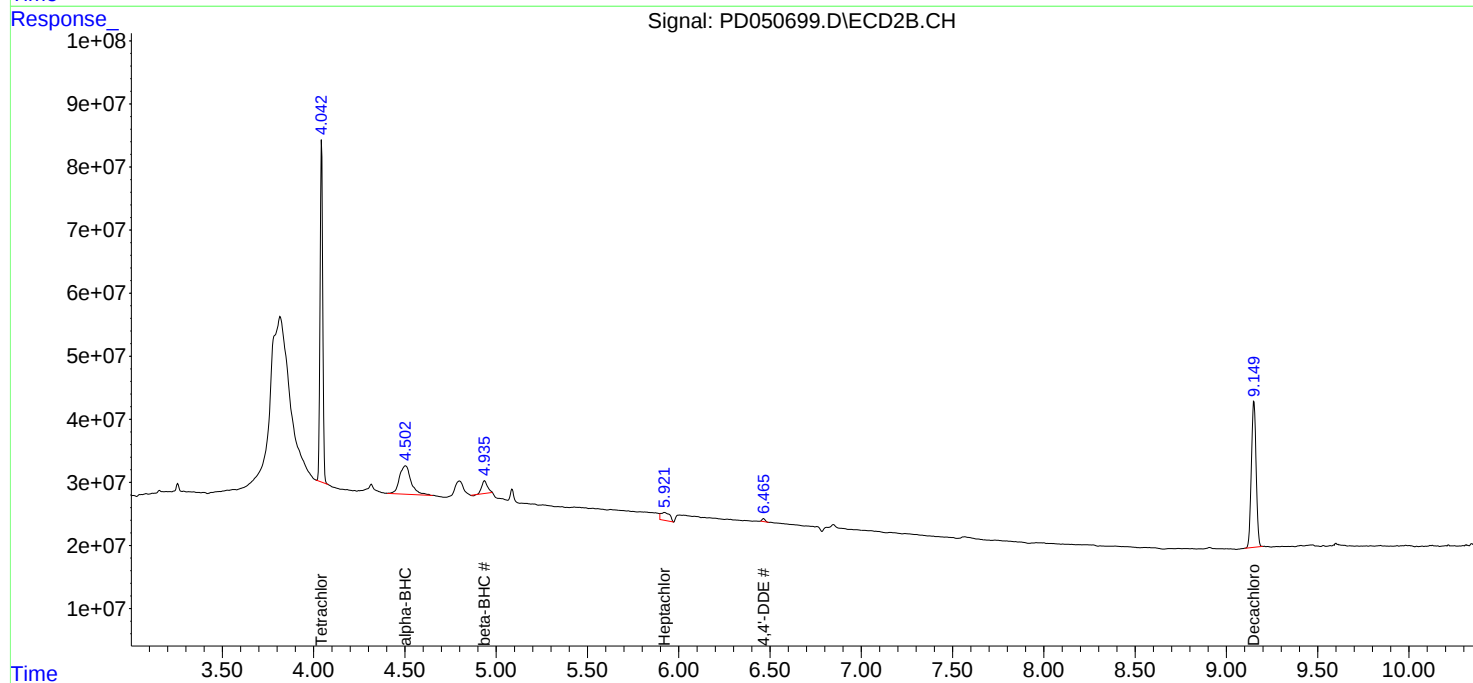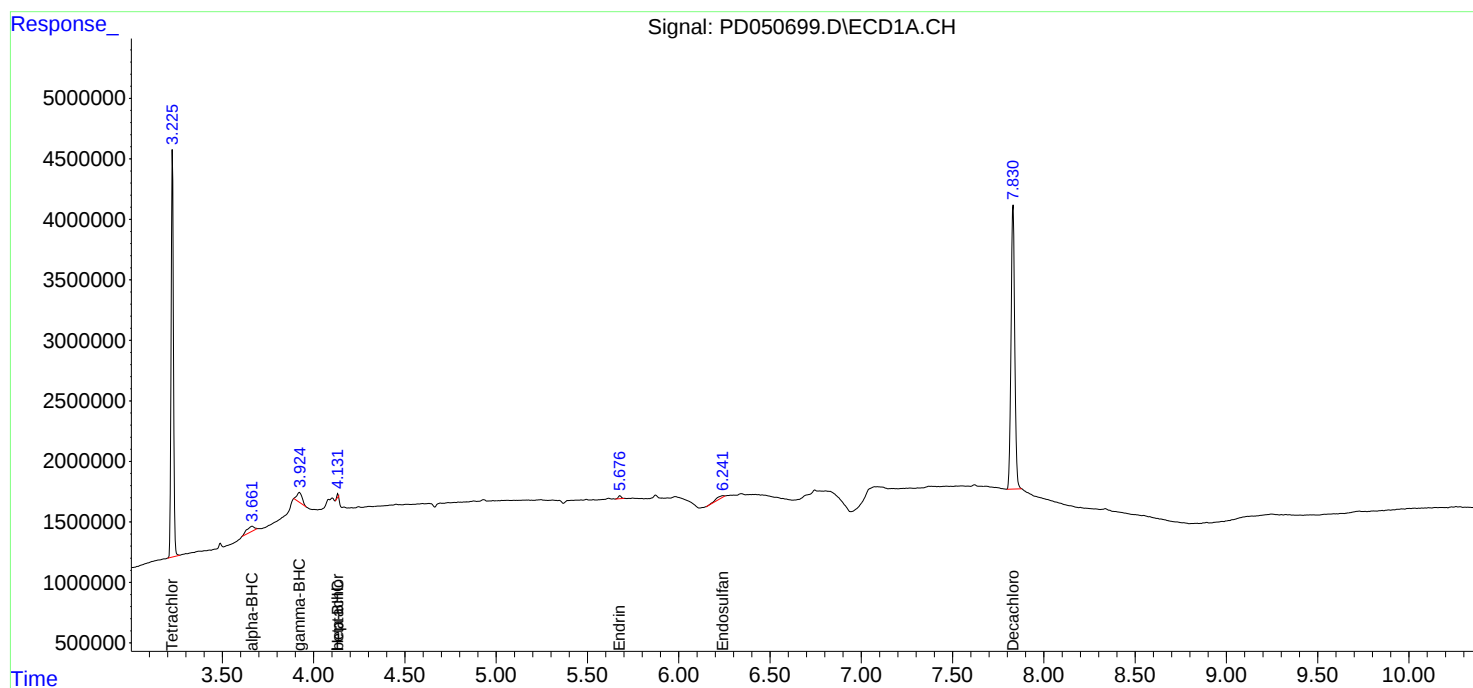


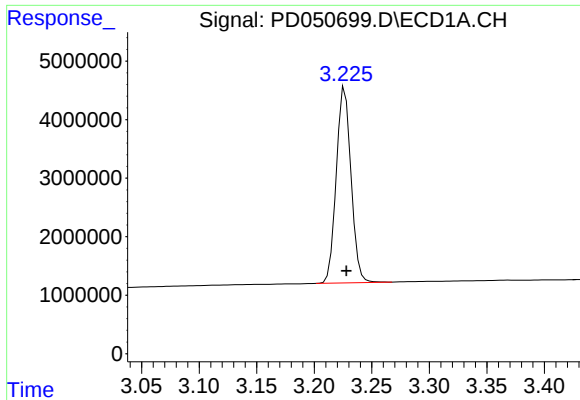

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: -0.001 min
Response: 29864862
Conc: 20.52 ng/ml

Instrument :
ECD_D
ClientSampleId :

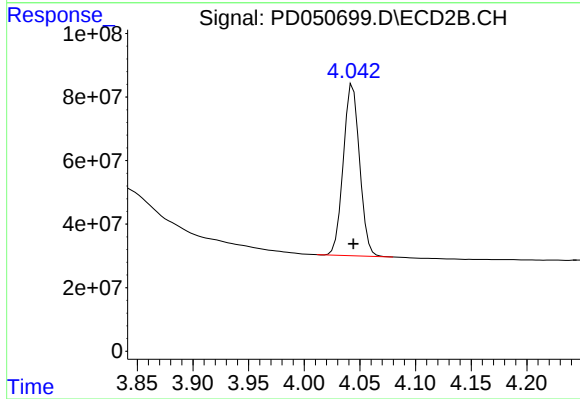


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 550090191
Conc: 19.97 ng/ml

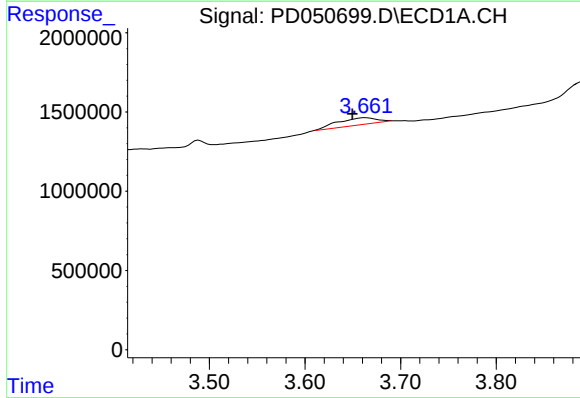


#2 alpha-BHC

R.T.: 3.664 min
Delta R.T.: 0.014 min
Response: 1342038
Conc: 0.57 ng/ml

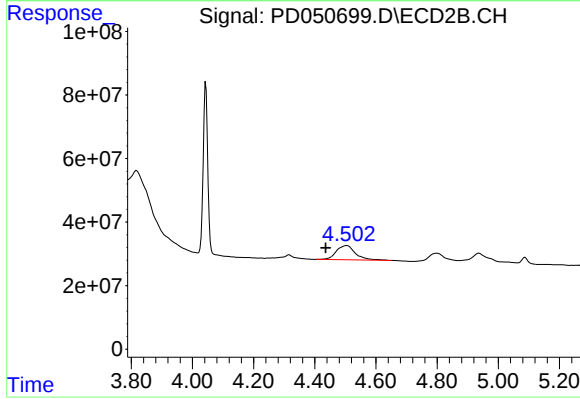

#2 alpha-BHC


R.T.: 4.504 min
Delta R.T.: 0.067 min
Response: 197647926
Conc: 4.66 ng/ml

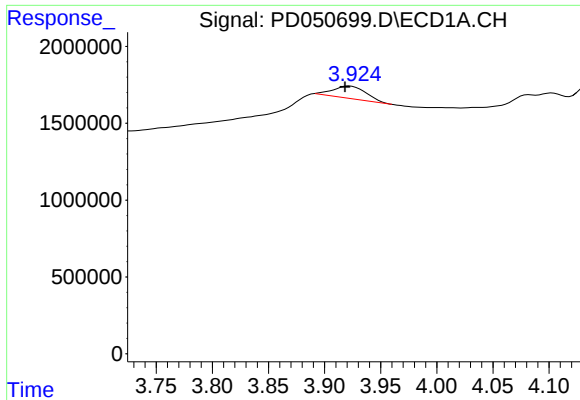

#3 gamma-BHC (Lindane)


R.T.: 3.922 min
Delta R.T.: 0.004 min
Response: 1560925
Conc: 0.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

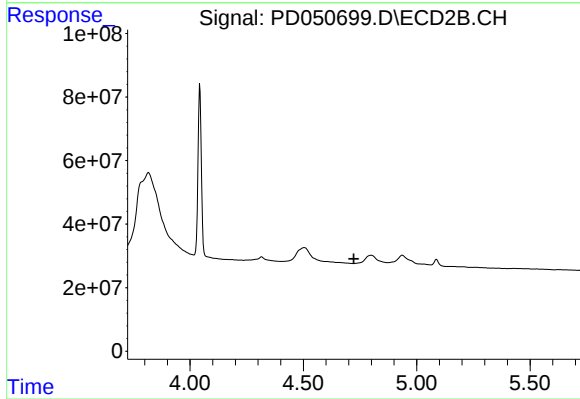


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

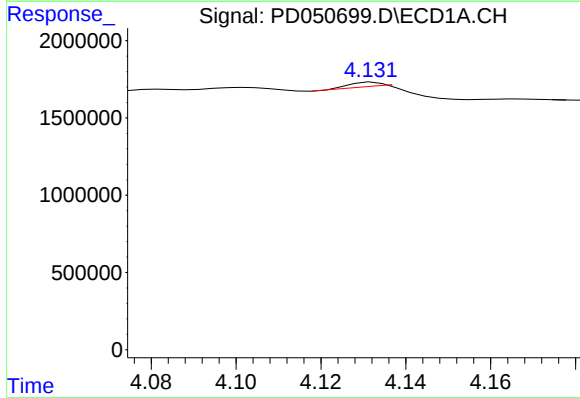


#4 Heptachlor

R.T.: 4.132 min
Delta R.T.: -0.065 min
Response: 214500
Conc: 0.10 ng/ml

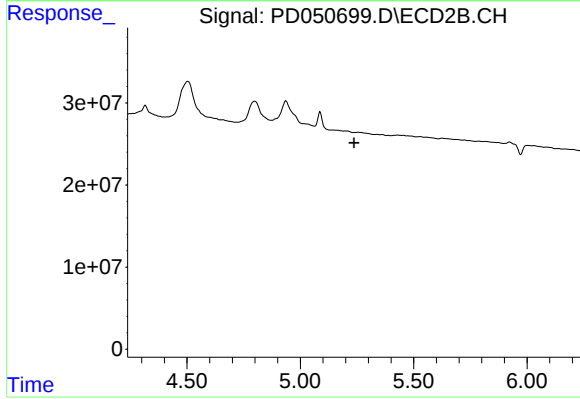

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.238 min
Response: 0
Conc: N.D.

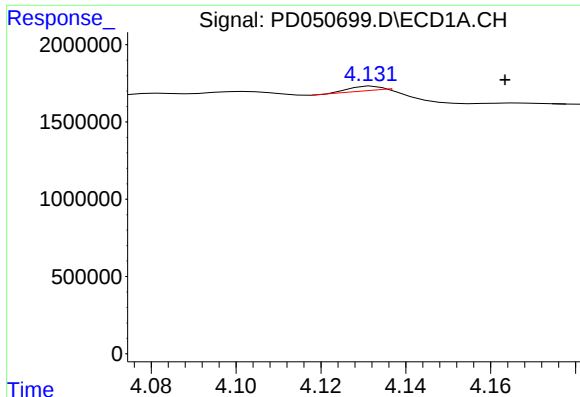

#6 beta-BHC


R.T.: 4.132 min
Delta R.T.: -0.031 min
Response: 214500
Conc: 0.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

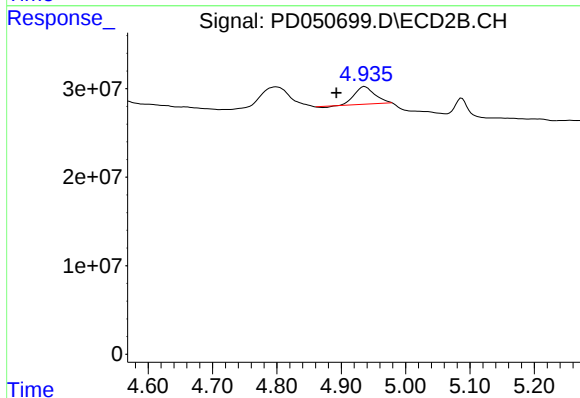


#6 beta-BHC

R.T.: 4.936 min
Delta R.T.: 0.044 min
Response: 43509671
Conc: 2.62 ng/ml

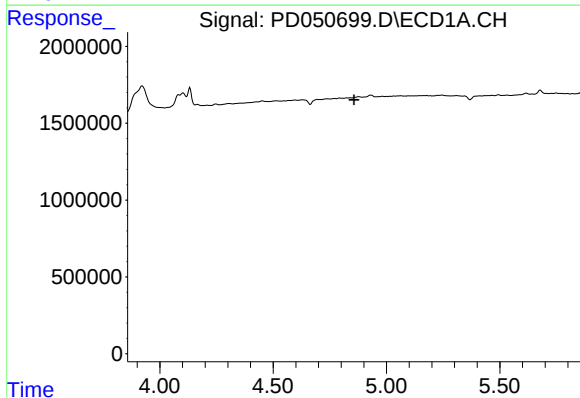


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.858 min
Response: 0
Conc: N.D.

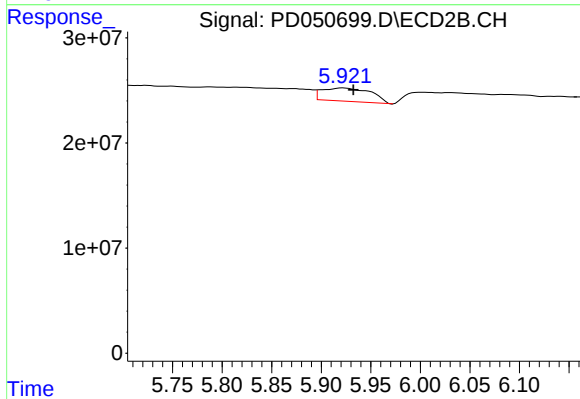

#8 Heptachlor epoxide


R.T.: 5.922 min
Delta R.T.: -0.010 min
Response: 43617413
Conc: 1.37 ng/ml

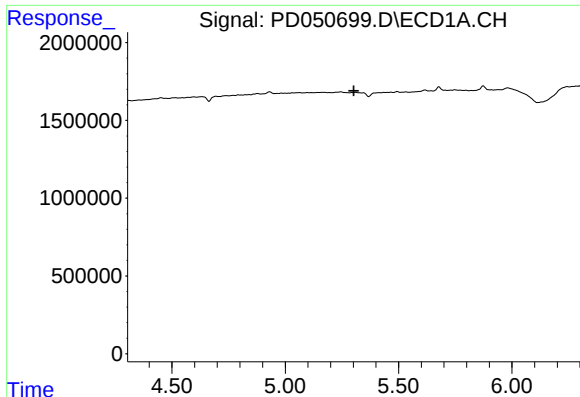

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.302 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

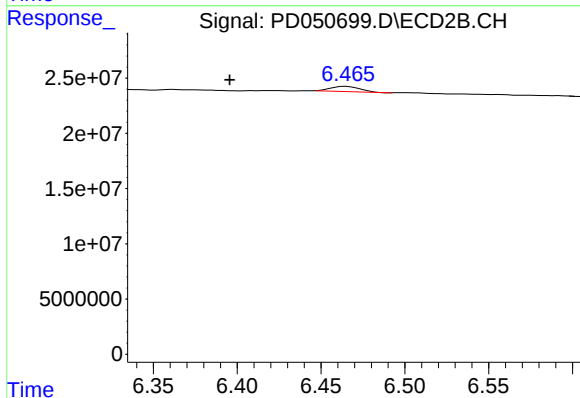


#12 4,4'-DDE

R.T.: 6.465 min
Delta R.T.: 0.069 min
Response: 5729915
Conc: 0.19 ng/ml

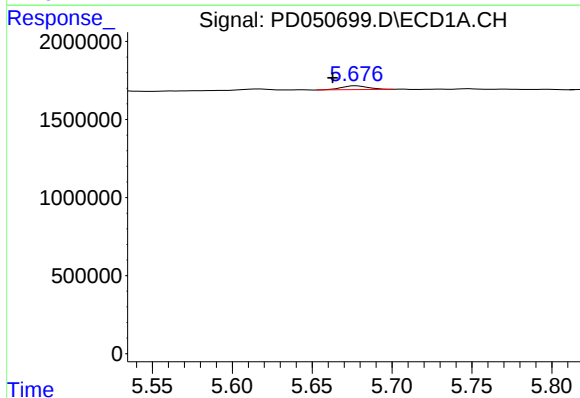


#14 Endrin

R.T.: 5.678 min
Delta R.T.: 0.015 min
Response: 281086
Conc: 0.15 ng/ml

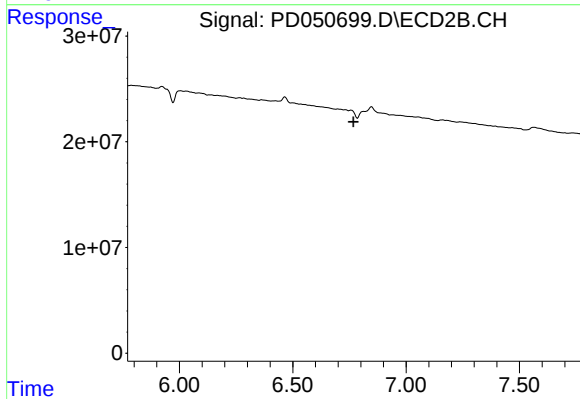

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.768 min
Response: 0
Conc: N.D.

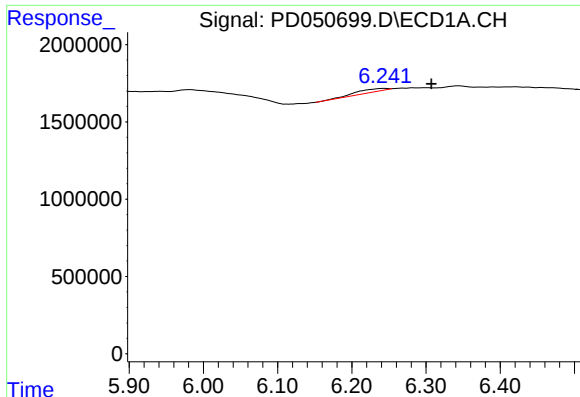

#19 Endosulfan Sulfate


R.T.: 6.244 min
Delta R.T.: -0.064 min
Response: 579708
Conc: 0.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

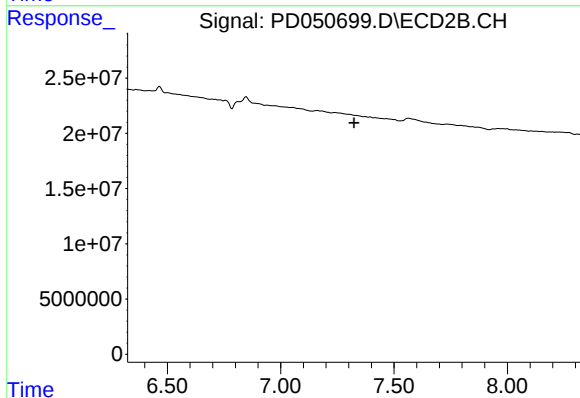


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.324 min
Response: 0
Conc: N.D.

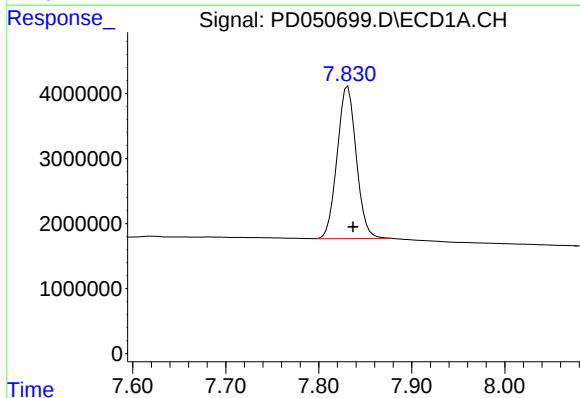

#28 Decachlorobiphenyl

R.T.: 7.831 min
Delta R.T.: -0.005 min
Response: 33414405
Conc: 22.57 ng/ml

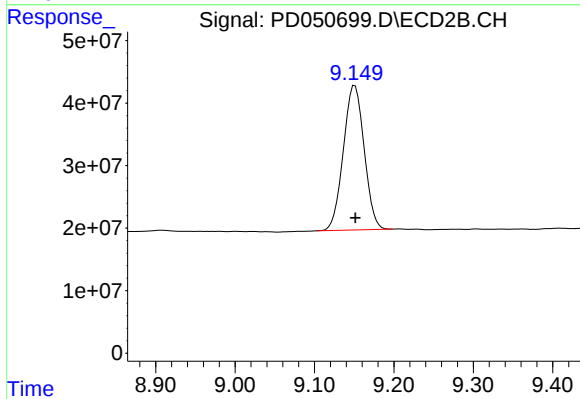

#28 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: 0.000 min
Response: 420768073
Conc: 20.79 ng/ml