

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121018\
 Data File : PD050726.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Dec 2018 22:23
 Operator : AJ\SJ
 Sample : J6316-14
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 03:52:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111618.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 16 02:59:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	4.044	31530769	505.5E6	21.668	18.352
28)	SA Decachlor...	7.830	9.149	28832312	372.3E6	19.477	18.392
Target Compounds							
2)	A alpha-BHC	3.665	0.000	721152	0	0.307	N.D. #
4)	MA Heptachlor	0.000	5.212	0	3382137	N.D.	0.089 #
5)	MB Aldrin	4.450	0.000	837543	0	0.365	N.D. #
6)	B beta-BHC	0.000	4.844f	0	3010074	N.D.	0.181 #
8)	B Heptachlo...	0.000	5.920	0	3325706	N.D.	0.105 #
14)	MA Endrin	0.000	6.770	0	2228352	N.D.	0.092 #
16)	A 4,4'-DDD	0.000	6.845f	0	128866	N.D.	0.006 #
23)	Chlordane-1	4.079	0.000	163283	0	2.424	N.D. #
24)	Chlordane-2	4.507	0.000	429694	0	5.460	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121018\
Data File : PD050726.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Dec 2018 22:23
Operator : AJ\SJ
Sample : J6316-14
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 03:52:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111618.M
Quant Title : GC Extractables
QLast Update : Fri Nov 16 02:59:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

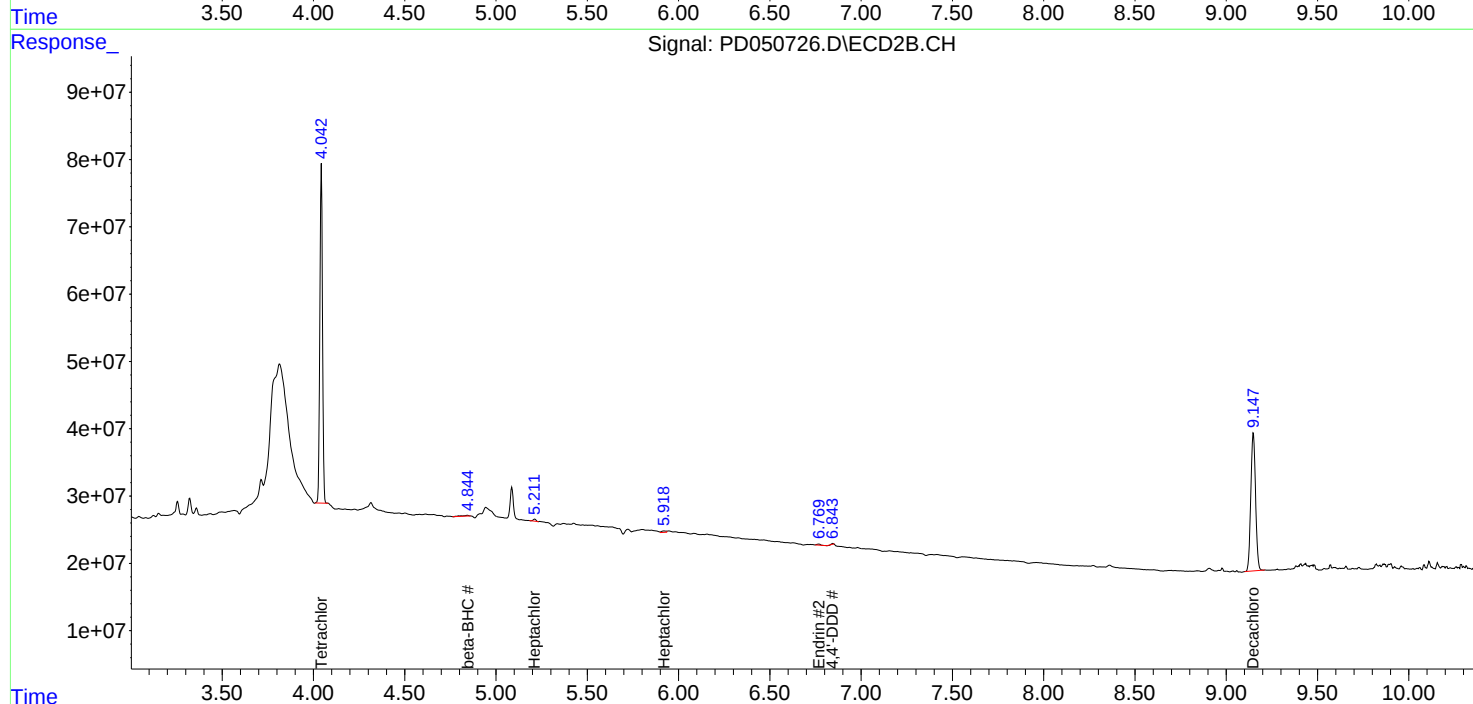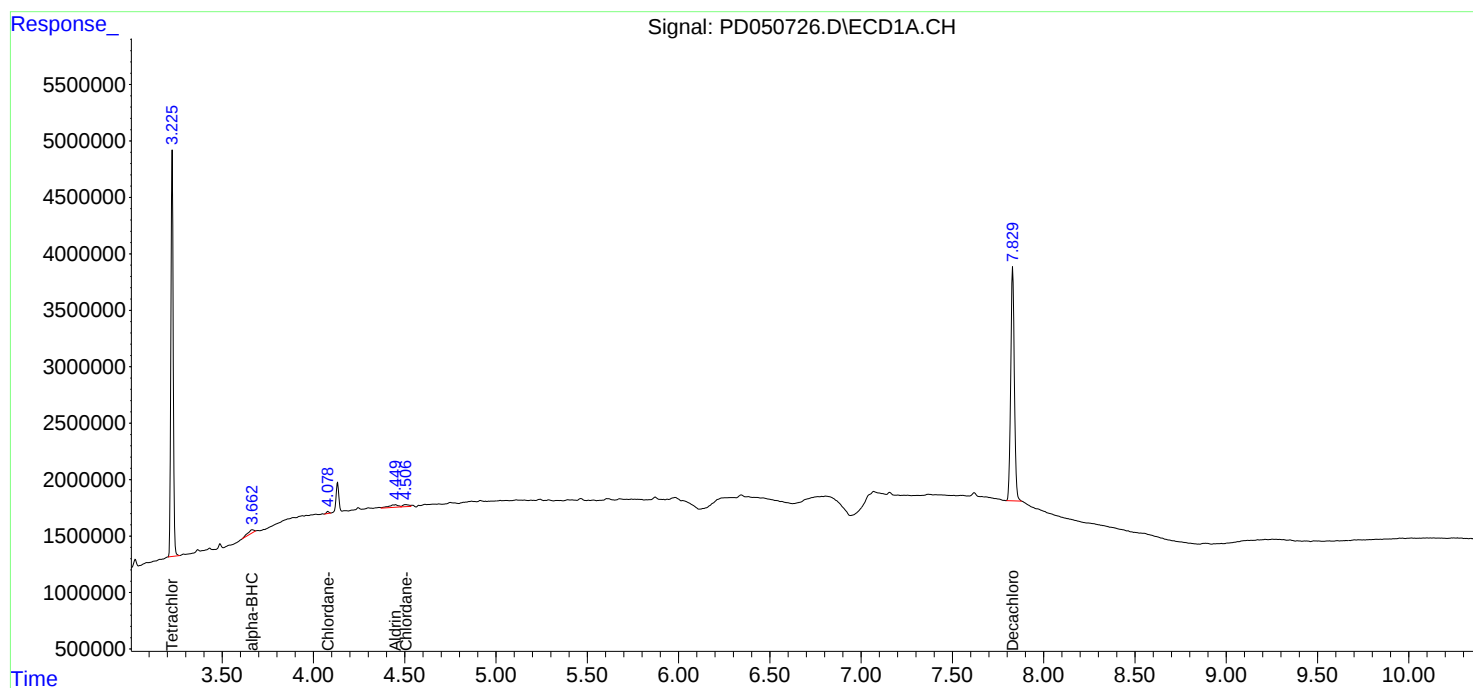


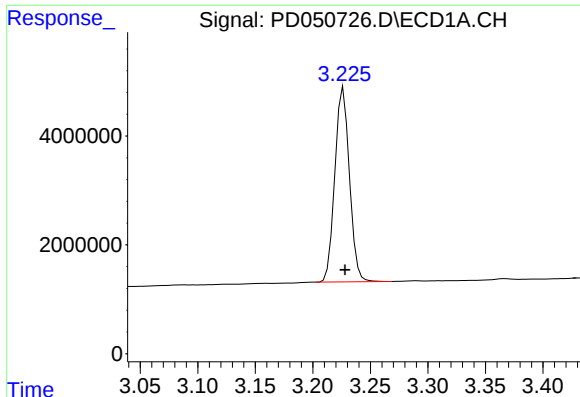

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: -0.001 min
Response: 31530769
Conc: 21.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

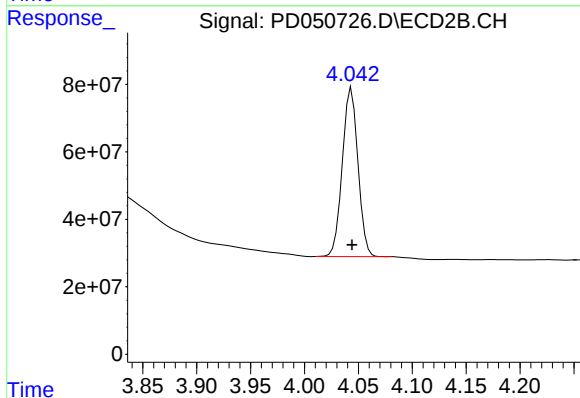


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 505480617
Conc: 18.35 ng/ml

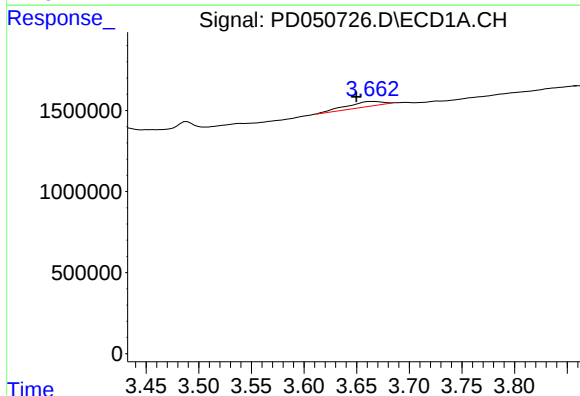


#2 alpha-BHC

R.T.: 3.665 min
Delta R.T.: 0.015 min
Response: 721152
Conc: 0.31 ng/ml

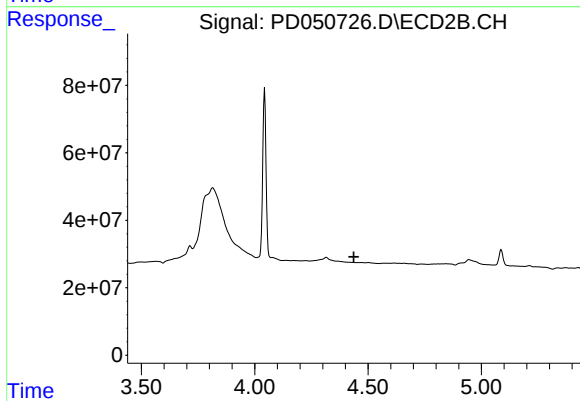

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.436 min
Response: 0
Conc: N.D.

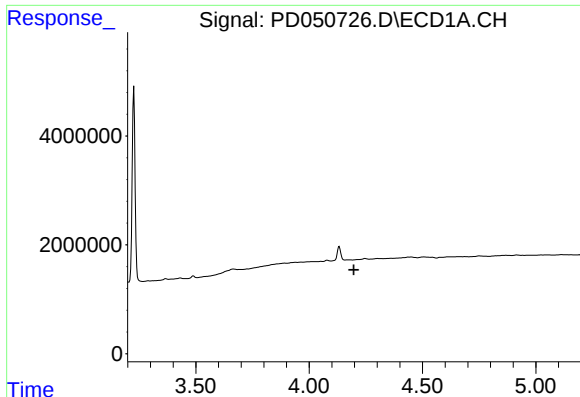

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.197 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

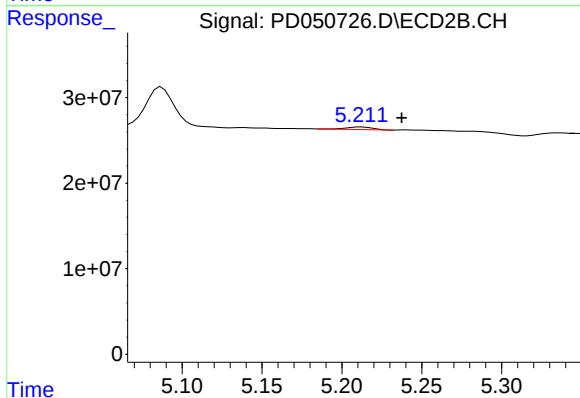


#4 Heptachlor

R.T.: 5.212 min
Delta R.T.: -0.025 min
Response: 3382137
Conc: 0.09 ng/ml

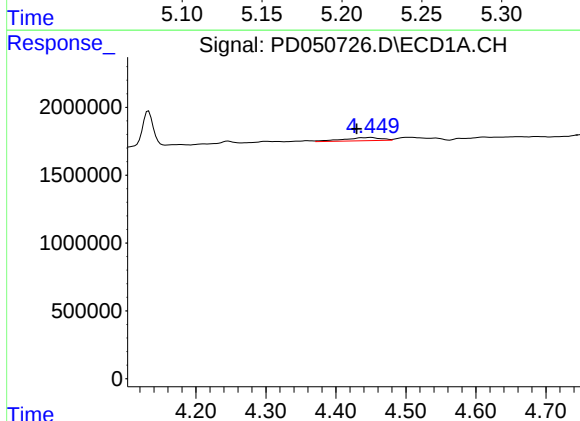


#5 Aldrin

R.T.: 4.450 min
Delta R.T.: 0.021 min
Response: 837543
Conc: 0.37 ng/ml

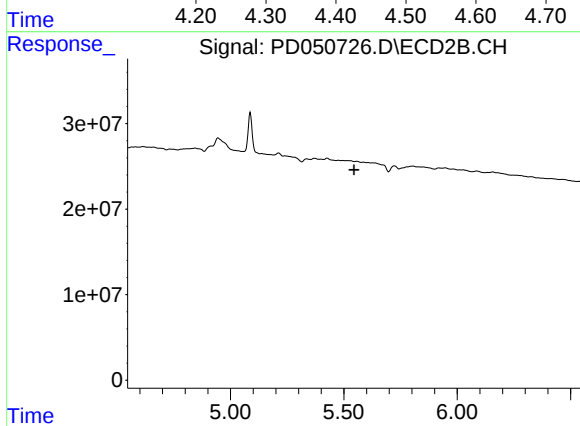

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

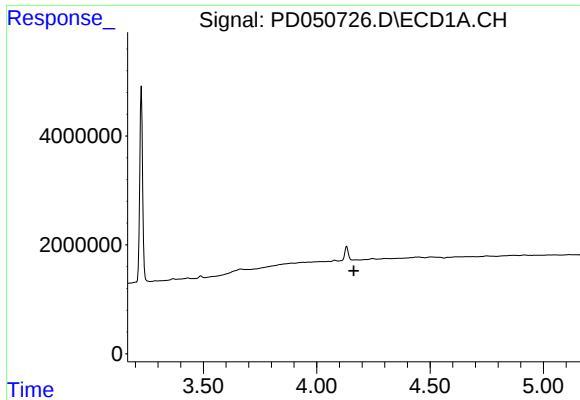

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

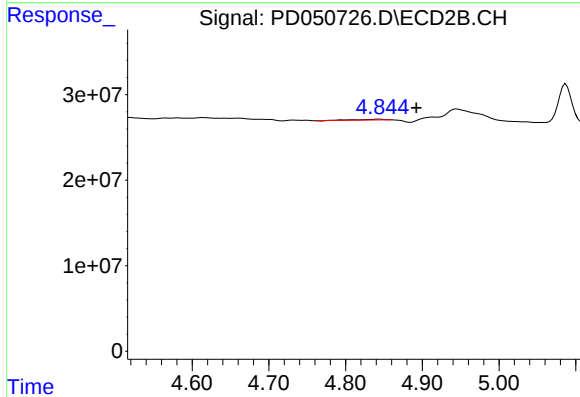


#6 beta-BHC

R.T.: 4.844 min
Delta R.T.: -0.048 min
Response: 3010074
Conc: 0.18 ng/ml

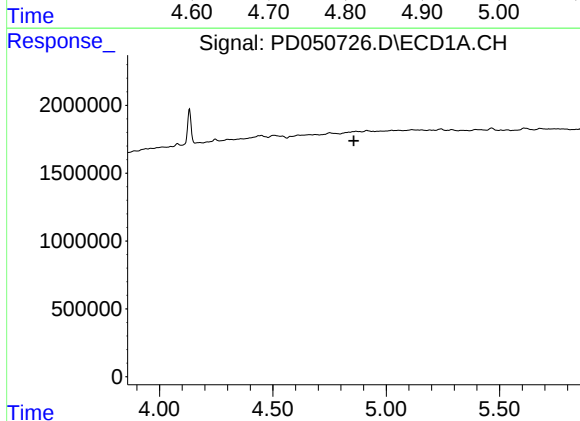


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.858 min
Response: 0
Conc: N.D.

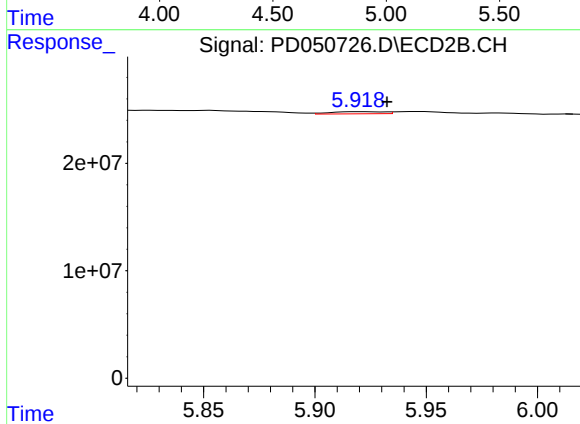

#8 Heptachlor epoxide


R.T.: 5.920 min
Delta R.T.: -0.013 min
Response: 3325706
Conc: 0.10 ng/ml

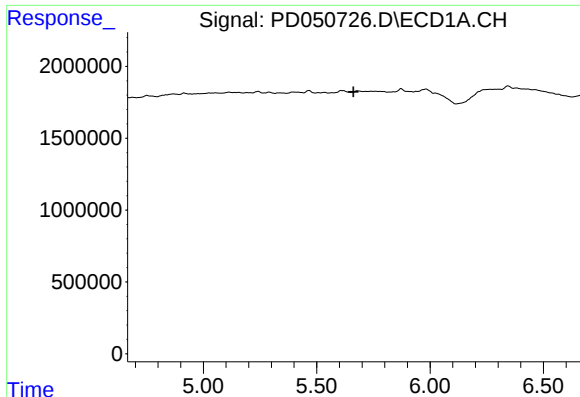

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.663 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

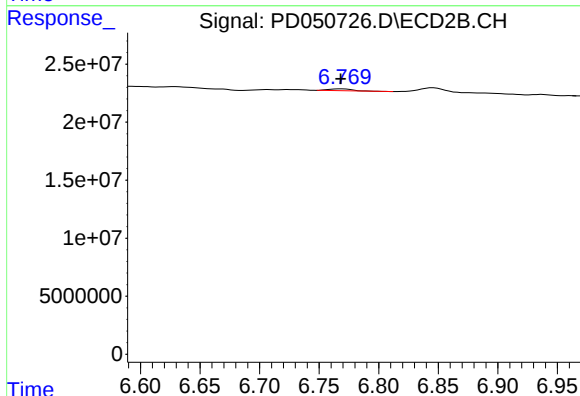


#14 Endrin

R.T.: 6.770 min
Delta R.T.: 0.002 min
Response: 2228352
Conc: 0.09 ng/ml

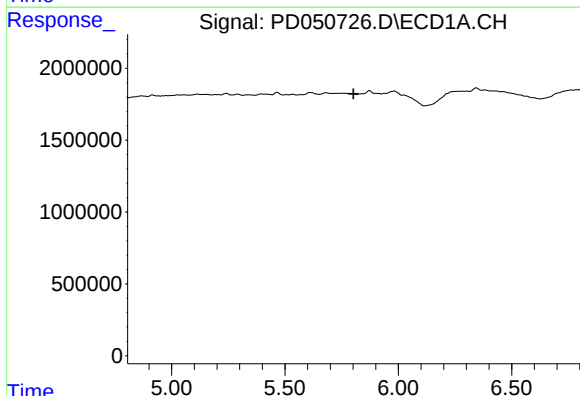


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.803 min
Response: 0
Conc: N.D.

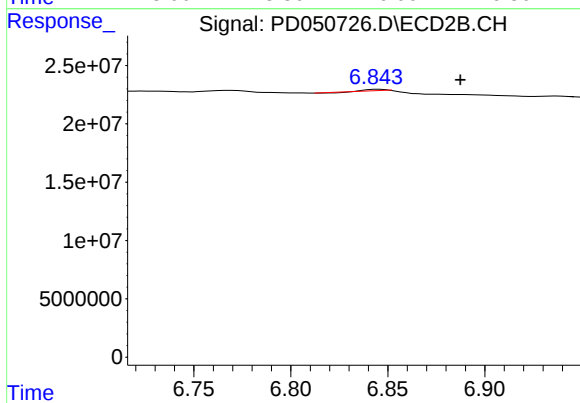

#16 4,4'-DDD


R.T.: 6.845 min
Delta R.T.: -0.042 min
Response: 128866
Conc: 0.01 ng/ml

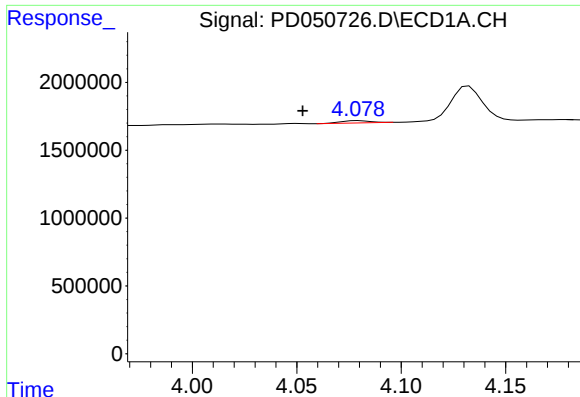

#23 Chlordane-1


R.T.: 4.079 min
Delta R.T.: 0.027 min
Response: 163283
Conc: 2.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

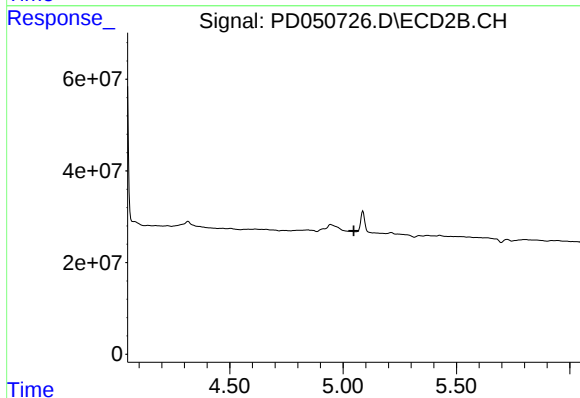


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.048 min
Response: 0
Conc: N.D.

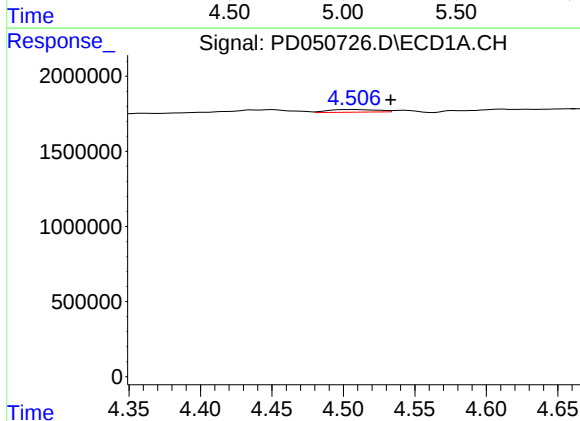


#24 Chlordane-2

R.T.: 4.507 min
Delta R.T.: -0.026 min
Response: 429694
Conc: 5.46 ng/ml

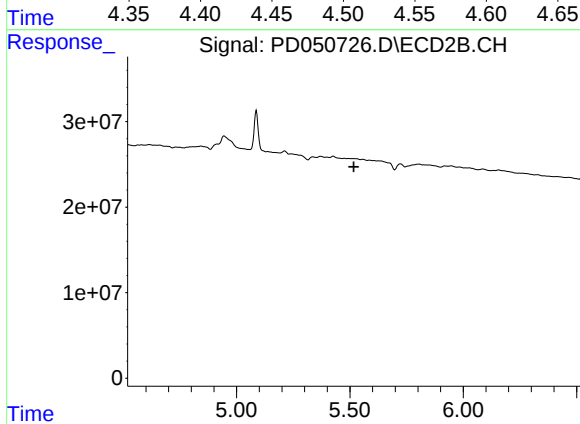

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.518 min
Response: 0
Conc: N.D.

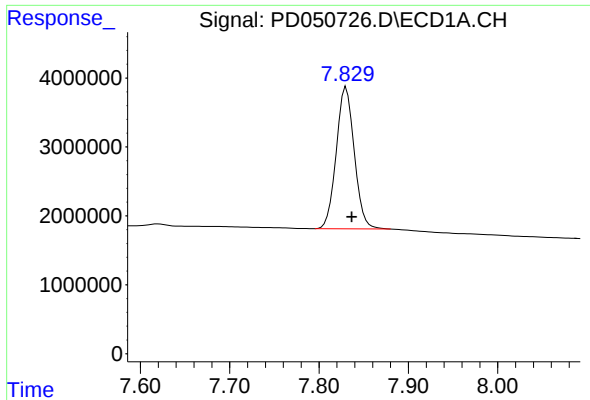

#28 Decachlorobiphenyl

R.T.: 7.830 min
Delta R.T.: -0.006 min
Response: 28832312
Conc: 19.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

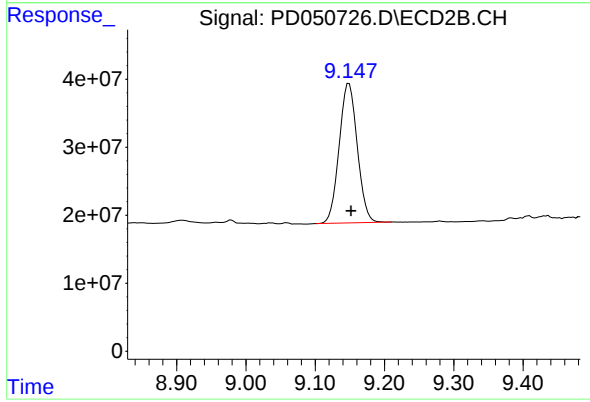

#28 Decachlorobiphenyl

R.T.: 9.149 min
Delta R.T.: -0.003 min
Response: 372287035
Conc: 18.39 ng/ml