

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121018\
 Data File : PD050728.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Dec 2018 22:51
 Operator : AJ\SJ
 Sample : J6316-22
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 03:53:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111618.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 16 02:59:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	4.043	29753297	506.0E6	20.446	18.370
28)	SA Decachlor...	7.830	9.149	28436471	373.4E6	19.209	18.446
Target Compounds							
2)	A alpha-BHC	3.666	4.499f	637186	1892889	0.271	0.045 #
5)	MB Aldrin	4.424	0.000	135523	0	0.059	N.D. #
6)	B beta-BHC	4.133	4.848f	-75259	2099028	N.D.	0.127
10)	B gamma-Chl...	0.000	6.154	0	9680981	N.D.	0.305 #
14)	MA Endrin	0.000	6.768	0	2868364	N.D.	0.119 #
16)	A 4,4'-DDD	0.000	6.846f	0	599283	N.D.	0.026 #
23)	Chlordane-1	4.079	0.000	145675	0	2.163	N.D. #
24)	Chlordane-2	0.000	5.459	0	417105	N.D.	0.334 #
25)	Chlordane-3	0.000	6.154	0	9680981	N.D.	2.403 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121018\
Data File : PD050728.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Dec 2018 22:51
Operator : AJ\SJ
Sample : J6316-22
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 03:53:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111618.M
Quant Title : GC Extractables
QLast Update : Fri Nov 16 02:59:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

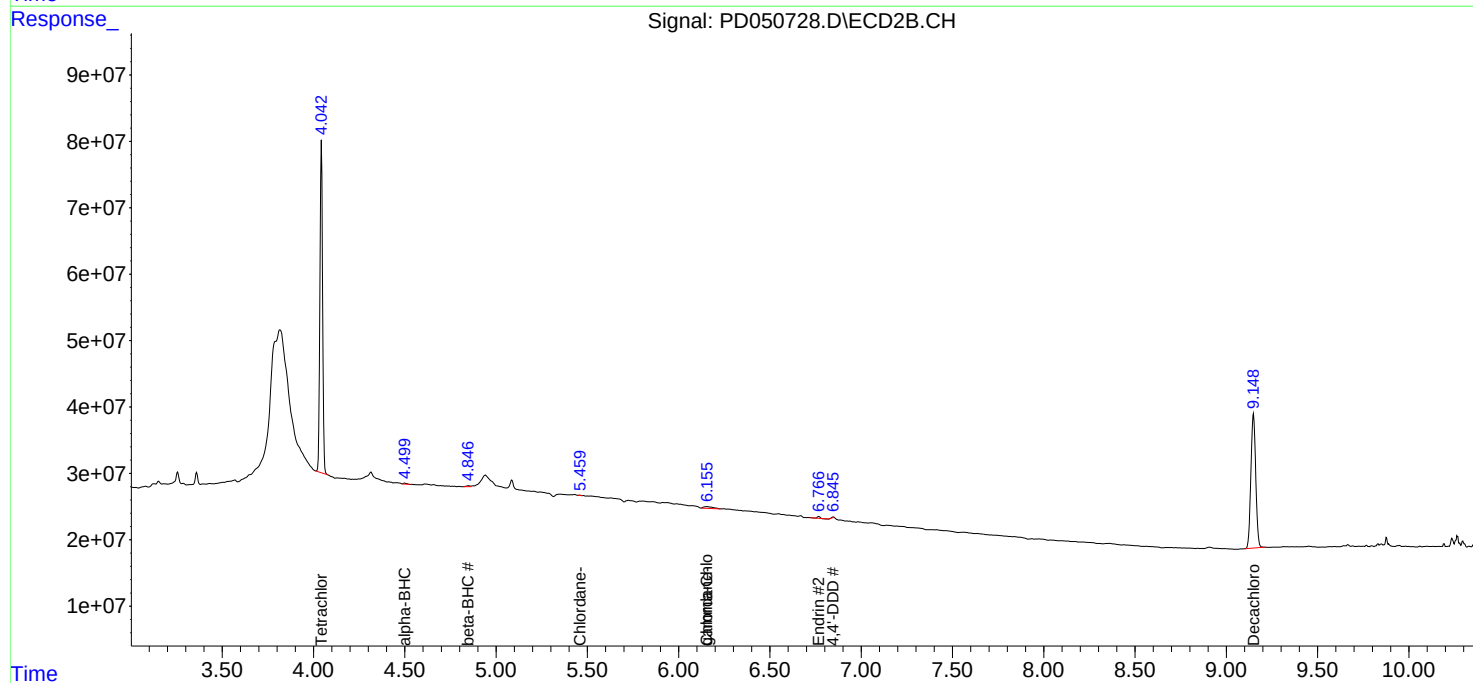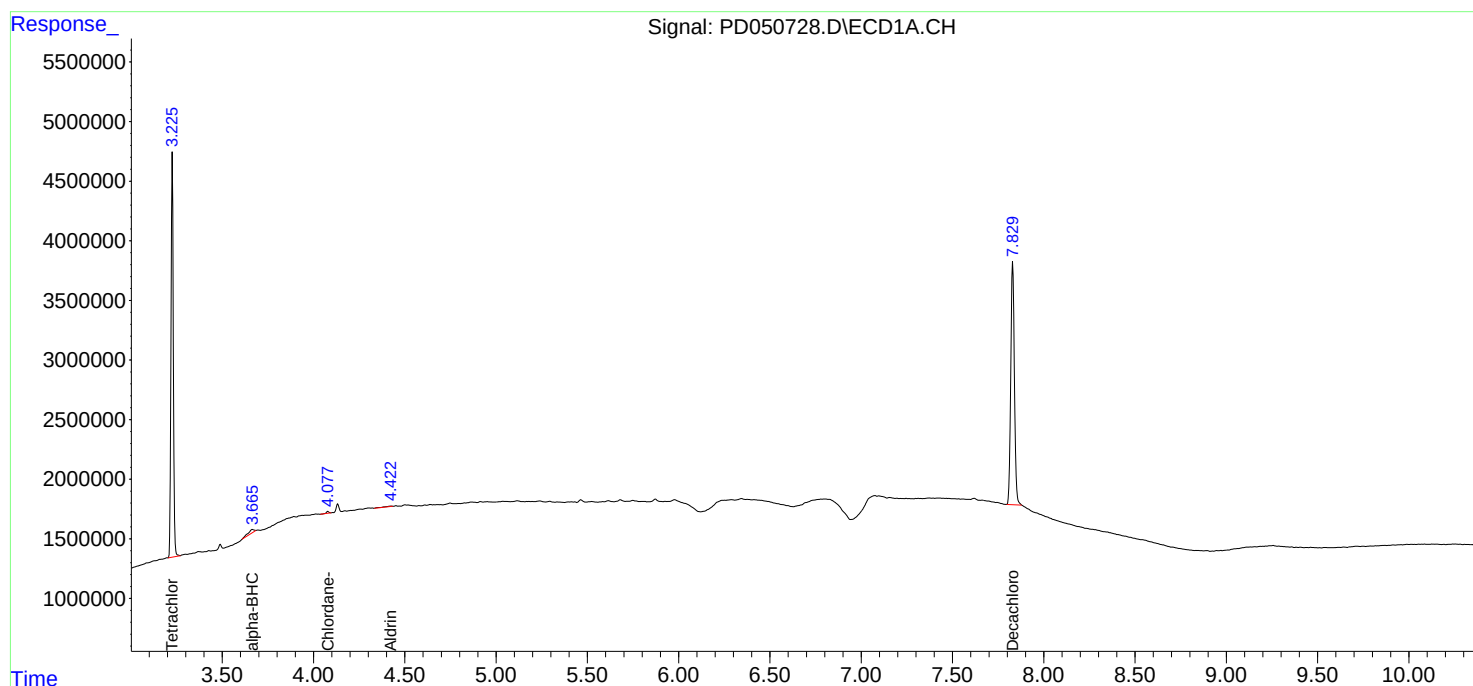


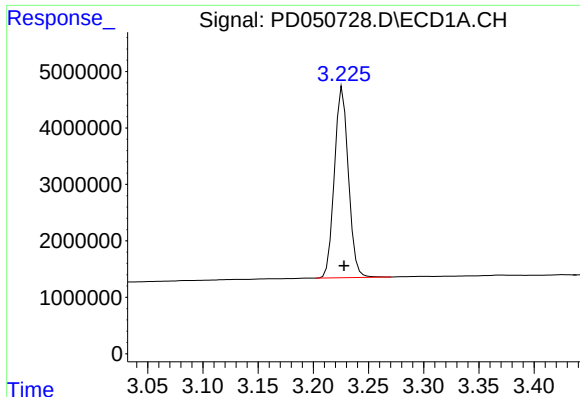

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: -0.001 min
Response: 29753297
Conc: 20.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

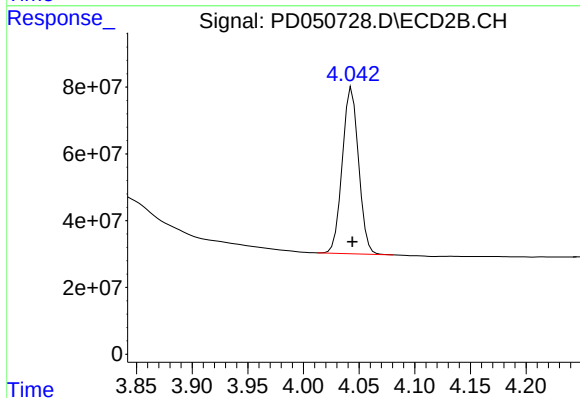


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 505988273
Conc: 18.37 ng/ml

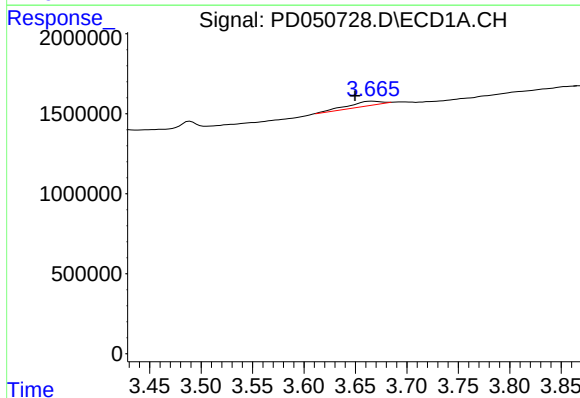


#2 alpha-BHC

R.T.: 3.666 min
Delta R.T.: 0.016 min
Response: 637186
Conc: 0.27 ng/ml

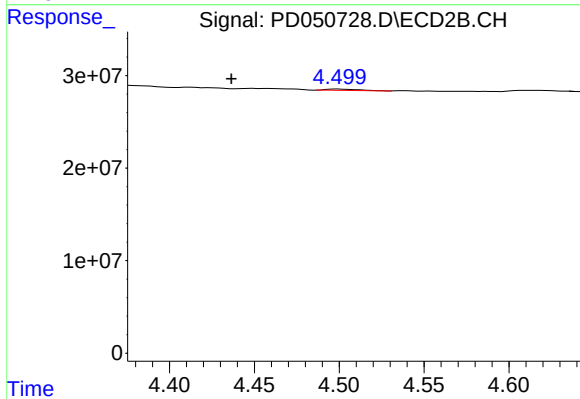

#2 alpha-BHC


R.T.: 4.499 min
Delta R.T.: 0.063 min
Response: 1892889
Conc: 0.04 ng/ml

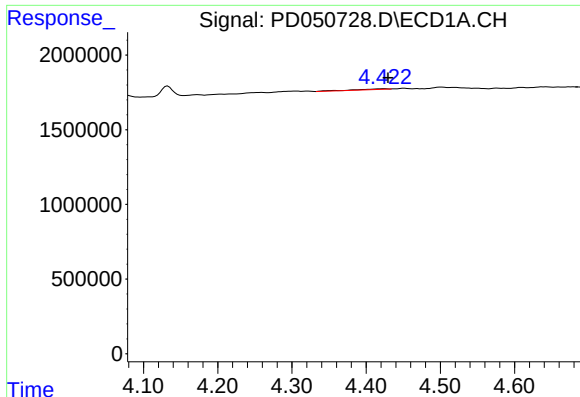

#5 Aldrin


R.T.: 4.424 min
Delta R.T.: -0.005 min
Response: 135523
Conc: 0.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

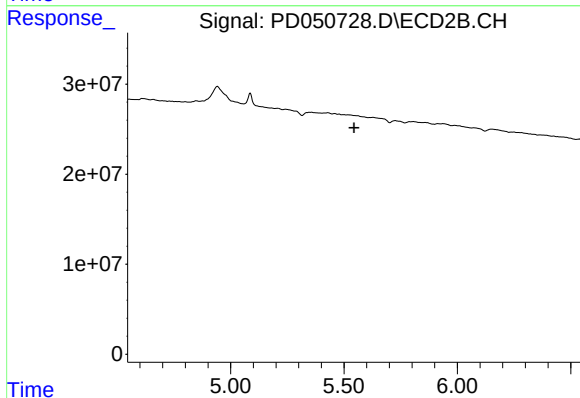


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.545 min
Response: 0
Conc: N.D.

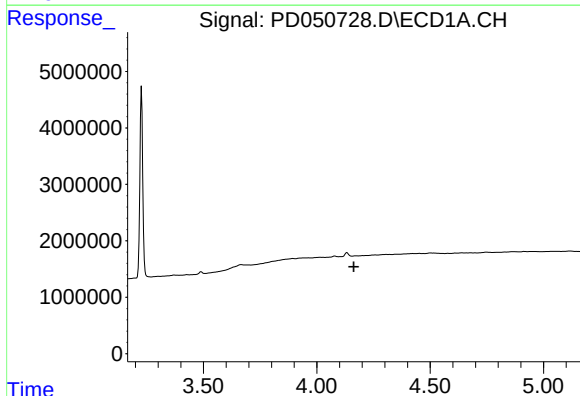


#6 beta-BHC

R.T.: 4.133 min
Delta R.T.: -0.031 min
Response: -75259
Conc: N.D.

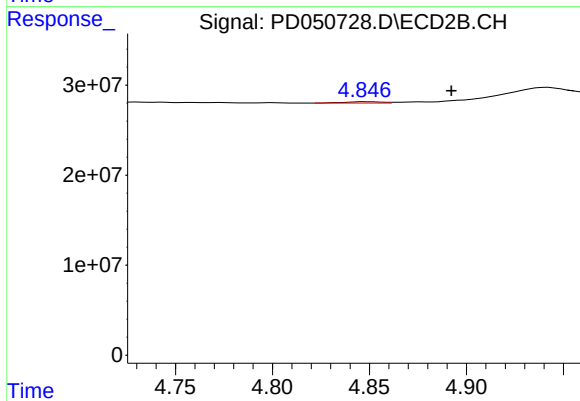

#6 beta-BHC


R.T.: 4.848 min
Delta R.T.: -0.044 min
Response: 2099028
Conc: 0.13 ng/ml

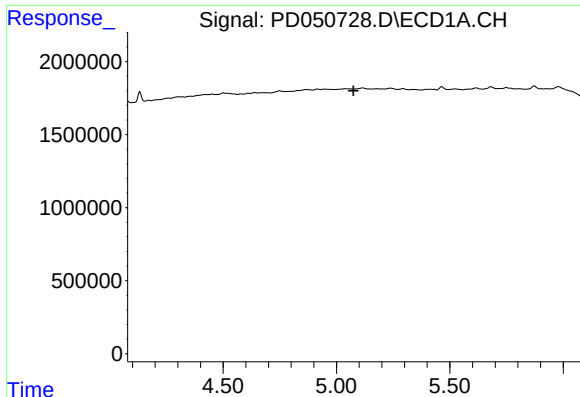

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.075 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

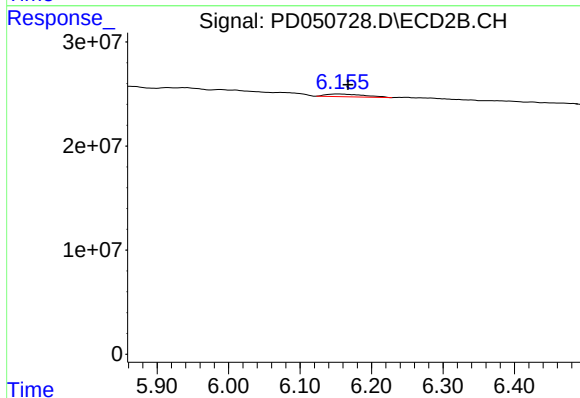


#10 gamma-Chlordane

R.T.: 6.154 min
Delta R.T.: -0.013 min
Response: 9680981
Conc: 0.31 ng/ml

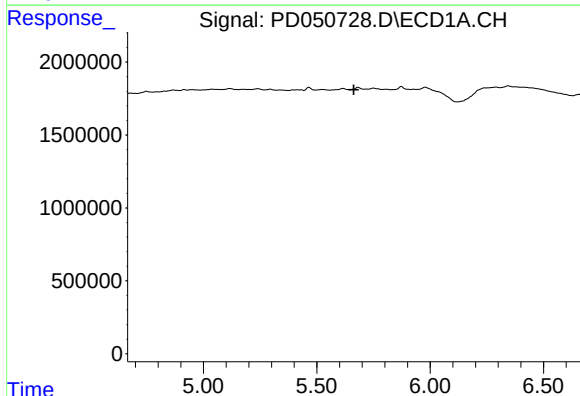


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.663 min
Response: 0
Conc: N.D.

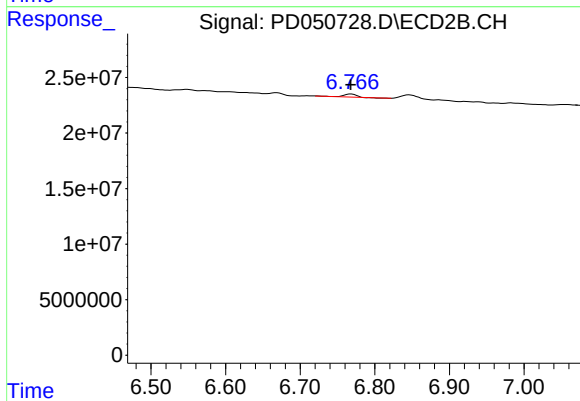

#14 Endrin


R.T.: 6.768 min
Delta R.T.: 0.000 min
Response: 2868364
Conc: 0.12 ng/ml

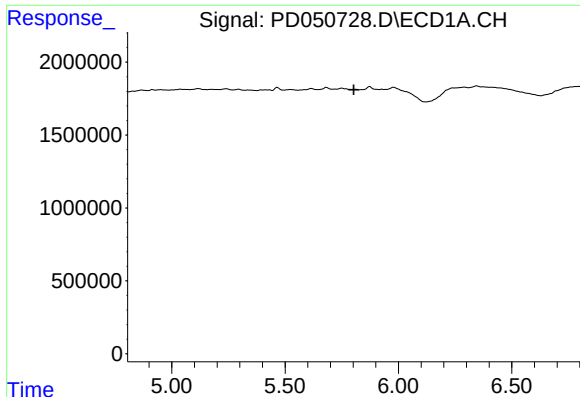

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.803 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

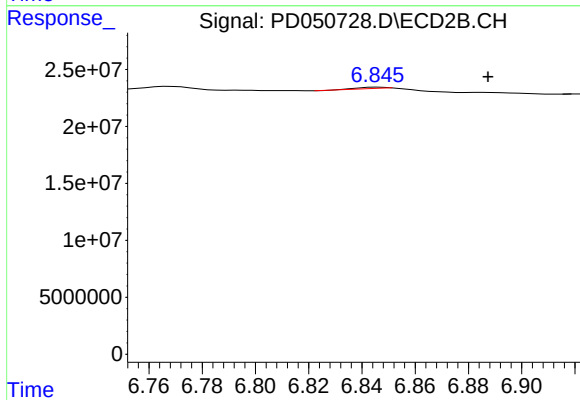


#16 4,4'-DDD

R.T.: 6.846 min
Delta R.T.: -0.041 min
Response: 599283
Conc: 0.03 ng/ml

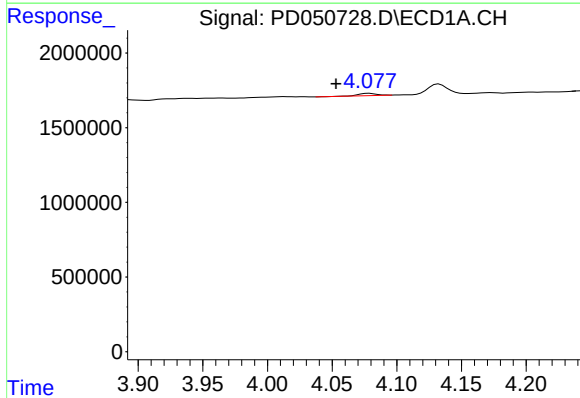


#23 Chlordane-1

R.T.: 4.079 min
Delta R.T.: 0.026 min
Response: 145675
Conc: 2.16 ng/ml

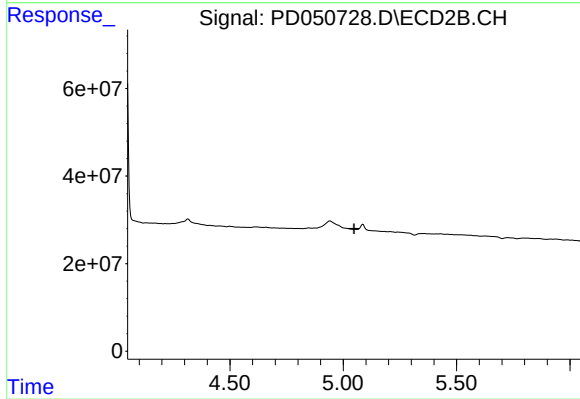

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.048 min
Response: 0
Conc: N.D.

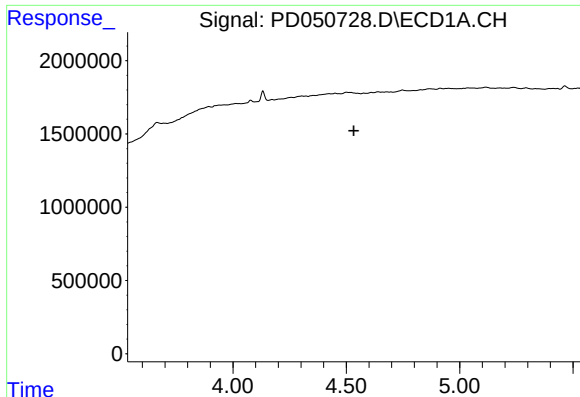

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.533 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

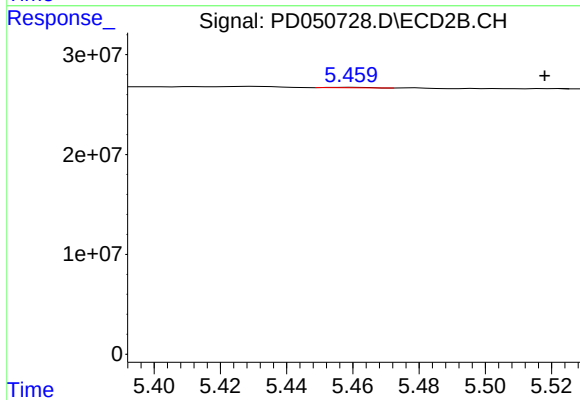


#24 Chlordane-2

R.T.: 5.459 min
Delta R.T.: -0.059 min
Response: 417105
Conc: 0.33 ng/ml

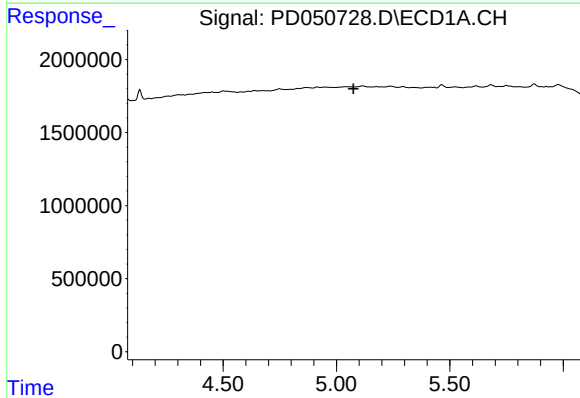


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.076 min
Response: 0
Conc: N.D.

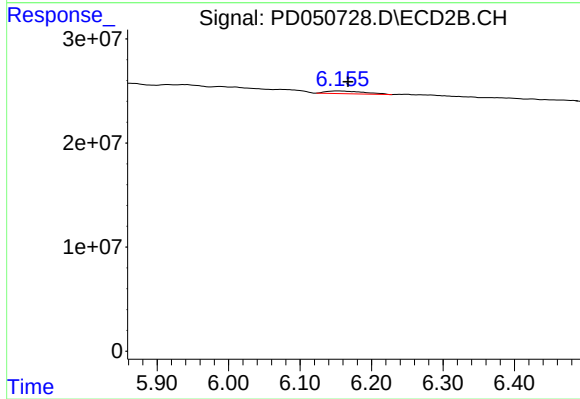

#25 Chlordane-3


R.T.: 6.154 min
Delta R.T.: -0.013 min
Response: 9680981
Conc: 2.40 ng/ml

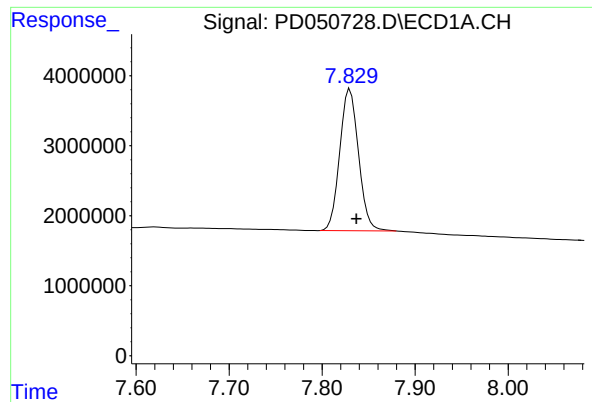

#28 Decachlorobiphenyl

R.T.: 7.830 min
Delta R.T.: -0.007 min
Response: 28436471
Conc: 19.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

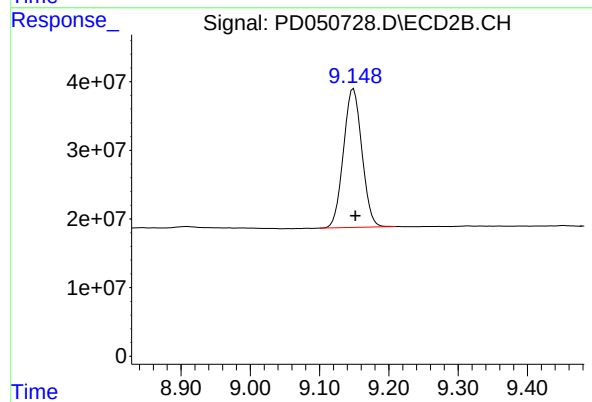

#28 Decachlorobiphenyl

R.T.: 9.149 min
Delta R.T.: -0.003 min
Response: 373382666
Conc: 18.45 ng/ml