

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121020\
 Data File : PD060691.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2020 15:20
 Operator : DD\AJ
 Sample : INDA338
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3038

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 04:47:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 04 03:58:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.501	4.022	21335427	81238301	18.262	20.654
27)	SA Decachlor...	8.288	9.106	52938706	125.7E6	35.511	38.842
Target Compounds							
2)	A alpha-BHC	3.942	4.413	30392553	120.1E6	18.047	20.345
3)	MA gamma-BHC...	4.227	4.698	29152030	109.9E6	18.073	20.496
4)	MA Heptachlor	4.533	5.210	31114638	108.2E6	18.529	20.569
9)	A Endosulfan I	5.571	6.260	26824615	85774841	18.462	20.039
13)	MA Dieldrin	5.816	6.518	57754764	187.7E6	36.367	40.192
14)	MA Endrin	6.074	6.736	47362501	148.3E6	36.605	40.216
16)	A 4,4'-DDD	6.199	6.855	46404932	147.4E6	36.116	39.999
17)	MA 4,4'-DDT	6.442	7.155	48246421	144.7E6	37.043	40.334
20)	A Methoxychlor	6.989	7.611	120.3E6	359.5E6	176.946	199.249

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121020\
Data File : PD060691.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2020 15:20
Operator : DD\AJ
Sample : INDA338
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 04:47:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 04 03:58:39 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

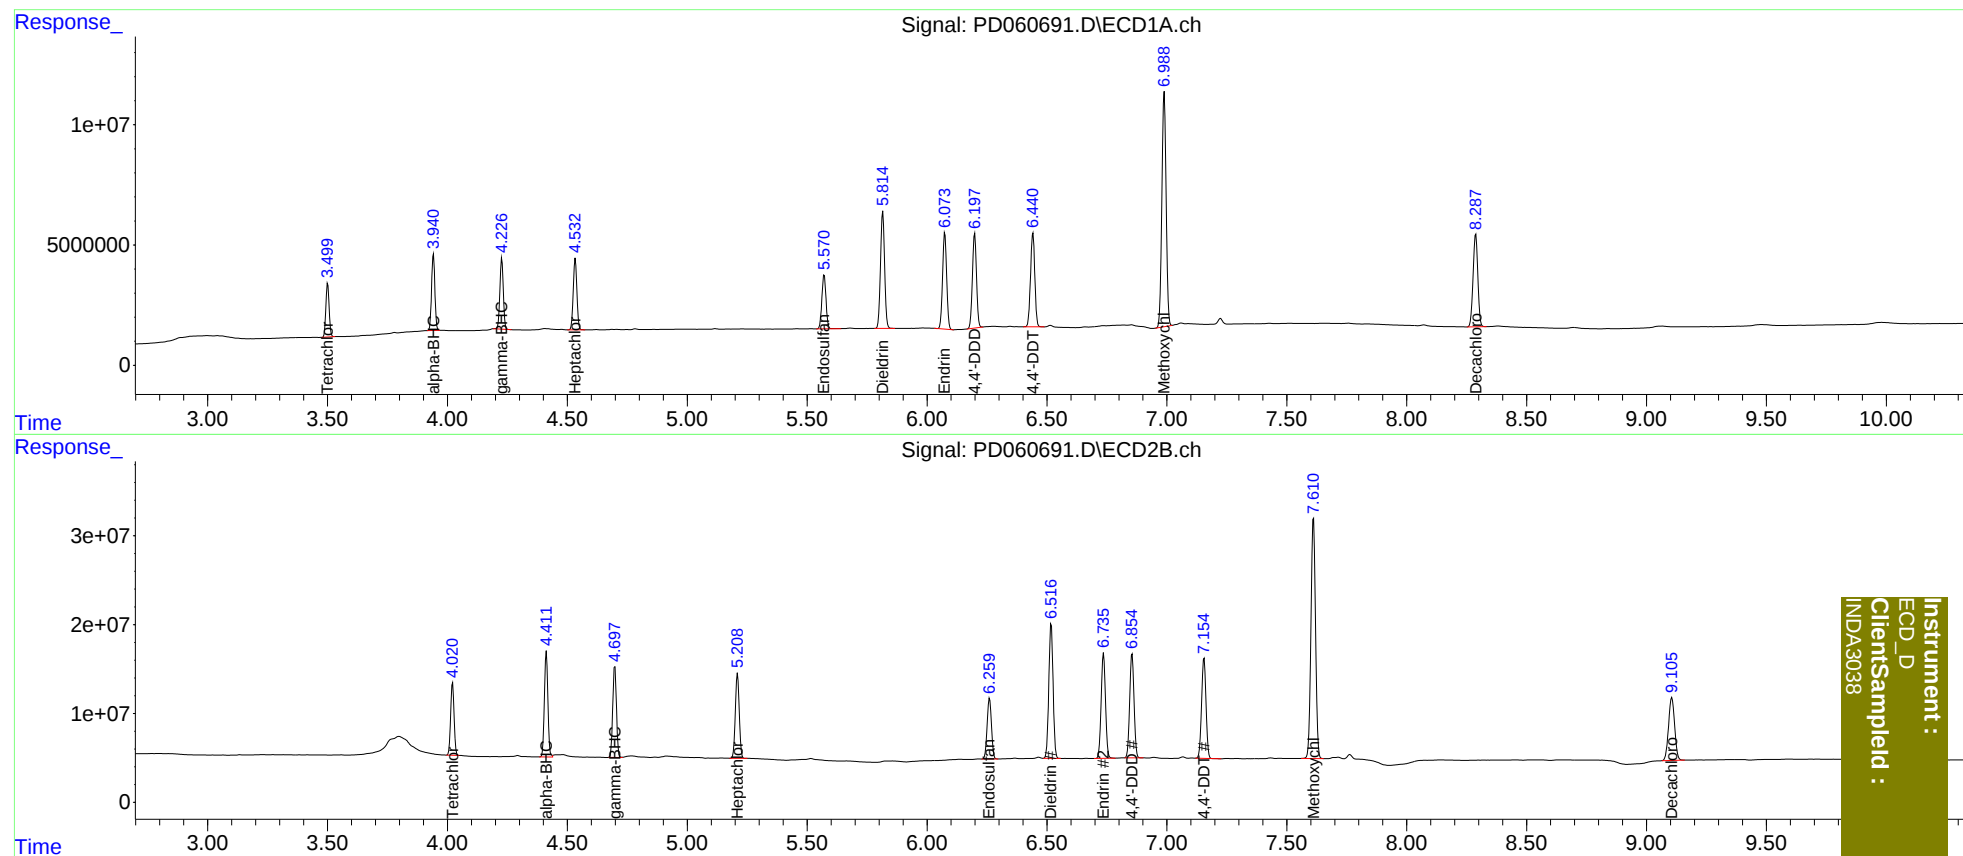

Instrument :
ECD_D
ClientSampled :
INDA3038