

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121020\
 Data File : PD060685.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2020 13:56
 Operator : DD\AJ
 Sample : L4941-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0B34

Manual Integrations
 APPROVED

Ankita
 12/11/2020 4:57:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 04:45:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 04 03:58:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.501	4.022	12394973	47597298	10.609	12.101
2) SA Decachlor...	8.288	9.107	22547356	52680124	15.125	16.274
Target Compounds						
5) MB Aldrin	4.785	5.516	40518041	142.7E6	25.191	28.667
12) B 4,4'-DDE	5.680	6.362	1277969	8601931	0.849	1.948 #
17) MA 4,4'-DDT	6.439	7.153	3694241	8431797	2.836m	2.350m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121020\
Data File : PD060685.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2020 13:56
Operator : DD\AJ
Sample : L4941-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 04:45:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 04 03:58:39 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

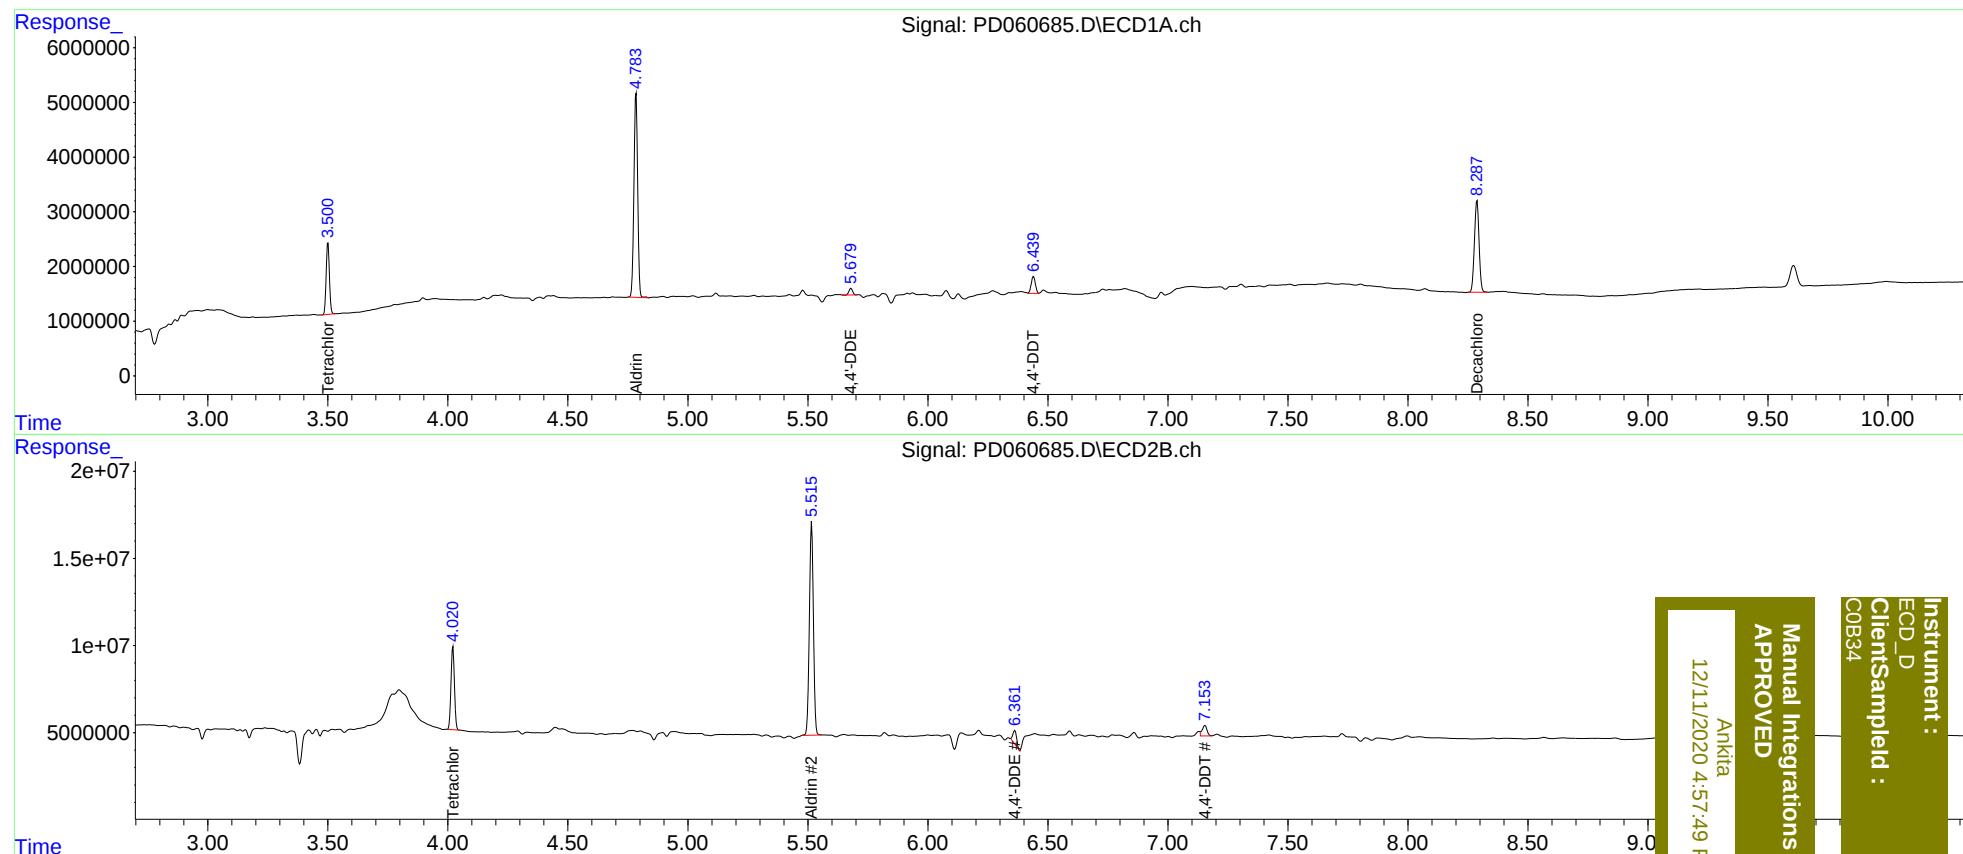

Manual Integrations
APPROVED

Ankita
12/11/2020 4:57:49 PM

Instrument :
ECD_D
ClientSampled :
C0B34