

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121021\
 Data File : PD067259.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2021 13:01
 Operator : AR\AJ
 Sample : M4977-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BI-WEEKLY-DECANT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 21:52:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 17:33:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.966	25904877	66988953	12.537	9.229 #
28)	SA Decachlor...	8.162	9.023	8368998	23527960	7.387	4.680 #
Target Compounds							
6)	B beta-BHC	4.397	4.811	46855207	57878053	34.326	13.130 #
10)	B gamma-Chl...	5.368	6.069	17853242	15459046	6.139m	2.100m#
11)	B alpha-Chl...	5.416	6.140	16165253	16564426	5.690m	2.274m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121021\
Data File : PD067259.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2021 13:01
Operator : AR\AJ
Sample : M4977-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 21:52:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 17:33:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

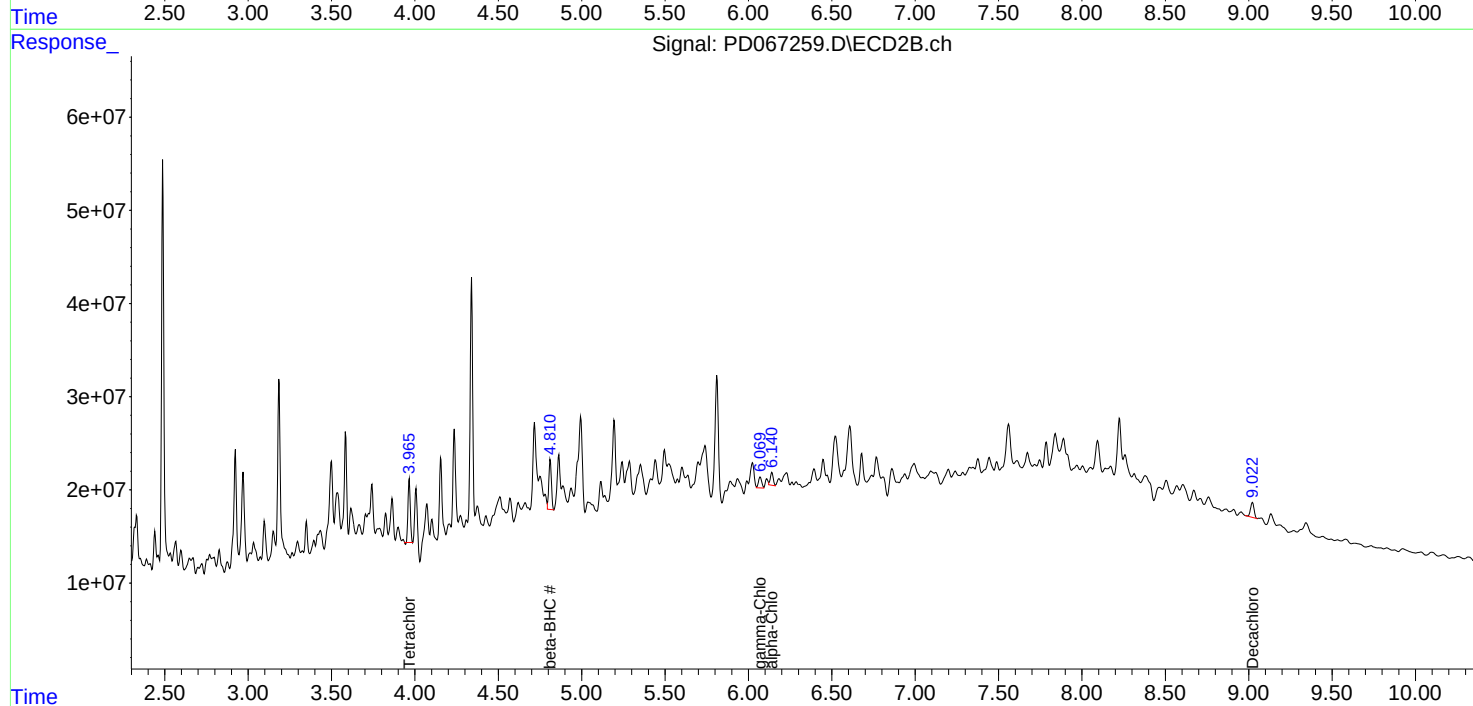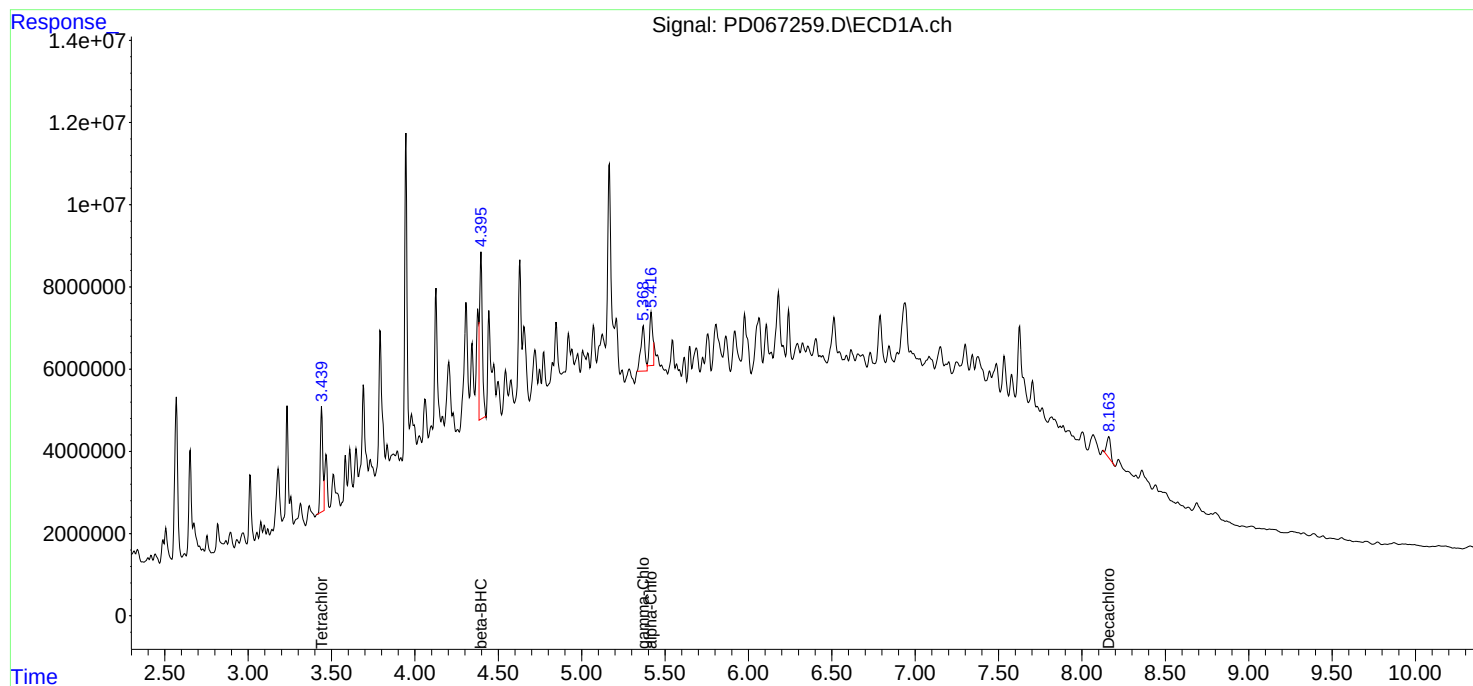


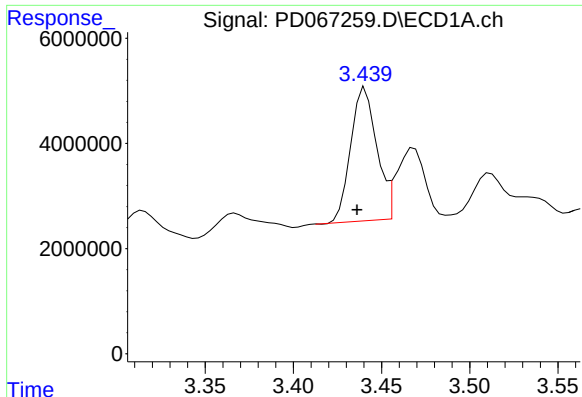

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.005 min
Response: 25904877
Conc: 12.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANT

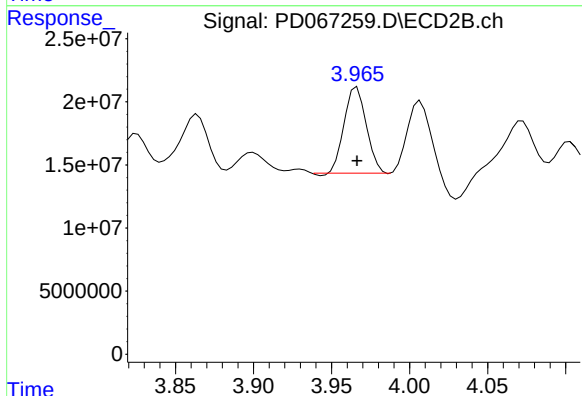


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 66988953
Conc: 9.23 ng/ml

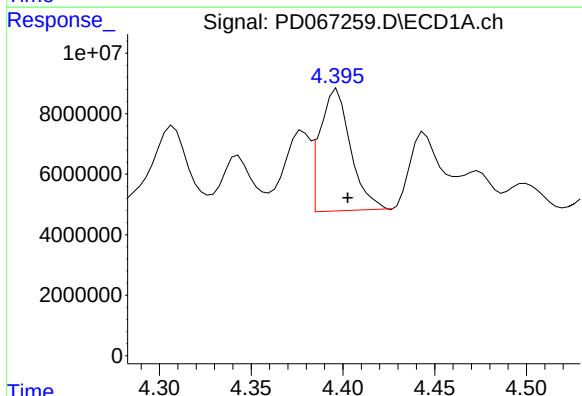


#6 beta-BHC

R.T.: 4.397 min
Delta R.T.: -0.006 min
Response: 46855207
Conc: 34.33 ng/ml

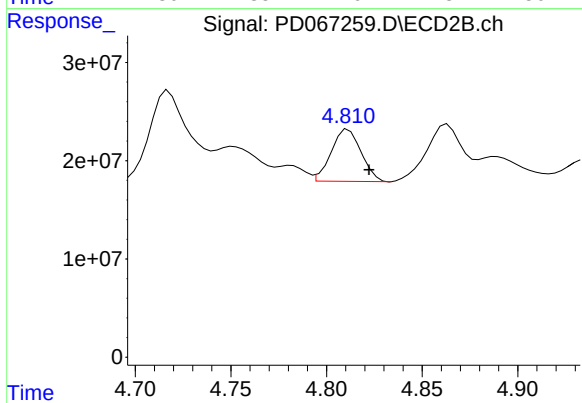

#6 beta-BHC


R.T.: 4.811 min
Delta R.T.: -0.011 min
Response: 57878053
Conc: 13.13 ng/ml

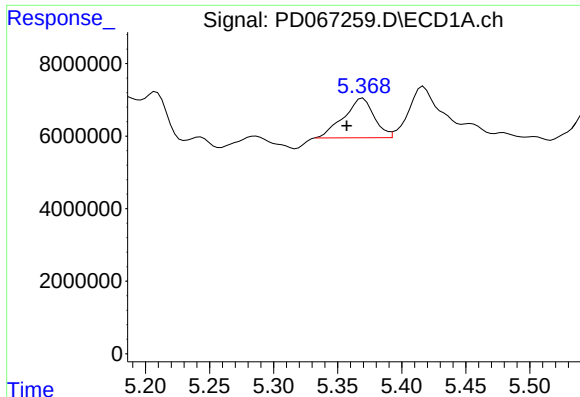

#10 gamma-Chlordane


R.T.: 5.368 min
Delta R.T.: 0.011 min
Response: 17853242
Conc: 6.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANT

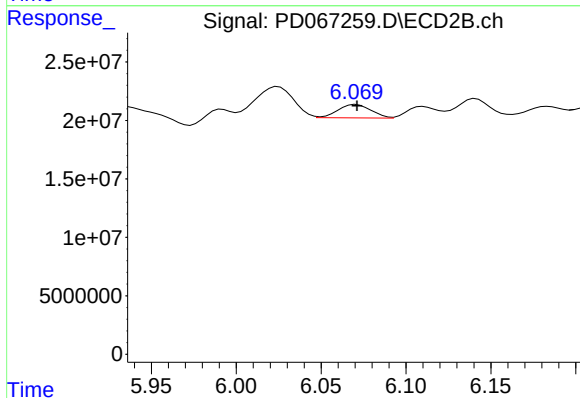


#10 gamma-Chlordane

R.T.: 6.069 min
Delta R.T.: -0.002 min
Response: 15459046
Conc: 2.10 ng/ml m

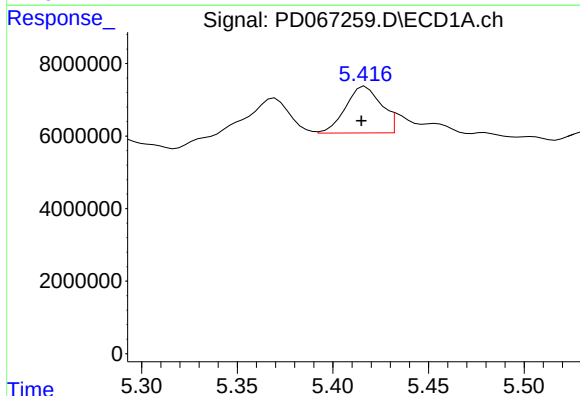


#11 alpha-Chlordane

R.T.: 5.416 min
Delta R.T.: 0.000 min
Response: 16165253
Conc: 5.69 ng/ml m

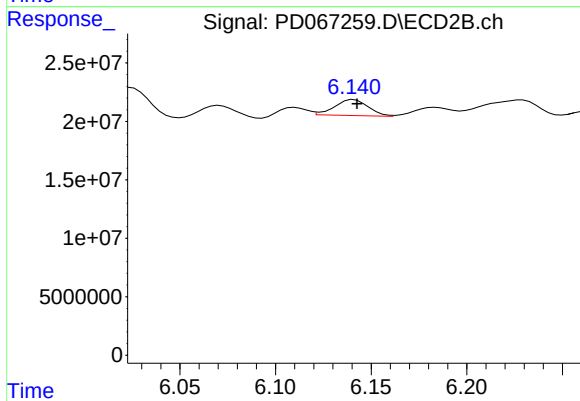

#11 alpha-Chlordane


R.T.: 6.140 min
Delta R.T.: -0.003 min
Response: 16564426
Conc: 2.27 ng/ml m

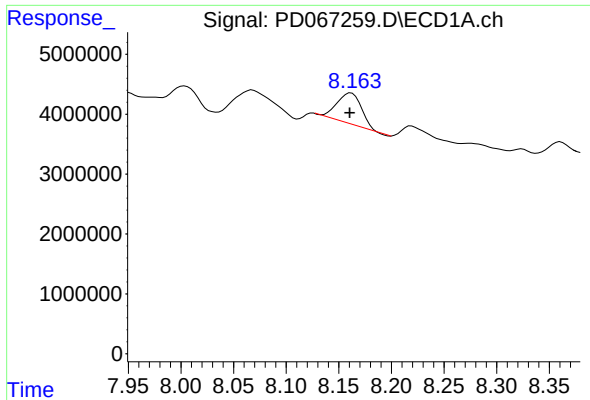

#28 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.001 min
Response: 8368998
Conc: 7.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANT

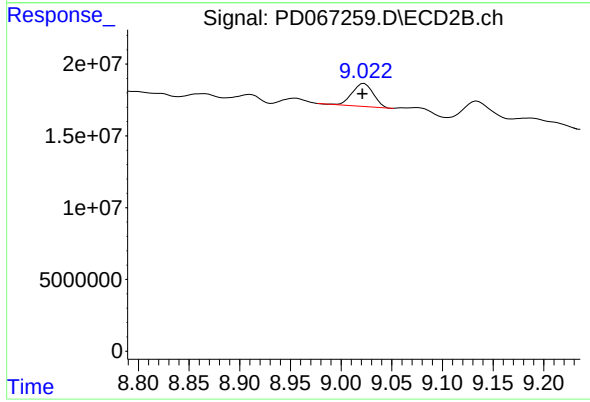

#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.002 min
Response: 23527960
Conc: 4.68 ng/ml