

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121025\
 Data File : PD091536.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2025 15:29
 Operator : AR\AJ
 Sample : Q3812-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 OR-02-120825

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/11/2025
 Supervised By : Yogesh Patel 12/11/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 01:54:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120825.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 04:29:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.869	42914781	607.2E6	12.356m	15.411m
28)	SA Decachlor...	9.064	8.058	73551532	535.1E6	14.150	12.921

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121025\
Data File : PD091536.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2025 15:29
Operator : AR\AJ
Sample : Q3812-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
OR-02-120825


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/11/2025
Supervised By : Yogesh Patel 12/11/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 01:54:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120825.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 04:29:17 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

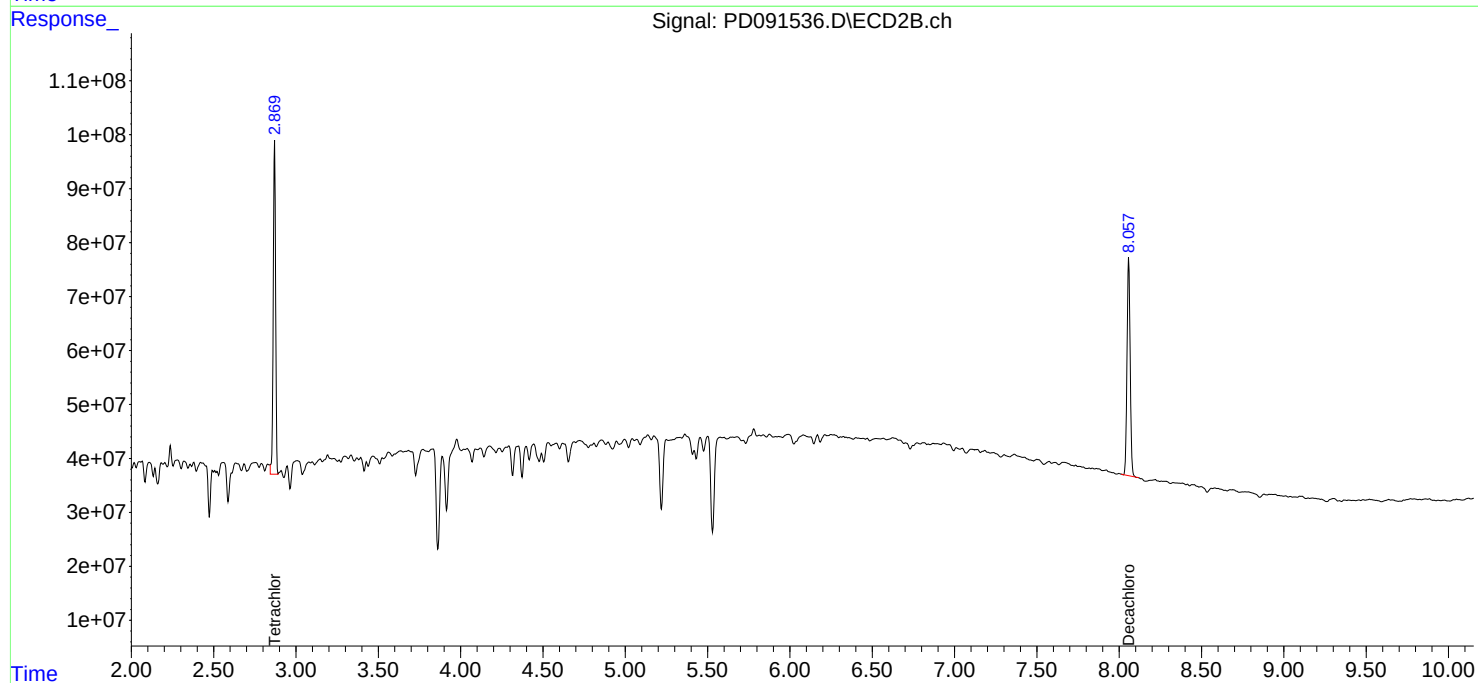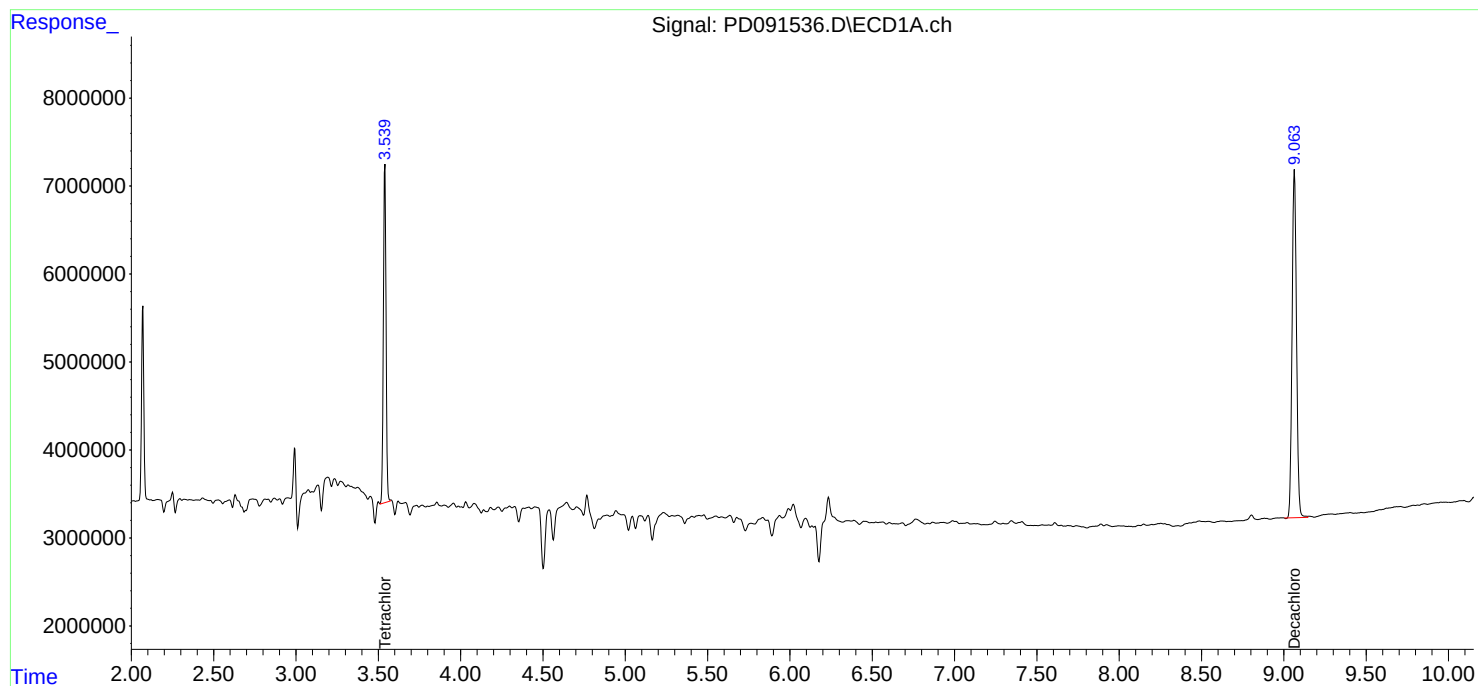

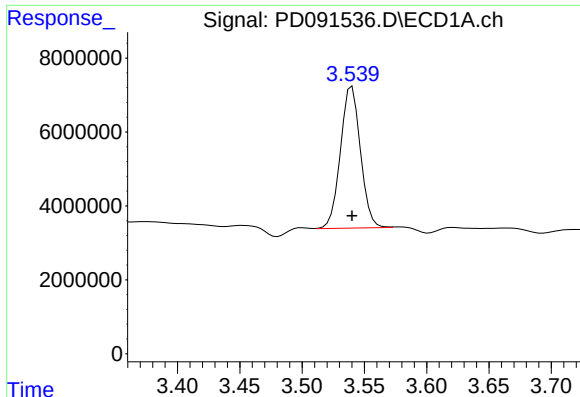


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: -0.001 min
Response: 42914781
Conc: 12.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
OR-02-120825


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/11/2025
Supervised By :Yogesh Patel 12/11/2025

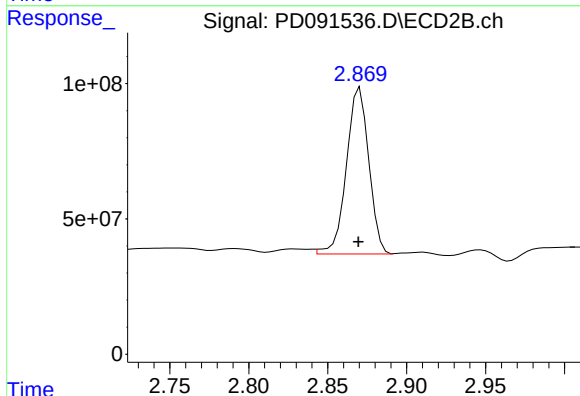


#1 Tetrachloro-m-xylene

R.T.: 2.869 min
Delta R.T.: 0.000 min
Response: 607235493
Conc: 15.41 ng/ml m

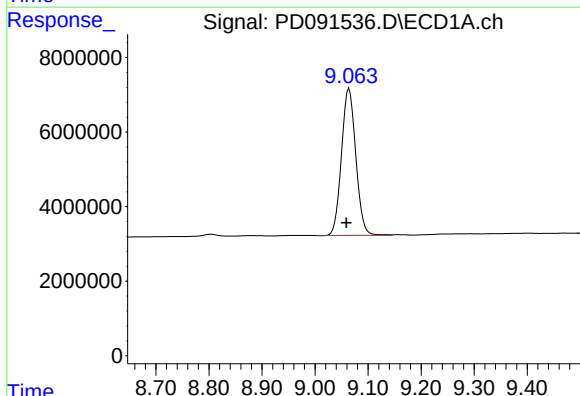

#28 Decachlorobiphenyl

R.T.: 9.064 min
Delta R.T.: 0.005 min
Response: 73551532
Conc: 14.15 ng/ml

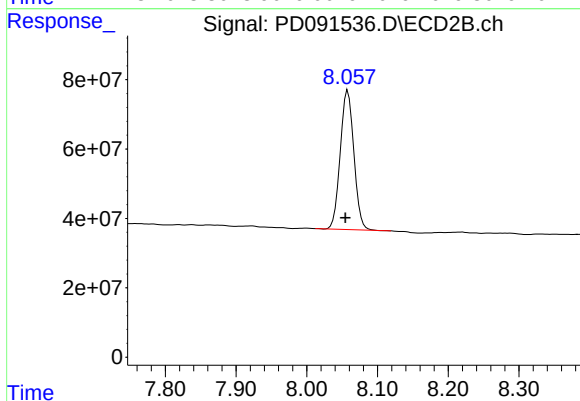

#28 Decachlorobiphenyl

R.T.: 8.058 min
Delta R.T.: 0.003 min
Response: 535059938
Conc: 12.92 ng/ml